

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB022223\
 Data File : FB029369.D
 Signal(s) : FID2B.CH
 Acq On : 22 Feb 2023 15:23
 Operator : YP/AJ
 Sample : 01627-07
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 11 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Feb 23 00:25:22 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB020623.M
 Quant Title :
 QLast Update : Mon Feb 06 14:33:16 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.792	205342	21.349 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.710	87710	5.528 ng/ml
2) t	2,2,4-Trimethylpentane	7.416	103796	6.026 ng/mlm
3) t	n-Heptane	7.754	35448	1.959 ng/ml
4) t	Benzene	7.887	40929	1.965 ng/ml
6) t	Toluene	10.621	120275	5.935 ng/ml
7) t	Ethylbenzene	13.058	37603	1.970 ng/ml
8) t	m-Xylene	13.190	74078	3.908 ng/ml
9) t	O-Xylene	13.916	74593	4.088 ng/ml
10) t	1,2,4-Trimethylbenzene	16.191	74805	3.975 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB022223\
Data File : FB029369.D
Signal(s) : FID2B.CH
Acq On : 22 Feb 2023 15:23
Operator : YP/AJ
Sample : 01627-07
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 11 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Feb 23 00:25:22 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB020623.M
Quant Title :
QLast Update : Mon Feb 06 14:33:16 2023
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

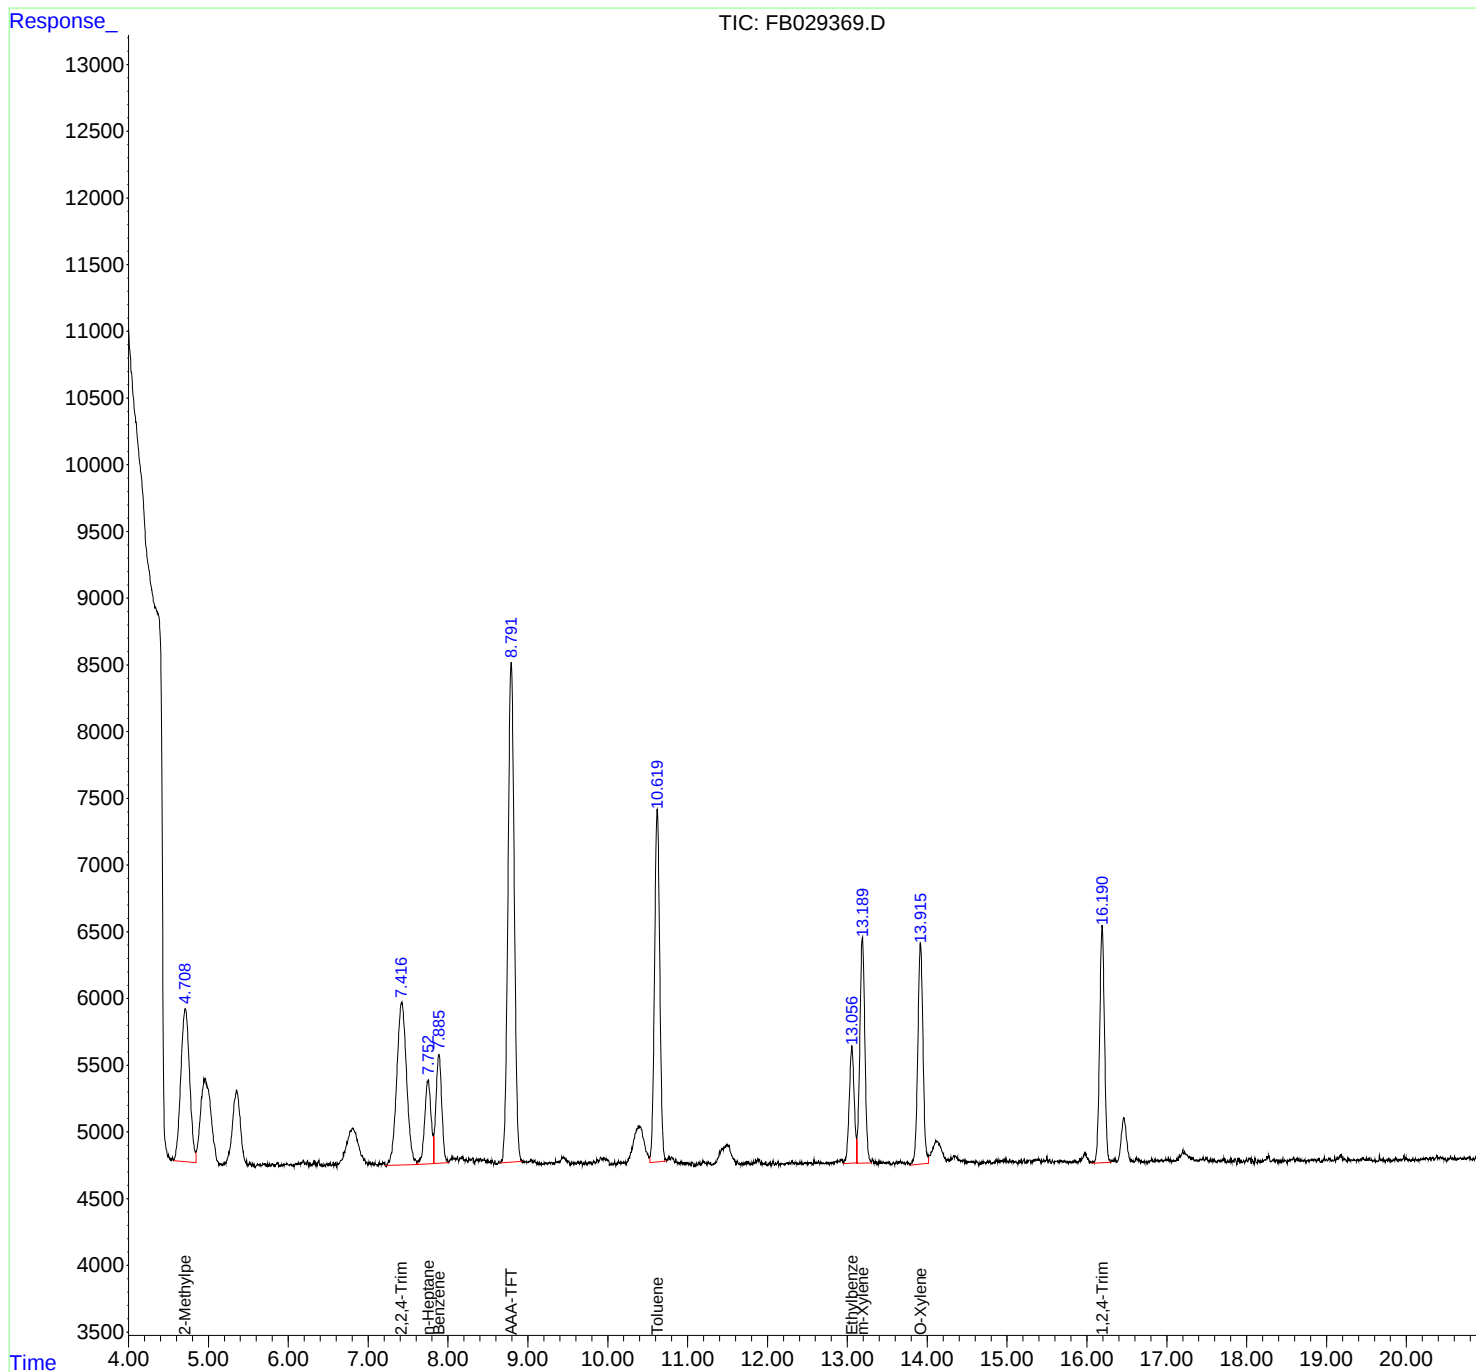

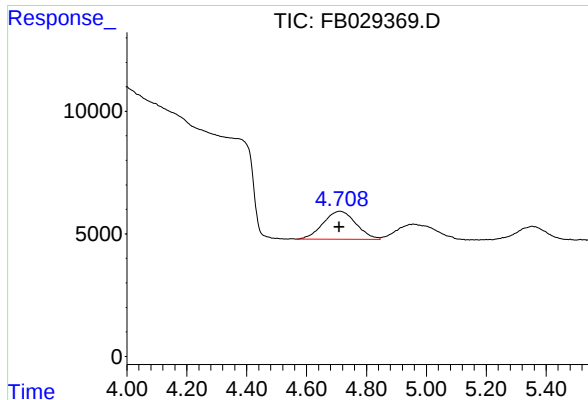


#1 2-Methylpentane

R.T.: 4.710 min
Delta R.T.: 0.001 min
Response: 87710
Conc: 5.53 ng/ml

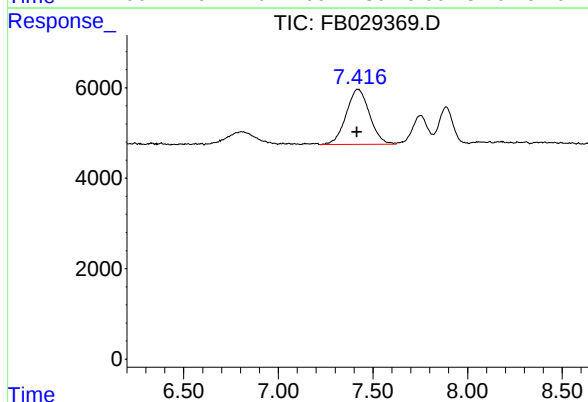


#2 2,2,4-Trimethylpentane

R.T.: 7.416 min
Delta R.T.: 0.002 min
Response: 103796
Conc: 6.03 ng/ml m

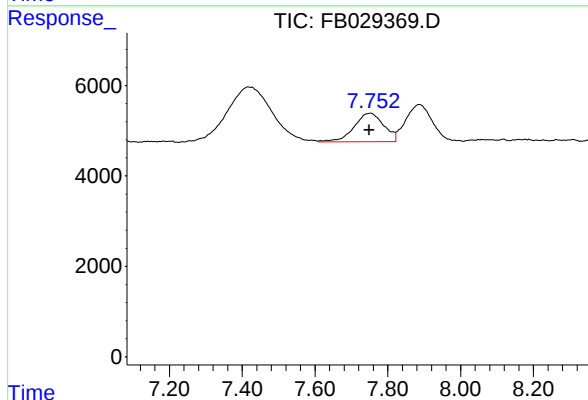


#3 n-Heptane

R.T.: 7.754 min
Delta R.T.: 0.005 min
Response: 35448
Conc: 1.96 ng/ml

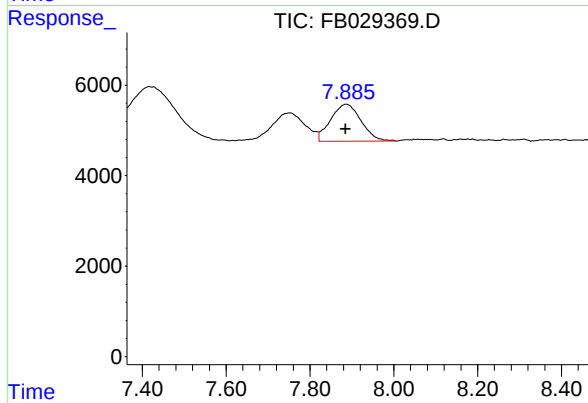


#4 Benzene

R.T.: 7.887 min
Delta R.T.: 0.002 min
Response: 40929
Conc: 1.96 ng/ml

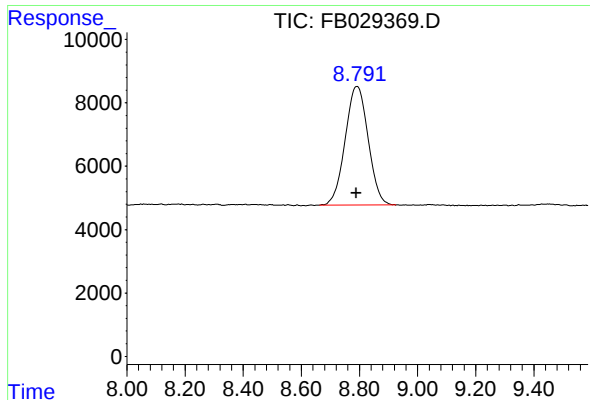


#5 AAA-TFT

R.T.: 8.792 min
Delta R.T.: 0.003 min
Response: 205342
Conc: 21.35 ng/ml

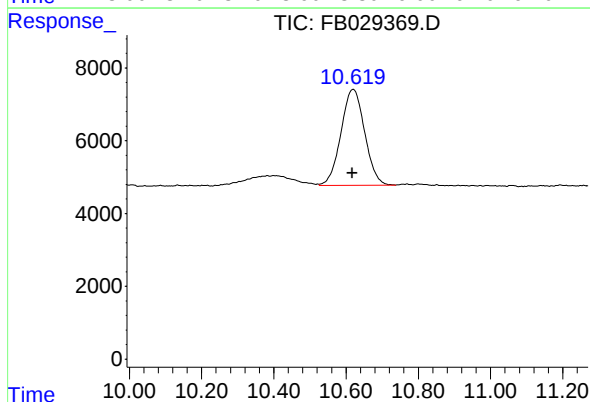


#6 Toluene

R.T.: 10.621 min
Delta R.T.: 0.004 min
Response: 120275
Conc: 5.94 ng/ml

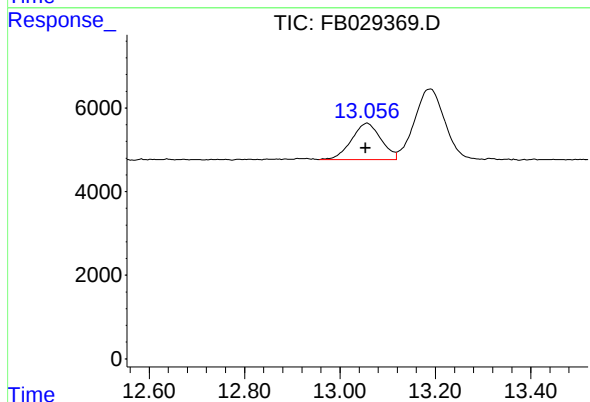


#7 Ethylbenzene

R.T.: 13.058 min
Delta R.T.: 0.004 min
Response: 37603
Conc: 1.97 ng/ml

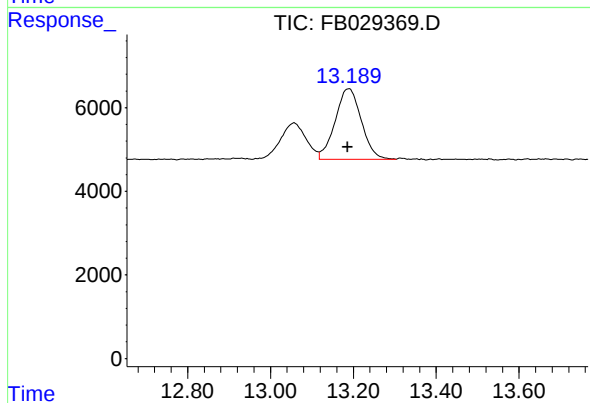


#8 m-Xylene

R.T.: 13.190 min
Delta R.T.: 0.004 min
Response: 74078
Conc: 3.91 ng/ml

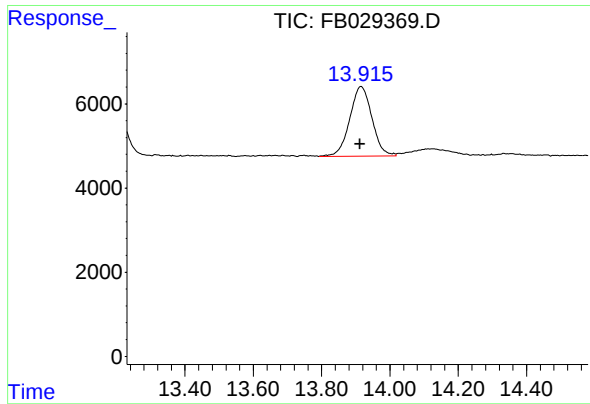

#9 O-Xylene

R.T.: 13.916 min
Delta R.T.: 0.003 min
Response: 74593
Conc: 4.09 ng/ml

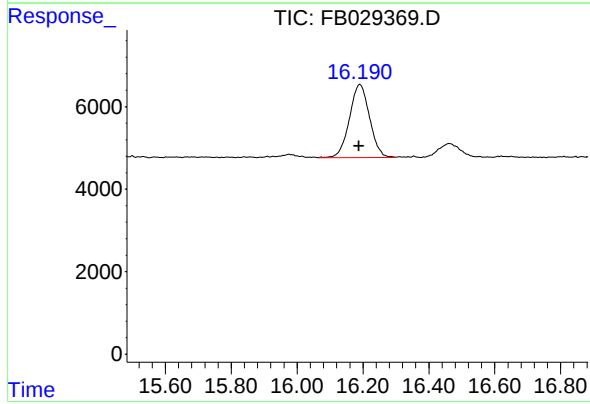

#10 1,2,4-Trimethylbenzene

R.T.: 16.191 min
Delta R.T.: 0.003 min
Response: 74805
Conc: 3.98 ng/ml