

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB022321\
 Data File : FB025450.D
 Signal(s) : FID2B.CH
 Acq On : 23 Feb 2021 13:07
 Operator : DD/AJ
 Sample : M1458-02
 Misc : 5.00g/5.00ml DI WATER
 ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Feb 24 02:04:03 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB021921.M
 Quant Title :
 QLast Update : Mon Feb 22 11:51:04 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.804	467356	18.425 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.693	250854	7.117 ng/ml
2) t 2,2,4-Trimethylpentane	7.422	273124	7.355 ng/ml
3) t n-Heptane	7.764	86872	2.400 ng/ml
4) t Benzene	7.901	107336	2.323 ng/ml
6) t Toluene	10.636	307171	6.870 ng/ml
7) t Ethylbenzene	13.077	99655	2.469 ng/ml
8) t m-Xylene	13.210	194647	4.839 ng/ml
9) t O-Xylene	13.937	185428	4.790 ng/ml
10) t 1,2,4-Trimethylbenzene	16.216	153746	4.580 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB022321\
Data File : FB025450.D
Signal(s) : FID2B.CH
Acq On : 23 Feb 2021 13:07
Operator : DD/AJ
Sample : M1458-02
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Feb 24 02:04:03 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB021921.M
Quant Title :
QLast Update : Mon Feb 22 11:51:04 2021
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

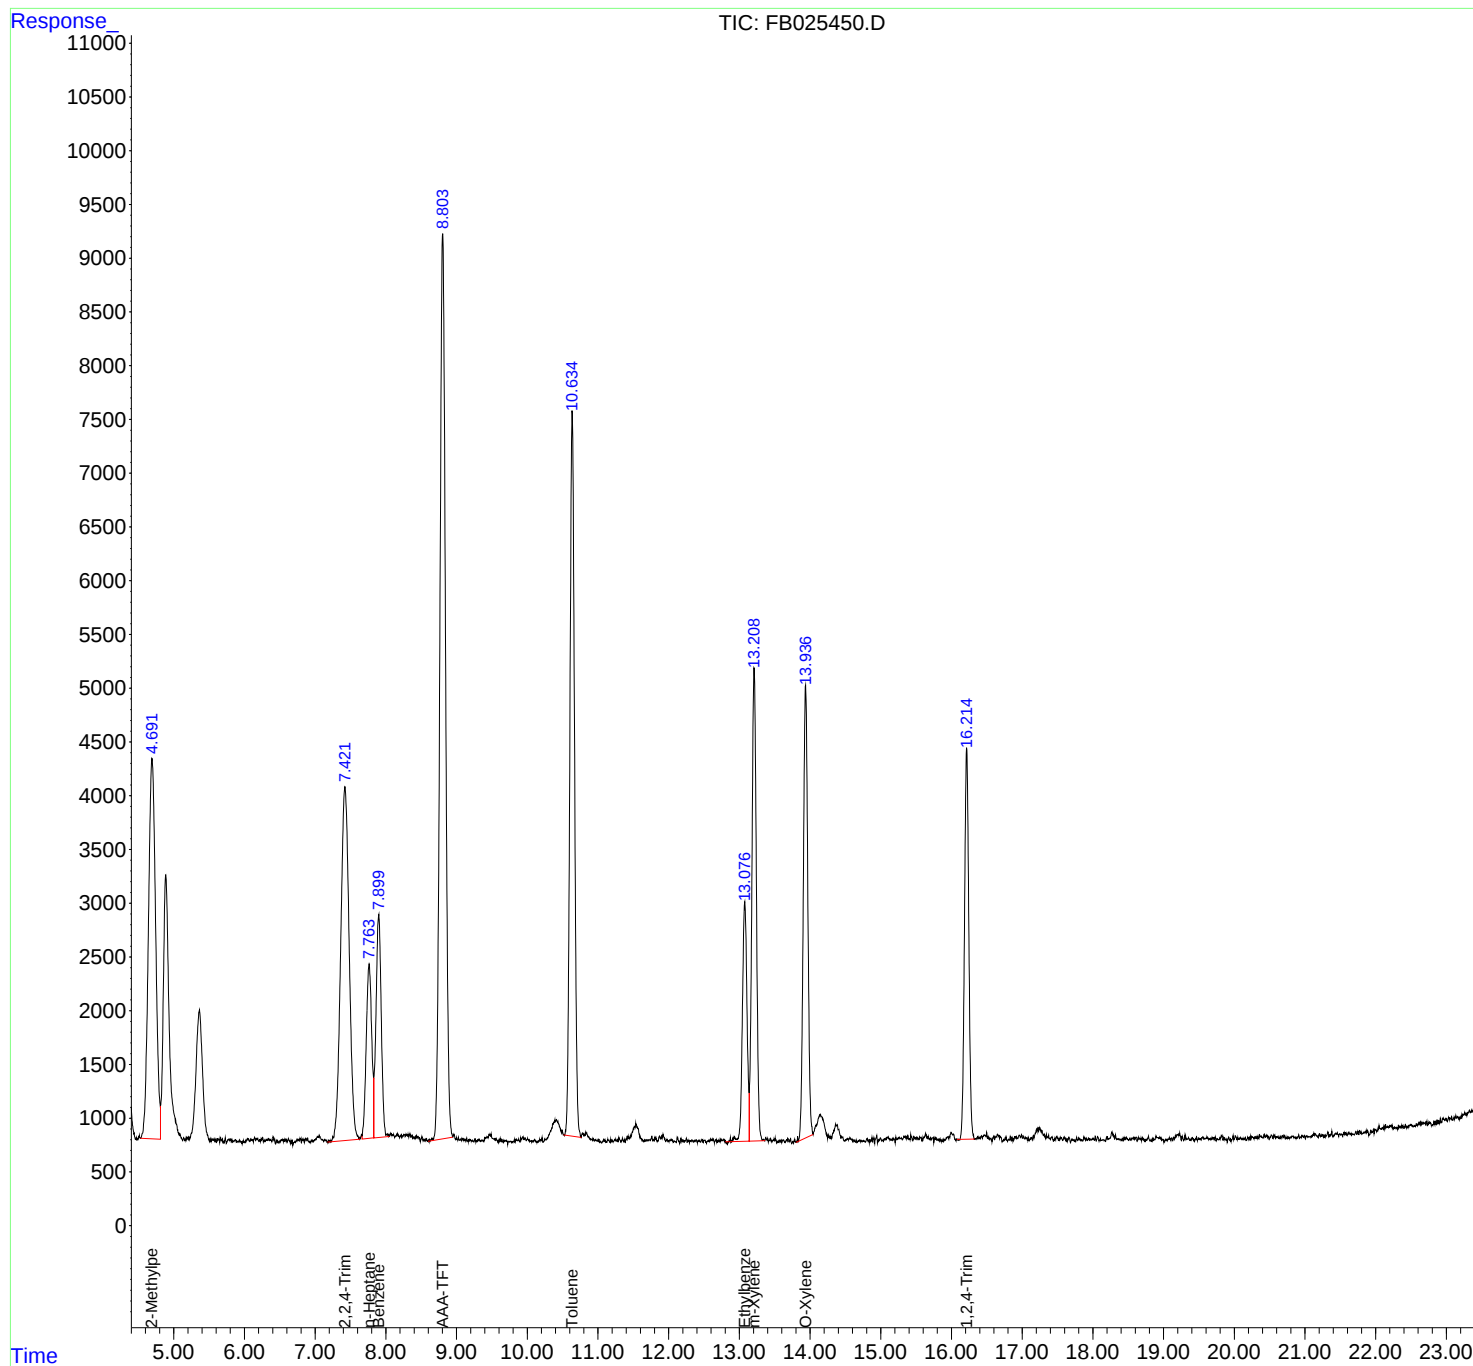

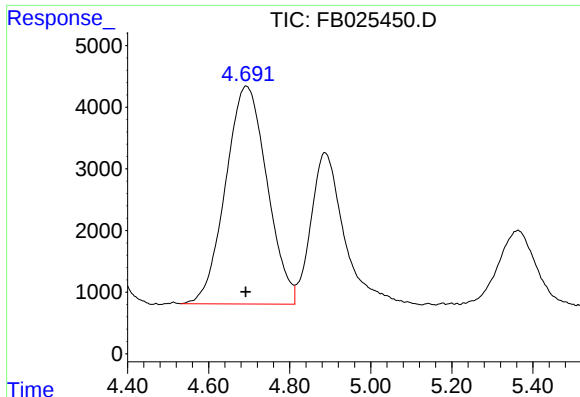


#1 2-Methylpentane

R.T.: 4.693 min
Delta R.T.: 0.001 min
Response: 250854
Conc: 7.12 ng/ml

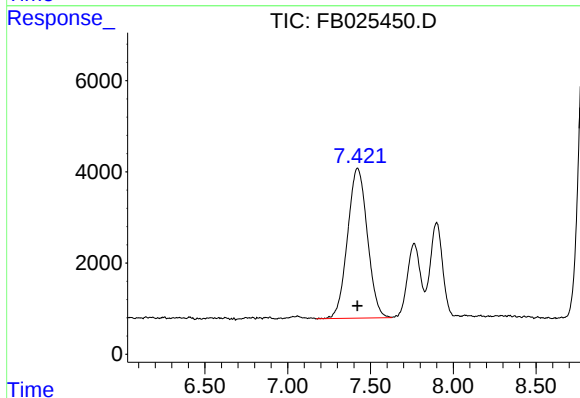


#2 2,2,4-Trimethylpentane

R.T.: 7.422 min
Delta R.T.: 0.000 min
Response: 273124
Conc: 7.36 ng/ml

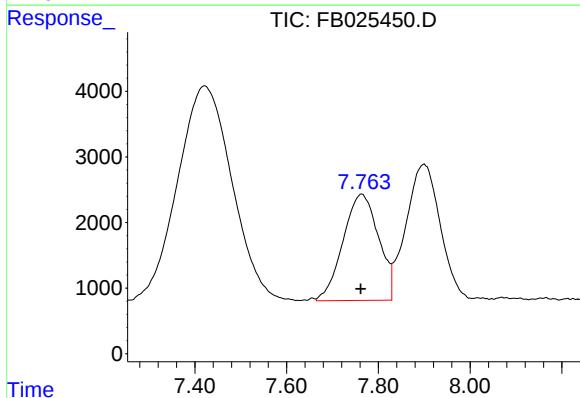


#3 n-Heptane

R.T.: 7.764 min
Delta R.T.: 0.003 min
Response: 86872
Conc: 2.40 ng/ml

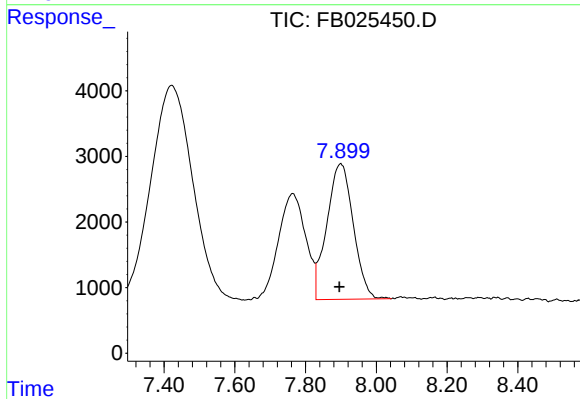


#4 Benzene

R.T.: 7.901 min
Delta R.T.: 0.005 min
Response: 107336
Conc: 2.32 ng/ml

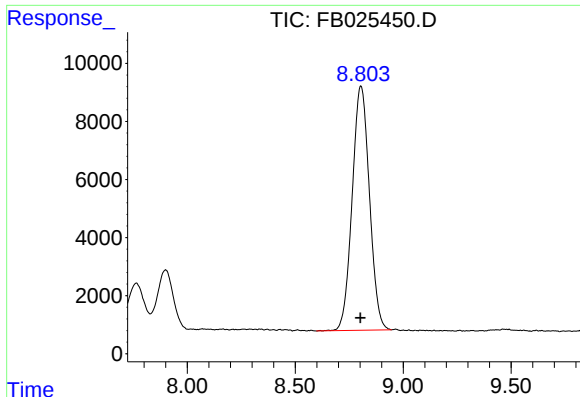


#5 AAA-TFT

R.T.: 8.804 min
Delta R.T.: 0.002 min
Response: 467356
Conc: 18.43 ng/ml

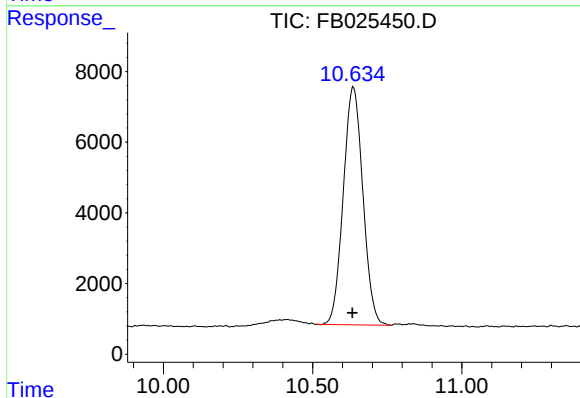


#6 Toluene

R.T.: 10.636 min
Delta R.T.: 0.002 min
Response: 307171
Conc: 6.87 ng/ml

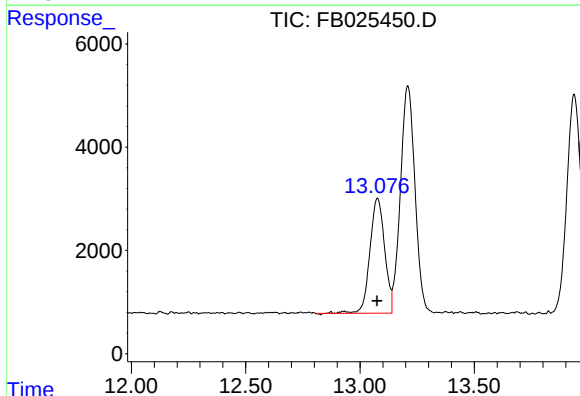


#7 Ethylbenzene

R.T.: 13.077 min
Delta R.T.: 0.003 min
Response: 99655
Conc: 2.47 ng/ml

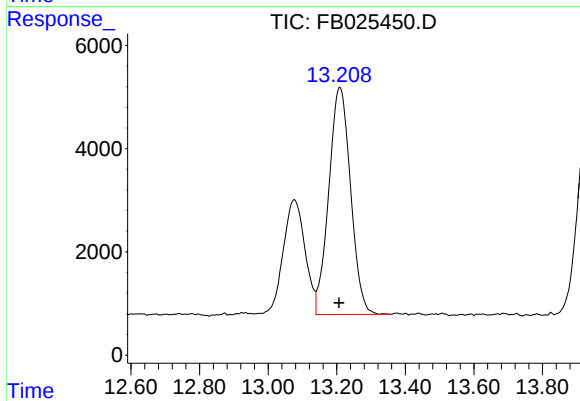


#8 m-Xylene

R.T.: 13.210 min
Delta R.T.: 0.003 min
Response: 194647
Conc: 4.84 ng/ml

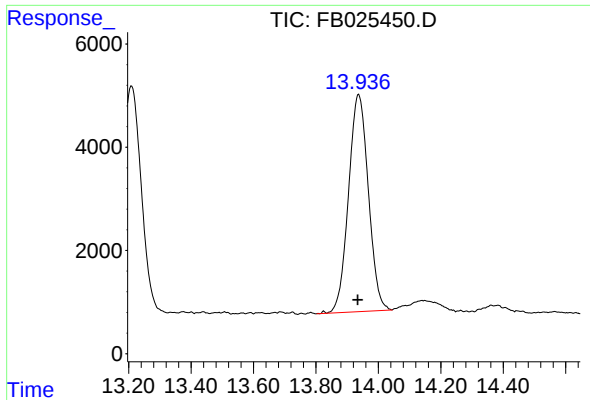

#9 O-Xylene

R.T.: 13.937 min
Delta R.T.: 0.003 min
Response: 185428
Conc: 4.79 ng/ml

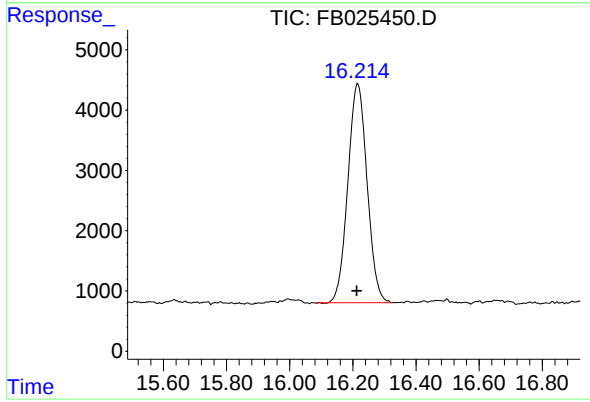

#10 1,2,4-Trimethylbenzene

R.T.: 16.216 min
Delta R.T.: 0.004 min
Response: 153746
Conc: 4.58 ng/ml