

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB022323\
 Data File : FB029373.D
 Signal(s) : FID2B.CH
 Acq On : 23 Feb 2023 9:29
 Operator : YP/AJ
 Sample : VBF0223S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 2 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Feb 24 01:28:48 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB020623.M
 Quant Title :
 QLast Update : Mon Feb 06 14:33:16 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.789	199706	20.763 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.715	27795	1.752 ng/ml
2) t	2,2,4-Trimethylpentane	7.417	24160	1.403 ng/ml
3) t	n-Heptane	7.754	10671	0.590 ng/ml
4) t	Benzene	7.886	6794	0.326 ng/ml
6) t	Toluene	10.619	23463	1.158 ng/ml
7) t	Ethylbenzene	13.052	7907	0.414 ng/ml
8) t	m-Xylene	13.187	13600	0.717 ng/ml
9) t	O-Xylene	13.913	12238	0.671 ng/ml
10) t	1,2,4-Trimethylbenzene	16.189	14937	0.794 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB022323\
Data File : FB029373.D
Signal(s) : FID2B.CH
Acq On : 23 Feb 2023 9:29
Operator : YP/AJ
Sample : VBF0223S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 2 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Feb 24 01:28:48 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB020623.M
Quant Title :
QLast Update : Mon Feb 06 14:33:16 2023
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

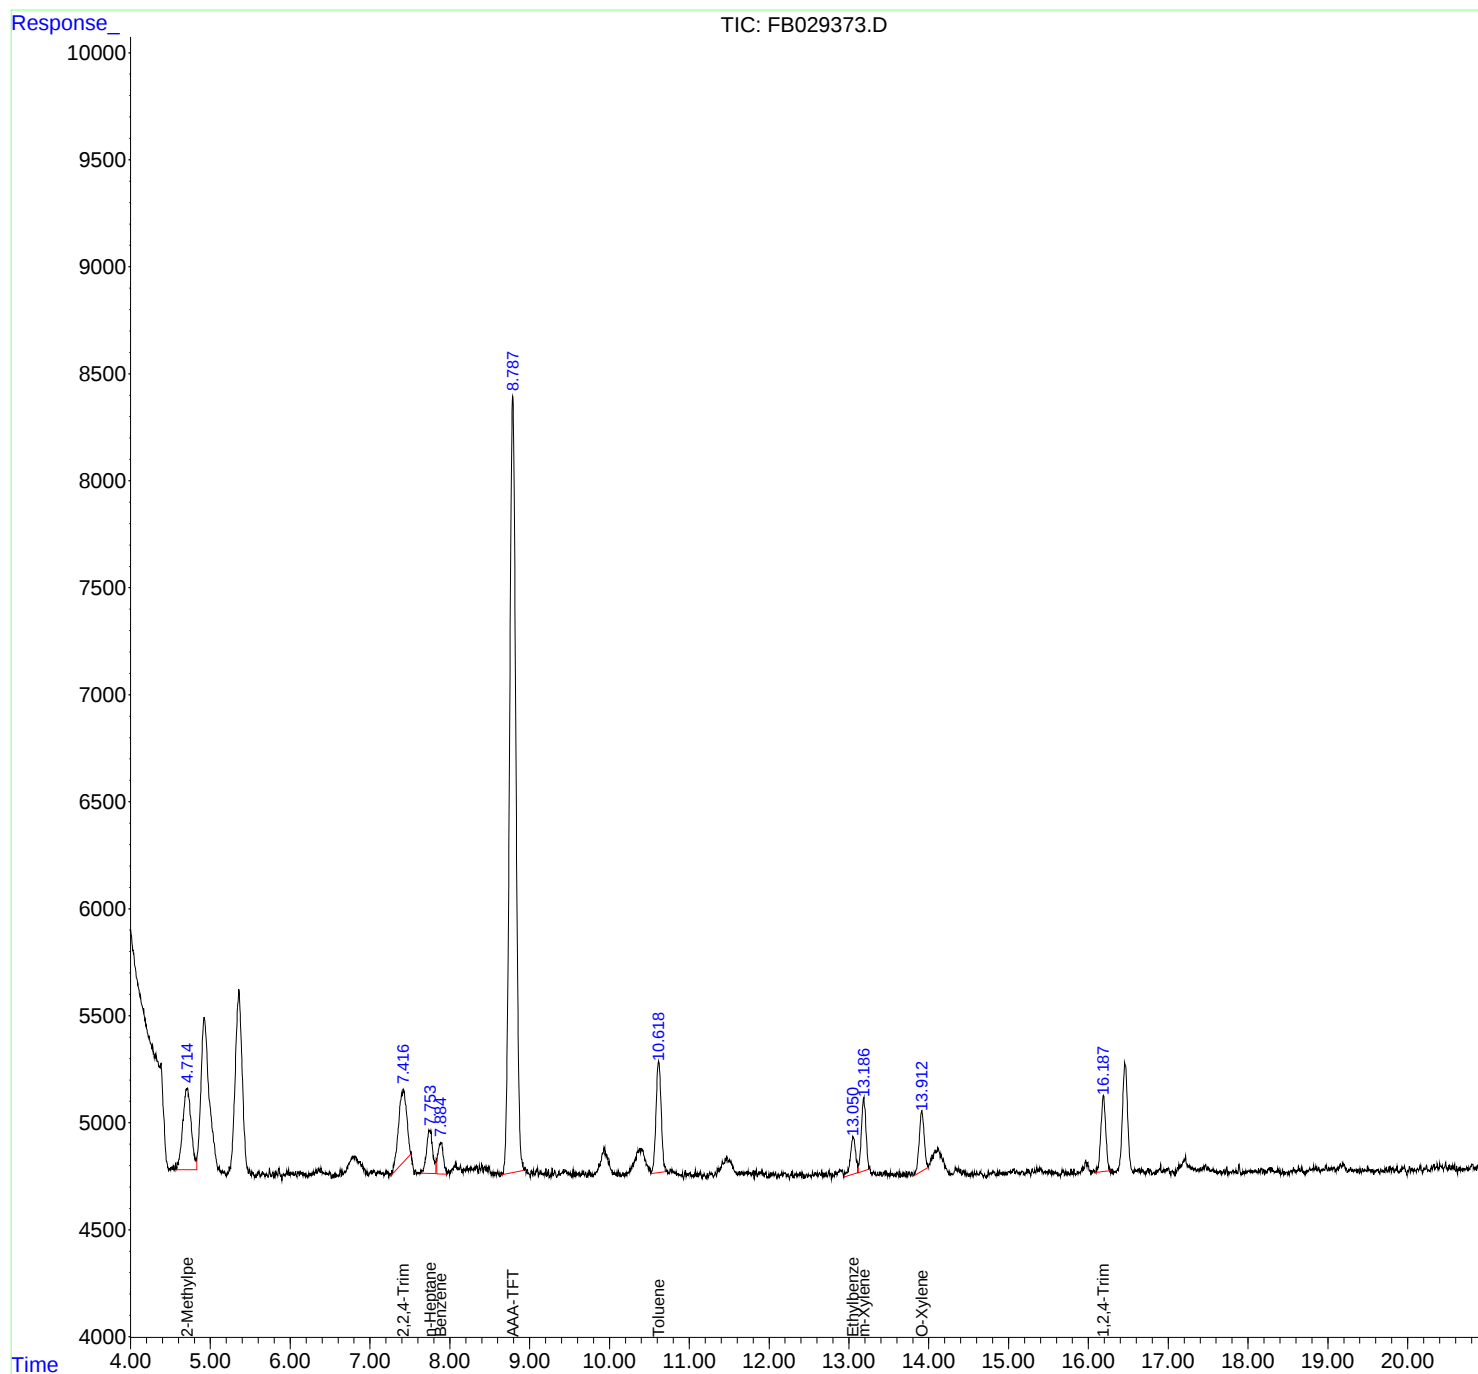

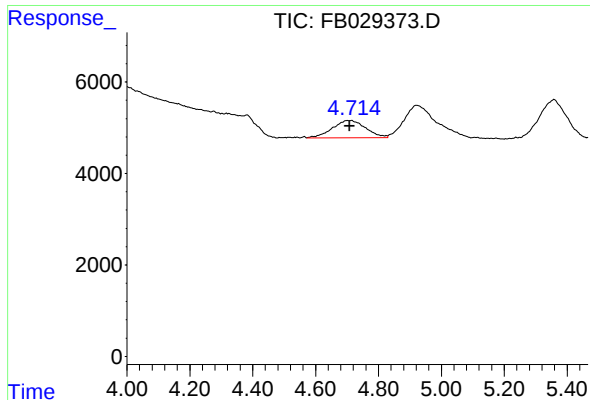


#1 2-Methylpentane

R.T.: 4.715 min
Delta R.T.: 0.006 min
Response: 27795
Conc: 1.75 ng/ml

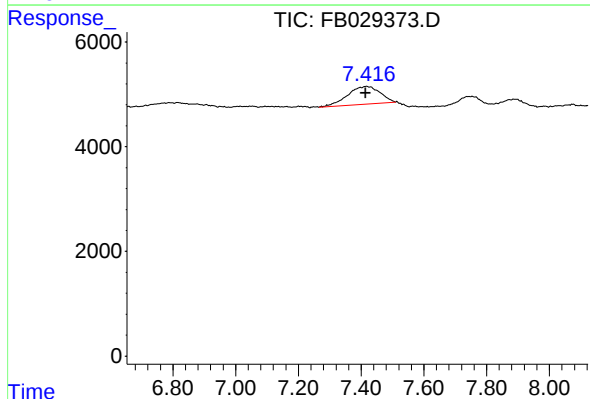


#2 2,2,4-Trimethylpentane

R.T.: 7.417 min
Delta R.T.: 0.003 min
Response: 24160
Conc: 1.40 ng/ml

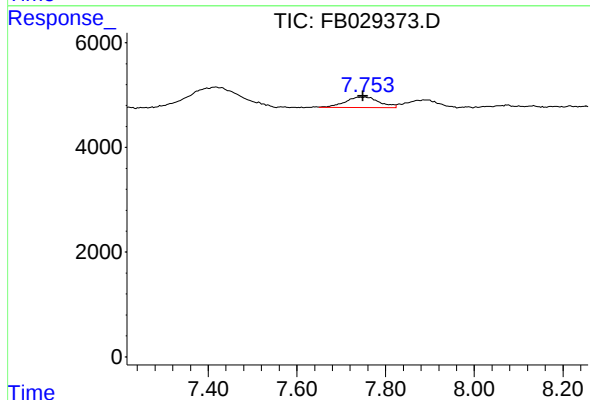


#3 n-Heptane

R.T.: 7.754 min
Delta R.T.: 0.006 min
Response: 10671
Conc: 0.59 ng/ml

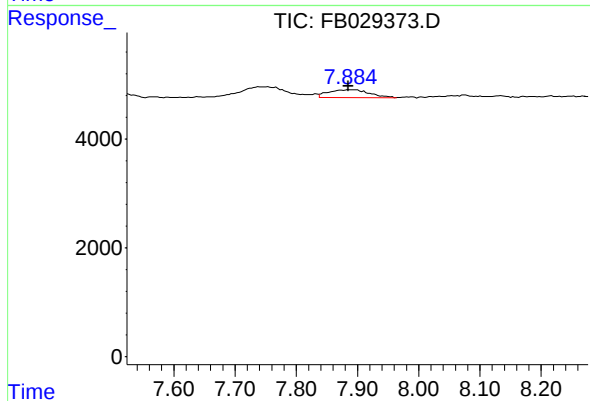


#4 Benzene

R.T.: 7.886 min
Delta R.T.: 0.001 min
Response: 6794
Conc: 0.33 ng/ml

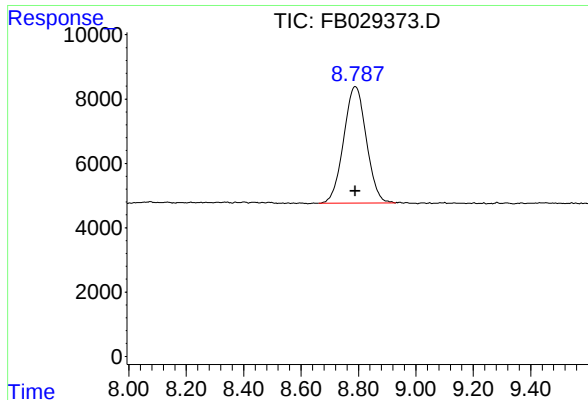


#5 AAA-TFT

R.T.: 8.789 min
Delta R.T.: 0.000 min
Response: 199706
Conc: 20.76 ng/ml

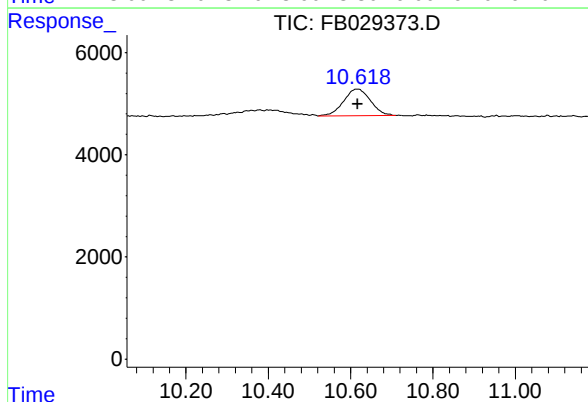


#6 Toluene

R.T.: 10.619 min
Delta R.T.: 0.002 min
Response: 23463
Conc: 1.16 ng/ml

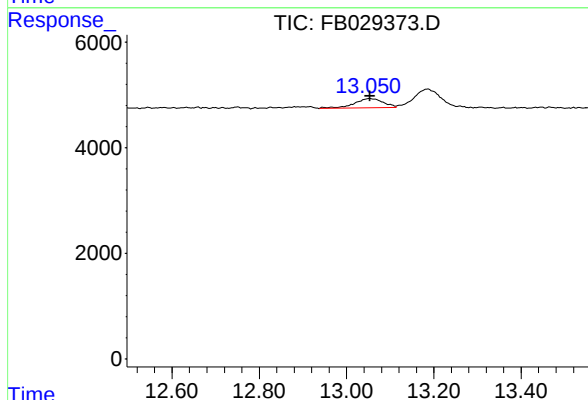


#7 Ethylbenzene

R.T.: 13.052 min
Delta R.T.: -0.002 min
Response: 7907
Conc: 0.41 ng/ml

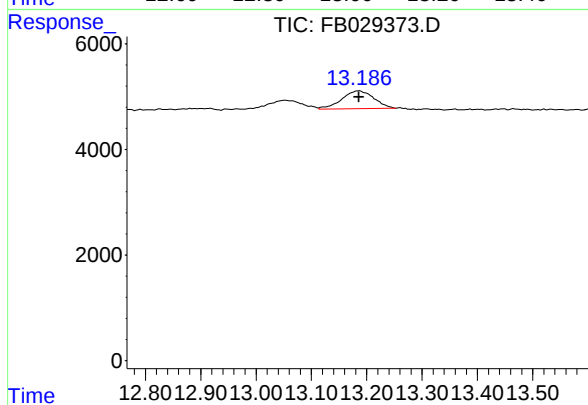


#8 m-Xylene

R.T.: 13.187 min
Delta R.T.: 0.001 min
Response: 13600
Conc: 0.72 ng/ml

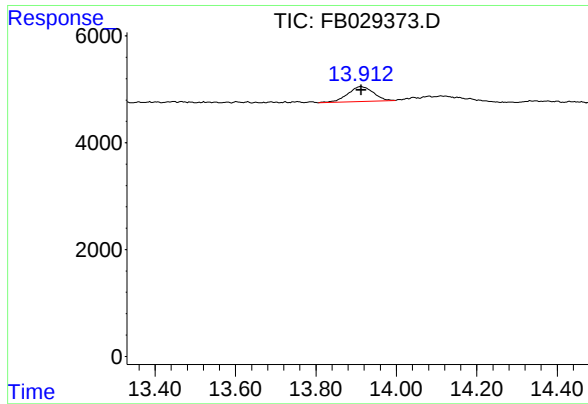

#9 O-Xylene

R.T.: 13.913 min
Delta R.T.: 0.000 min
Response: 12238
Conc: 0.67 ng/ml

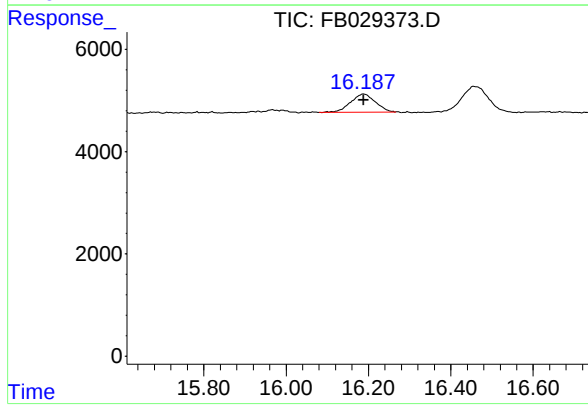

#10 1,2,4-Trimethylbenzene

R.T.: 16.189 min
Delta R.T.: 0.000 min
Response: 14937
Conc: 0.79 ng/ml