

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB022323\
 Data File : FB029376.D
 Signal(s) : FID2B.CH
 Acq On : 23 Feb 2023 11:20
 Operator : YP/AJ
 Sample : 01627-03
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 5 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Feb 24 01:29:07 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB020623.M
 Quant Title :
 QLast Update : Mon Feb 06 14:33:16 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.792	234602	24.391 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.709	21196	1.336 ng/ml
2) t	2,2,4-Trimethylpentane	7.423	26525	1.540 ng/ml
3) t	n-Heptane	7.743	2394	0.132 ng/ml
4) t	Benzene	7.887	10101	0.485 ng/ml
6) t	Toluene	10.621	31263	1.543 ng/ml
7) t	Ethylbenzene	13.057	9967	0.522 ng/ml
8) t	m-Xylene	13.191	20053	1.058 ng/ml
9) t	O-Xylene	13.917	19232	1.054 ng/ml
10) t	1,2,4-Trimethylbenzene	16.193	22986	1.221 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB022323\
Data File : FB029376.D
Signal(s) : FID2B.CH
Acq On : 23 Feb 2023 11:20
Operator : YP/AJ
Sample : 01627-03
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 5 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Feb 24 01:29:07 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB020623.M
Quant Title :
QLast Update : Mon Feb 06 14:33:16 2023
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

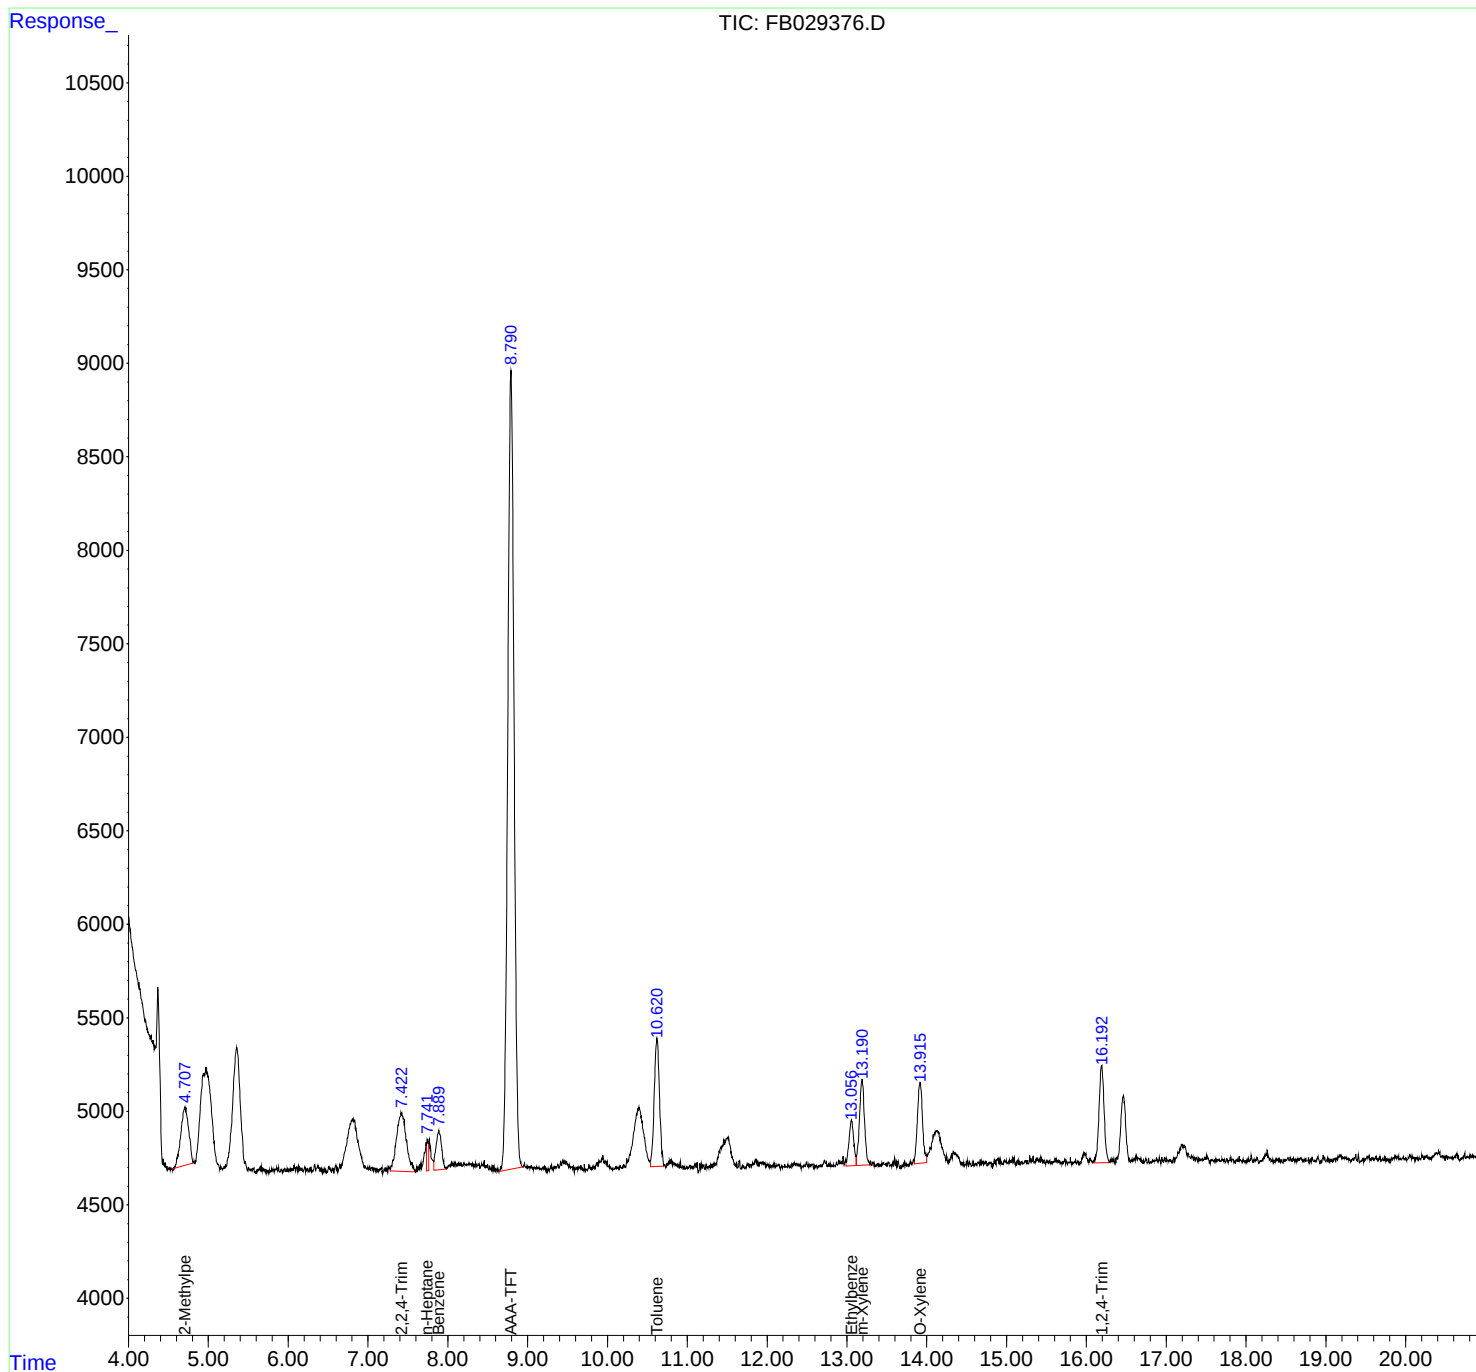

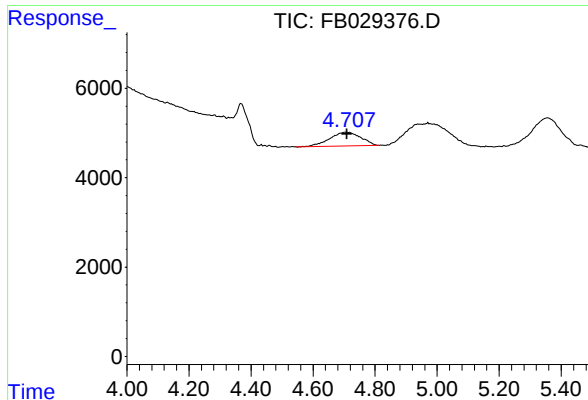


#1 2-Methylpentane

R.T.: 4.709 min
Delta R.T.: 0.000 min
Response: 21196
Conc: 1.34 ng/ml

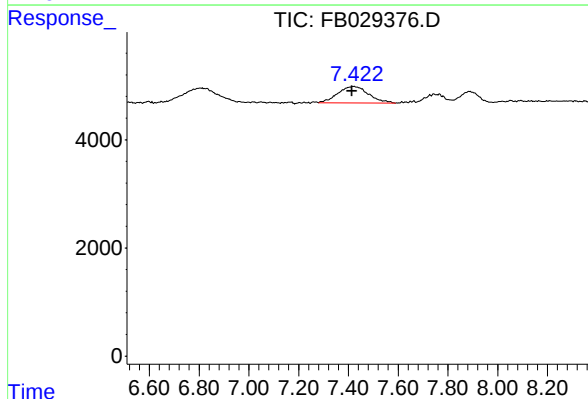


#2 2,2,4-Trimethylpentane

R.T.: 7.423 min
Delta R.T.: 0.009 min
Response: 26525
Conc: 1.54 ng/ml

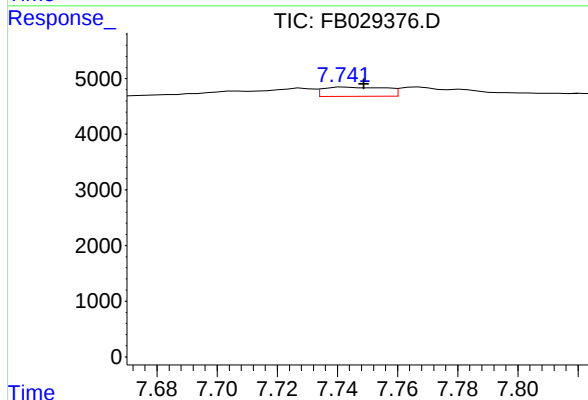


#3 n-Heptane

R.T.: 7.743 min
Delta R.T.: -0.006 min
Response: 2394
Conc: 0.13 ng/ml

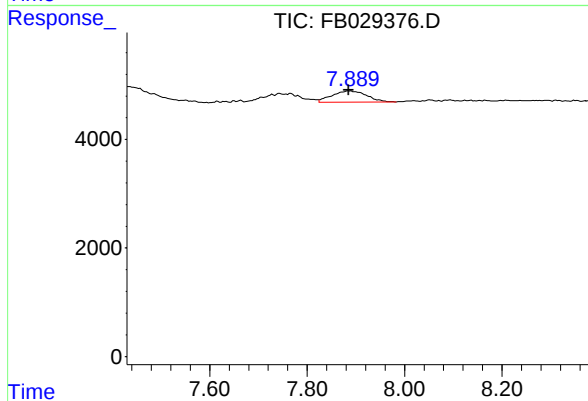


#4 Benzene

R.T.: 7.887 min
Delta R.T.: 0.002 min
Response: 10101
Conc: 0.48 ng/ml

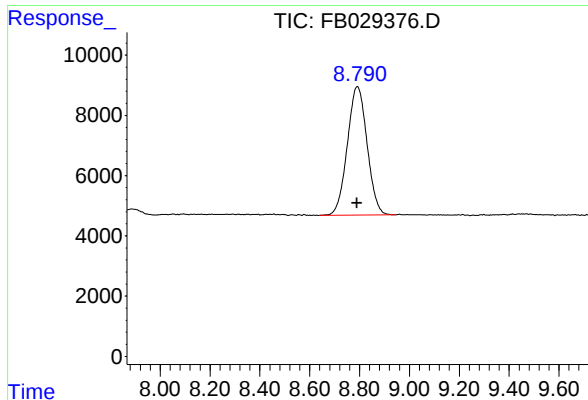


#5 AAA-TFT

R.T.: 8.792 min
Delta R.T.: 0.003 min
Response: 234602
Conc: 24.39 ng/ml

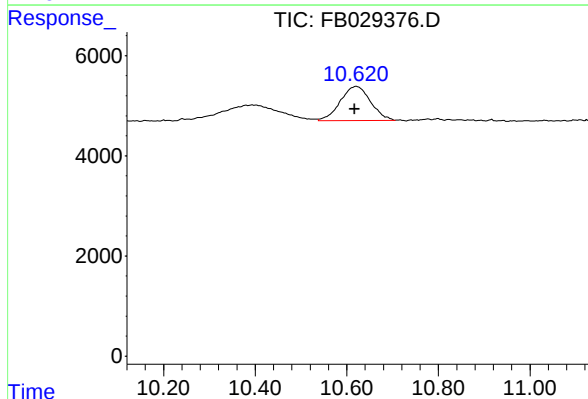


#6 Toluene

R.T.: 10.621 min
Delta R.T.: 0.004 min
Response: 31263
Conc: 1.54 ng/ml

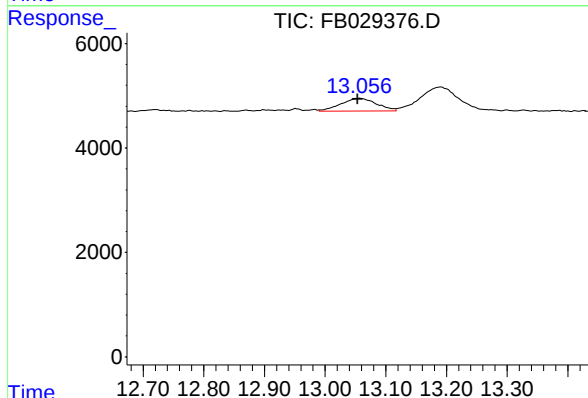


#7 Ethylbenzene

R.T.: 13.057 min
Delta R.T.: 0.003 min
Response: 9967
Conc: 0.52 ng/ml

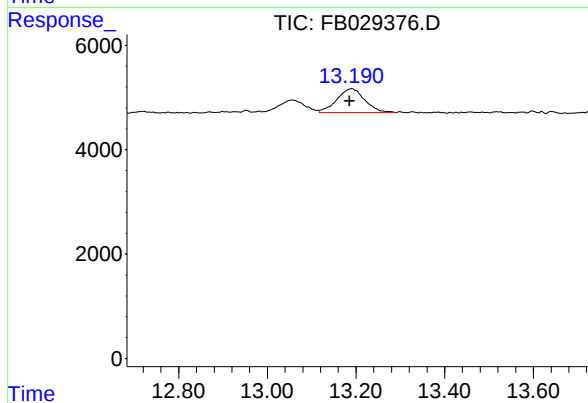


#8 m-Xylene

R.T.: 13.191 min
Delta R.T.: 0.005 min
Response: 20053
Conc: 1.06 ng/ml

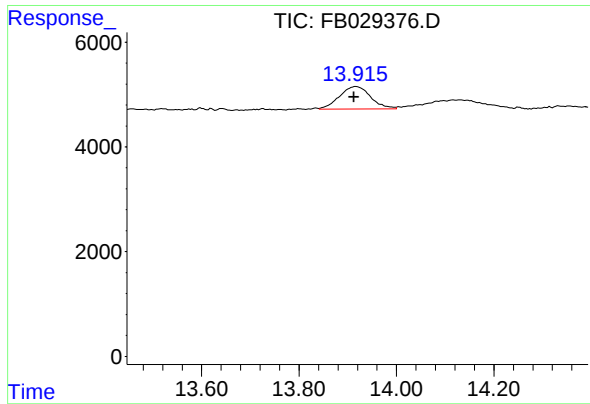

#9 O-Xylene

R.T.: 13.917 min
Delta R.T.: 0.004 min
Response: 19232
Conc: 1.05 ng/ml

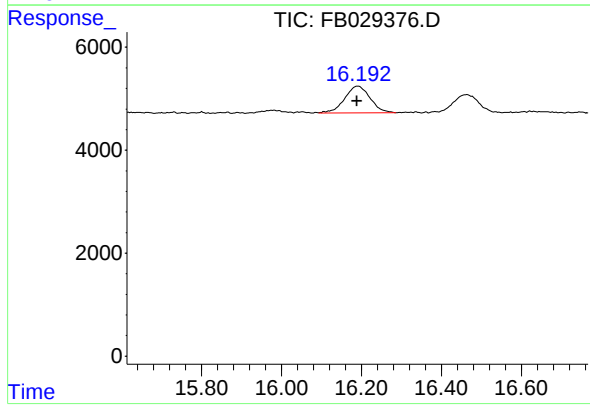

#10 1,2,4-Trimethylbenzene

R.T.: 16.193 min
Delta R.T.: 0.005 min
Response: 22986
Conc: 1.22 ng/ml