

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB022323\
 Data File : FB029386.D
 Signal(s) : FID2B.CH
 Acq On : 23 Feb 2023 18:14
 Operator : YP/AJ
 Sample : 01627-09
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 15 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Feb 24 01:29:58 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB020623.M
 Quant Title :
 QLast Update : Mon Feb 06 14:33:16 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.793	188384	19.586 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.713	16033	1.010 ng/ml
2) t	2,2,4-Trimethylpentane	7.412	19709	1.144 ng/ml
3) t	n-Heptane	7.743	6359	0.351 ng/ml
4) t	Benzene	7.890	8577	0.412 ng/ml
6) t	Toluene	10.623	24884	1.228 ng/ml
7) t	Ethylbenzene	13.054	6963	0.365 ng/ml
8) t	m-Xylene	13.193	15353	0.810 ng/ml
9) t	O-Xylene	13.918	15157	0.831 ng/ml
10) t	1,2,4-Trimethylbenzene	16.188	19243	1.023 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB022323\
Data File : FB029386.D
Signal(s) : FID2B.CH
Acq On : 23 Feb 2023 18:14
Operator : YP/AJ
Sample : 01627-09
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 15 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Feb 24 01:29:58 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB020623.M
Quant Title :
QLast Update : Mon Feb 06 14:33:16 2023
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

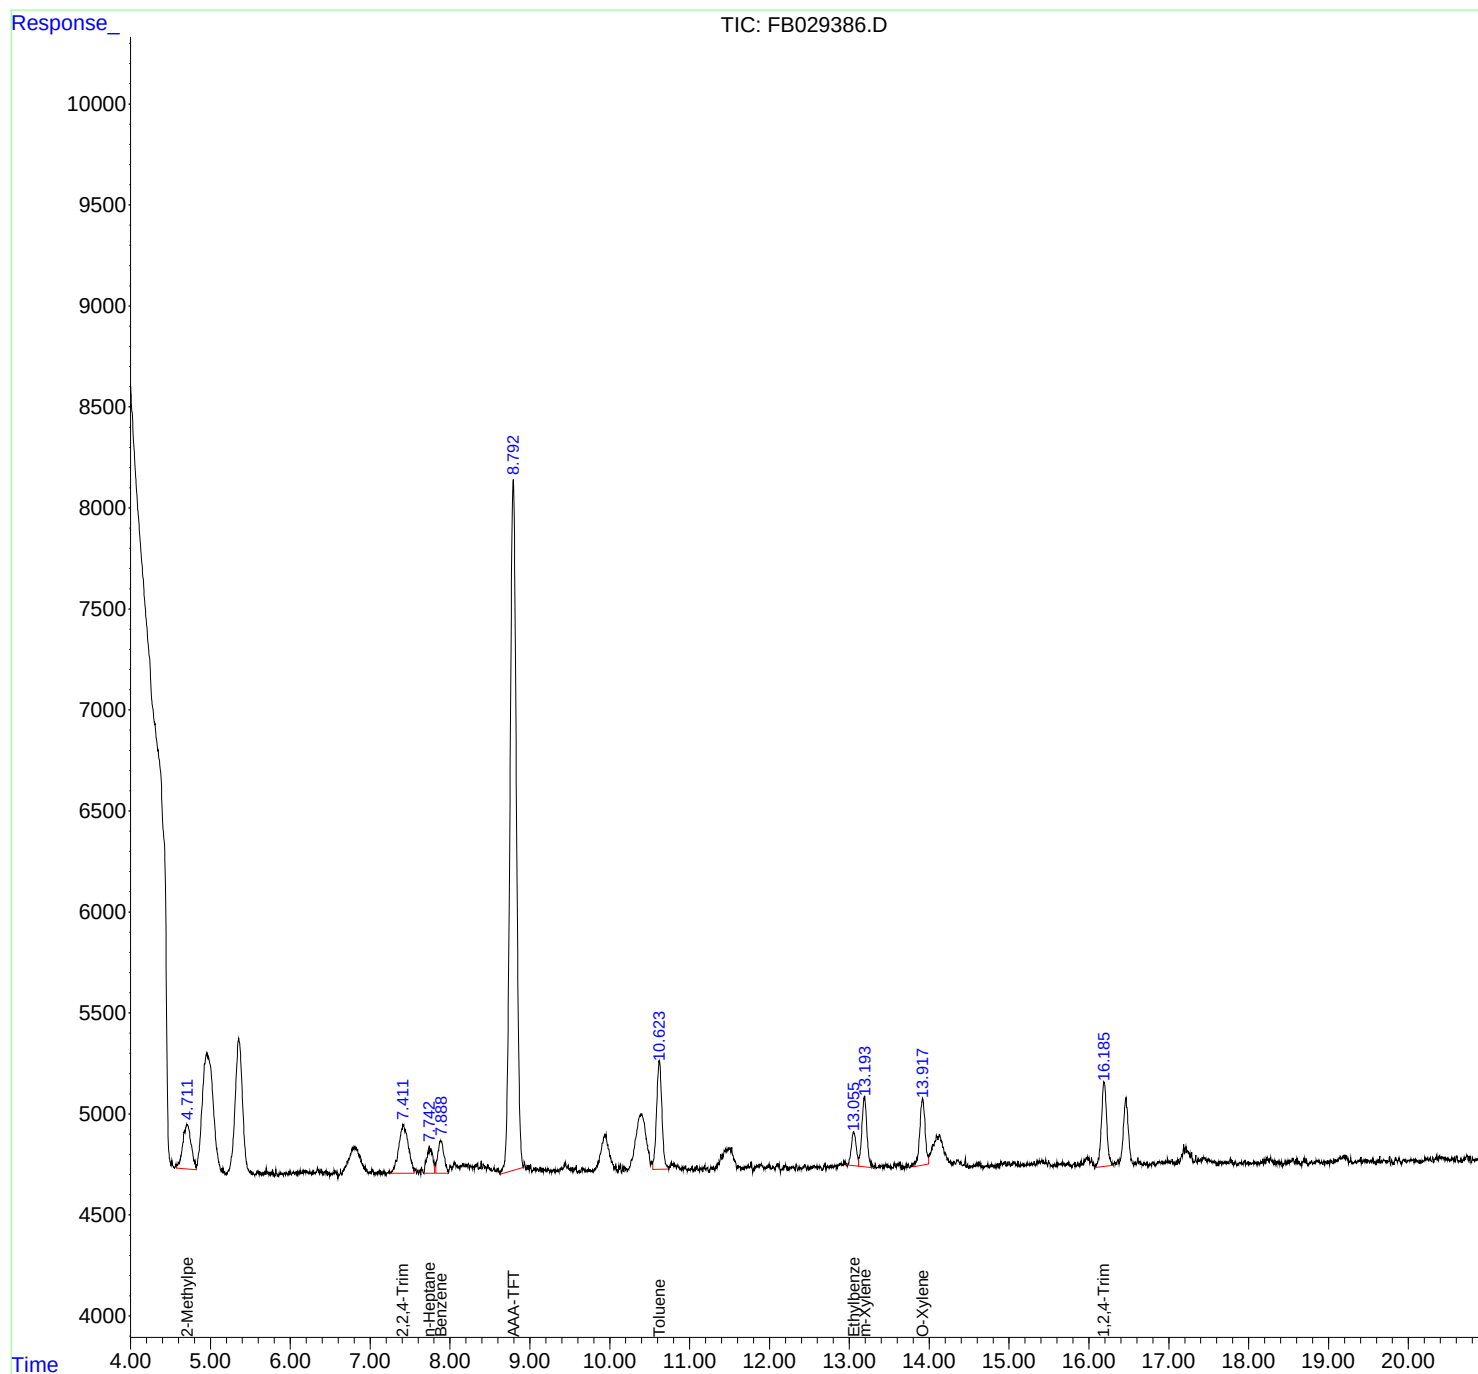

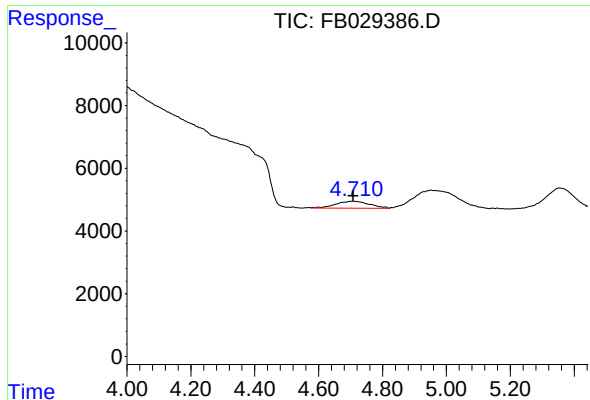


#1 2-Methylpentane

R.T.: 4.713 min
Delta R.T.: 0.004 min
Response: 16033
Conc: 1.01 ng/ml

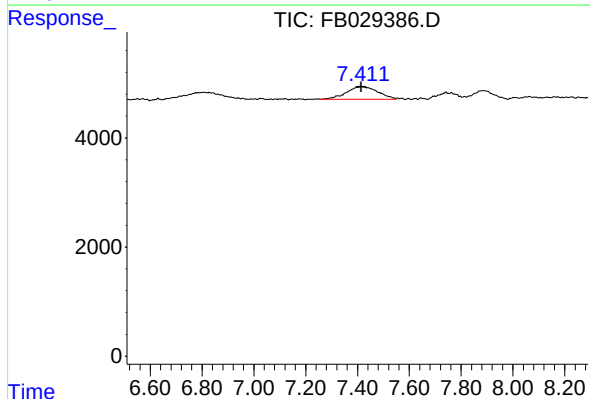


#2 2,2,4-Trimethylpentane

R.T.: 7.412 min
Delta R.T.: -0.002 min
Response: 19709
Conc: 1.14 ng/ml

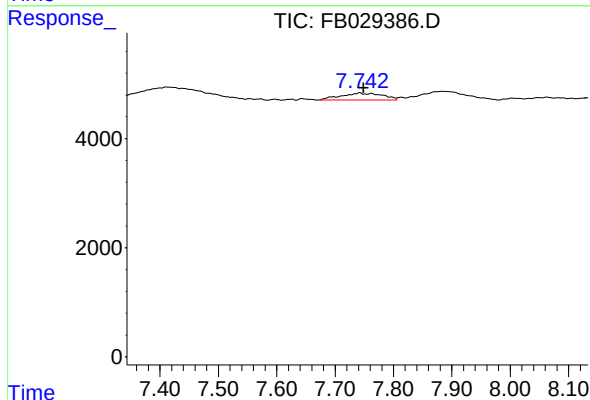


#3 n-Heptane

R.T.: 7.743 min
Delta R.T.: -0.006 min
Response: 6359
Conc: 0.35 ng/ml

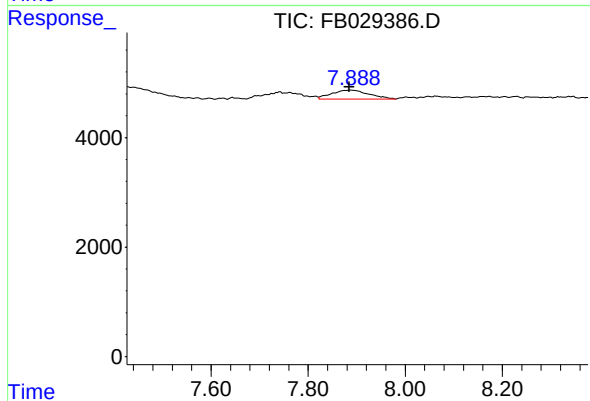


#4 Benzene

R.T.: 7.890 min
Delta R.T.: 0.005 min
Response: 8577
Conc: 0.41 ng/ml

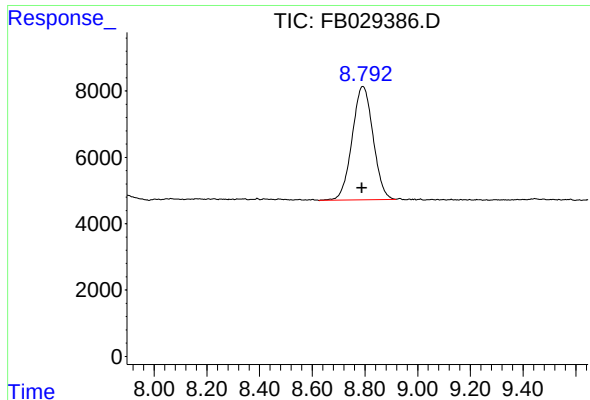


#5 AAA-TFT

R.T.: 8.793 min
Delta R.T.: 0.003 min
Response: 188384
Conc: 19.59 ng/ml

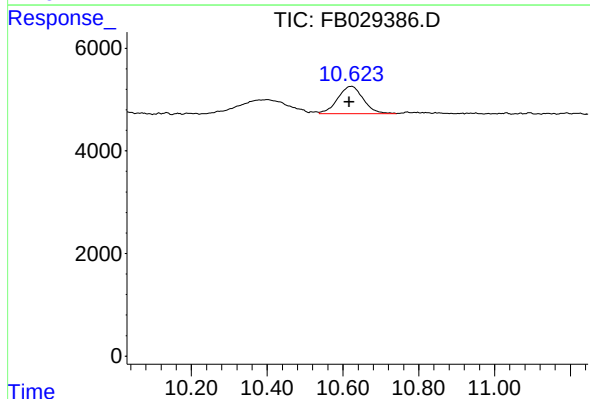


#6 Toluene

R.T.: 10.623 min
Delta R.T.: 0.006 min
Response: 24884
Conc: 1.23 ng/ml

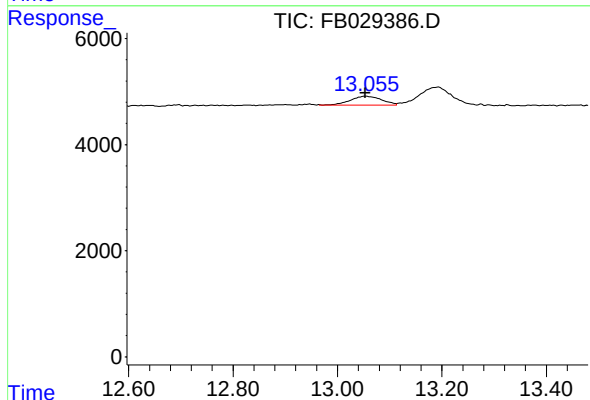


#7 Ethylbenzene

R.T.: 13.054 min
Delta R.T.: 0.000 min
Response: 6963
Conc: 0.36 ng/ml

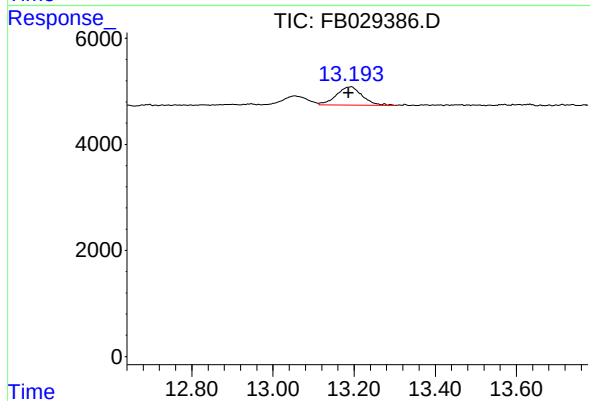


#8 m-Xylene

R.T.: 13.193 min
Delta R.T.: 0.007 min
Response: 15353
Conc: 0.81 ng/ml

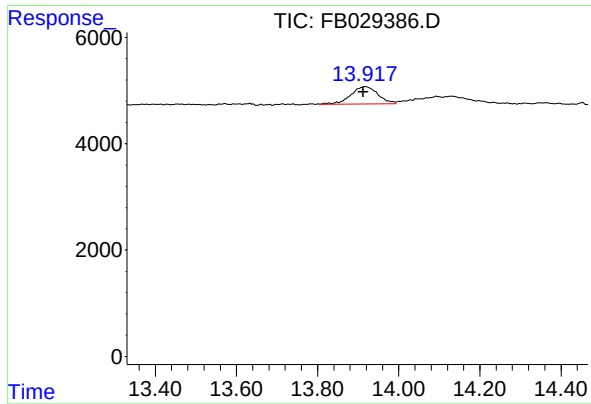

#9 O-Xylene

R.T.: 13.918 min
Delta R.T.: 0.005 min
Response: 15157
Conc: 0.83 ng/ml

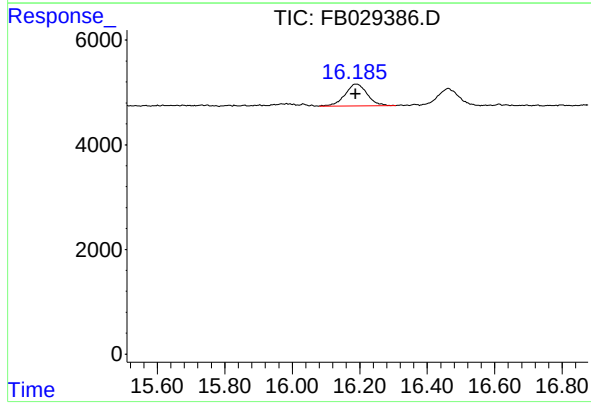

#10 1,2,4-Trimethylbenzene

R.T.: 16.188 min
Delta R.T.: 0.000 min
Response: 19243
Conc: 1.02 ng/ml