

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB022323\
 Data File : FB029375.D
 Signal(s) : FID2B.CH
 Acq On : 23 Feb 2023 10:43
 Operator : YP/AJ
 Sample : BSF0223S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Feb 24 01:29:01 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB020623.M
 Quant Title :
 QLast Update : Mon Feb 06 14:33:16 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.791	208733	21.702 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.706	424810	26.773 ng/ml
2) t 2,2,4-Trimethylpentane	7.416	486855	28.267 ng/ml
3) t n-Heptane	7.749	163311	9.026 ng/ml
4) t Benzene	7.887	202642	9.729 ng/ml
6) t Toluene	10.619	597208	29.470 ng/ml
7) t Ethylbenzene	13.055	186190	9.755 ng/ml
8) t m-Xylene	13.188	369284	19.479 ng/ml
9) t O-Xylene	13.915	360244	19.744 ng/ml
10) t 1,2,4-Trimethylbenzene	16.190	358319	19.041 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB022323\
Data File : FB029375.D
Signal(s) : FID2B.CH
Acq On : 23 Feb 2023 10:43
Operator : YP/AJ
Sample : BSF0223S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Feb 24 01:29:01 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB020623.M
Quant Title :
QLast Update : Mon Feb 06 14:33:16 2023
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

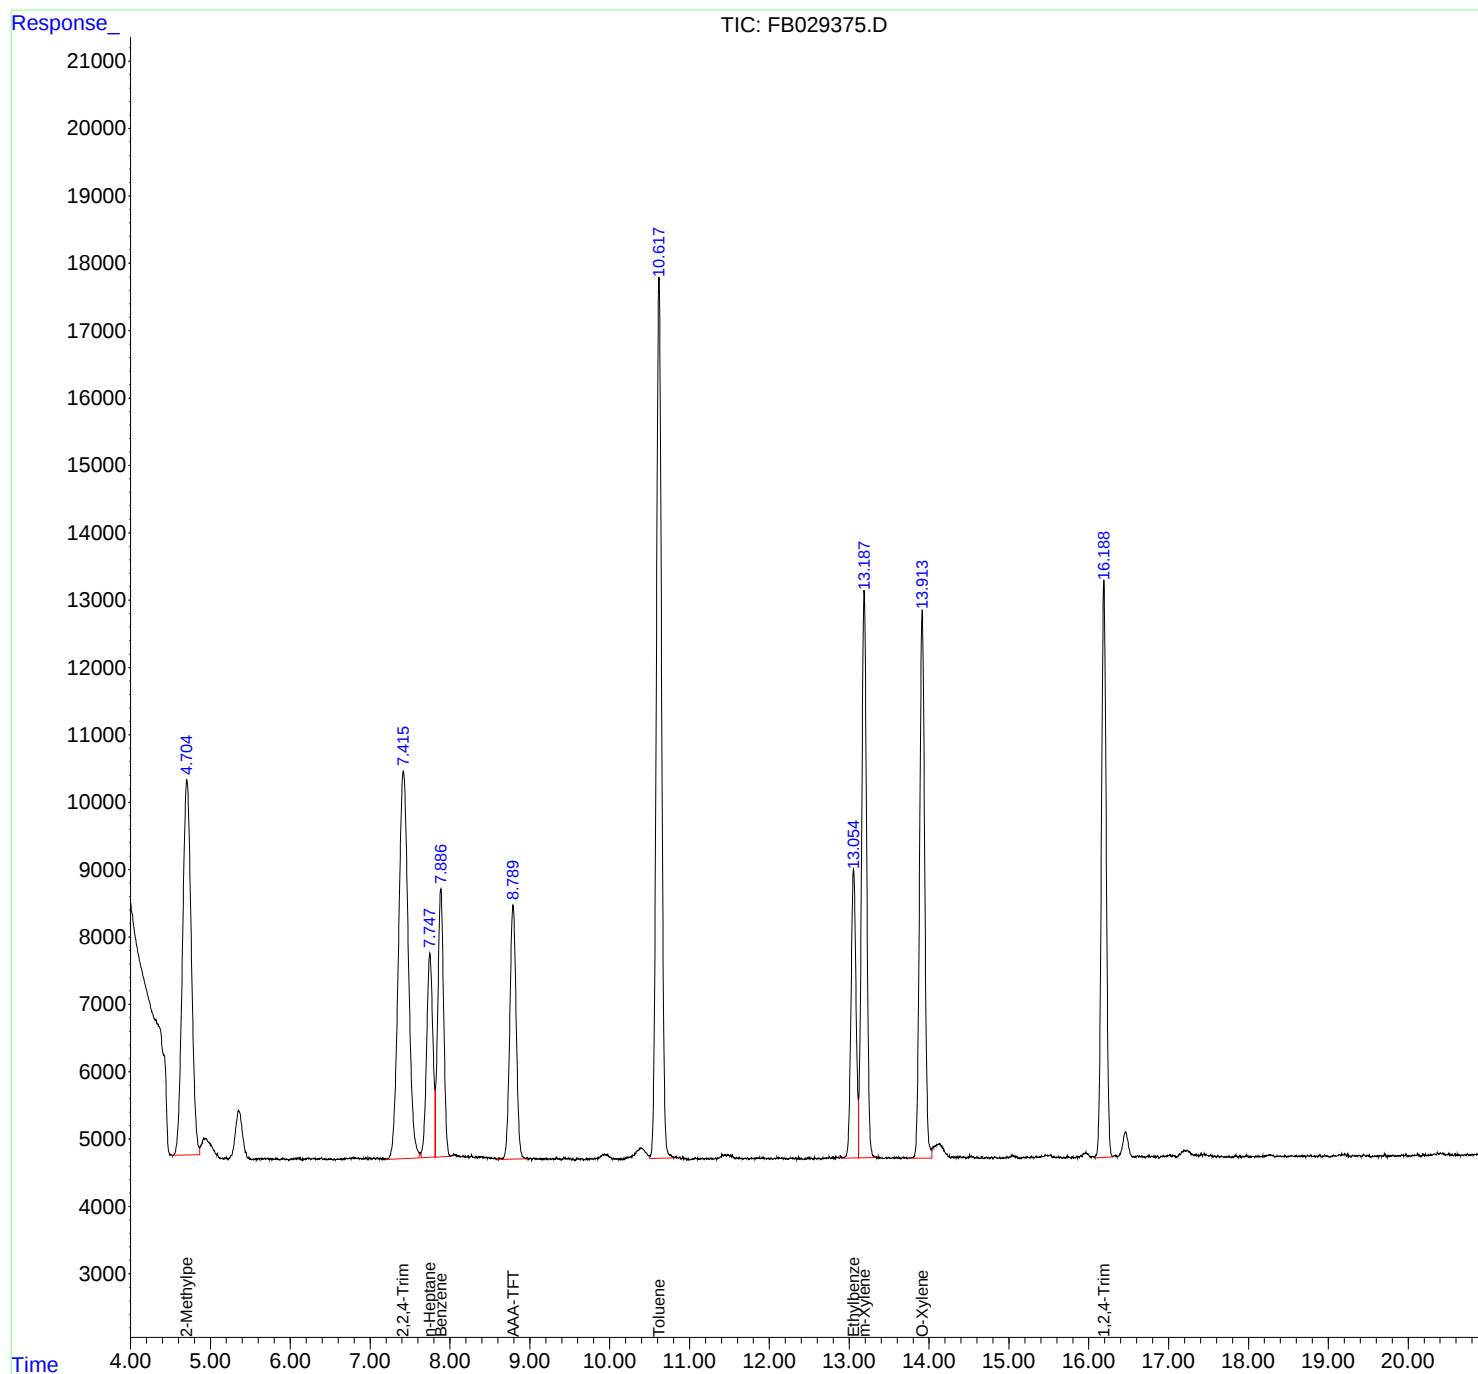

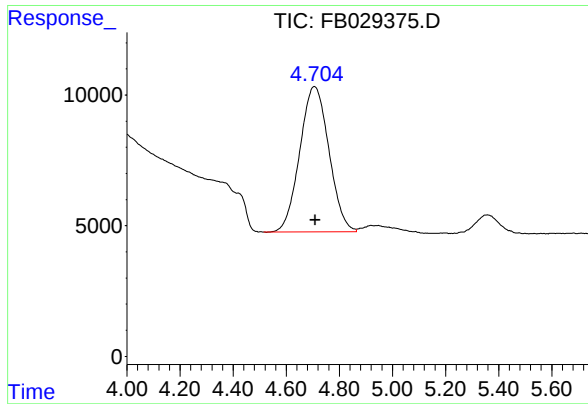


#1 2-Methylpentane

R.T.: 4.706 min
Delta R.T.: -0.003 min
Response: 424810
Conc: 26.77 ng/ml

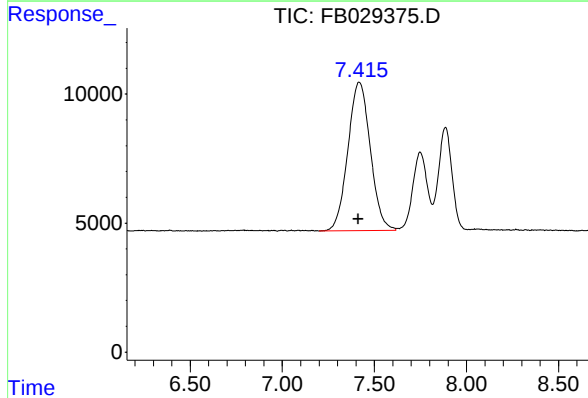


#2 2,2,4-Trimethylpentane

R.T.: 7.416 min
Delta R.T.: 0.002 min
Response: 486855
Conc: 28.27 ng/ml

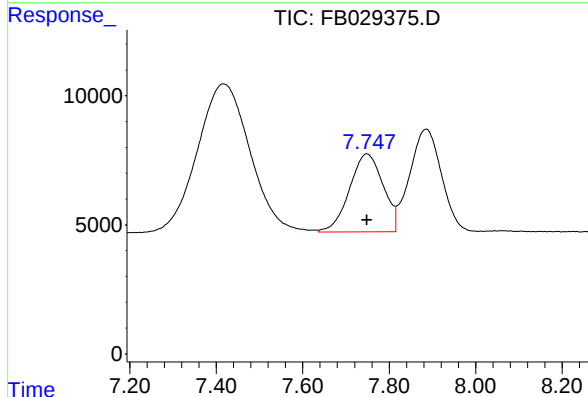


#3 n-Heptane

R.T.: 7.749 min
Delta R.T.: 0.000 min
Response: 163311
Conc: 9.03 ng/ml

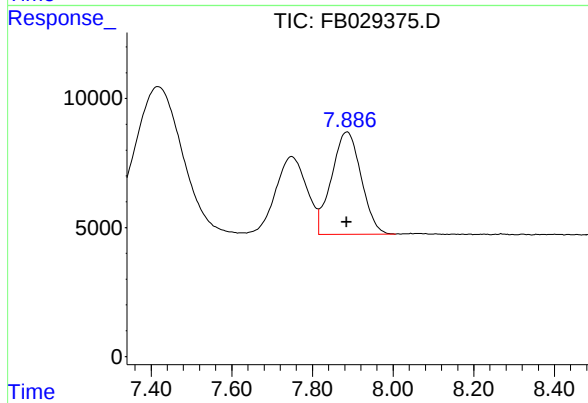


#4 Benzene

R.T.: 7.887 min
Delta R.T.: 0.002 min
Response: 202642
Conc: 9.73 ng/ml

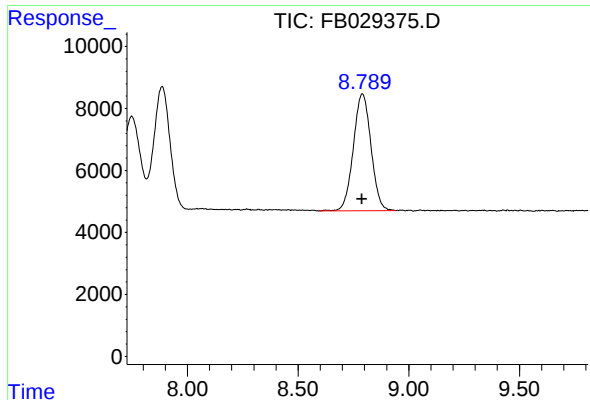


#5 AAA-TFT

R.T.: 8.791 min
Delta R.T.: 0.001 min
Response: 208733
Conc: 21.70 ng/ml

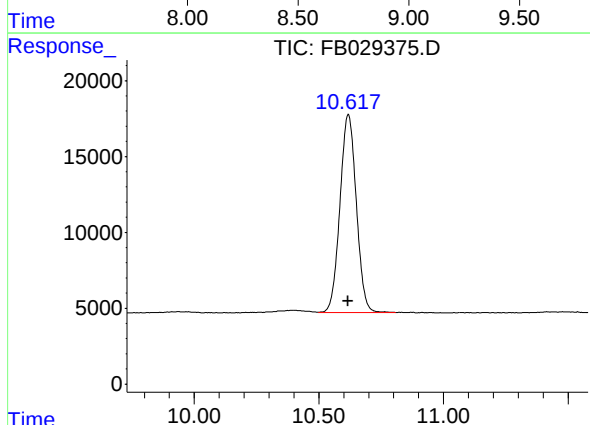


#6 Toluene

R.T.: 10.619 min
Delta R.T.: 0.002 min
Response: 597208
Conc: 29.47 ng/ml

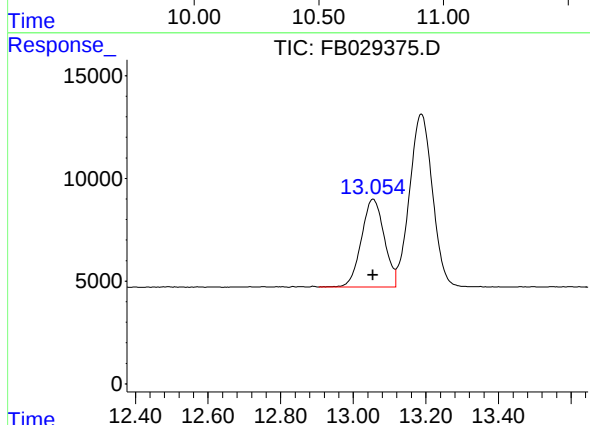


#7 Ethylbenzene

R.T.: 13.055 min
Delta R.T.: 0.001 min
Response: 186190
Conc: 9.76 ng/ml

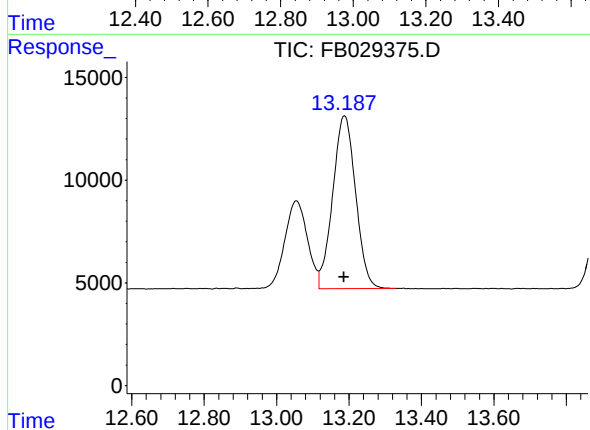


#8 m-Xylene

R.T.: 13.188 min
Delta R.T.: 0.002 min
Response: 369284
Conc: 19.48 ng/ml

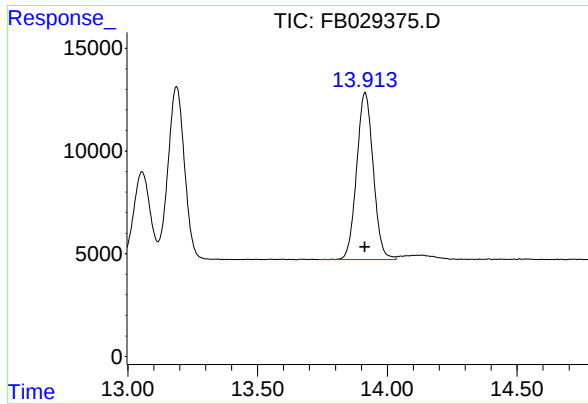

#9 O-Xylene

R.T.: 13.915 min
Delta R.T.: 0.002 min
Response: 360244
Conc: 19.74 ng/ml

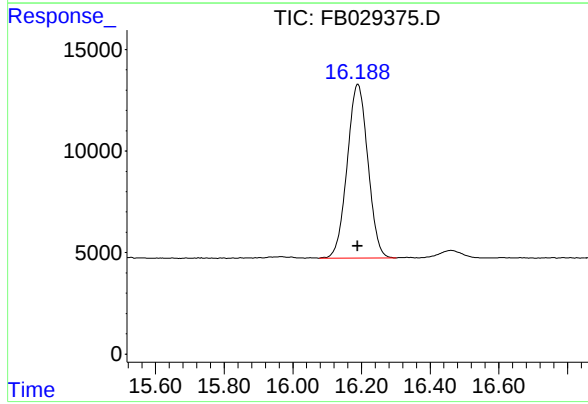

#10 1,2,4-Trimethylbenzene

R.T.: 16.190 min
Delta R.T.: 0.002 min
Response: 358319
Conc: 19.04 ng/ml