

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB022323\
 Data File : FB029384.D
 Signal(s) : FID2B.CH
 Acq On : 23 Feb 2023 17:00
 Operator : YP/AJ
 Sample : BSF0223W1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 13 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Feb 24 01:29:48 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB020623.M
 Quant Title :
 QLast Update : Mon Feb 06 14:33:16 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.791	201769	20.978 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.709	435583	27.452 ng/ml
2) t 2,2,4-Trimethylpentane	7.419	501506	29.118 ng/ml
3) t n-Heptane	7.750	165178	9.129 ng/ml
4) t Benzene	7.887	209595	10.062 ng/ml
6) t Toluene	10.619	611966	30.198 ng/ml
7) t Ethylbenzene	13.056	190897	10.002 ng/ml
8) t m-Xylene	13.189	378513	19.966 ng/ml
9) t O-Xylene	13.915	367284	20.130 ng/ml
10) t 1,2,4-Trimethylbenzene	16.190	361744	19.223 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB022323\
Data File : FB029384.D
Signal(s) : FID2B.CH
Acq On : 23 Feb 2023 17:00
Operator : YP/AJ
Sample : BSF0223W1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 13 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Feb 24 01:29:48 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB020623.M
Quant Title :
QLast Update : Mon Feb 06 14:33:16 2023
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

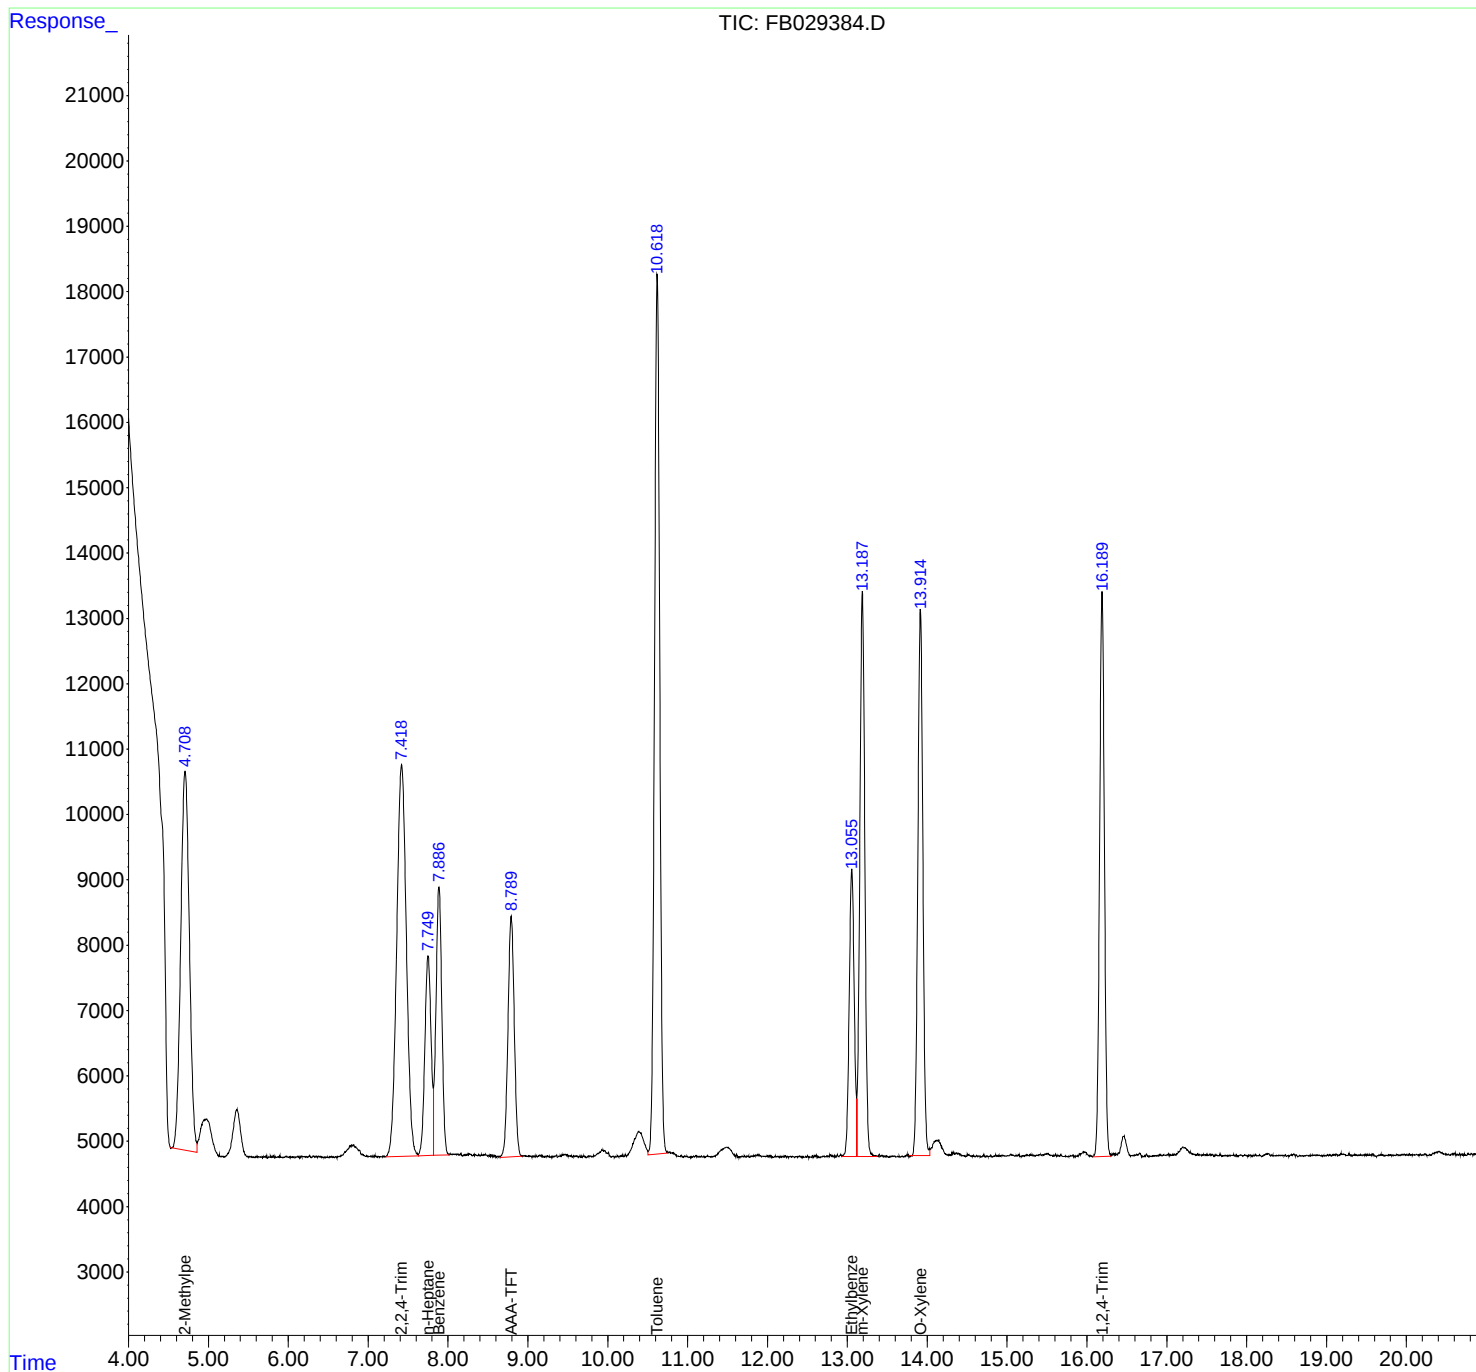

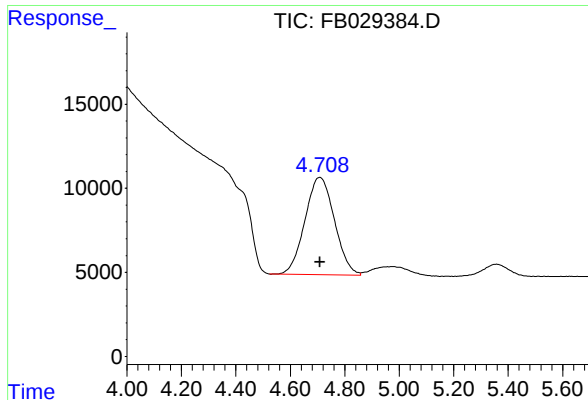


#1 2-Methylpentane

R.T.: 4.709 min
Delta R.T.: 0.000 min
Response: 435583
Conc: 27.45 ng/ml

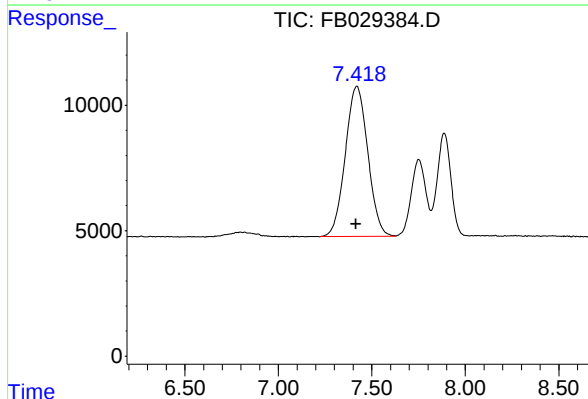


#2 2,2,4-Trimethylpentane

R.T.: 7.419 min
Delta R.T.: 0.005 min
Response: 501506
Conc: 29.12 ng/ml

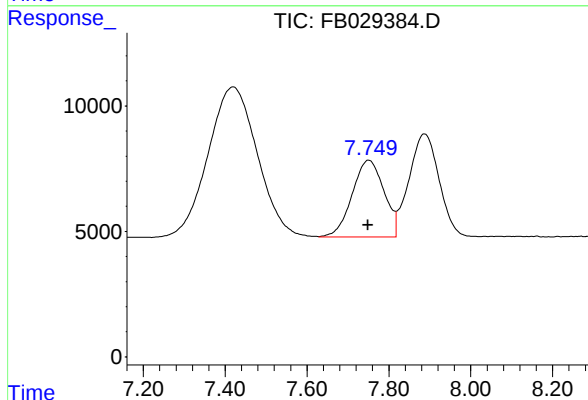


#3 n-Heptane

R.T.: 7.750 min
Delta R.T.: 0.002 min
Response: 165178
Conc: 9.13 ng/ml

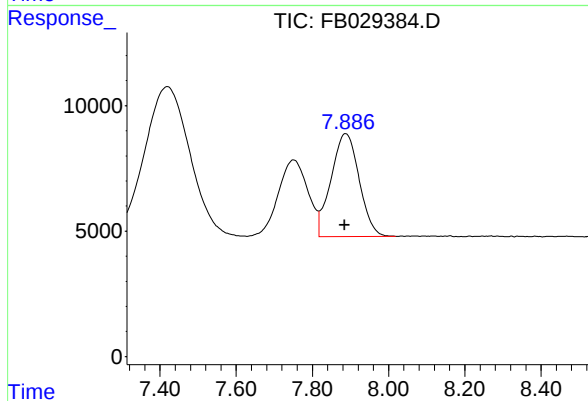


#4 Benzene

R.T.: 7.887 min
Delta R.T.: 0.003 min
Response: 209595
Conc: 10.06 ng/ml

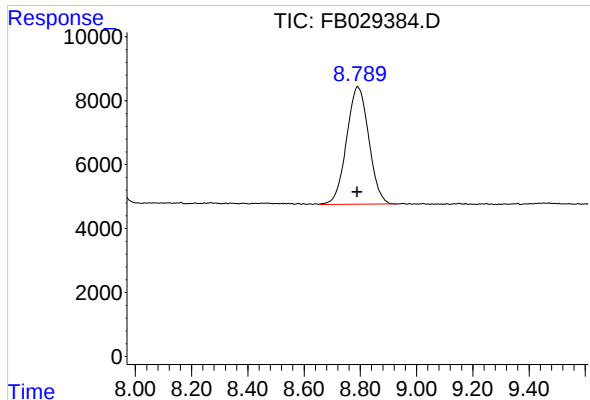


#5 AAA-TFT

R.T.: 8.791 min
Delta R.T.: 0.001 min
Response: 201769
Conc: 20.98 ng/ml

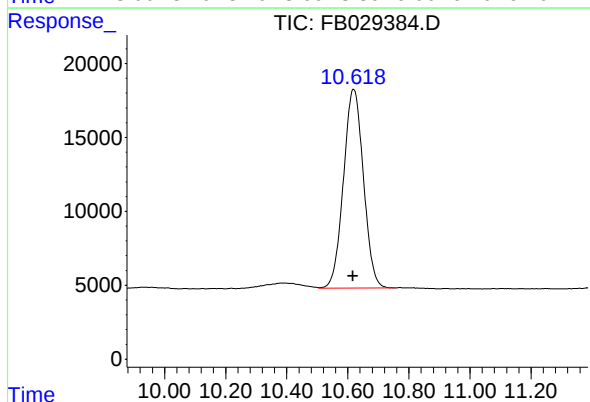


#6 Toluene

R.T.: 10.619 min
Delta R.T.: 0.002 min
Response: 611966
Conc: 30.20 ng/ml

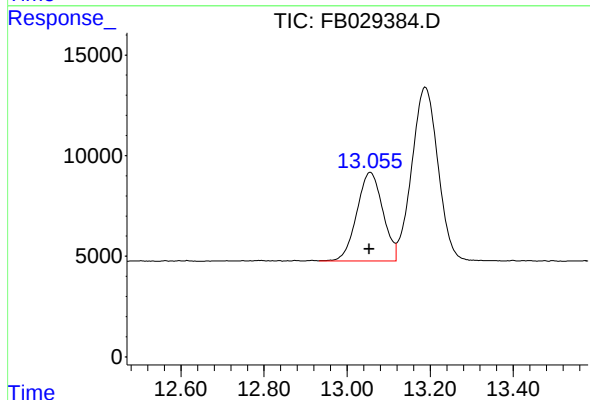


#7 Ethylbenzene

R.T.: 13.056 min
Delta R.T.: 0.002 min
Response: 190897
Conc: 10.00 ng/ml

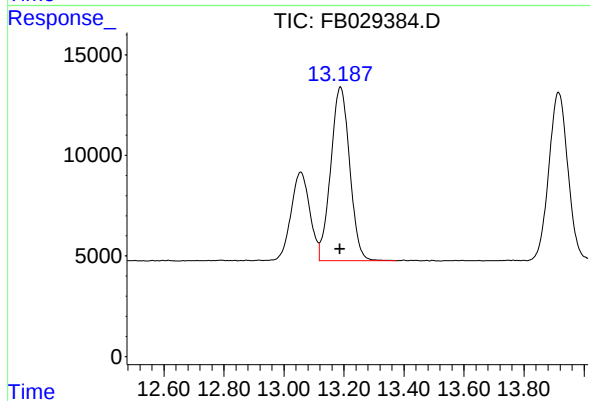


#8 m-Xylene

R.T.: 13.189 min
Delta R.T.: 0.003 min
Response: 378513
Conc: 19.97 ng/ml

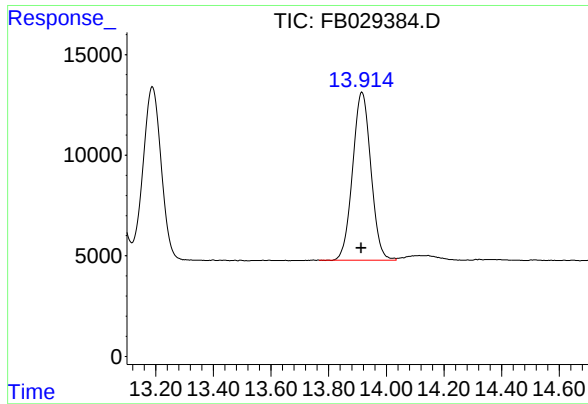

#9 O-Xylene

R.T.: 13.915 min
Delta R.T.: 0.003 min
Response: 367284
Conc: 20.13 ng/ml

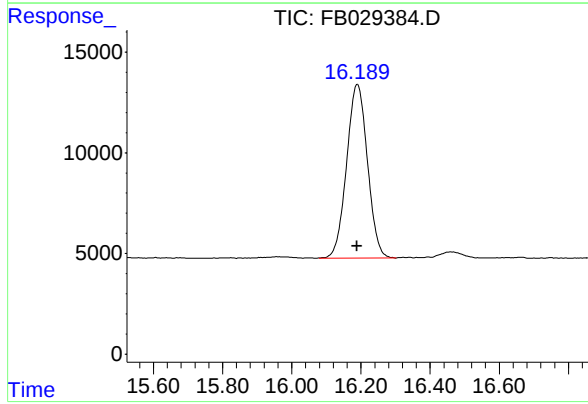

#10 1,2,4-Trimethylbenzene

R.T.: 16.190 min
Delta R.T.: 0.002 min
Response: 361744
Conc: 19.22 ng/ml