

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB022323\
 Data File : FB029385.D
 Signal(s) : FID2B.CH
 Acq On : 23 Feb 2023 17:37
 Operator : YP/AJ
 Sample : BSF0223W2
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 14 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Feb 24 01:29:53 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB020623.M
 Quant Title :
 QLast Update : Mon Feb 06 14:33:16 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.792	244920	25.464 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.711	470152	29.631 ng/ml
2) t 2,2,4-Trimethylpentane	7.422	555026	32.225 ng/ml
3) t n-Heptane	7.751	180293	9.964 ng/ml
4) t Benzene	7.888	228874	10.988 ng/ml
6) t Toluene	10.620	663655	32.749 ng/ml
7) t Ethylbenzene	13.056	204979	10.740 ng/ml
8) t m-Xylene	13.189	410723	21.665 ng/ml
9) t O-Xylene	13.916	399439	21.892 ng/ml
10) t 1,2,4-Trimethylbenzene	16.191	389097	20.676 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB022323\
Data File : FB029385.D
Signal(s) : FID2B.CH
Acq On : 23 Feb 2023 17:37
Operator : YP/AJ
Sample : BSF0223W2
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 14 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Feb 24 01:29:53 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB020623.M
Quant Title :
QLast Update : Mon Feb 06 14:33:16 2023
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

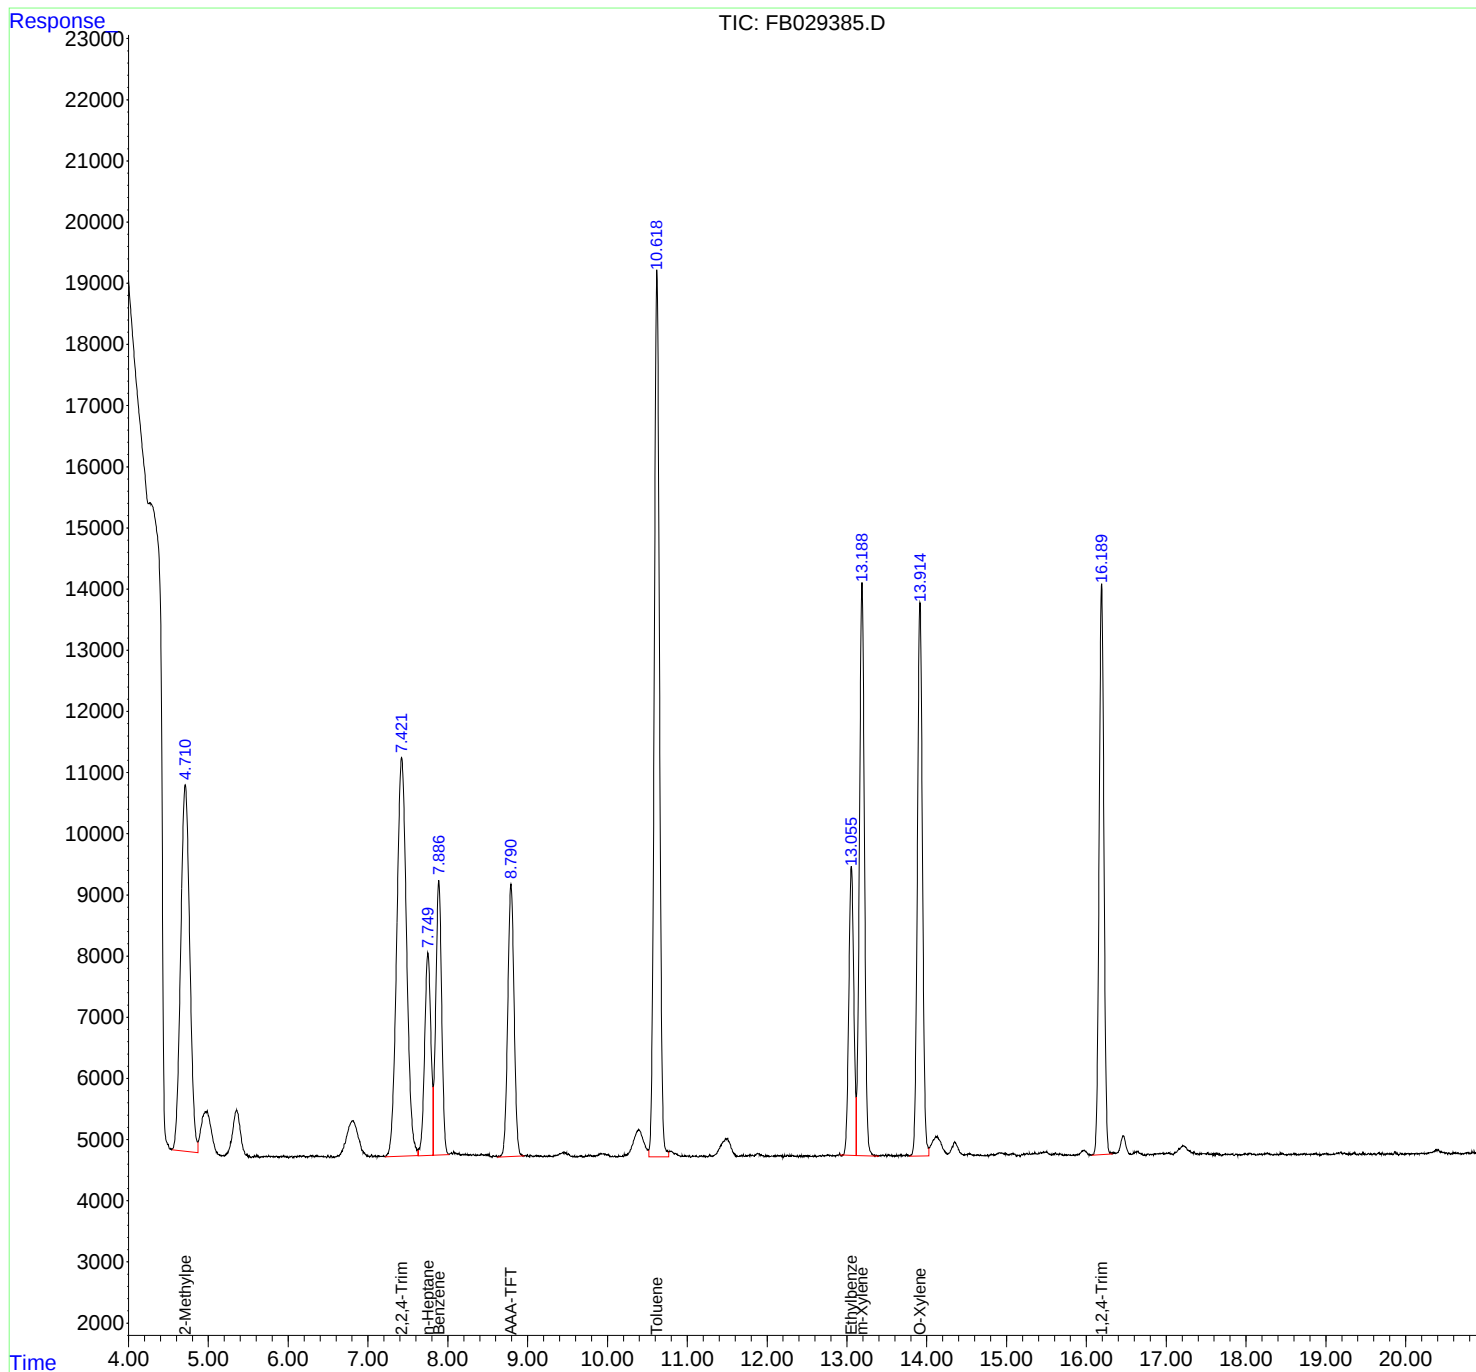

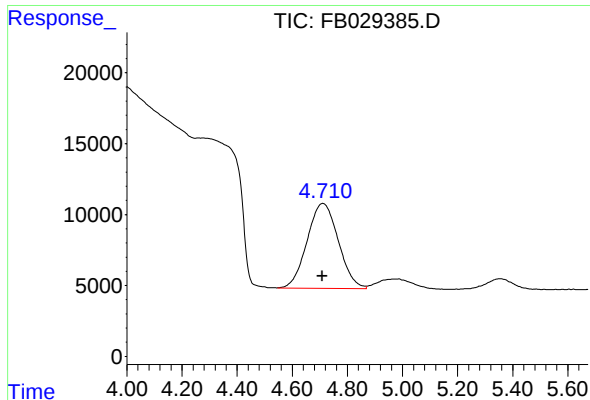


#1 2-Methylpentane

R.T.: 4.711 min
Delta R.T.: 0.002 min
Response: 470152
Conc: 29.63 ng/ml

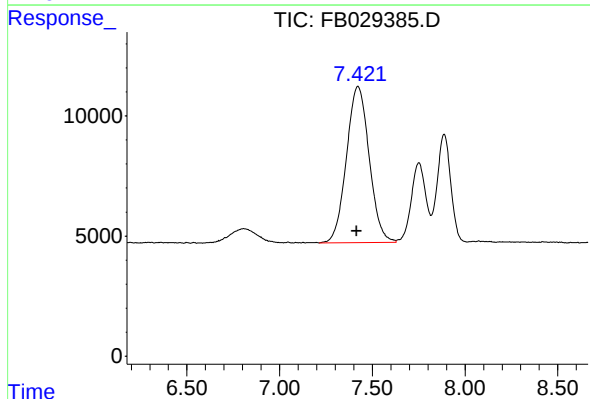


#2 2,2,4-Trimethylpentane

R.T.: 7.422 min
Delta R.T.: 0.007 min
Response: 555026
Conc: 32.22 ng/ml

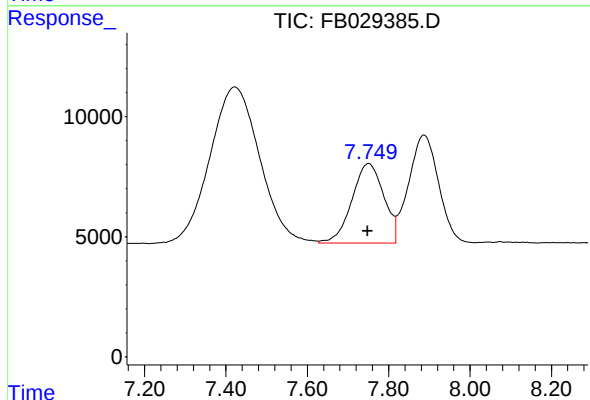


#3 n-Heptane

R.T.: 7.751 min
Delta R.T.: 0.002 min
Response: 180293
Conc: 9.96 ng/ml

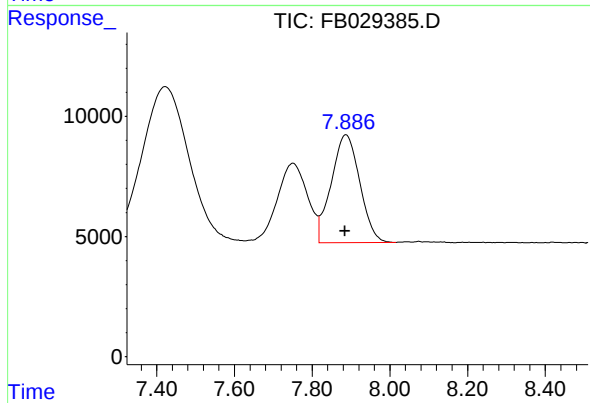


#4 Benzene

R.T.: 7.888 min
Delta R.T.: 0.003 min
Response: 228874
Conc: 10.99 ng/ml

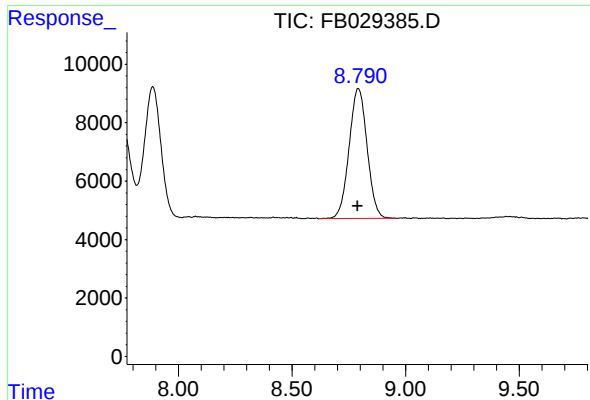


#5 AAA-TFT

R.T.: 8.792 min
Delta R.T.: 0.002 min
Response: 244920
Conc: 25.46 ng/ml

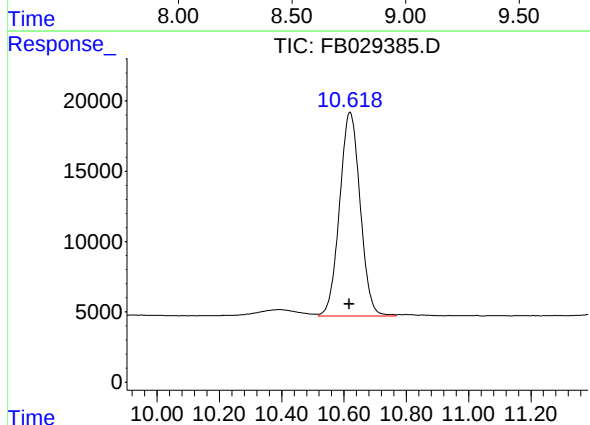


#6 Toluene

R.T.: 10.620 min
Delta R.T.: 0.003 min
Response: 663655
Conc: 32.75 ng/ml

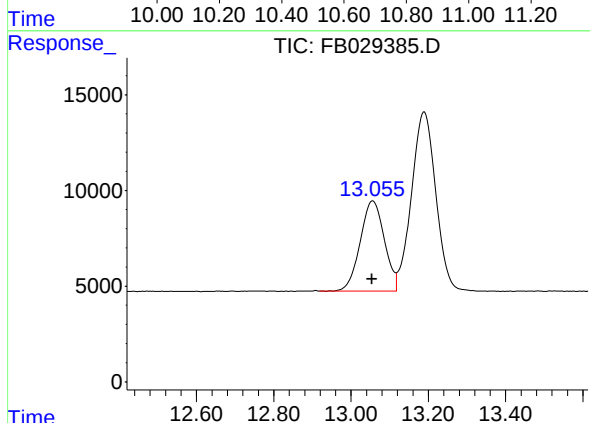


#7 Ethylbenzene

R.T.: 13.056 min
Delta R.T.: 0.002 min
Response: 204979
Conc: 10.74 ng/ml

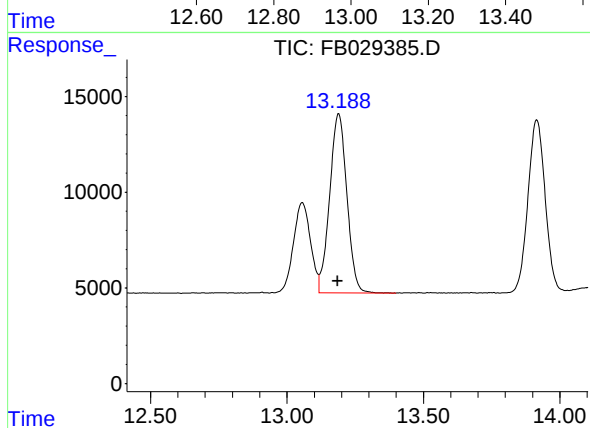


#8 m-Xylene

R.T.: 13.189 min
Delta R.T.: 0.003 min
Response: 410723
Conc: 21.67 ng/ml

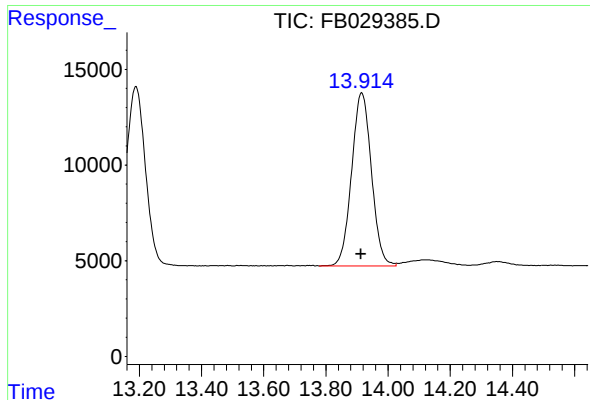

#9 O-Xylene

R.T.: 13.916 min
Delta R.T.: 0.003 min
Response: 399439
Conc: 21.89 ng/ml

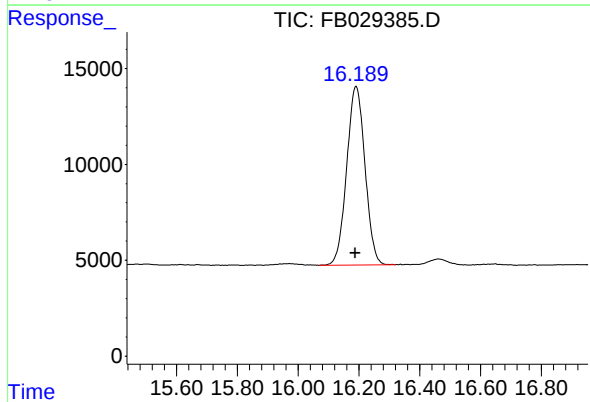

#10 1,2,4-Trimethylbenzene

R.T.: 16.191 min
Delta R.T.: 0.003 min
Response: 389097
Conc: 20.68 ng/ml