

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB022323\
 Data File : FB029387.D
 Signal(s) : FID2B.CH
 Acq On : 23 Feb 2023 20:06
 Operator : YP/AJ
 Sample : 20 PPB GRO STD
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 18 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Feb 24 01:30:03 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB020623.M
 Quant Title :
 QLast Update : Mon Feb 06 14:33:16 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.792	225321	23.426 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.708	416141	26.227 ng/ml
2) t 2,2,4-Trimethylpentane	7.419	464609	26.975 ng/ml
3) t n-Heptane	7.750	153992	8.511 ng/ml
4) t Benzene	7.888	200308	9.617 ng/ml
6) t Toluene	10.620	585670	28.901 ng/ml
7) t Ethylbenzene	13.056	183495	9.614 ng/ml
8) t m-Xylene	13.189	365134	19.260 ng/ml
9) t O-Xylene	13.915	356024	19.513 ng/ml
10) t 1,2,4-Trimethylbenzene	16.190	349470	18.570 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB022323\
Data File : FB029387.D
Signal(s) : FID2B.CH
Acq On : 23 Feb 2023 20:06
Operator : YP/AJ
Sample : 20 PPB GRO STD
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 18 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Feb 24 01:30:03 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB020623.M
Quant Title :
QLast Update : Mon Feb 06 14:33:16 2023
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

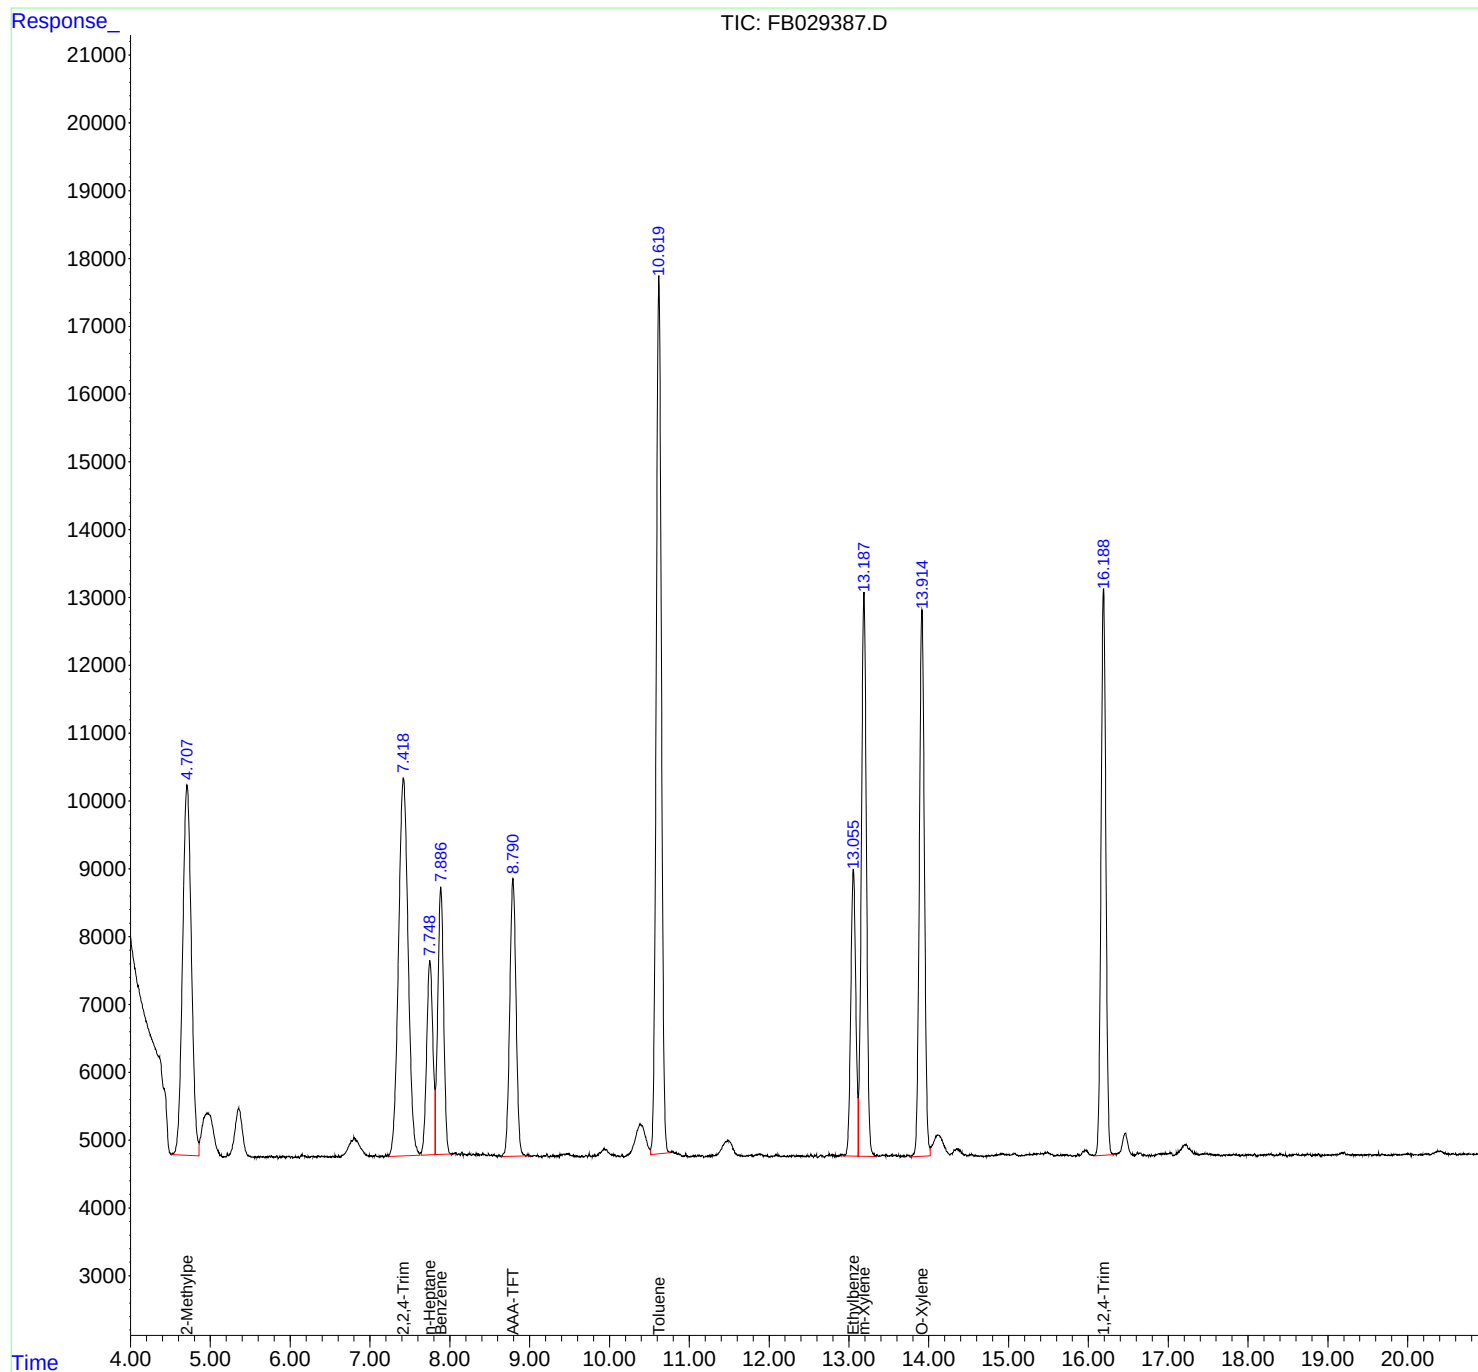

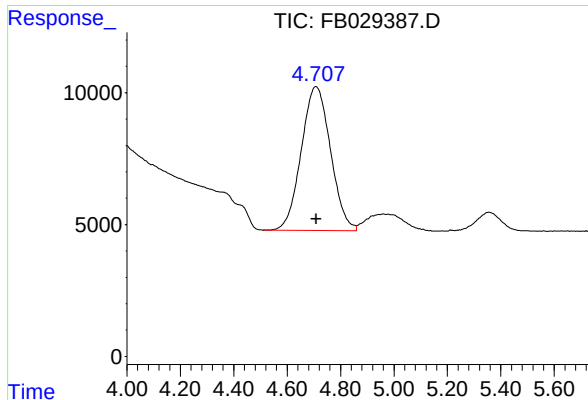


#1 2-Methylpentane

R.T.: 4.708 min
Delta R.T.: 0.000 min
Response: 416141
Conc: 26.23 ng/ml

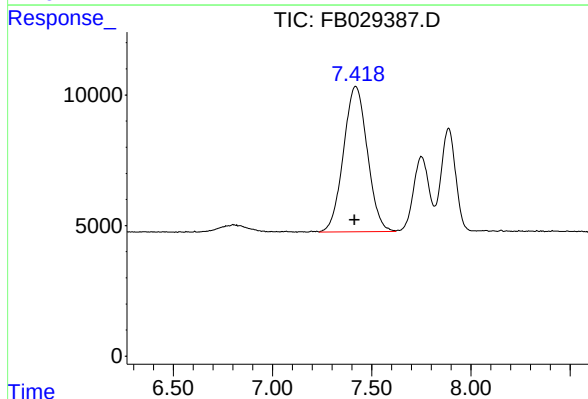


#2 2,2,4-Trimethylpentane

R.T.: 7.419 min
Delta R.T.: 0.005 min
Response: 464609
Conc: 26.98 ng/ml

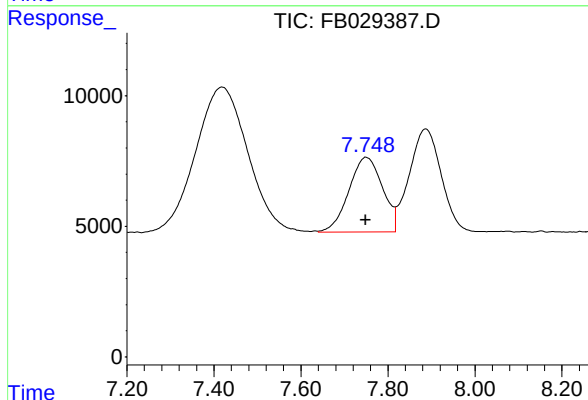


#3 n-Heptane

R.T.: 7.750 min
Delta R.T.: 0.000 min
Response: 153992
Conc: 8.51 ng/ml

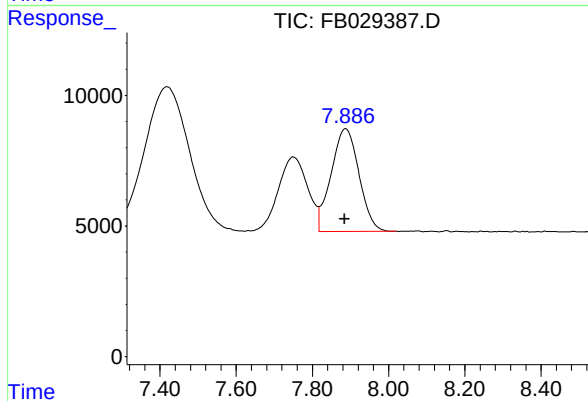


#4 Benzene

R.T.: 7.888 min
Delta R.T.: 0.003 min
Response: 200308
Conc: 9.62 ng/ml

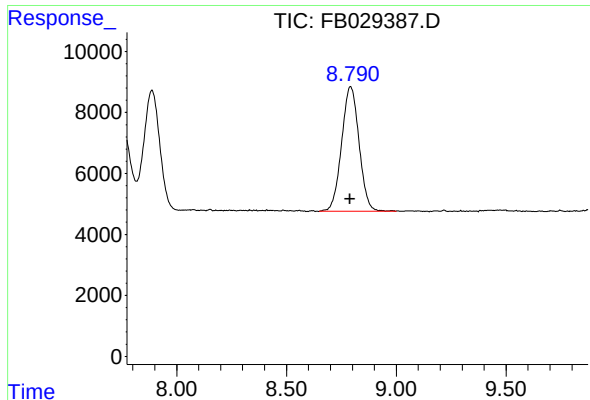


#5 AAA-TFT

R.T.: 8.792 min
Delta R.T.: 0.002 min
Response: 225321
Conc: 23.43 ng/ml

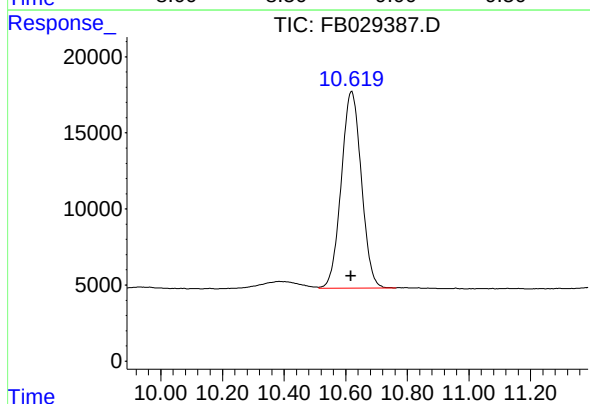


#6 Toluene

R.T.: 10.620 min
Delta R.T.: 0.003 min
Response: 585670
Conc: 28.90 ng/ml

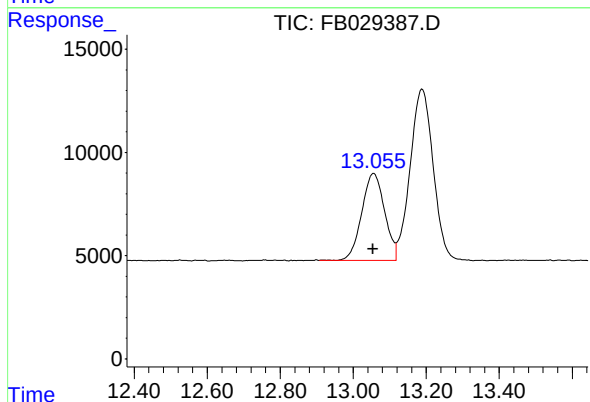


#7 Ethylbenzene

R.T.: 13.056 min
Delta R.T.: 0.002 min
Response: 183495
Conc: 9.61 ng/ml

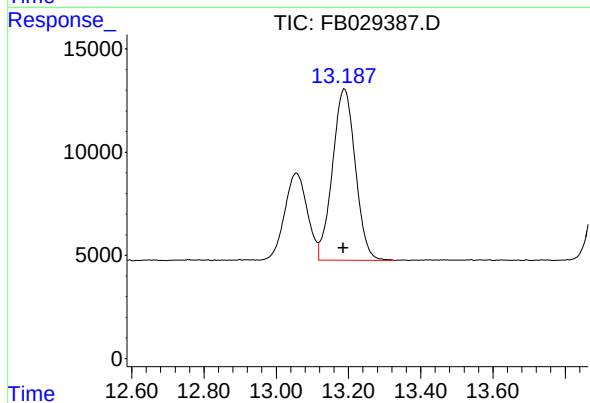


#8 m-Xylene

R.T.: 13.189 min
Delta R.T.: 0.003 min
Response: 365134
Conc: 19.26 ng/ml

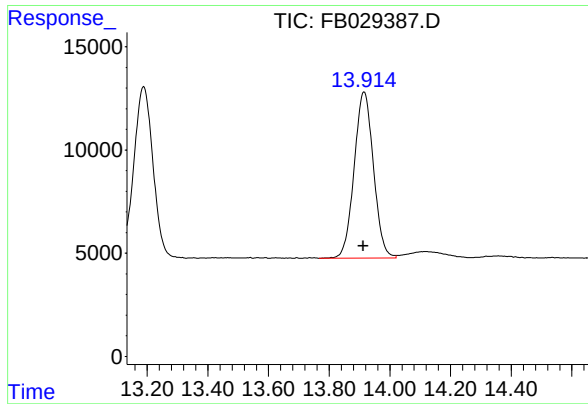

#9 O-Xylene

R.T.: 13.915 min
Delta R.T.: 0.003 min
Response: 356024
Conc: 19.51 ng/ml

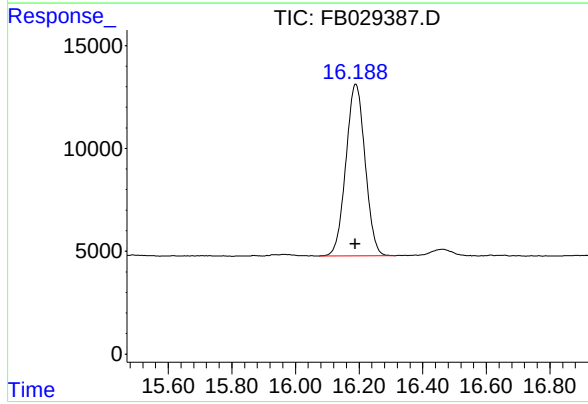

#10 1,2,4-Trimethylbenzene

R.T.: 16.190 min
Delta R.T.: 0.002 min
Response: 349470
Conc: 18.57 ng/ml