

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB022420\
 Data File : FB023709.D
 Signal(s) : FID2B.CH
 Acq On : 24 Feb 2020 10:58
 Operator : DD/AJ
 Sample : L1659-02
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Feb 25 00:17:59 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB020620.M
 Quant Title :
 QLast Update : Thu Feb 06 11:13:47 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.795	421590	20.707 ng/ml
Target Compounds			
6) t Toluene	10.625	4490	0.113 ng/ml
8) t m-Xylene	13.207	485	0.014 ng/ml
9) t O-Xylene	13.944	3765	0.109 ng/ml
10) t 1,2,4-Trimethylbenzene	16.216	4615	0.158 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB022420\
Data File : FB023709.D
Signal(s) : FID2B.CH
Acq On : 24 Feb 2020 10:58
Operator : DD/AJ
Sample : L1659-02
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 4 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Feb 25 00:17:59 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB020620.M
Quant Title :
QLast Update : Thu Feb 06 11:13:47 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

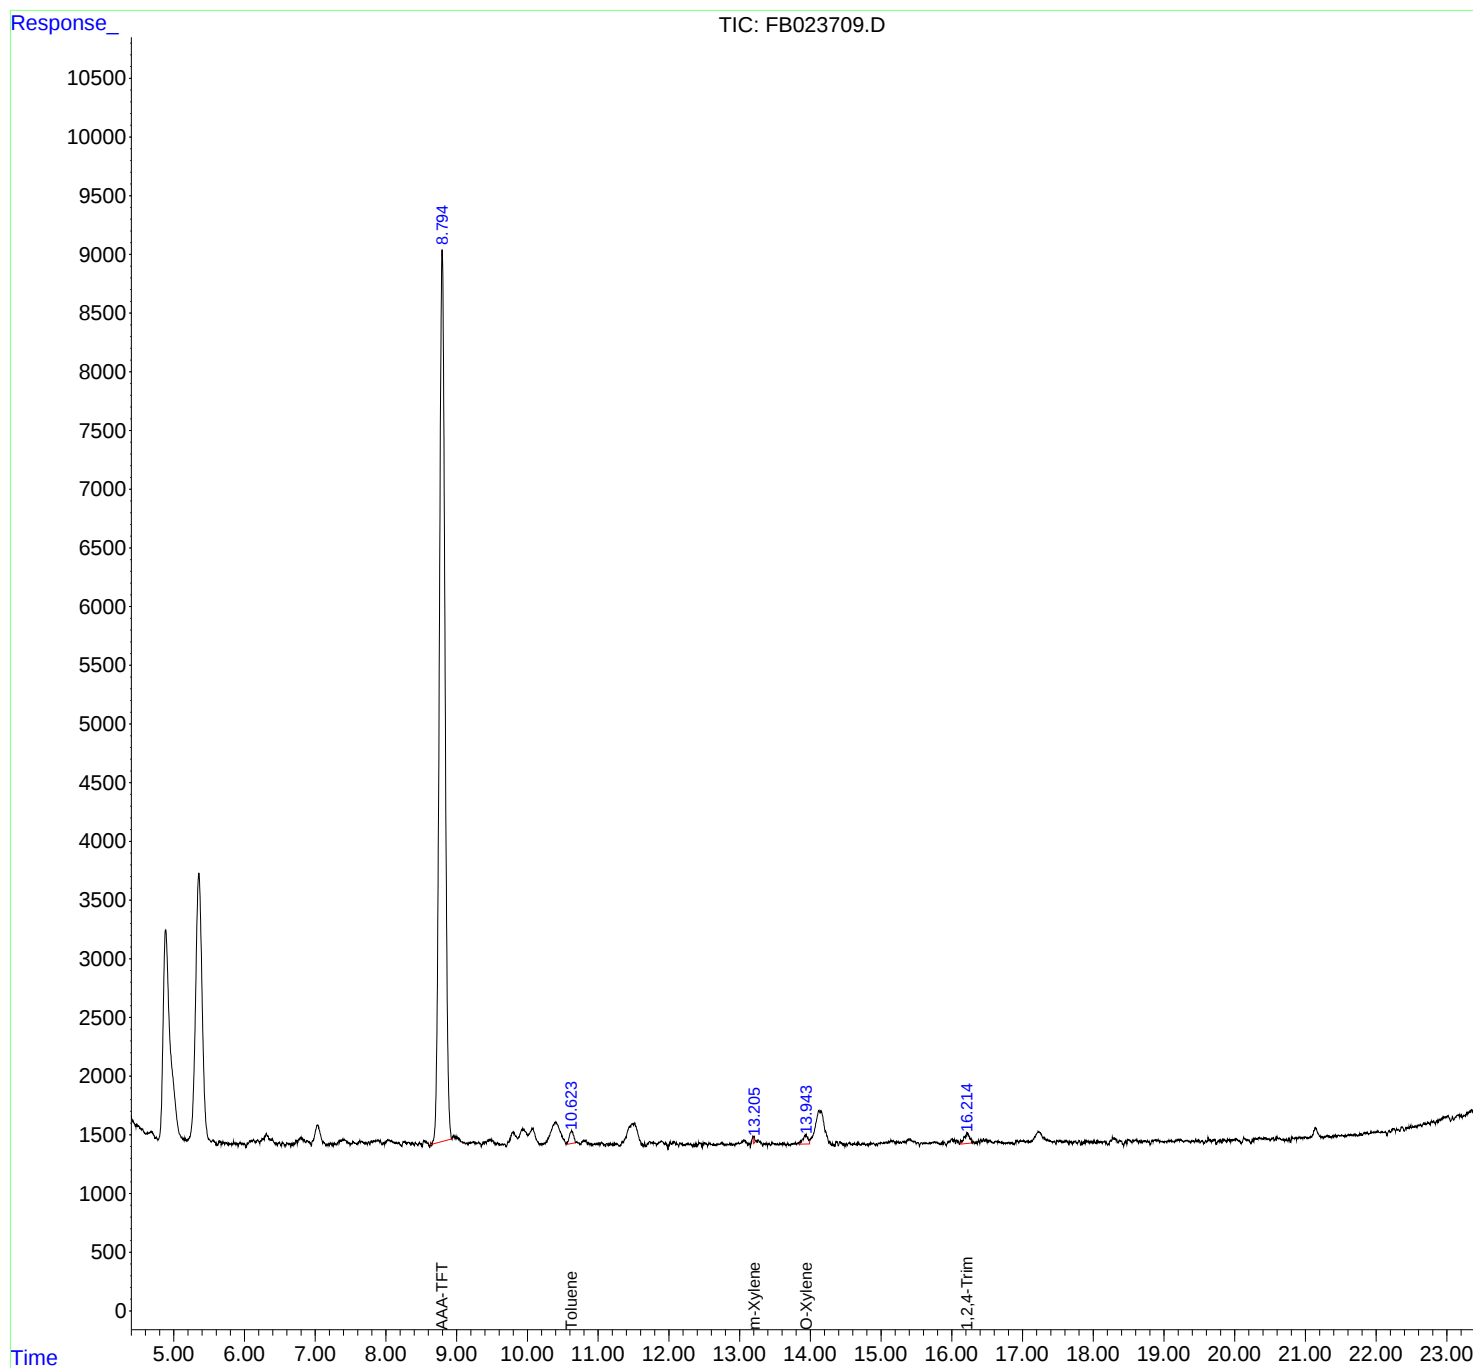

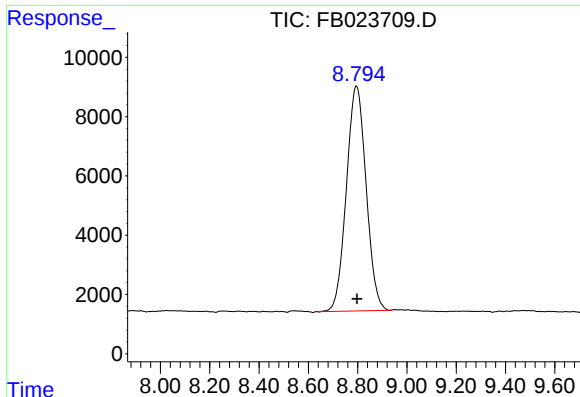


#5 AAA-TFT

R.T.: 8.795 min
Delta R.T.: -0.003 min
Response: 421590
Conc: 20.71 ng/ml

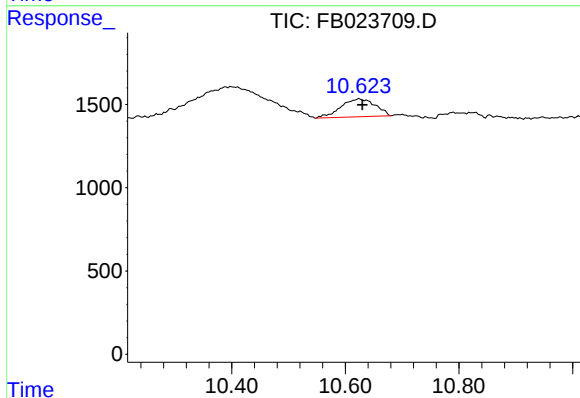


#6 Toluene

R.T.: 10.625 min
Delta R.T.: -0.005 min
Response: 4490
Conc: 0.11 ng/ml

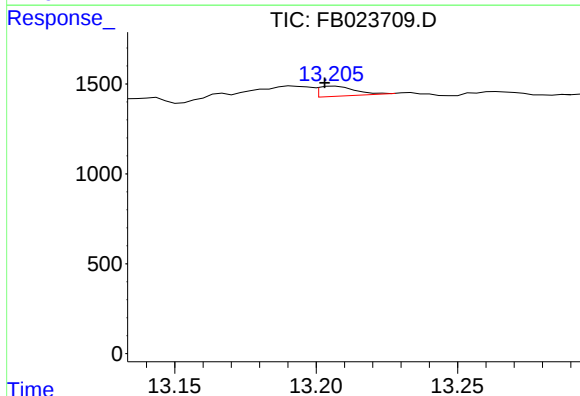


#8 m-Xylene

R.T.: 13.207 min
Delta R.T.: 0.004 min
Response: 485
Conc: 0.01 ng/ml

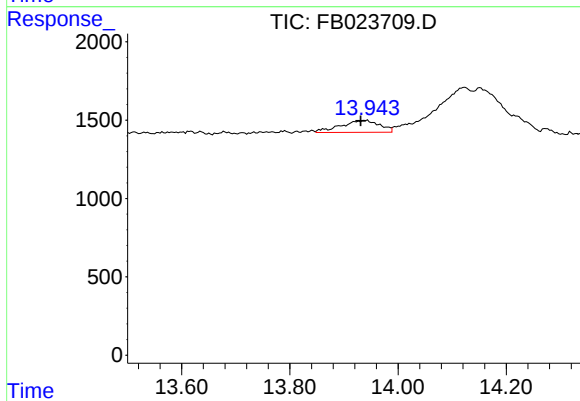

#9 O-Xylene

R.T.: 13.944 min
Delta R.T.: 0.012 min
Response: 3765
Conc: 0.11 ng/ml

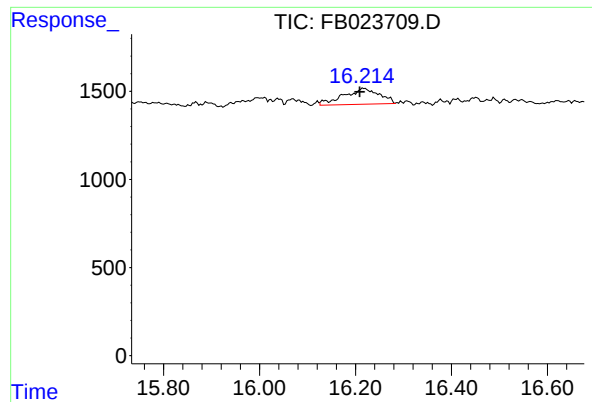

#10 1,2,4-Trimethylbenzene

R.T.: 16.216 min
Delta R.T.: 0.007 min
Response: 4615
Conc: 0.16 ng/ml