

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB022420\
 Data File : FB023711.D
 Signal(s) : FID2B.CH
 Acq On : 24 Feb 2020 11:58
 Operator : DD/AJ
 Sample : L1659-03MS
 Misc : 5.07g/5.00ml DI WATER
 ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Feb 25 00:18:09 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB020620.M
 Quant Title :
 QLast Update : Thu Feb 06 11:13:47 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.796	465625	22.870 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.689	854314	28.392 ng/ml
2) t 2,2,4-Trimethylpentane	7.414	945358	28.971 ng/ml
3) t n-Heptane	7.755	290587	9.032 ng/ml
4) t Benzene	7.890	417851	10.216 ng/ml
6) t Toluene	10.627	1207849	30.428 ng/ml
7) t Ethylbenzene	13.068	373947	10.059 ng/ml
8) t m-Xylene	13.201	720873	20.186 ng/ml
9) t O-Xylene	13.928	693471	20.107 ng/ml
10) t 1,2,4-Trimethylbenzene	16.207	582892	19.909 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB022420\
Data File : FB023711.D
Signal(s) : FID2B.CH
Acq On : 24 Feb 2020 11:58
Operator : DD/AJ
Sample : L1659-03MS
Misc : 5.07g/5.00ml DI WATER
ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Feb 25 00:18:09 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB020620.M
Quant Title :
QLast Update : Thu Feb 06 11:13:47 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

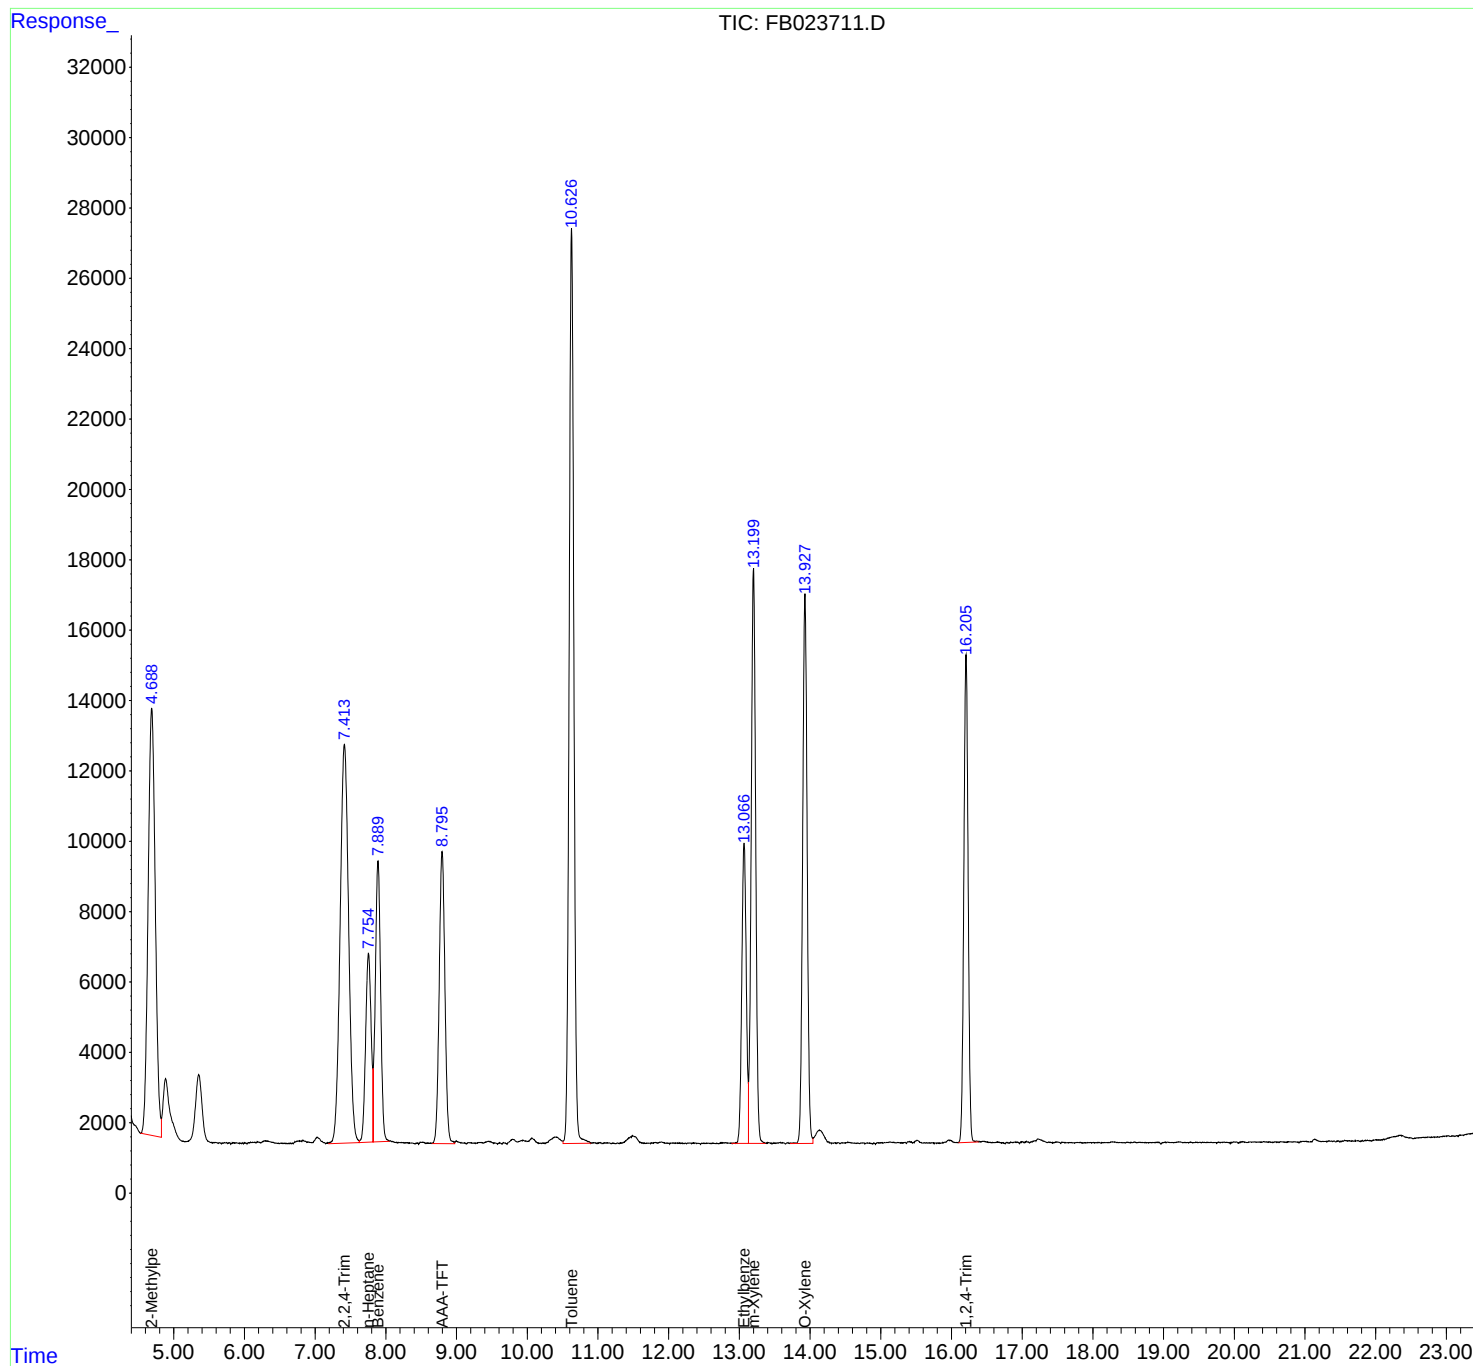

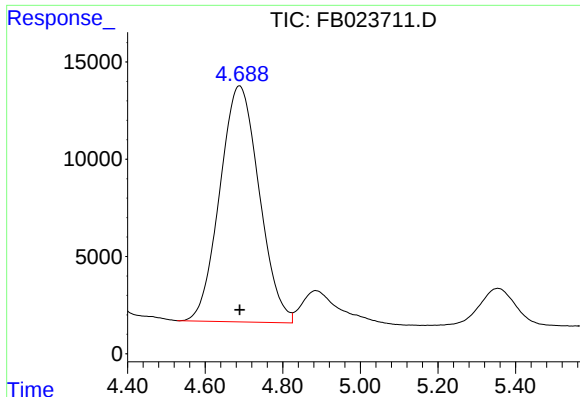


#1 2-Methylpentane

R.T.: 4.689 min
Delta R.T.: 0.000 min
Response: 854314
Conc: 28.39 ng/ml

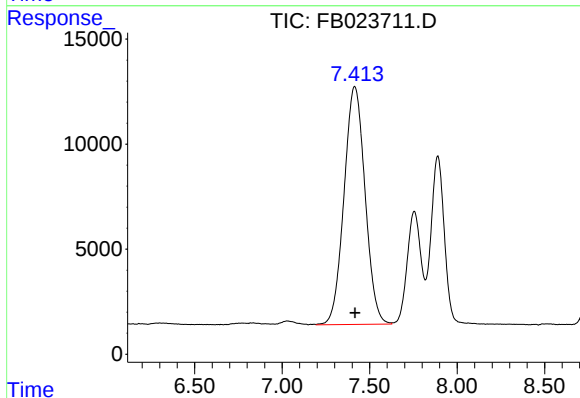


#2 2,2,4-Trimethylpentane

R.T.: 7.414 min
Delta R.T.: -0.004 min
Response: 945358
Conc: 28.97 ng/ml

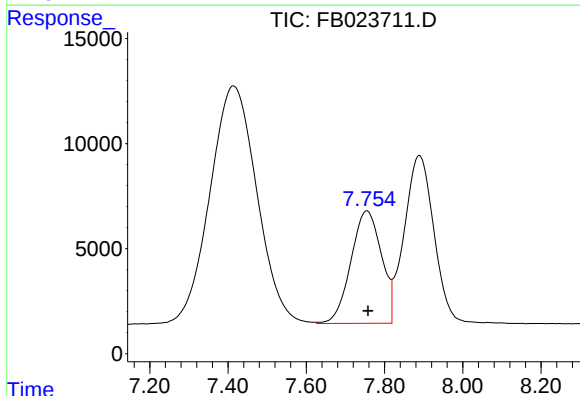


#3 n-Heptane

R.T.: 7.755 min
Delta R.T.: -0.002 min
Response: 290587
Conc: 9.03 ng/ml

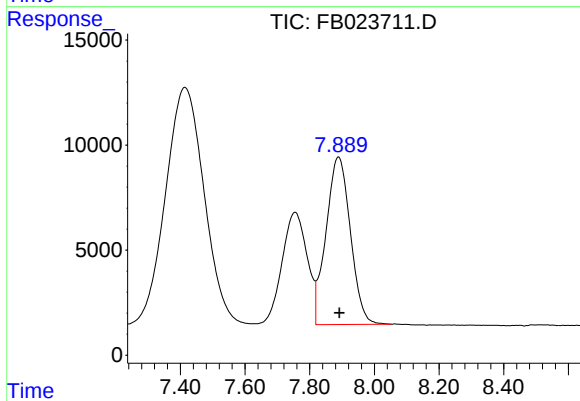


#4 Benzene

R.T.: 7.890 min
Delta R.T.: -0.002 min
Response: 417851
Conc: 10.22 ng/ml

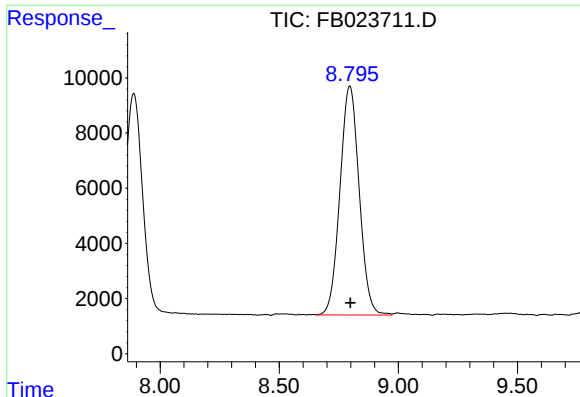


#5 AAA-TFT

R.T.: 8.796 min
Delta R.T.: -0.002 min
Response: 465625
Conc: 22.87 ng/ml

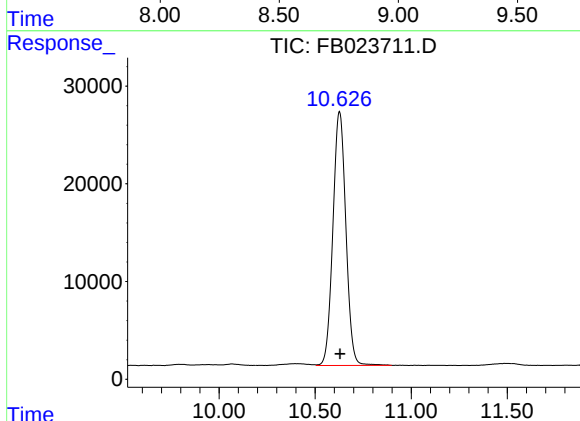


#6 Toluene

R.T.: 10.627 min
Delta R.T.: -0.003 min
Response: 1207849
Conc: 30.43 ng/ml

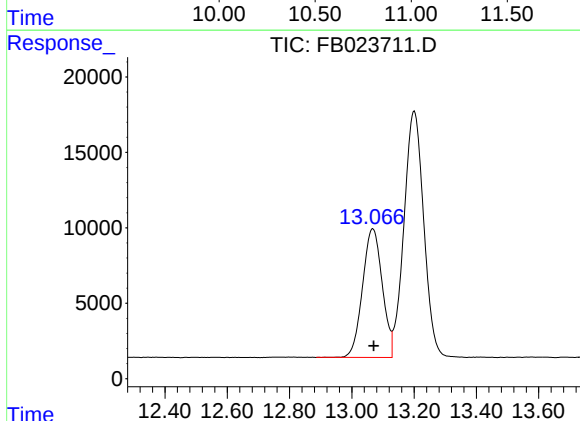


#7 Ethylbenzene

R.T.: 13.068 min
Delta R.T.: -0.003 min
Response: 373947
Conc: 10.06 ng/ml

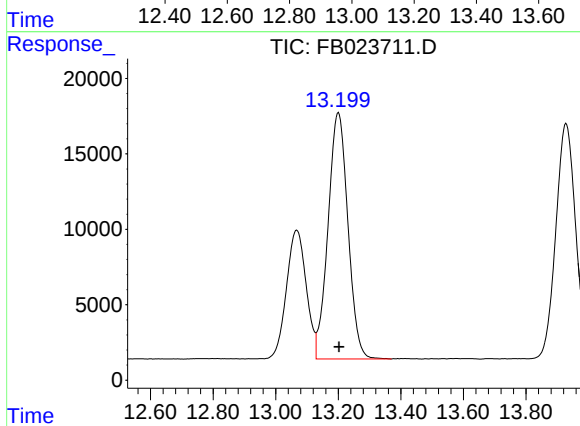


#8 m-Xylene

R.T.: 13.201 min
Delta R.T.: -0.002 min
Response: 720873
Conc: 20.19 ng/ml

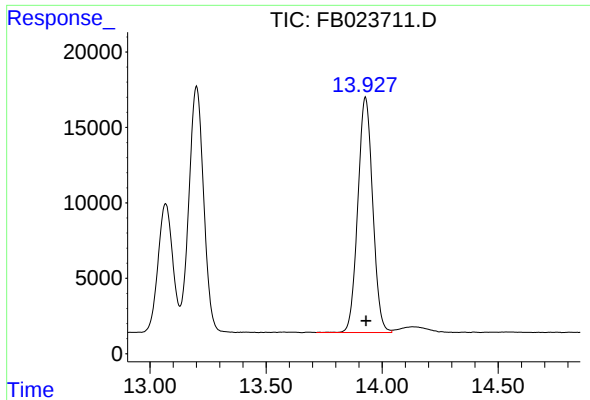

#9 O-Xylene

R.T.: 13.928 min
Delta R.T.: -0.003 min
Response: 693471
Conc: 20.11 ng/ml

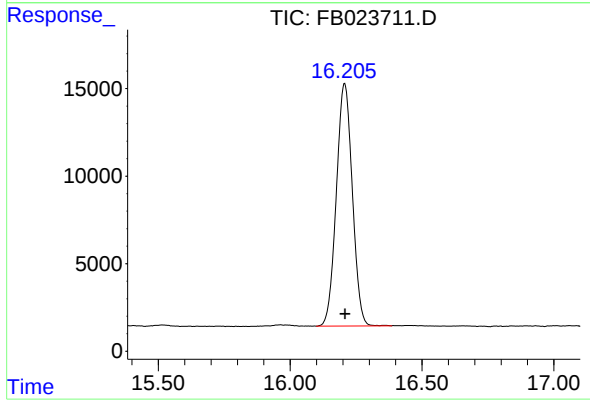

#10 1,2,4-Trimethylbenzene

R.T.: 16.207 min
Delta R.T.: -0.002 min
Response: 582892
Conc: 19.91 ng/ml