

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB022420\
 Data File : FB023712.D
 Signal(s) : FID2B.CH
 Acq On : 24 Feb 2020 12:28
 Operator : DD/AJ
 Sample : L1659-03MSD
 Misc : 5.09g/5.00ml DI WATER
 ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Feb 25 00:18:15 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB020620.M
 Quant Title :
 QLast Update : Thu Feb 06 11:13:47 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.797	463154	22.749 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.690	802777	26.679 ng/ml
2) t 2,2,4-Trimethylpentane	7.415	851862	26.106 ng/ml
3) t n-Heptane	7.756	260857	8.108 ng/ml
4) t Benzene	7.891	403040	9.854 ng/ml
6) t Toluene	10.628	1169753	29.469 ng/ml
7) t Ethylbenzene	13.068	353698	9.514 ng/ml
8) t m-Xylene	13.201	680446	19.054 ng/ml
9) t O-Xylene	13.929	656861	19.045 ng/ml
10) t 1,2,4-Trimethylbenzene	16.208	545101	18.618 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB022420\
Data File : FB023712.D
Signal(s) : FID2B.CH
Acq On : 24 Feb 2020 12:28
Operator : DD/AJ
Sample : L1659-03MSD
Misc : 5.09g/5.00ml DI WATER
ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Feb 25 00:18:15 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB020620.M
Quant Title :
QLast Update : Thu Feb 06 11:13:47 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

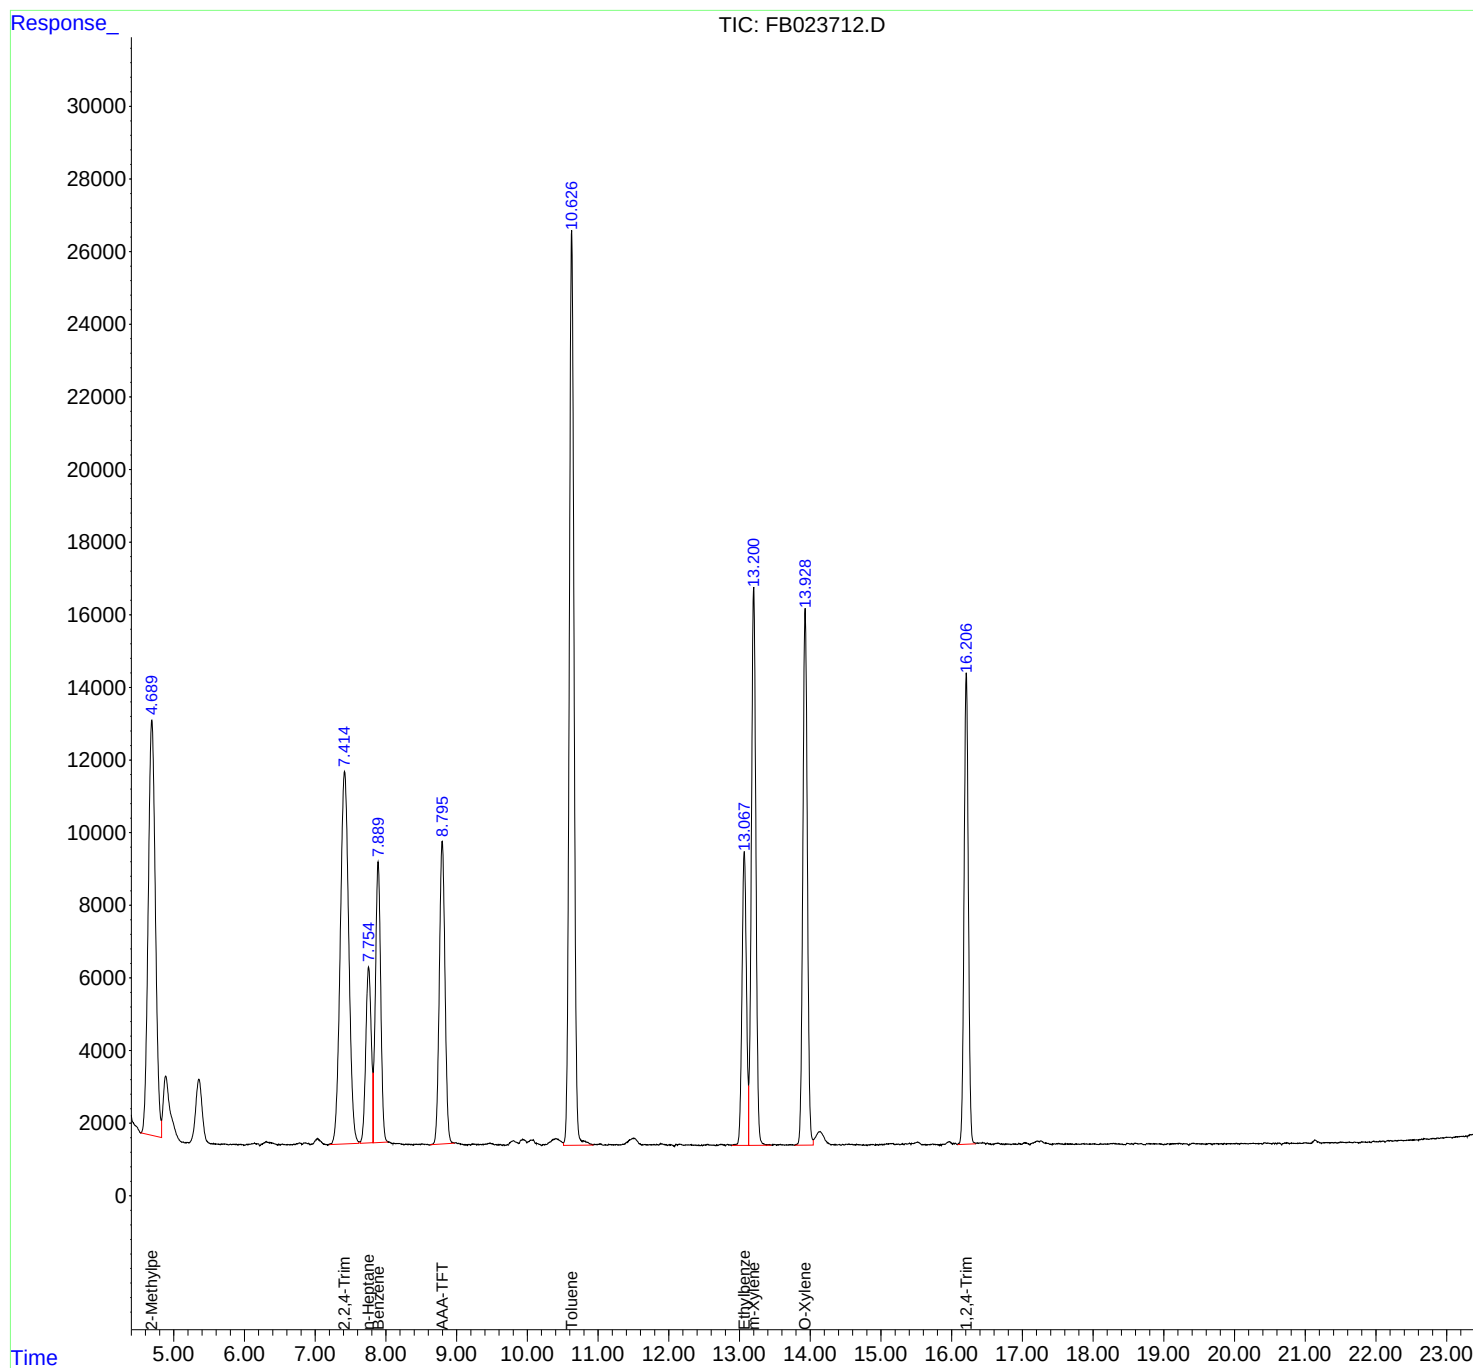

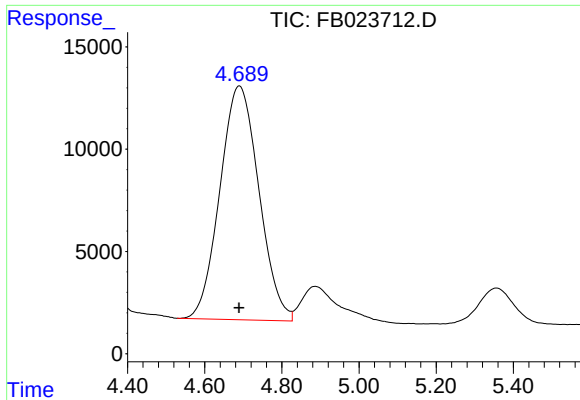


#1 2-Methylpentane

R.T.: 4.690 min
Delta R.T.: 0.001 min
Response: 802777
Conc: 26.68 ng/ml

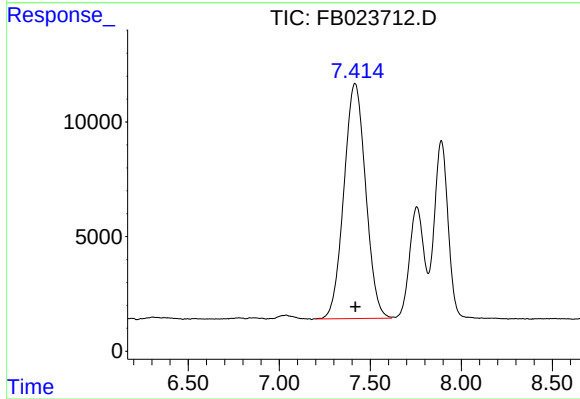


#2 2,2,4-Trimethylpentane

R.T.: 7.415 min
Delta R.T.: -0.002 min
Response: 851862
Conc: 26.11 ng/ml

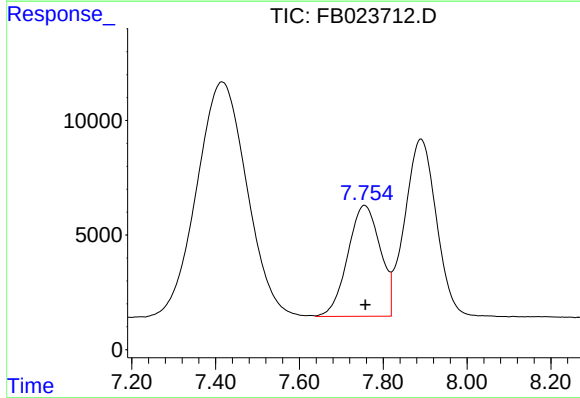


#3 n-Heptane

R.T.: 7.756 min
Delta R.T.: -0.002 min
Response: 260857
Conc: 8.11 ng/ml

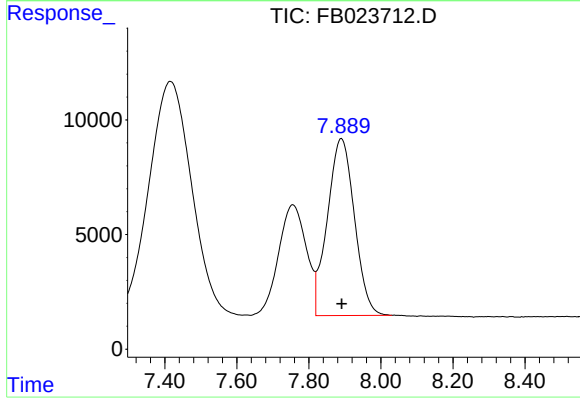


#4 Benzene

R.T.: 7.891 min
Delta R.T.: 0.000 min
Response: 403040
Conc: 9.85 ng/ml

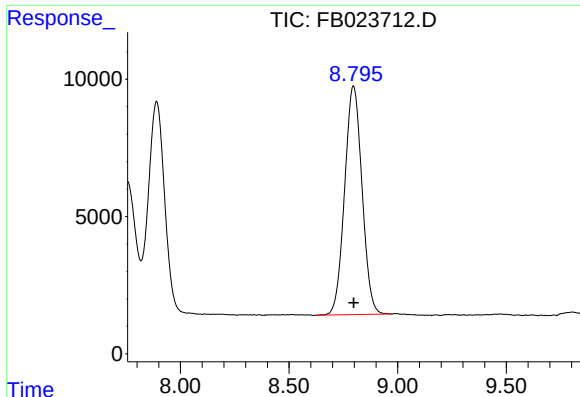


#5 AAA-TFT

R.T.: 8.797 min
Delta R.T.: -0.002 min
Response: 463154
Conc: 22.75 ng/ml

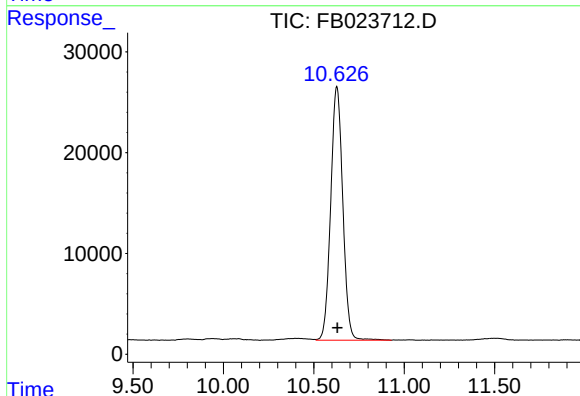


#6 Toluene

R.T.: 10.628 min
Delta R.T.: -0.003 min
Response: 1169753
Conc: 29.47 ng/ml

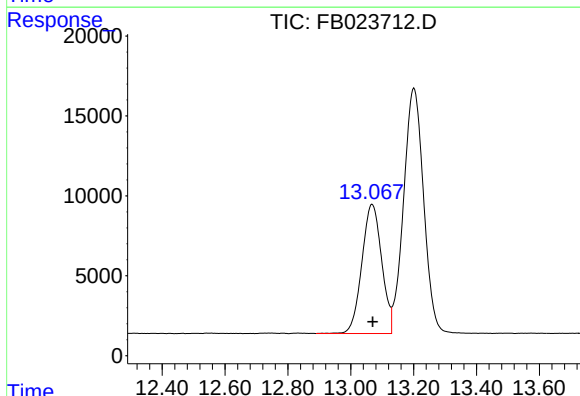


#7 Ethylbenzene

R.T.: 13.068 min
Delta R.T.: -0.002 min
Response: 353698
Conc: 9.51 ng/ml

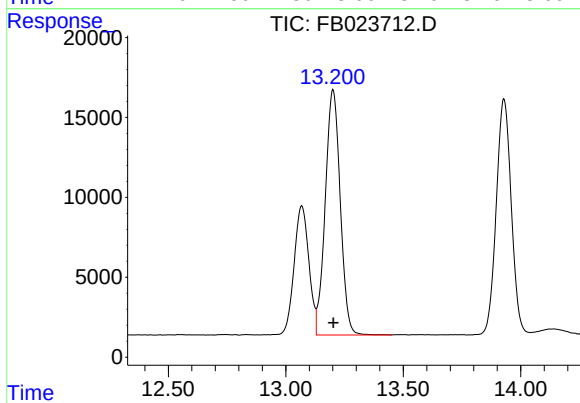


#8 m-Xylene

R.T.: 13.201 min
Delta R.T.: -0.002 min
Response: 680446
Conc: 19.05 ng/ml

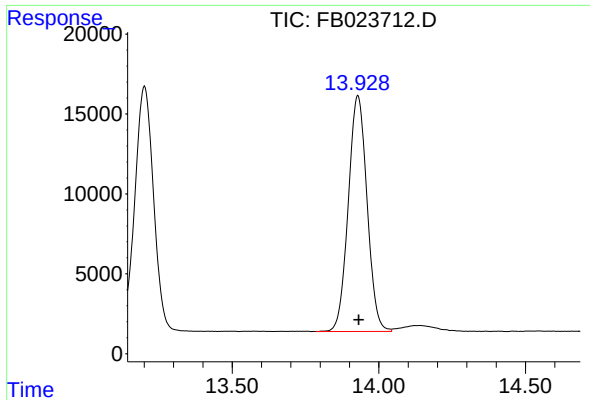

#9 O-Xylene

R.T.: 13.929 min
Delta R.T.: -0.002 min
Response: 656861
Conc: 19.05 ng/ml

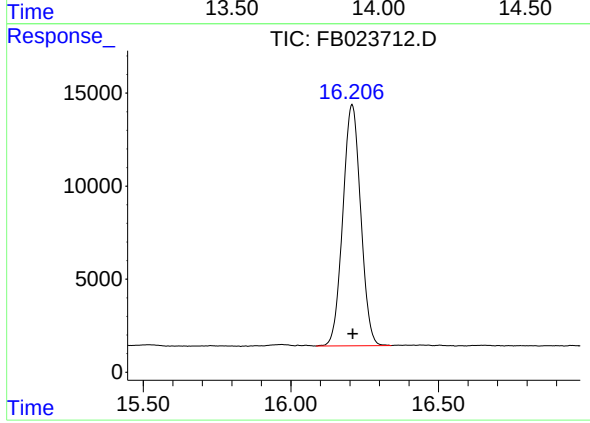

#10 1,2,4-Trimethylbenzene

R.T.: 16.208 min
Delta R.T.: -0.001 min
Response: 545101
Conc: 18.62 ng/ml