

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB022420\
Data File : FB023713.D
Signal(s) : FID2B.CH
Acq On : 24 Feb 2020 12:58
Operator : DD/AJ
Sample : L1659-05
Misc : 5.06g/5.00ml DI WATER
ALS Vial : 8 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Feb 25 00:18:21 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB020620.M
Quant Title :
QLast Update : Thu Feb 06 11:13:47 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.798	466054	22.891 ng/ml
Target Compounds			
6) t Toluene	10.626	474	0.012 ng/ml
8) t m-Xylene	13.212	3140	0.088 ng/ml
9) t O-Xylene	13.886	1051	0.030 ng/ml
10) t 1,2,4-Trimethylbenzene	16.204	5742	0.196 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB022420\
Data File : FB023713.D
Signal(s) : FID2B.CH
Acq On : 24 Feb 2020 12:58
Operator : DD/AJ
Sample : L1659-05
Misc : 5.06g/5.00ml DI WATER
ALS Vial : 8 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Feb 25 00:18:21 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB020620.M
Quant Title :
QLast Update : Thu Feb 06 11:13:47 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

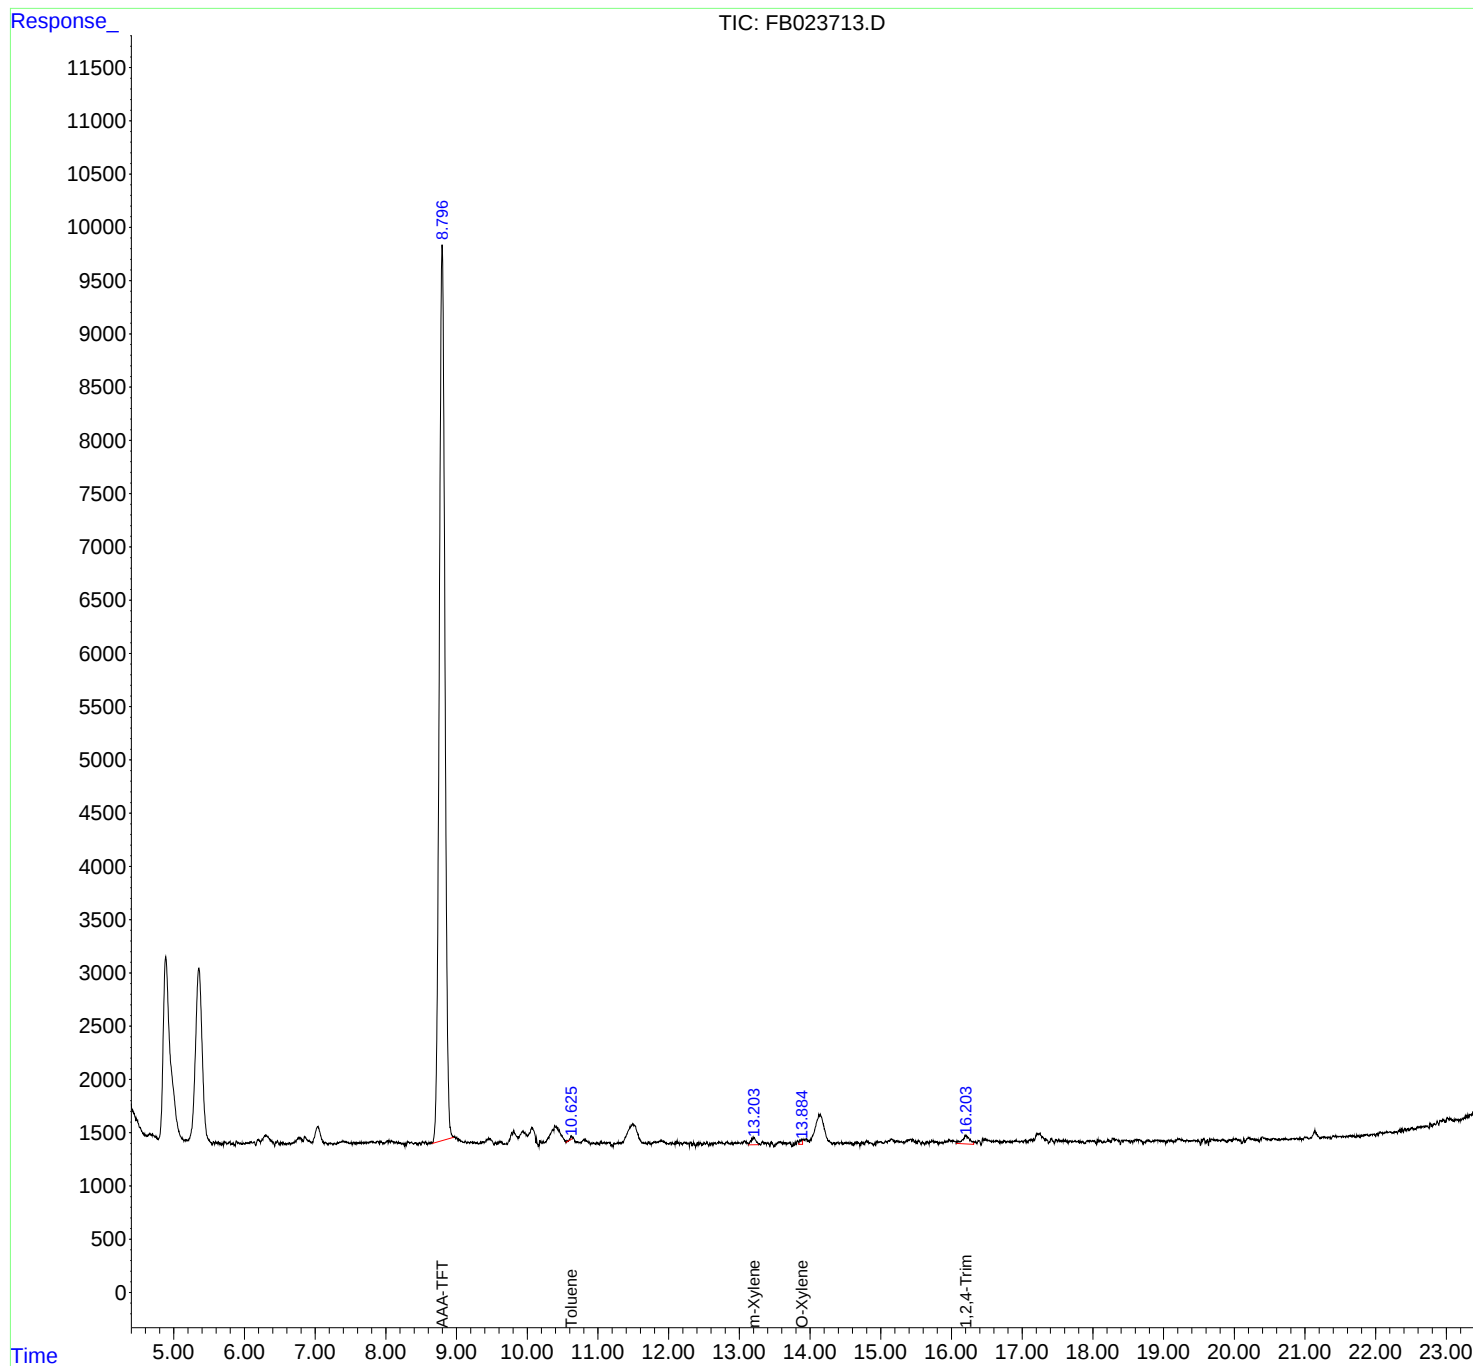

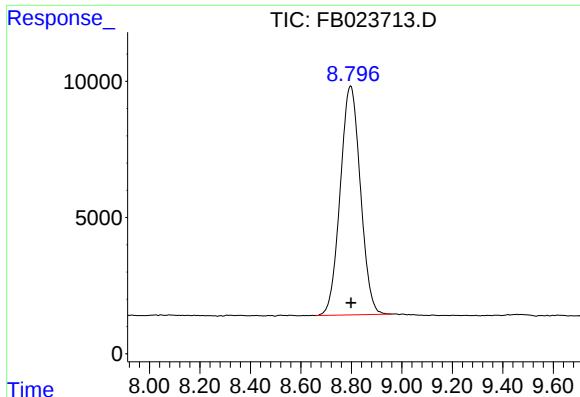


#5 AAA-TFT

R.T.: 8.798 min
Delta R.T.: 0.000 min
Response: 466054
Conc: 22.89 ng/ml

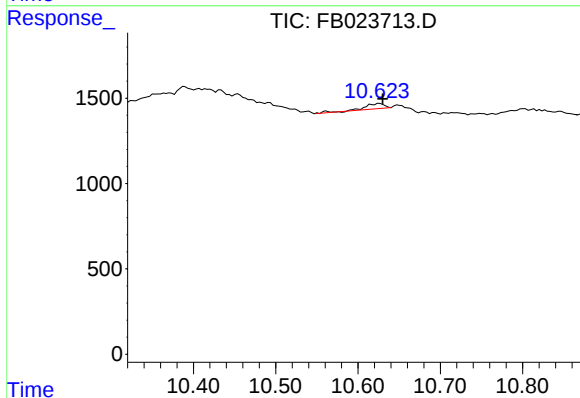


#6 Toluene

R.T.: 10.626 min
Delta R.T.: -0.004 min
Response: 474
Conc: 0.01 ng/ml

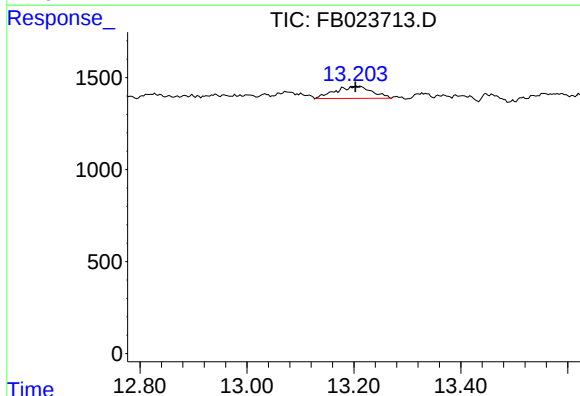


#8 m-Xylene

R.T.: 13.212 min
Delta R.T.: 0.008 min
Response: 3140
Conc: 0.09 ng/ml

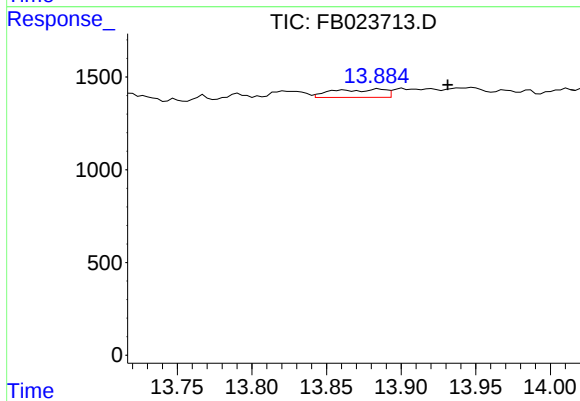

#9 O-Xylene

R.T.: 13.886 min
Delta R.T.: -0.045 min
Response: 1051
Conc: 0.03 ng/ml

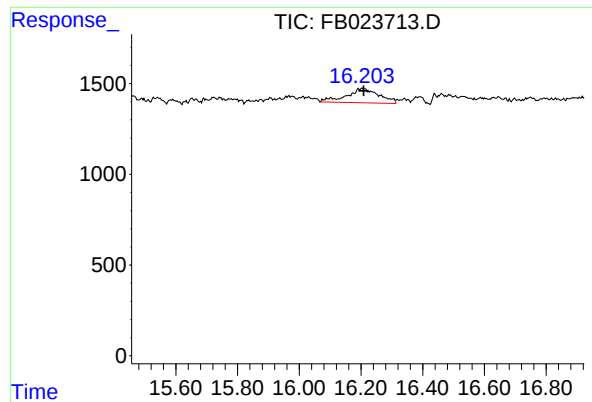

#10 1,2,4-Trimethylbenzene

R.T.: 16.204 min
Delta R.T.: -0.005 min
Response: 5742
Conc: 0.20 ng/ml