

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB022420\
 Data File : FB023708.D
 Signal(s) : FID2B.CH
 Acq On : 24 Feb 2020 10:20
 Operator : DD/AJ
 Sample : BSF0224S1
 Misc : 5.00g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Feb 25 00:17:53 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB020620.M
 Quant Title :
 QLast Update : Thu Feb 06 11:13:47 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.795	453139	22.257 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.687	912874	30.338 ng/ml
2) t 2,2,4-Trimethylpentane	7.414	1068226	32.736 ng/ml
3) t n-Heptane	7.753	339896	10.564 ng/ml
4) t Benzene	7.888	422875	10.339 ng/ml
6) t Toluene	10.626	1252083	31.543 ng/ml
7) t Ethylbenzene	13.067	386835	10.406 ng/ml
8) t m-Xylene	13.200	742495	20.791 ng/ml
9) t O-Xylene	13.928	715687	20.751 ng/ml
10) t 1,2,4-Trimethylbenzene	16.206	627155	21.420 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB022420\
Data File : FB023708.D
Signal(s) : FID2B.CH
Acq On : 24 Feb 2020 10:20
Operator : DD/AJ
Sample : BSF0224S1
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Feb 25 00:17:53 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB020620.M
Quant Title :
QLast Update : Thu Feb 06 11:13:47 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

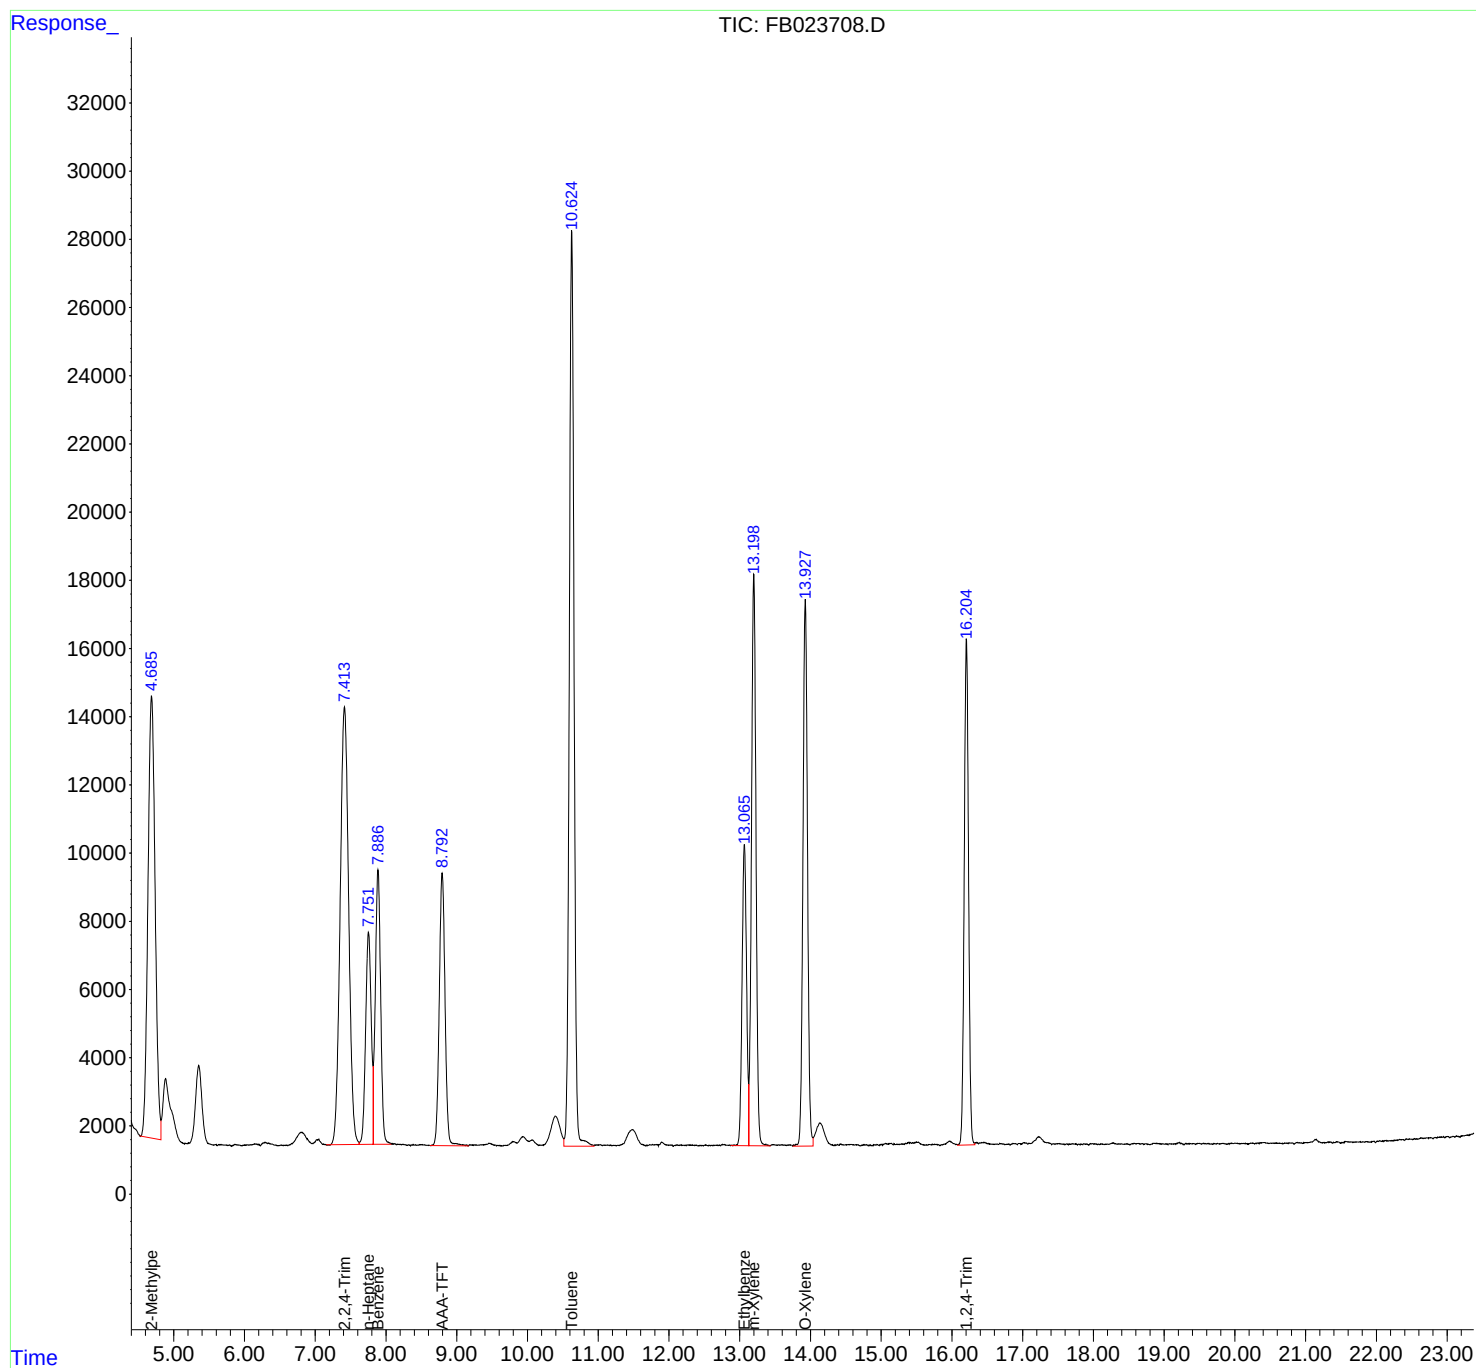

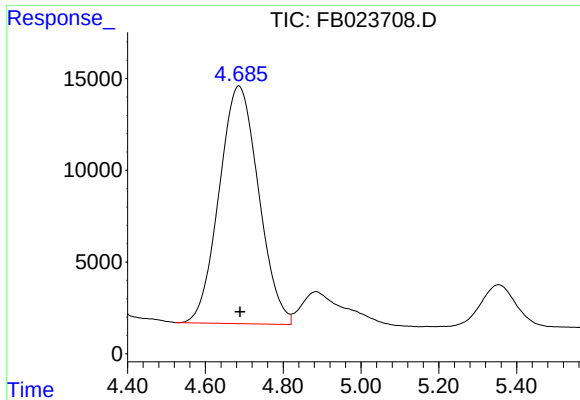


#1 2-Methylpentane

R.T.: 4.687 min
Delta R.T.: -0.002 min
Response: 912874
Conc: 30.34 ng/ml

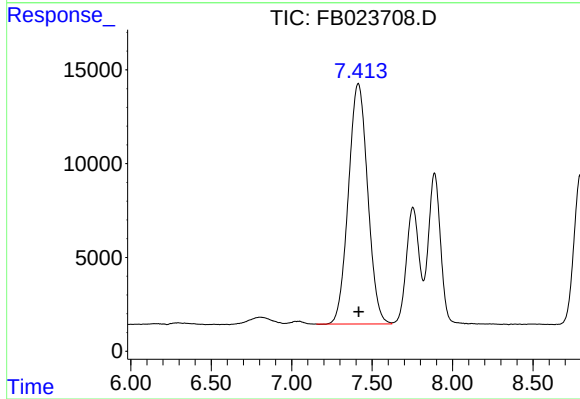


#2 2,2,4-Trimethylpentane

R.T.: 7.414 min
Delta R.T.: -0.004 min
Response: 1068226
Conc: 32.74 ng/ml

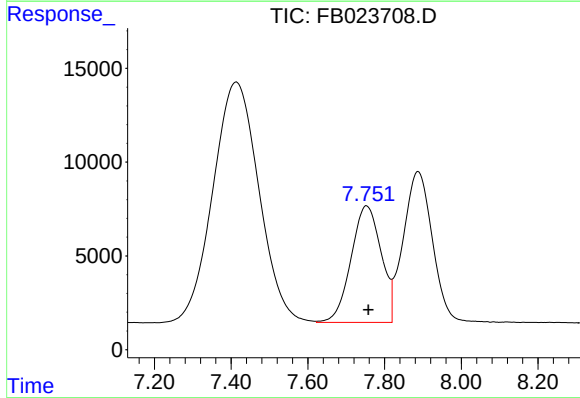


#3 n-Heptane

R.T.: 7.753 min
Delta R.T.: -0.005 min
Response: 339896
Conc: 10.56 ng/ml

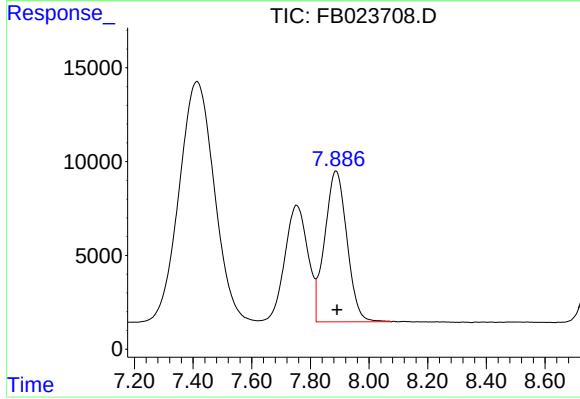


#4 Benzene

R.T.: 7.888 min
Delta R.T.: -0.004 min
Response: 422875
Conc: 10.34 ng/ml

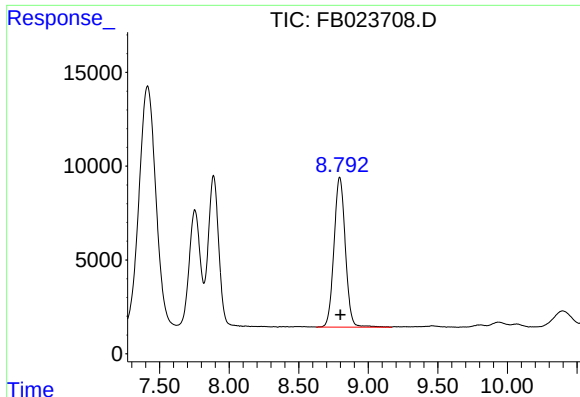


#5 AAA-TFT

R.T.: 8.795 min
Delta R.T.: -0.004 min
Response: 453139
Conc: 22.26 ng/ml

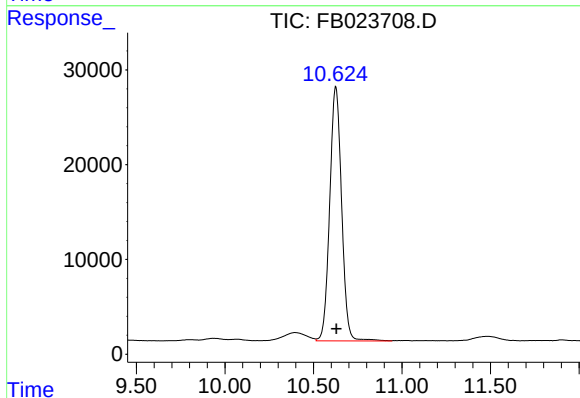


#6 Toluene

R.T.: 10.626 min
Delta R.T.: -0.004 min
Response: 1252083
Conc: 31.54 ng/ml

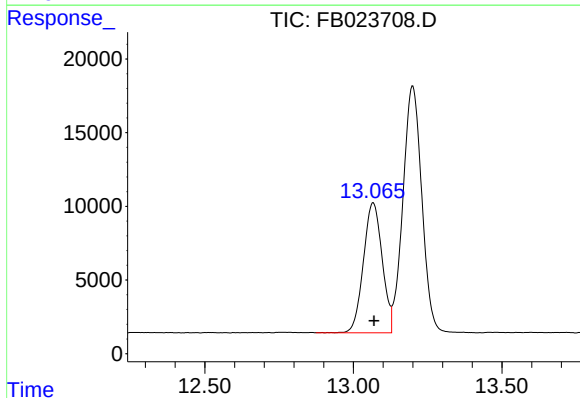


#7 Ethylbenzene

R.T.: 13.067 min
Delta R.T.: -0.004 min
Response: 386835
Conc: 10.41 ng/ml

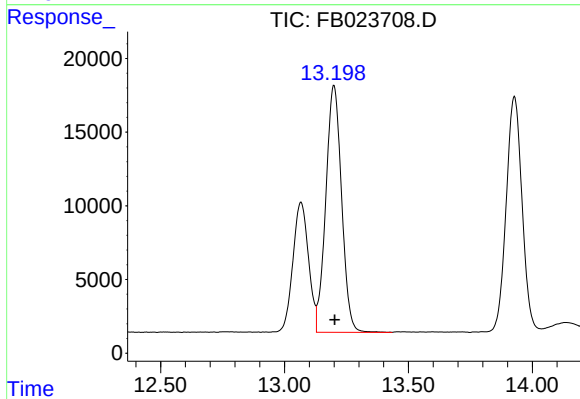


#8 m-Xylene

R.T.: 13.200 min
Delta R.T.: -0.003 min
Response: 742495
Conc: 20.79 ng/ml

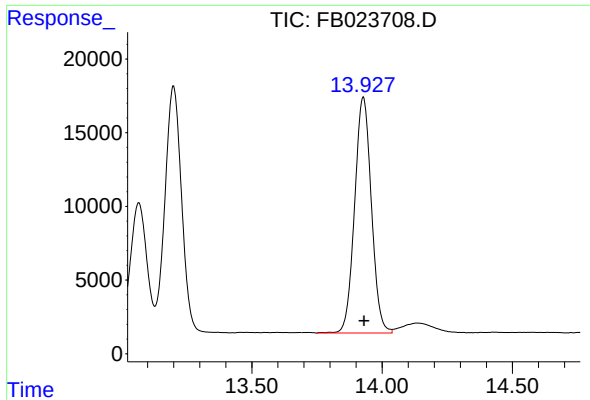

#9 O-Xylene

R.T.: 13.928 min
Delta R.T.: -0.003 min
Response: 715687
Conc: 20.75 ng/ml

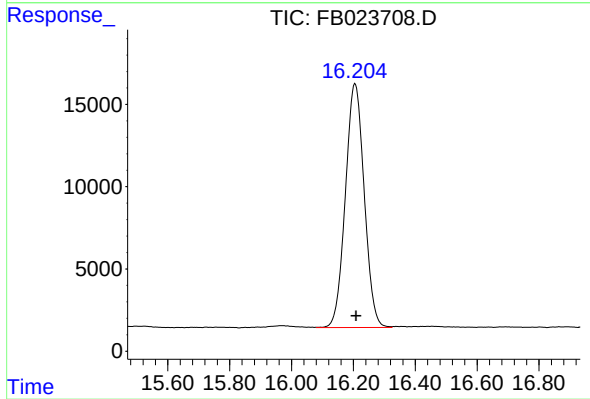

#10 1,2,4-Trimethylbenzene

R.T.: 16.206 min
Delta R.T.: -0.003 min
Response: 627155
Conc: 21.42 ng/ml