

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB022421\
Data File : FB025458.D
Signal(s) : FID2B.CH
Acq On : 24 Feb 2021 12:03
Operator : DD/AJ
Sample : M1472-03MSD
Misc : 5.08g/5.00ml DI WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Feb 25 00:19:37 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB021921.M
Quant Title :
QLast Update : Mon Feb 22 11:51:04 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
1) t 2-Methylpentane	4.719	13422702	380.841 ng/ml
2) t 2,2,4-Trimethylpentane	7.447	82222373	2214.328 ng/ml
3) t n-Heptane	7.779	75204907	2077.395 ng/ml
7) t Ethylbenzene	13.086	94703954	2346.460 ng/ml
8) t m-Xylene	13.210	21936697	545.304 ng/ml
9) t O-Xylene	13.869	59584718	1539.340 ng/ml
10) t 1,2,4-Trimethylbenzene	16.245	19201482	572.013 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB022421\
Data File : FB025458.D
Signal(s) : FID2B.CH
Acq On : 24 Feb 2021 12:03
Operator : DD/AJ
Sample : M1472-03MSD
Misc : 5.08g/5.00ml DI WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Feb 25 00:19:37 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB021921.M
Quant Title :
QLast Update : Mon Feb 22 11:51:04 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

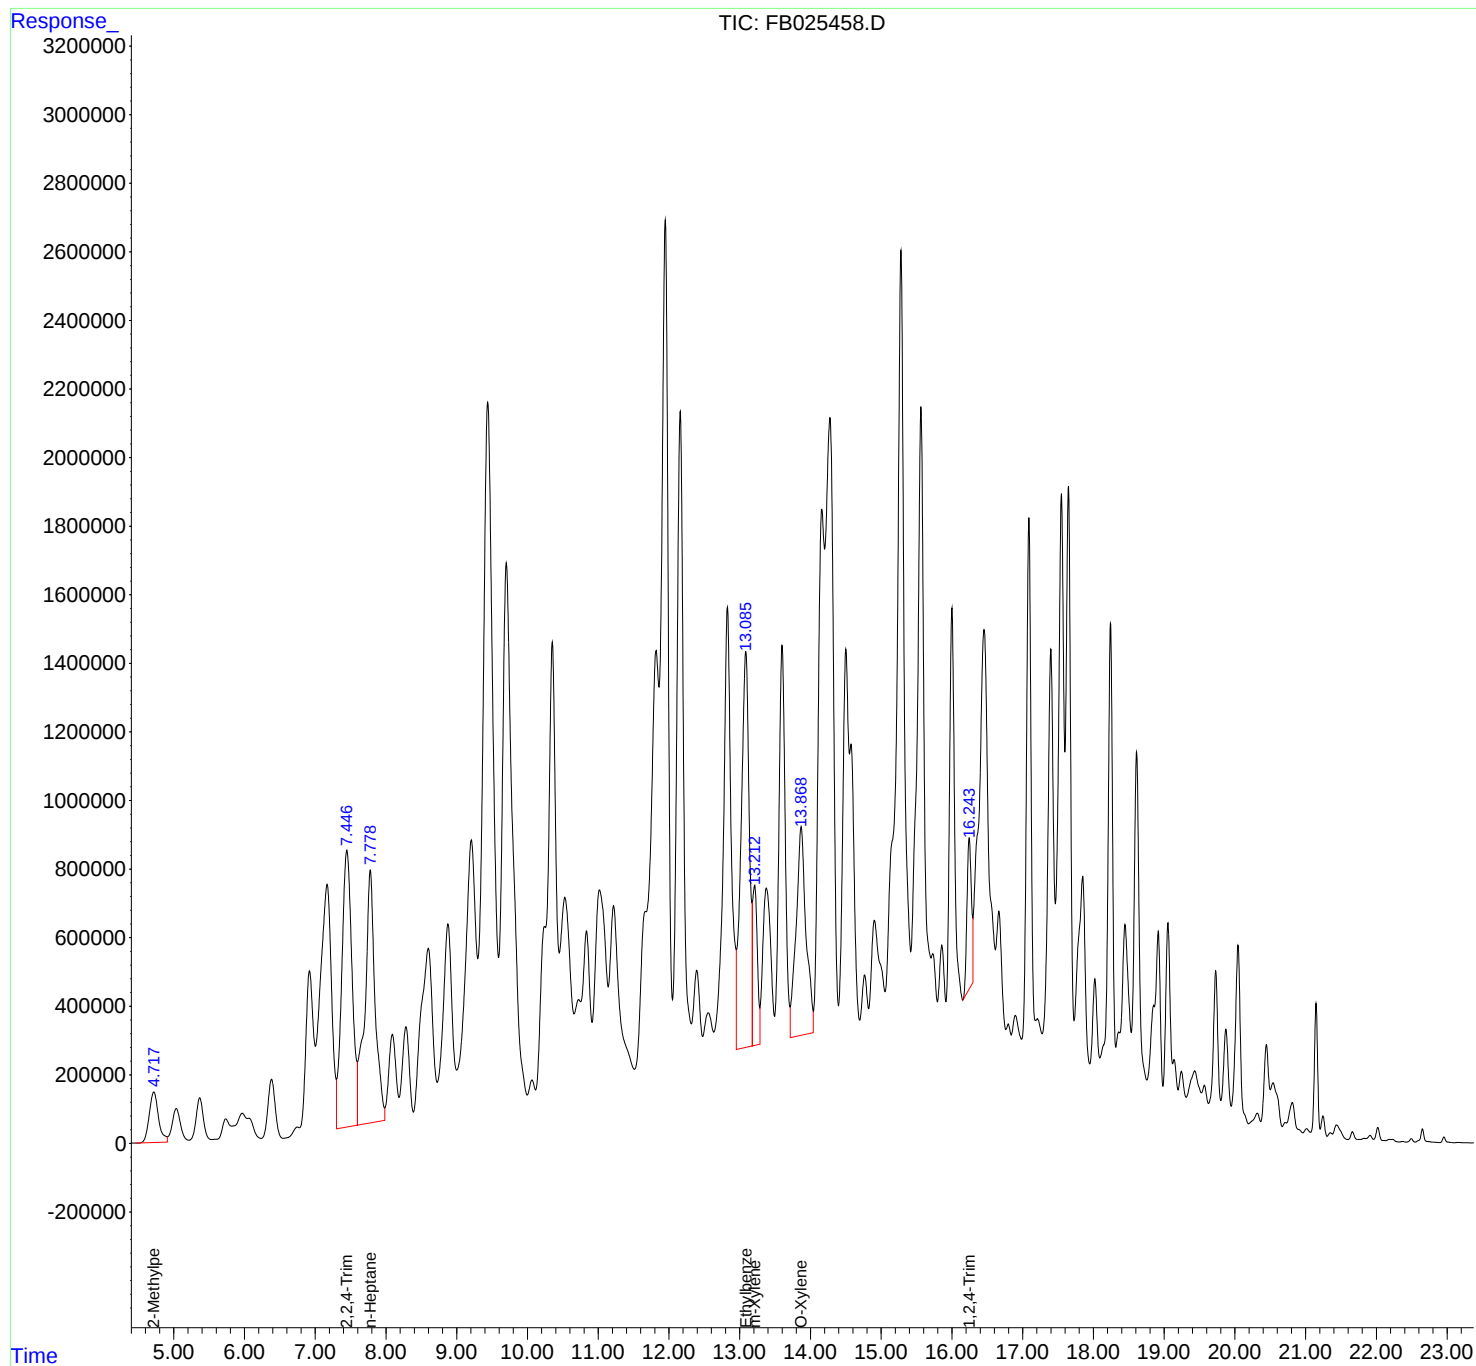


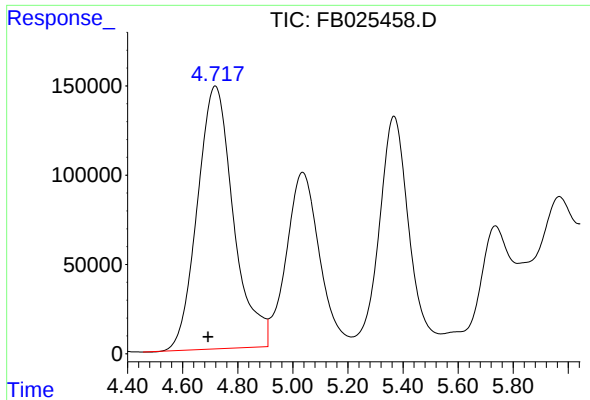

#1 2-Methylpentane


R.T.: 4.719 min
Delta R.T.: 0.027 min
Response: 13422702
Conc: 380.84 ng/ml

Instrument :
FID_B
ClientSampleId :

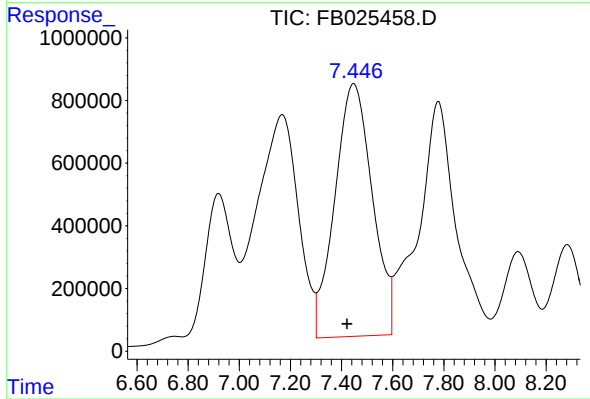


#2 2,2,4-Trimethylpentane

R.T.: 7.447 min
Delta R.T.: 0.025 min
Response: 82222373
Conc: 2214.33 ng/ml

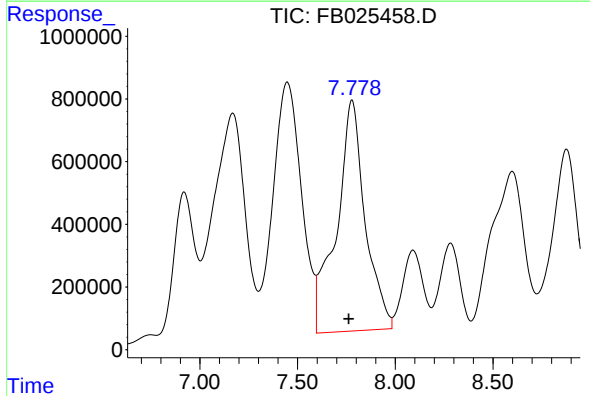


#3 n-Heptane

R.T.: 7.779 min
Delta R.T.: 0.017 min
Response: 75204907
Conc: 2077.39 ng/ml

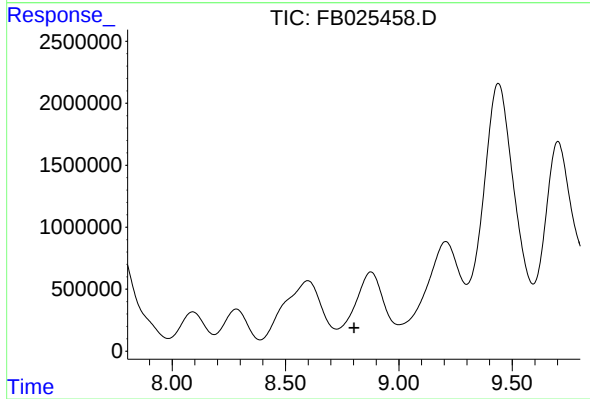

#5 AAA-TFT


R.T.: 0.000 min
Exp R.T.: 8.802 min
Response: 0
Conc: N.D.

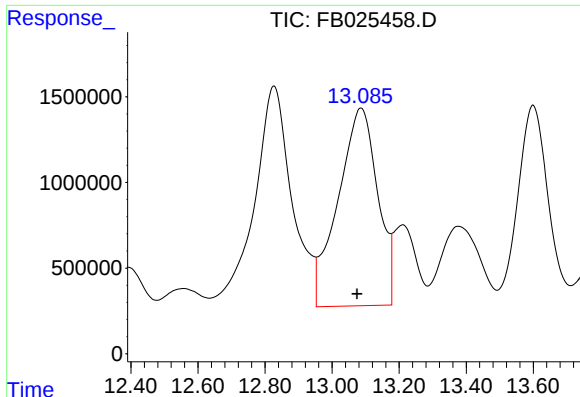

#7 Ethylbenzene


R.T.: 13.086 min
Delta R.T.: 0.012 min
Response: 94703954
Conc: 2346.46 ng/ml

Instrument :
FID_B
ClientSampleId :

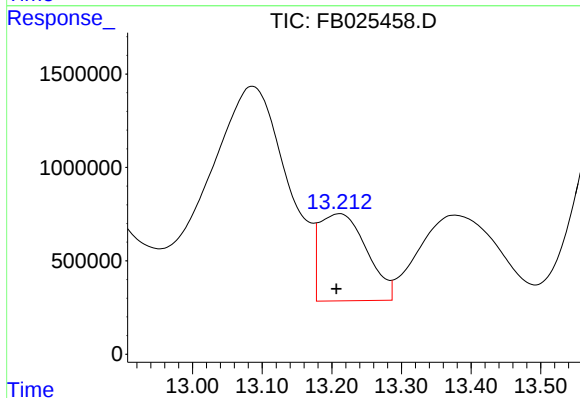


#8 m-Xylene

R.T.: 13.210 min
Delta R.T.: 0.003 min
Response: 21936697
Conc: 545.30 ng/ml

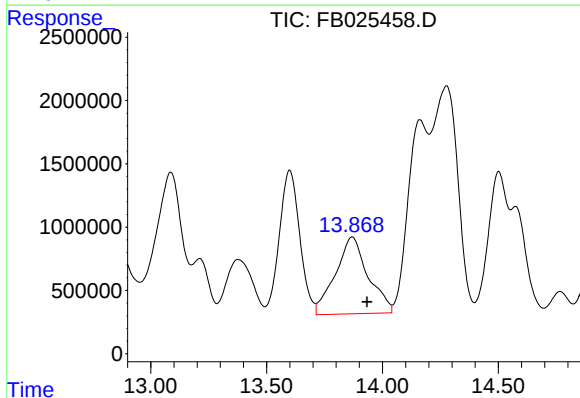

#9 o-Xylene

R.T.: 13.869 min
Delta R.T.: -0.065 min
Response: 59584718
Conc: 1539.34 ng/ml

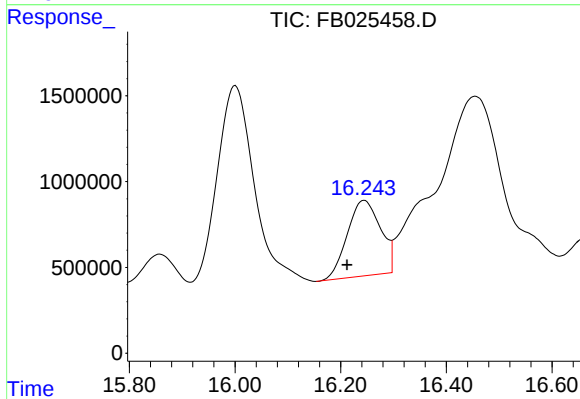

#10 1,2,4-Trimethylbenzene

R.T.: 16.245 min
Delta R.T.: 0.033 min
Response: 19201482
Conc: 572.01 ng/ml