

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB022421\
 Data File : FB025454.D
 Signal(s) : FID2B.CH
 Acq On : 24 Feb 2021 9:53
 Operator : DD/AJ
 Sample : BSF0224S1
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0224S1

Integration File: Calibration.e
 Quant Time: Feb 25 00:19:05 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB021921.M
 Quant Title :
 QLast Update : Mon Feb 22 11:51:04 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.799	487611	19.224 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.687	983295	27.899 ng/ml
2) t 2,2,4-Trimethylpentane	7.419	1088155	29.305 ng/ml
3) t n-Heptane	7.758	353831	9.774 ng/ml
4) t Benzene	7.893	429733	9.302 ng/ml
6) t Toluene	10.631	1229099	27.491 ng/ml
7) t Ethylbenzene	13.072	383507	9.502 ng/ml
8) t m-Xylene	13.205	767512	19.079 ng/ml
9) t O-Xylene	13.932	731736	18.904 ng/ml
10) t 1,2,4-Trimethylbenzene	16.210	634622	18.905 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB022421\
Data File : FB025454.D
Signal(s) : FID2B.CH
Acq On : 24 Feb 2021 9:53
Operator : DD/AJ
Sample : BSF0224S1
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0224S1

Integration File: Calibration.e
Quant Time: Feb 25 00:19:05 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB021921.M
Quant Title :
QLast Update : Mon Feb 22 11:51:04 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

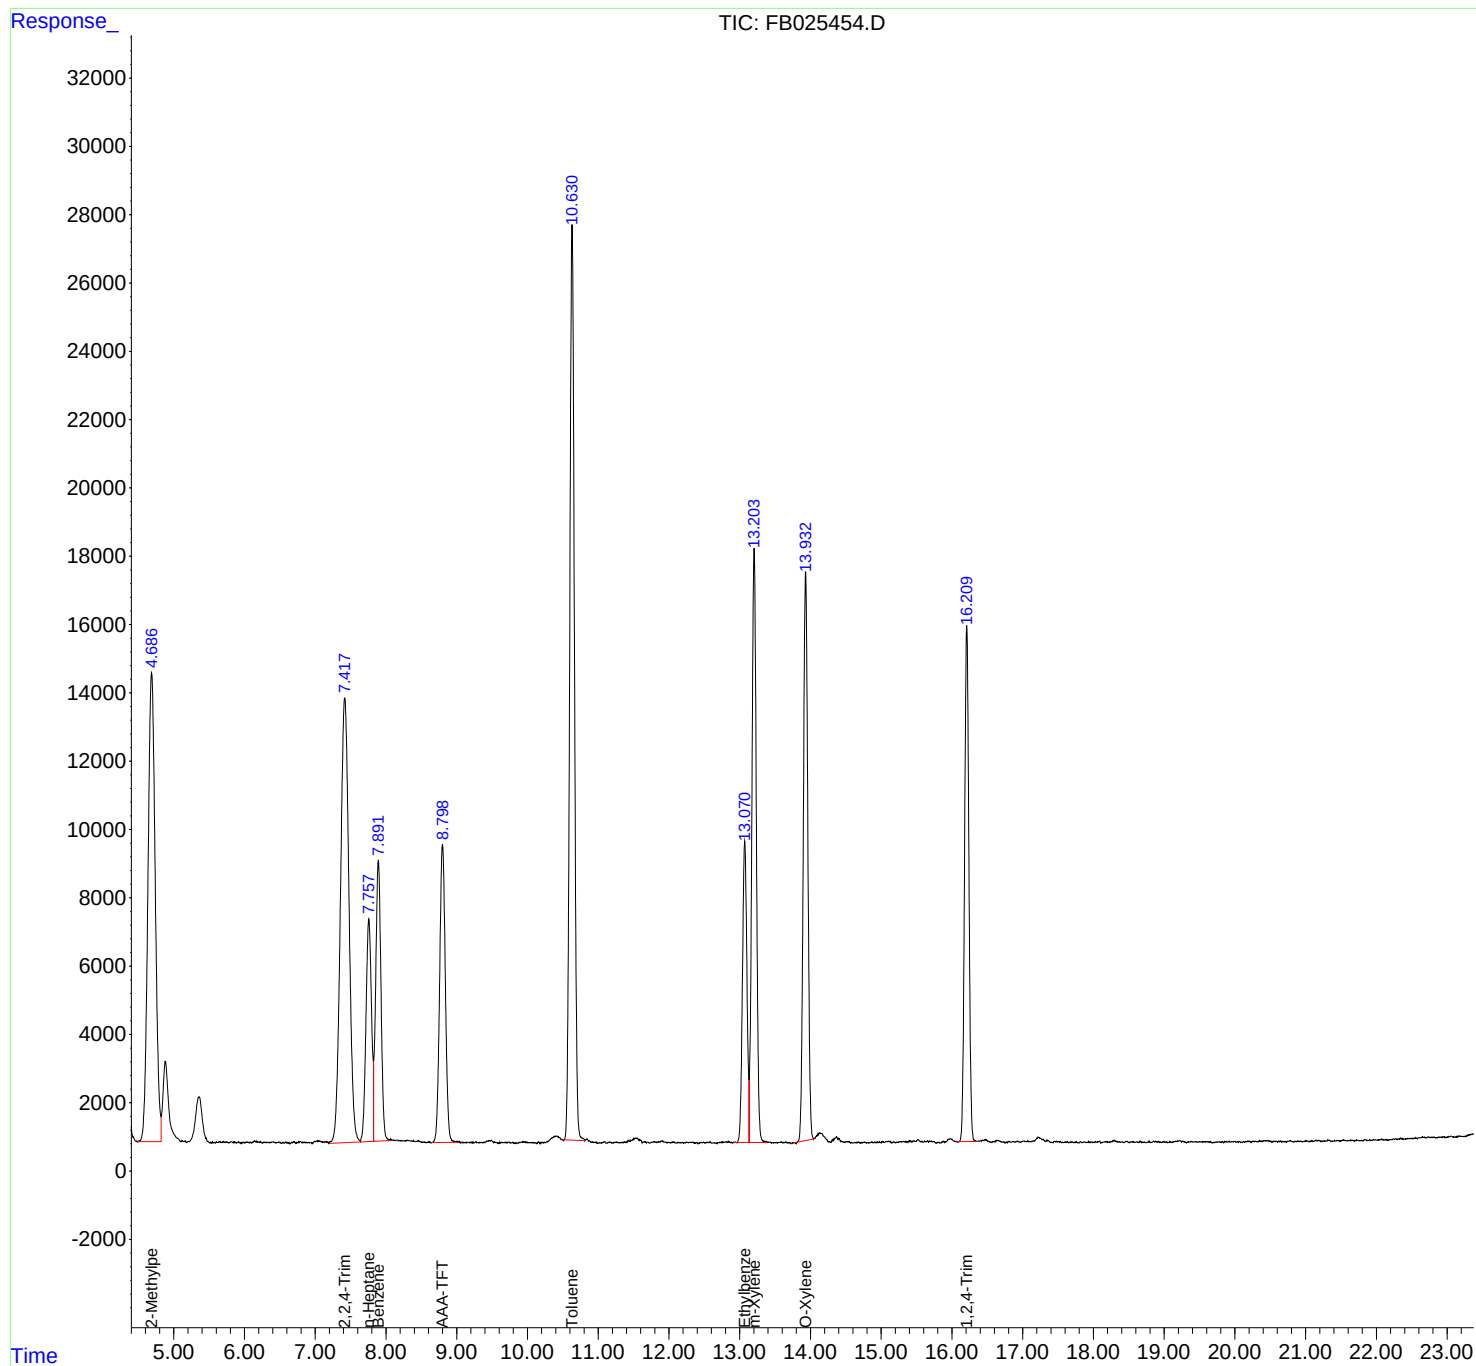


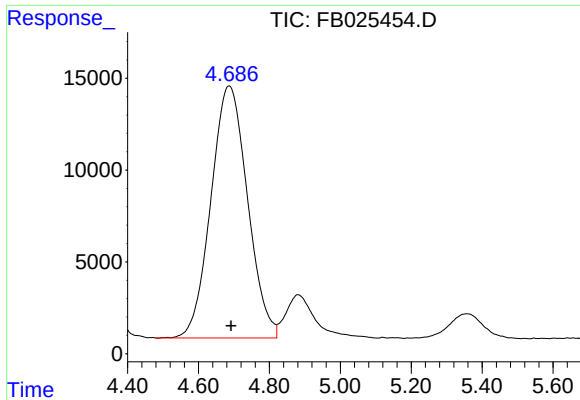

#1 2-Methylpentane


R.T.: 4.687 min
Delta R.T.: -0.005 min
Response: 983295
Conc: 27.90 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0224S1

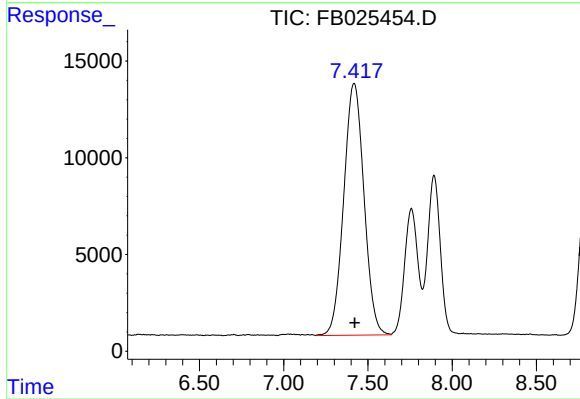


#2 2,2,4-Trimethylpentane

R.T.: 7.419 min
Delta R.T.: -0.003 min
Response: 1088155
Conc: 29.31 ng/ml

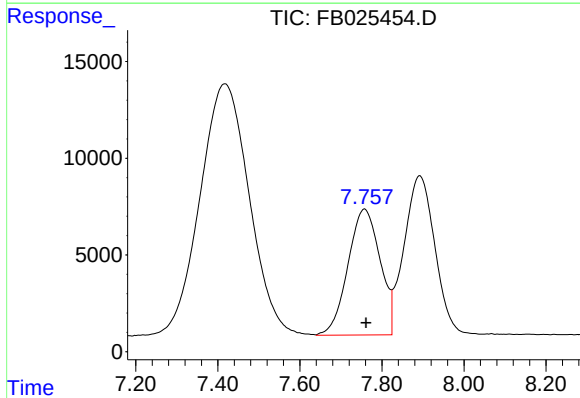


#3 n-Heptane

R.T.: 7.758 min
Delta R.T.: -0.003 min
Response: 353831
Conc: 9.77 ng/ml

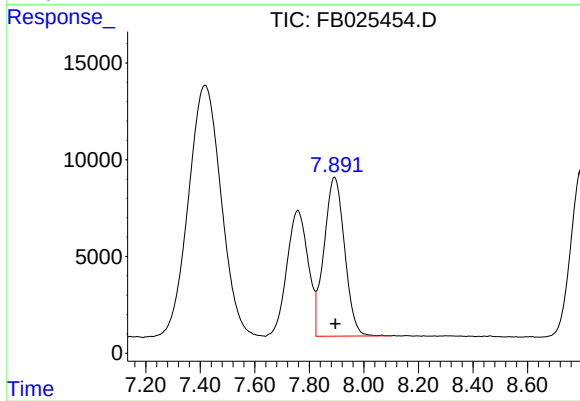

#4 Benzene


R.T.: 7.893 min
Delta R.T.: -0.003 min
Response: 429733
Conc: 9.30 ng/ml

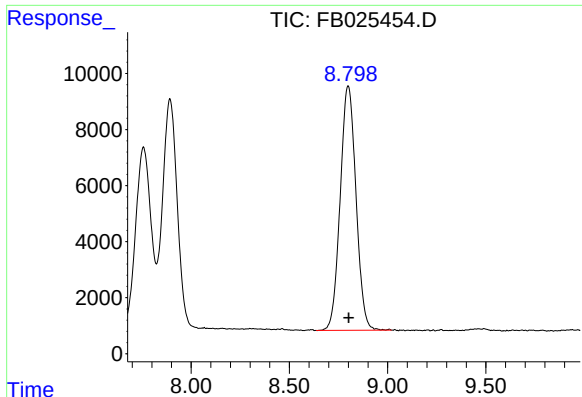

#5 AAA-TFT


R.T.: 8.799 min
Delta R.T.: -0.003 min
Response: 487611
Conc: 19.22 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0224S1

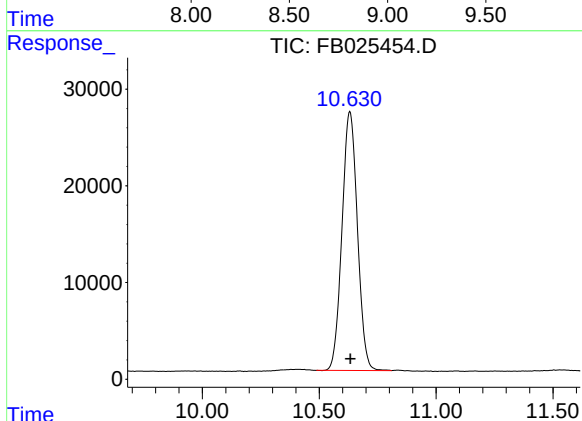


#6 Toluene

R.T.: 10.631 min
Delta R.T.: -0.002 min
Response: 1229099
Conc: 27.49 ng/ml

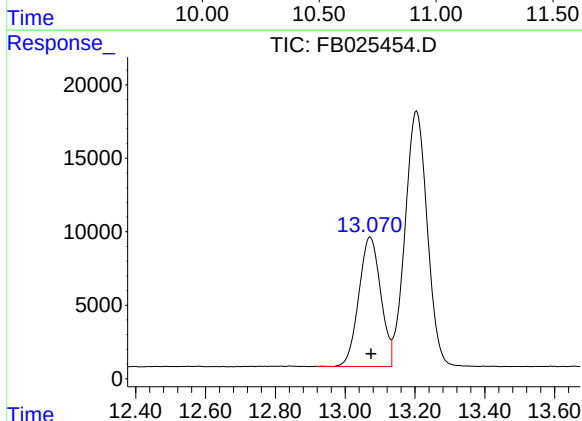


#7 Ethylbenzene

R.T.: 13.072 min
Delta R.T.: -0.002 min
Response: 383507
Conc: 9.50 ng/ml

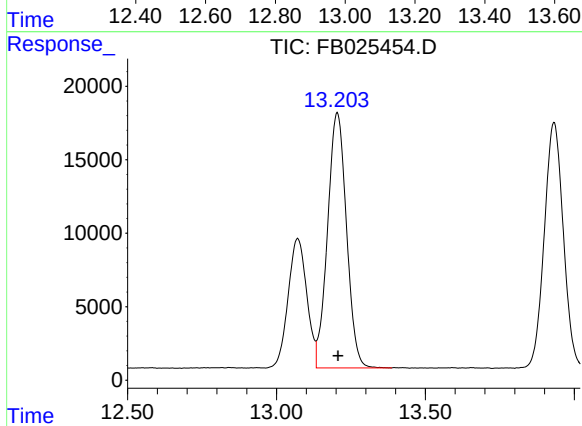

#8 m-Xylene


R.T.: 13.205 min
Delta R.T.: -0.002 min
Response: 767512
Conc: 19.08 ng/ml

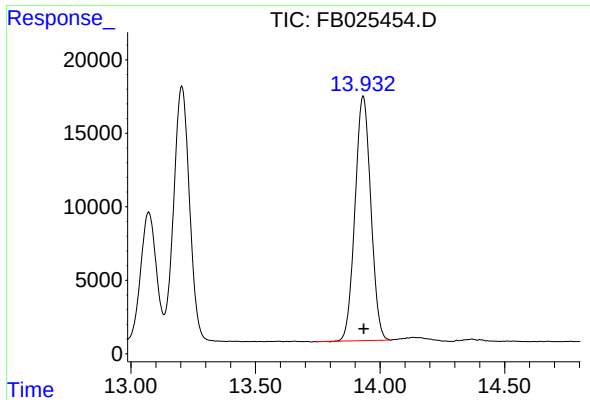

#9 O-Xylene

R.T.: 13.932 min
Delta R.T.: -0.002 min
Response: 731736
Conc: 18.90 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0224S1

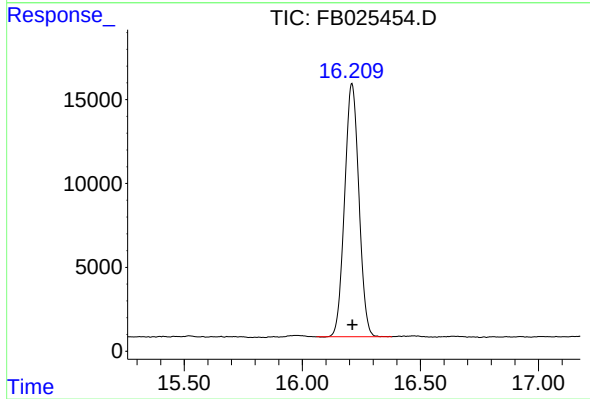

#10 1,2,4-Trimethylbenzene

R.T.: 16.210 min
Delta R.T.: -0.002 min
Response: 634622
Conc: 18.91 ng/ml