

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB022519\
 Data File : FB019881.D
 Signal(s) : FID2B.CH
 Acq On : 25 Feb 2019 10:06
 Operator : MJ/SJ
 Sample : BSF0225S1
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Feb 25 10:42:22 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB012919.M
 Quant Title :
 QLast Update : Tue Jan 29 12:07:12 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.040	214392	19.169 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.895	580883	31.702 ng/ml
2) t 2,2,4-Trimethylpentane	7.654	567102	32.466 ng/ml
3) t n-Heptane	7.994	174418	10.477 ng/ml
4) t Benzene	8.132	193424	10.045 ng/ml
6) t Toluene	10.887	513075	29.479 ng/ml
7) t Ethylbenzene	13.339	206997	9.560 ng/ml
8) t m-Xylene	13.473	431178	19.091 ng/ml
9) t O-Xylene	14.205	416163	18.819 ng/ml
10) t 1,2,4-Trimethylbenzene	16.491	428282	18.817 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB022519\
Data File : FB019881.D
Signal(s) : FID2B.CH
Acq On : 25 Feb 2019 10:06
Operator : MJ/SJ
Sample : BSF0225S1
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Feb 25 10:42:22 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB012919.M
Quant Title :
QLast Update : Tue Jan 29 12:07:12 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

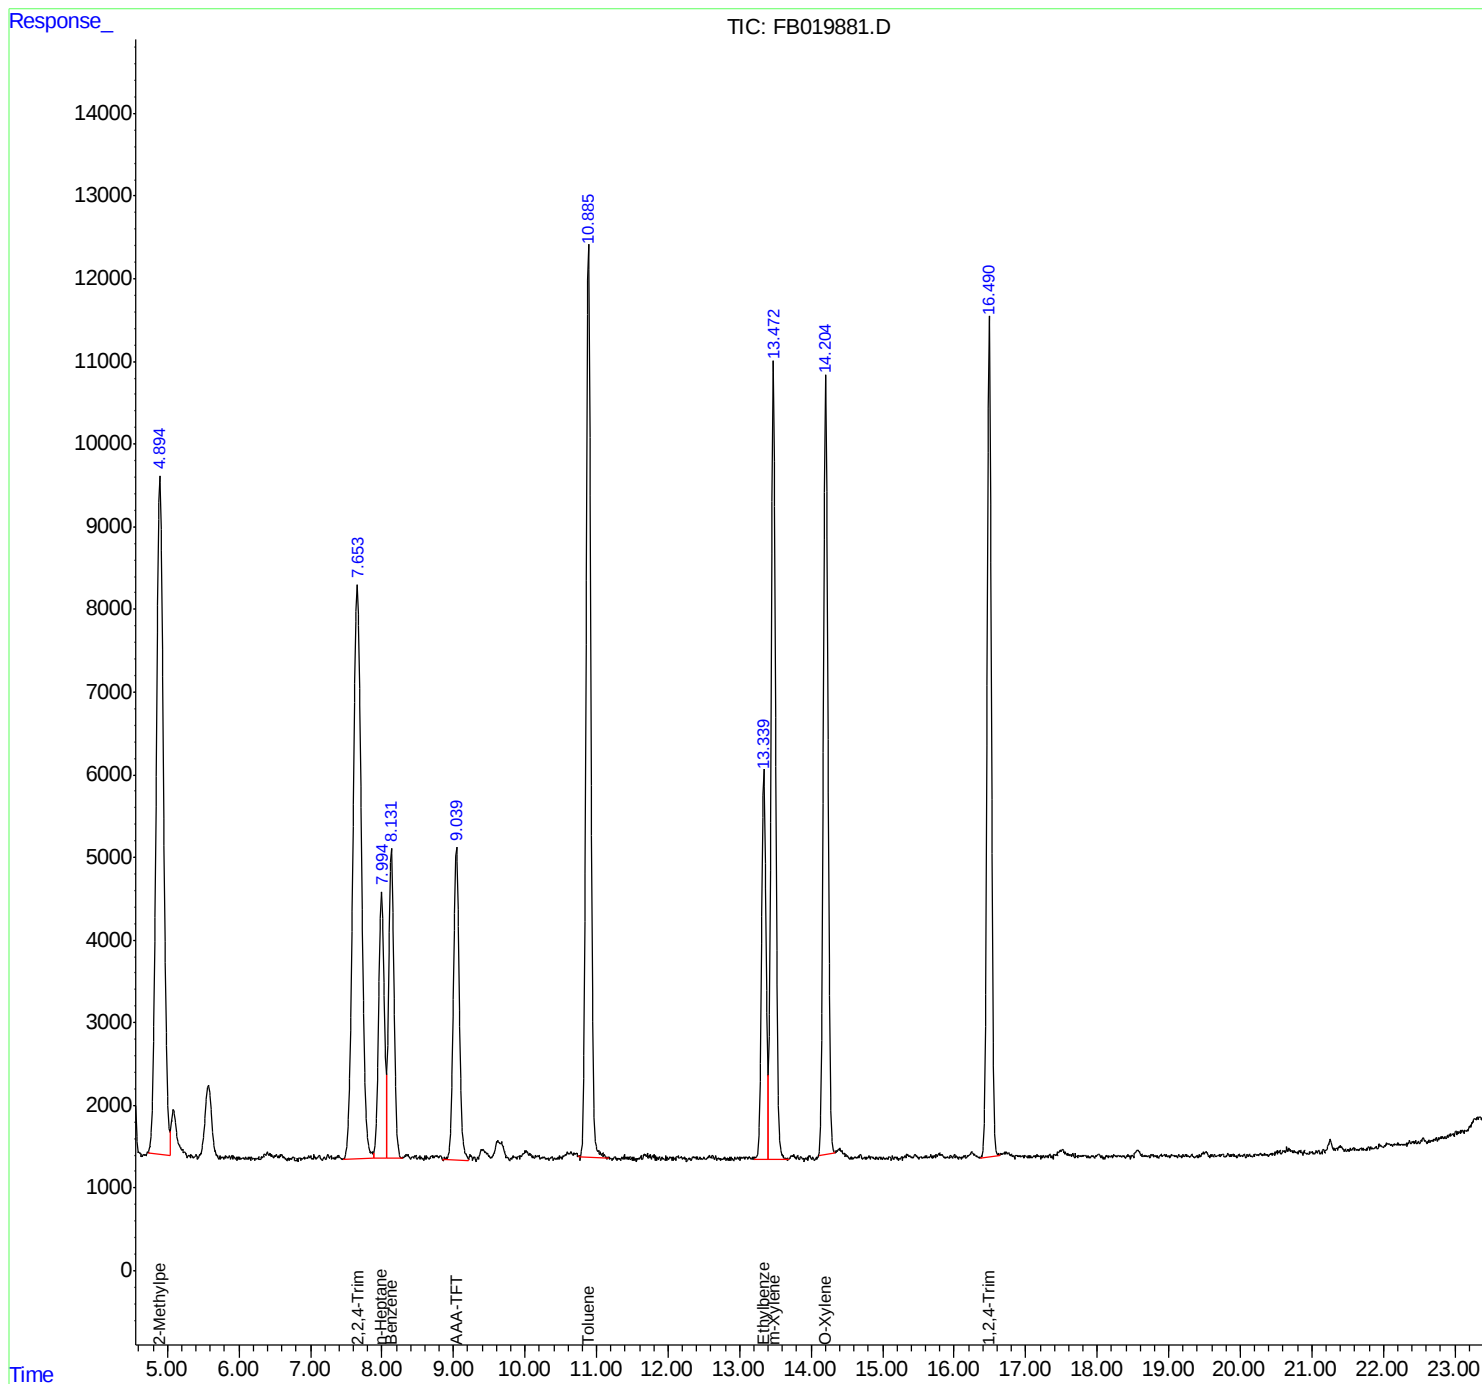

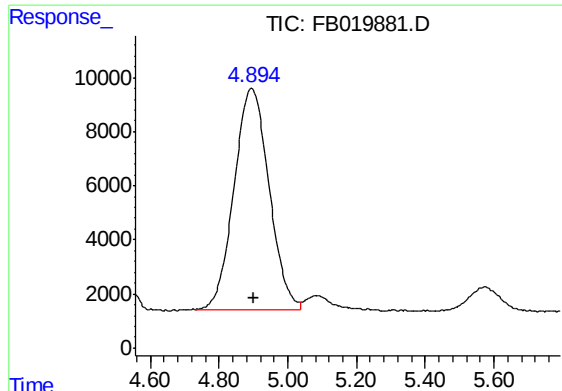


#1 2-Methylpentane

R.T.: 4.895 min
Delta R.T.: -0.007 min
Response: 580883
Conc: 31.70 ng/ml

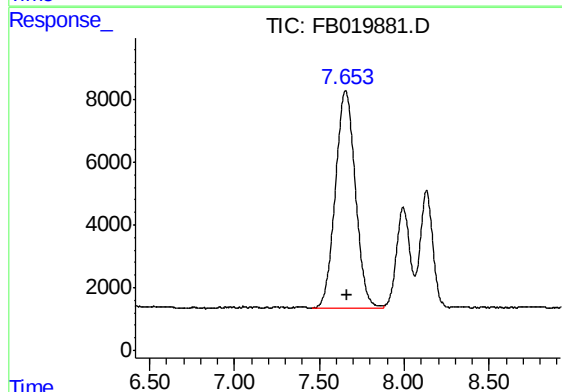


#2 2,2,4-Trimethylpentane

R.T.: 7.654 min
Delta R.T.: -0.010 min
Response: 567102
Conc: 32.47 ng/ml

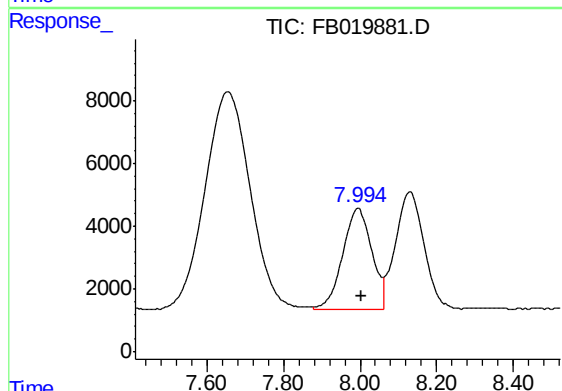


#3 n-Heptane

R.T.: 7.994 min
Delta R.T.: -0.010 min
Response: 174418
Conc: 10.48 ng/ml

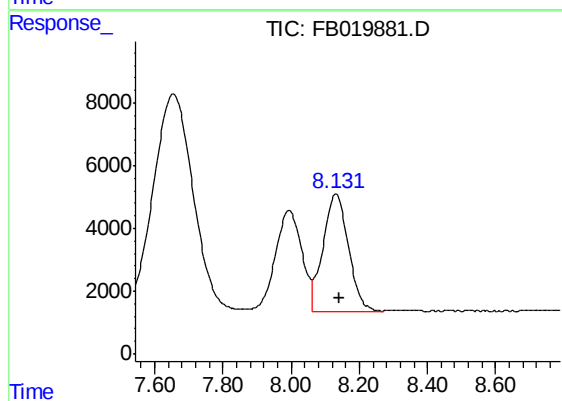


#4 Benzene

R.T.: 8.132 min
Delta R.T.: -0.009 min
Response: 193424
Conc: 10.05 ng/ml

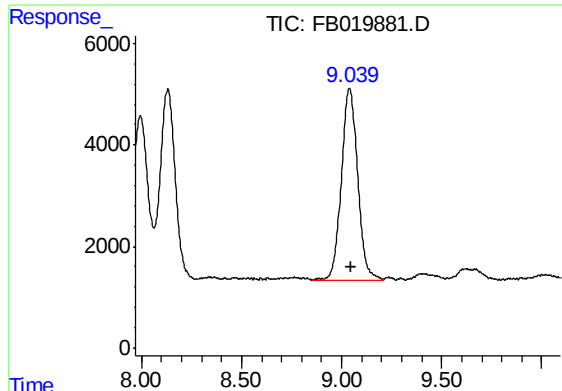


#5 AAA-TFT

R.T.: 9.040 min
Delta R.T.: -0.009 min
Response: 214392
Conc: 19.17 ng/ml

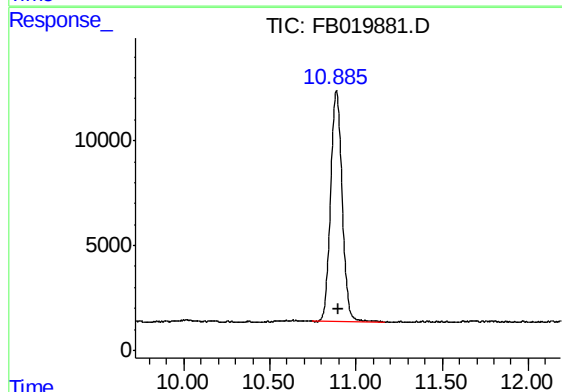


#6 Toluene

R.T.: 10.887 min
Delta R.T.: -0.010 min
Response: 513075
Conc: 29.48 ng/ml

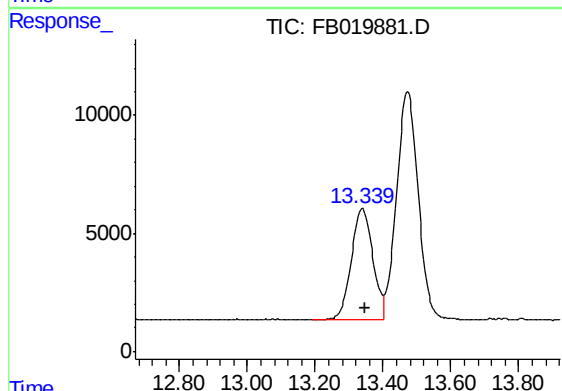


#7 Ethylbenzene

R.T.: 13.339 min
Delta R.T.: -0.009 min
Response: 206997
Conc: 9.56 ng/ml

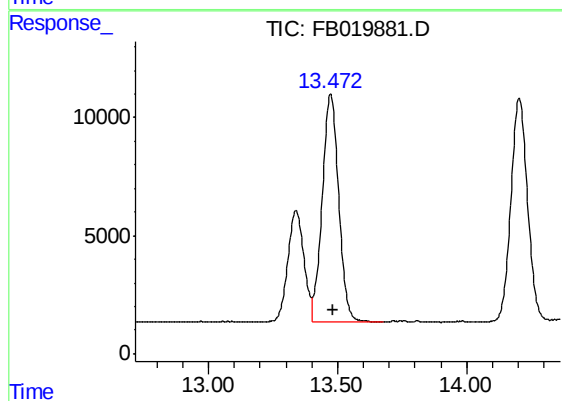


#8 m-Xylene

R.T.: 13.473 min
Delta R.T.: -0.009 min
Response: 431178
Conc: 19.09 ng/ml

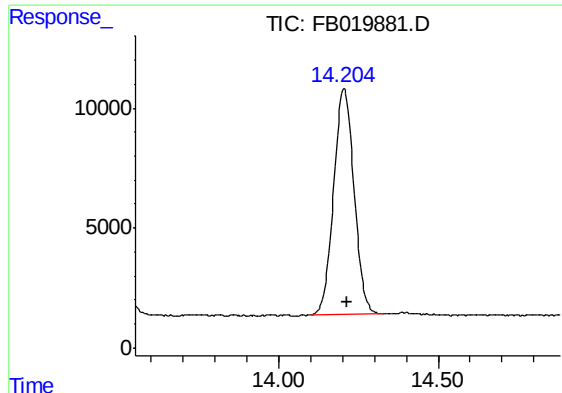

#9 O-Xylene

R.T.: 14.205 min
Delta R.T.: -0.009 min
Response: 416163
Conc: 18.82 ng/ml

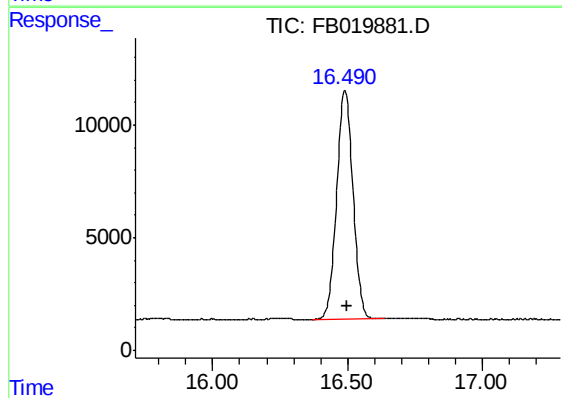

#10 1,2,4-Trimethylbenzene

R.T.: 16.491 min
Delta R.T.: -0.009 min
Response: 428282
Conc: 18.82 ng/ml