

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB022519\
 Data File : FB019887.D
 Signal(s) : FID2B.CH
 Acq On : 25 Feb 2019 13:04
 Operator : MJ/SJ
 Sample : K1586-01MSD
 Misc : 5.05g/5.00ml DI WATER
 ALS Vial : 9 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Feb 25 13:21:11 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB012919.M
 Quant Title :
 QLast Update : Tue Jan 29 12:07:12 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.042	236432	21.140 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.896	546379	29.819 ng/ml
2) t 2,2,4-Trimethylpentane	7.657	536790	30.730 ng/ml
3) t n-Heptane	7.997	142489	8.559 ng/ml
4) t Benzene	8.134	198334	10.300 ng/ml
6) t Toluene	10.889	501052	28.788 ng/ml
7) t Ethylbenzene	13.341	203716	9.408 ng/ml
8) t m-Xylene	13.475	423024	18.730 ng/ml
9) t O-Xylene	14.206	415654	18.796 ng/ml
10) t 1,2,4-Trimethylbenzene	16.493	413430	18.164 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB022519\
Data File : FB019887.D
Signal(s) : FID2B.CH
Acq On : 25 Feb 2019 13:04
Operator : MJ/SJ
Sample : K1586-01MSD
Misc : 5.05g/5.00ml DI WATER
ALS Vial : 9 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Feb 25 13:21:11 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB012919.M
Quant Title :
QLast Update : Tue Jan 29 12:07:12 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

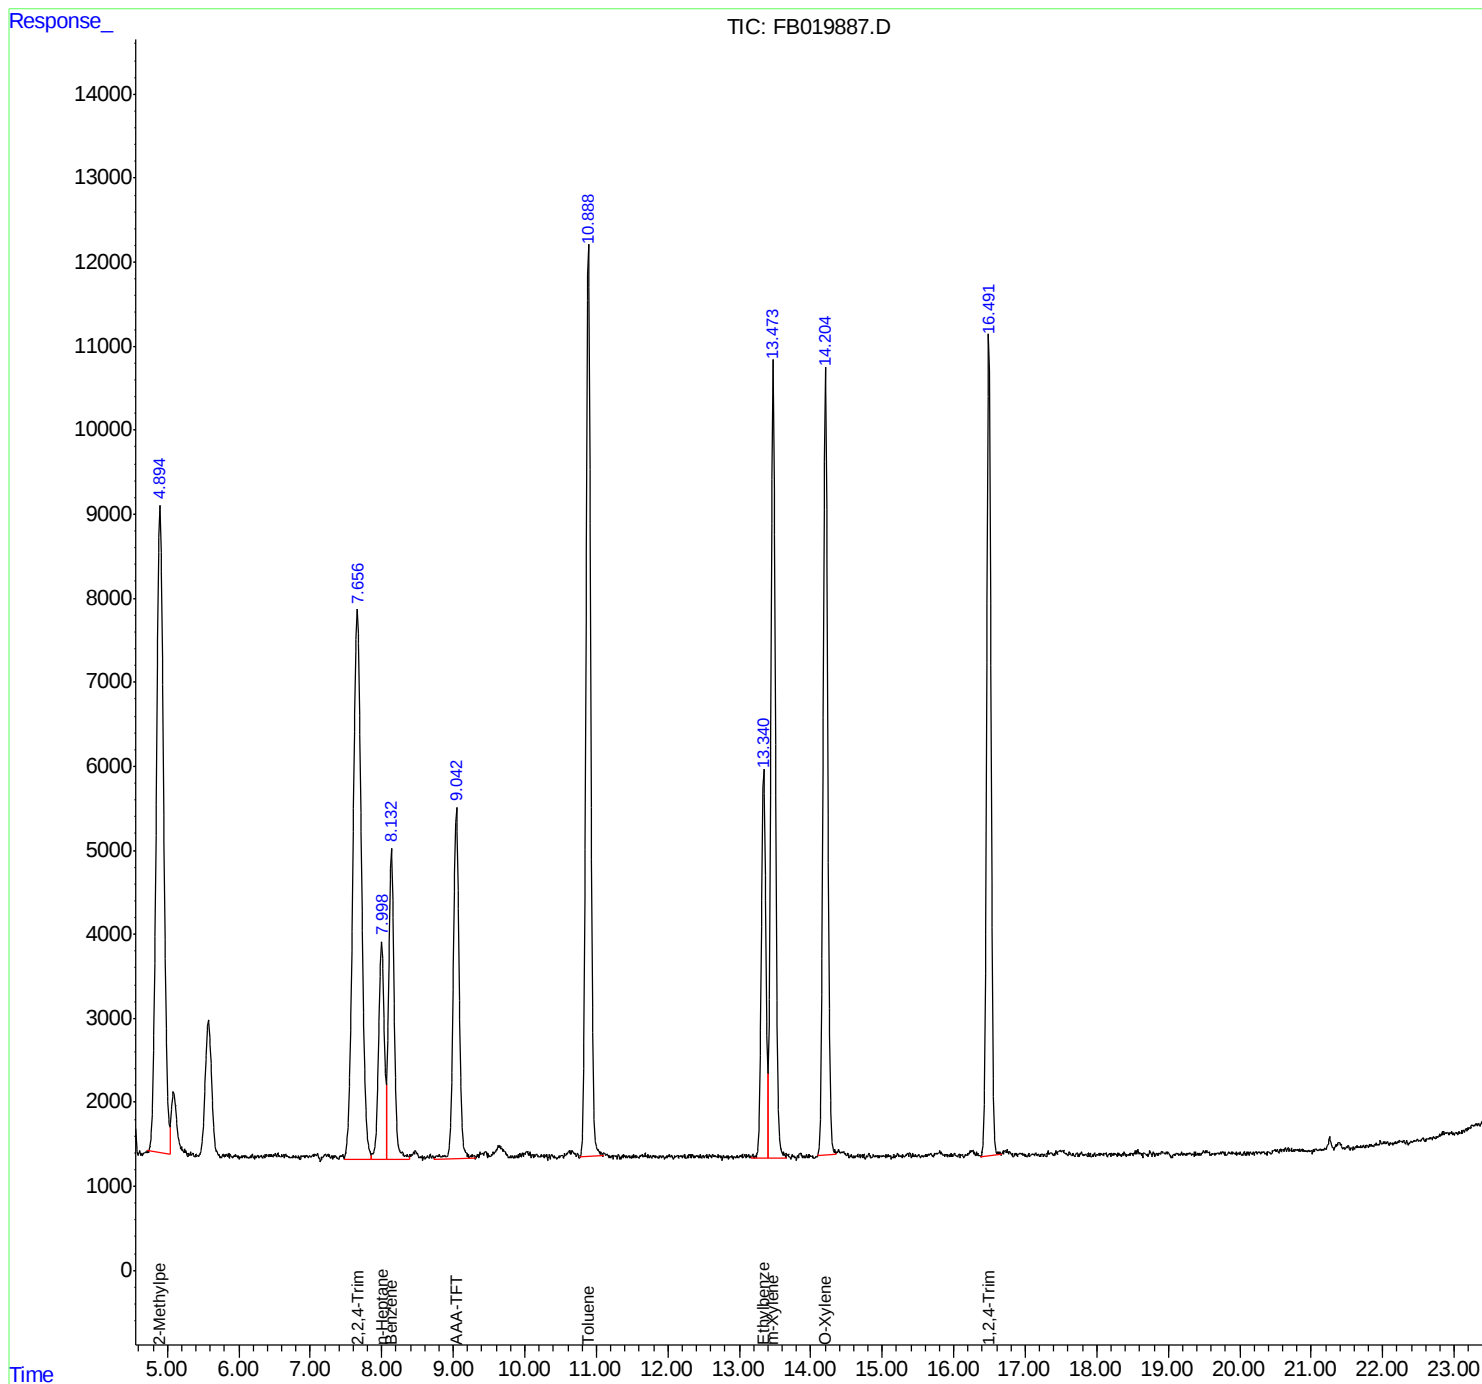

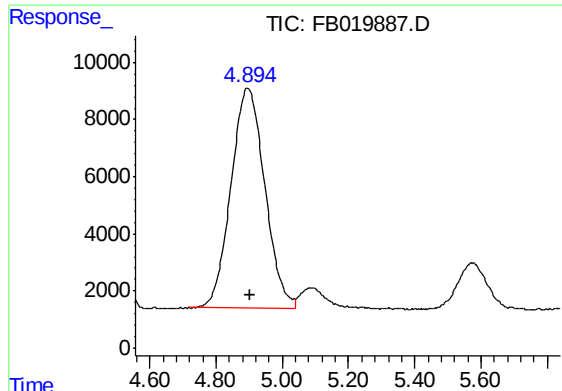


#1 2-Methylpentane

R.T.: 4.896 min
Delta R.T.: -0.006 min
Response: 546379
Conc: 29.82 ng/ml

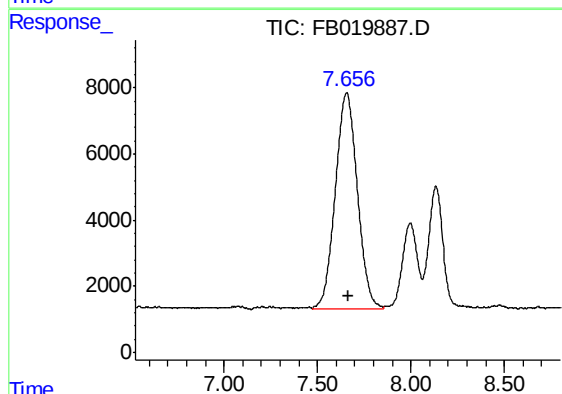


#2 2,2,4-Trimethylpentane

R.T.: 7.657 min
Delta R.T.: -0.008 min
Response: 536790
Conc: 30.73 ng/ml

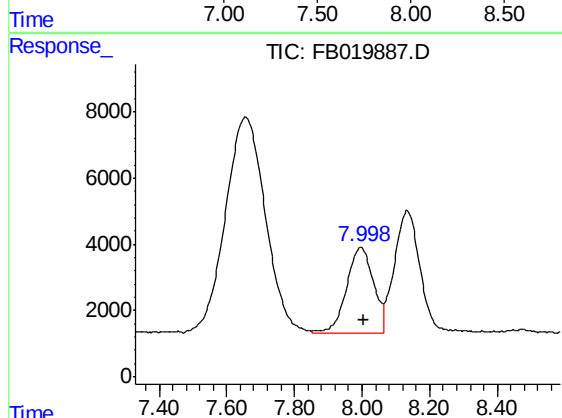


#3 n-Heptane

R.T.: 7.997 min
Delta R.T.: -0.008 min
Response: 142489
Conc: 8.56 ng/ml

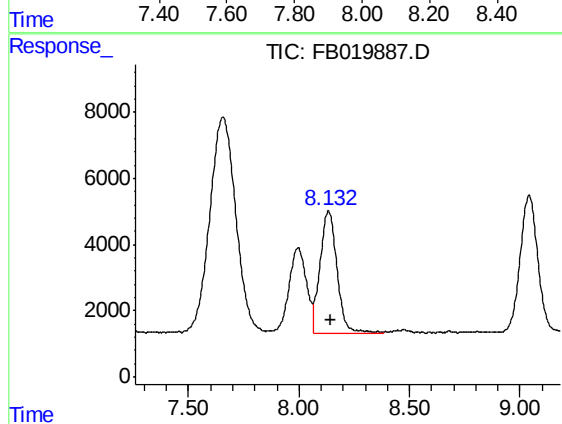


#4 Benzene

R.T.: 8.134 min
Delta R.T.: -0.008 min
Response: 198334
Conc: 10.30 ng/ml

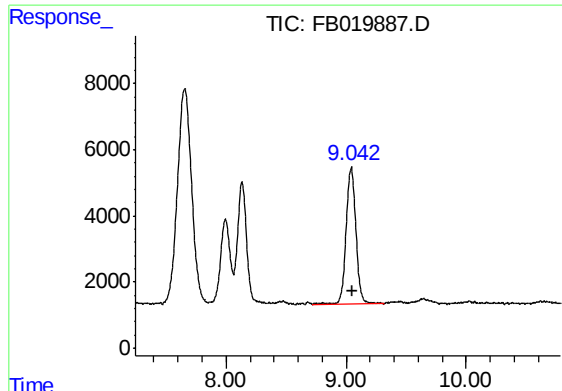


#5 AAA-TFT

R.T.: 9.042 min
Delta R.T.: -0.007 min
Response: 236432
Conc: 21.14 ng/ml

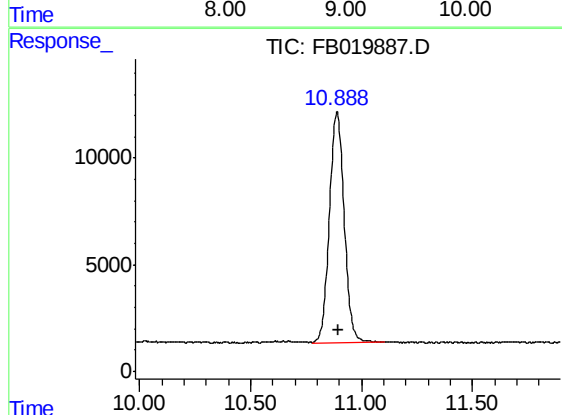


#6 Toluene

R.T.: 10.889 min
Delta R.T.: -0.008 min
Response: 501052
Conc: 28.79 ng/ml

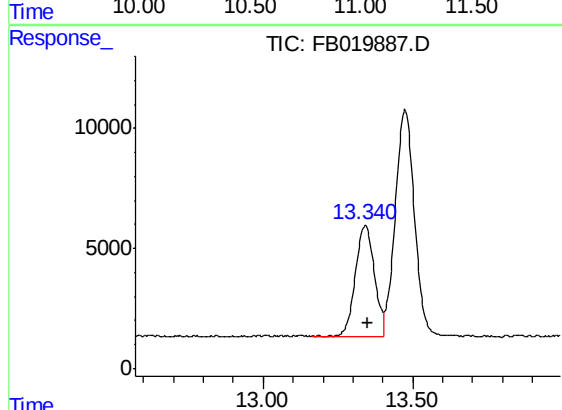


#7 Ethylbenzene

R.T.: 13.341 min
Delta R.T.: -0.007 min
Response: 203716
Conc: 9.41 ng/ml

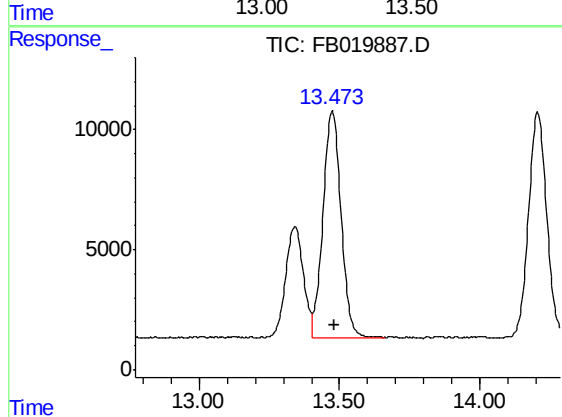


#8 m-Xylene

R.T.: 13.475 min
Delta R.T.: -0.007 min
Response: 423024
Conc: 18.73 ng/ml

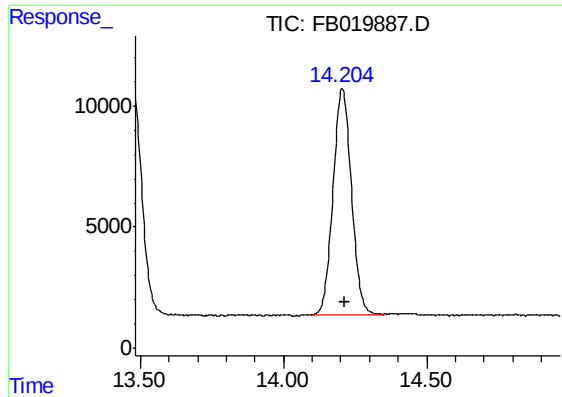

#9 O-Xylene

R.T.: 14.206 min
Delta R.T.: -0.008 min
Response: 415654
Conc: 18.80 ng/ml

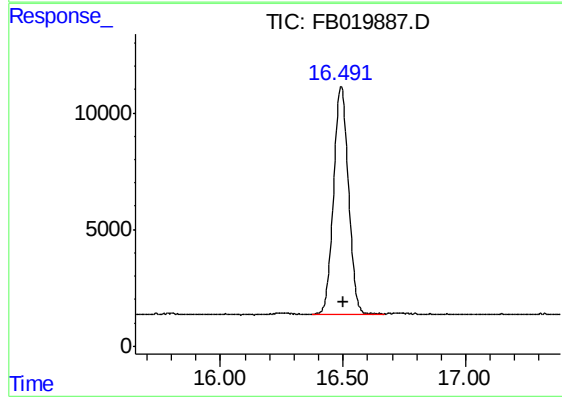

#10 1,2,4-Trimethylbenzene

R.T.: 16.493 min
Delta R.T.: -0.008 min
Response: 413430
Conc: 18.16 ng/ml