

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB022620\
 Data File : FB023727.D
 Signal(s) : FID2B.CH
 Acq On : 26 Feb 2020 10:54
 Operator : DD/AJ
 Sample : BSF0226S1
 Misc : 5.00g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Feb 27 00:21:29 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB020620.M
 Quant Title :
 QLast Update : Thu Feb 06 11:13:47 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.799	425168	20.883 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.689	917246	30.483 ng/ml
2) t 2,2,4-Trimethylpentane	7.418	1045737	32.047 ng/ml
3) t n-Heptane	7.757	329693	10.247 ng/ml
4) t Benzene	7.892	412687	10.090 ng/ml
6) t Toluene	10.630	1212491	30.545 ng/ml
7) t Ethylbenzene	13.070	363001	9.765 ng/ml
8) t m-Xylene	13.203	701404	19.641 ng/ml
9) t O-Xylene	13.930	677277	19.637 ng/ml
10) t 1,2,4-Trimethylbenzene	16.209	604636	20.651 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB022620\
Data File : FB023727.D
Signal(s) : FID2B.CH
Acq On : 26 Feb 2020 10:54
Operator : DD/AJ
Sample : BSF0226S1
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Feb 27 00:21:29 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB020620.M
Quant Title :
QLast Update : Thu Feb 06 11:13:47 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

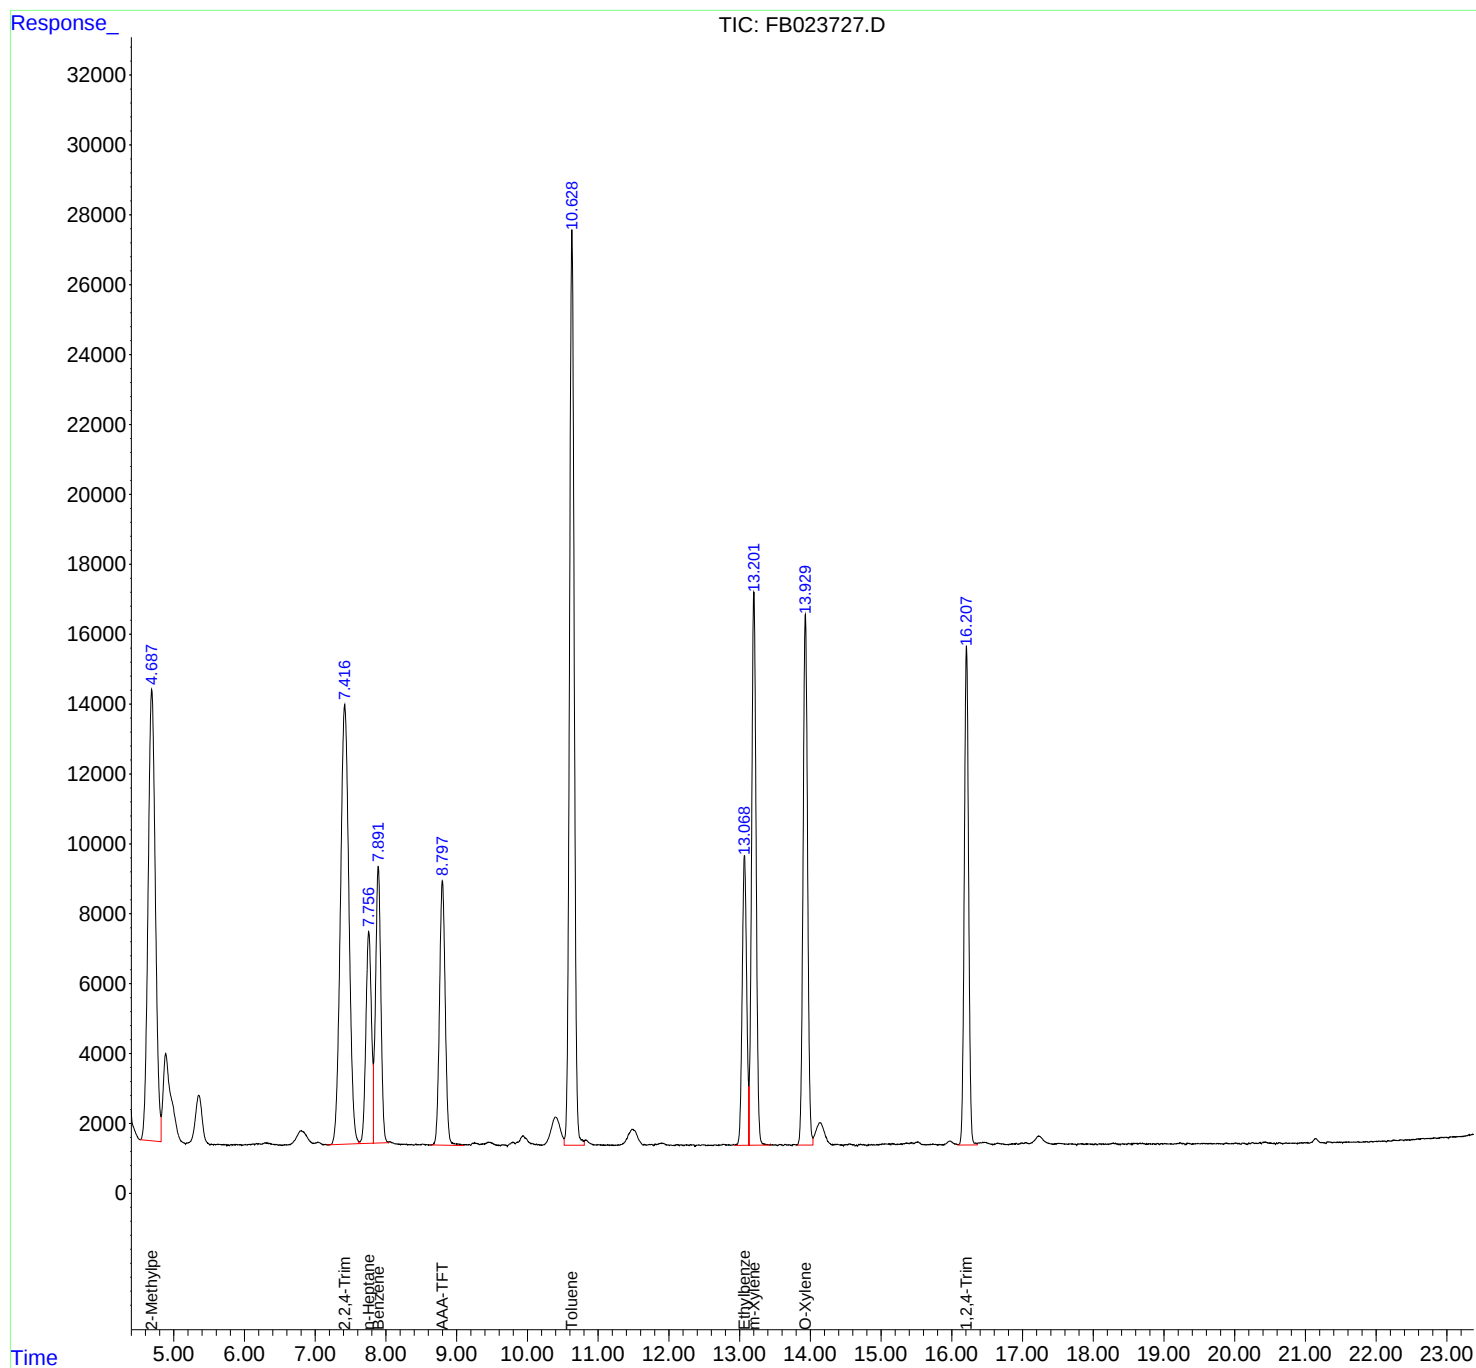

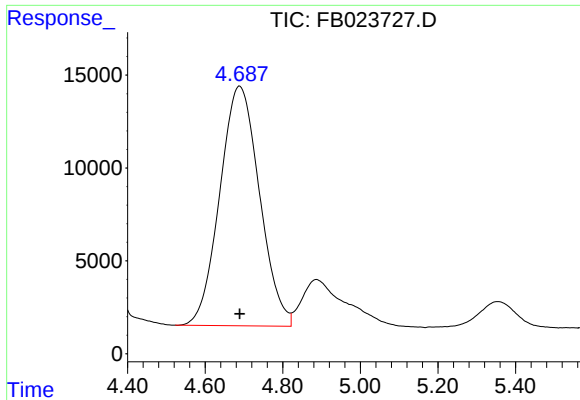


#1 2-Methylpentane

R.T.: 4.689 min
Delta R.T.: 0.000 min
Response: 917246
Conc: 30.48 ng/ml

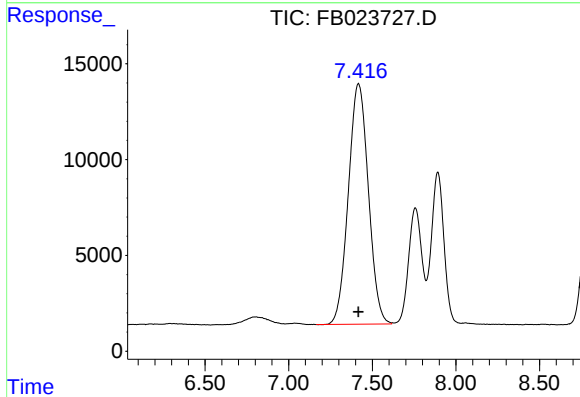


#2 2,2,4-Trimethylpentane

R.T.: 7.418 min
Delta R.T.: 0.000 min
Response: 1045737
Conc: 32.05 ng/ml

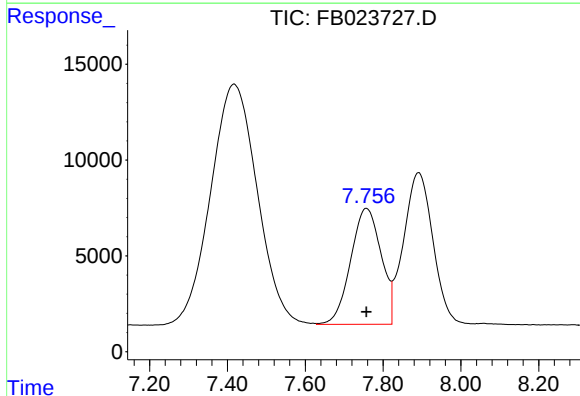


#3 n-Heptane

R.T.: 7.757 min
Delta R.T.: 0.000 min
Response: 329693
Conc: 10.25 ng/ml

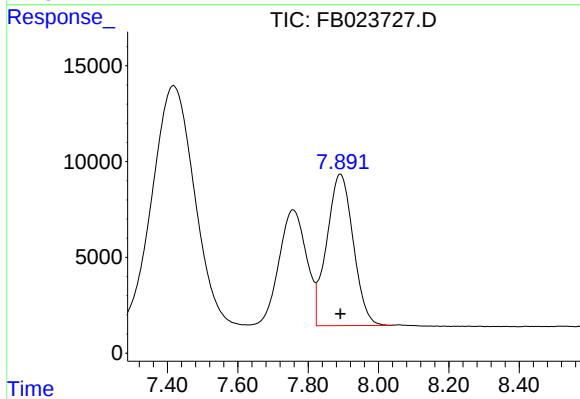


#4 Benzene

R.T.: 7.892 min
Delta R.T.: 0.000 min
Response: 412687
Conc: 10.09 ng/ml

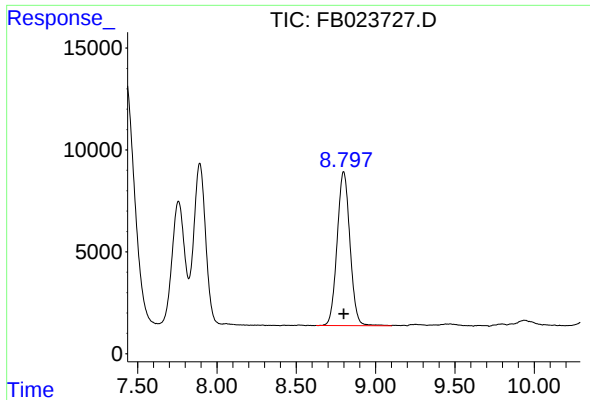


#5 AAA-TFT

R.T.: 8.799 min
Delta R.T.: 0.000 min
Response: 425168
Conc: 20.88 ng/ml

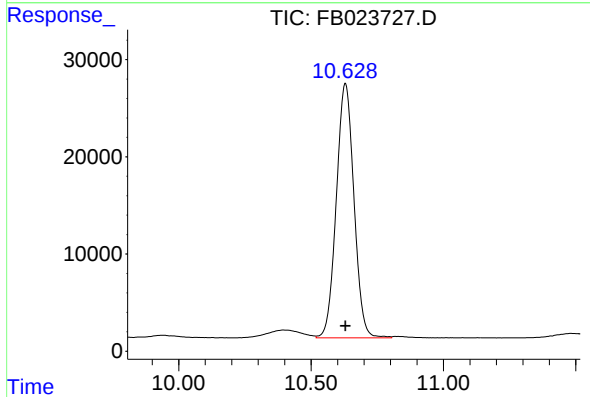


#6 Toluene

R.T.: 10.630 min
Delta R.T.: 0.000 min
Response: 1212491
Conc: 30.55 ng/ml

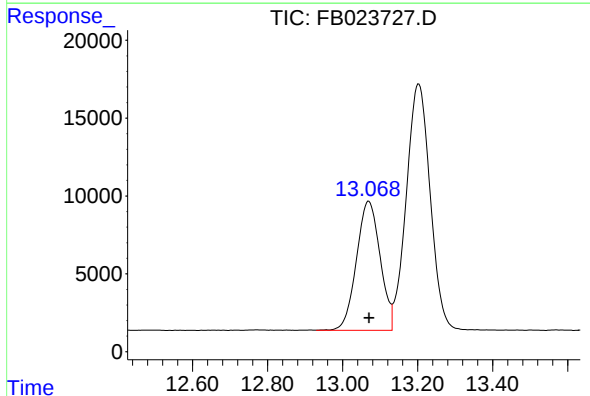


#7 Ethylbenzene

R.T.: 13.070 min
Delta R.T.: 0.000 min
Response: 363001
Conc: 9.76 ng/ml

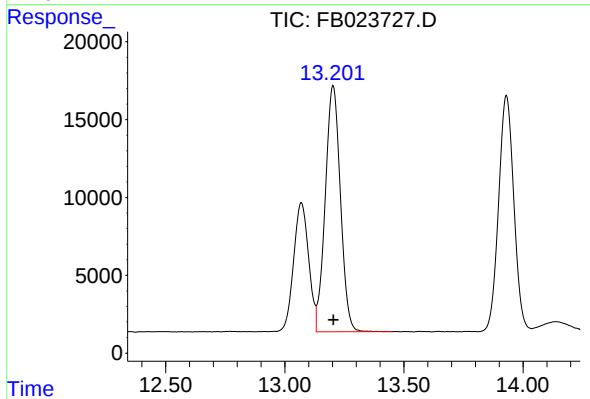

#8 m-Xylene

R.T.: 13.203 min
Delta R.T.: 0.000 min
Response: 701404
Conc: 19.64 ng/ml

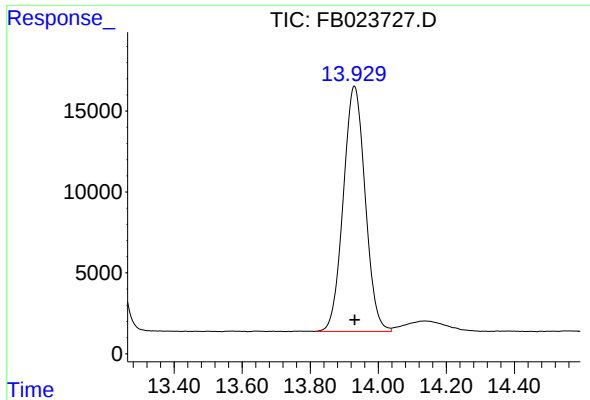


#9 O-Xylene

R.T.: 13.930 min

Delta R.T.: 0.000 min

Response: 677277

Conc: 19.64 ng/ml

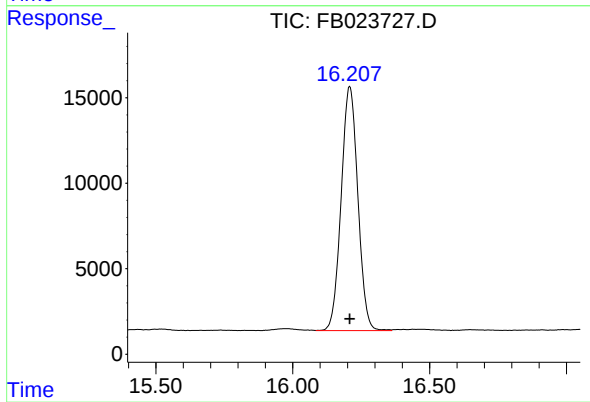

#10 1,2,4-Trimethylbenzene

R.T.: 16.209 min

Delta R.T.: 0.000 min

Response: 604636

Conc: 20.65 ng/ml