

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB022719\
Data File : FB019935.D
Signal(s) : FID2B.CH
Acq On : 27 Feb 2019 18:52
Operator : MJ/SJ
Sample : K1353-05
Misc : 5.04g/5.00ml DI WATER
ALS Vial : 20 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Feb 28 01:23:36 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB012919.M
Quant Title :
QLast Update : Tue Jan 29 12:07:12 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.043	200814	17.179 ng/ml
Target Compounds			
6) t Toluene	10.891	223179	12.759 ng/ml
8) t m-Xylene	13.477	7847	0.343 ng/ml
9) t O-Xylene	14.216	4840	0.217 ng/ml
10) t 1,2,4-Trimethylbenzene	16.495	88589	3.823 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB022719\
Data File : FB019935.D
Signal(s) : FID2B.CH
Acq On : 27 Feb 2019 18:52
Operator : MJ/SJ
Sample : K1353-05
Misc : 5.04g/5.00ml DI WATER
ALS Vial : 20 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Feb 28 01:23:36 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB012919.M
Quant Title :
QLast Update : Tue Jan 29 12:07:12 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

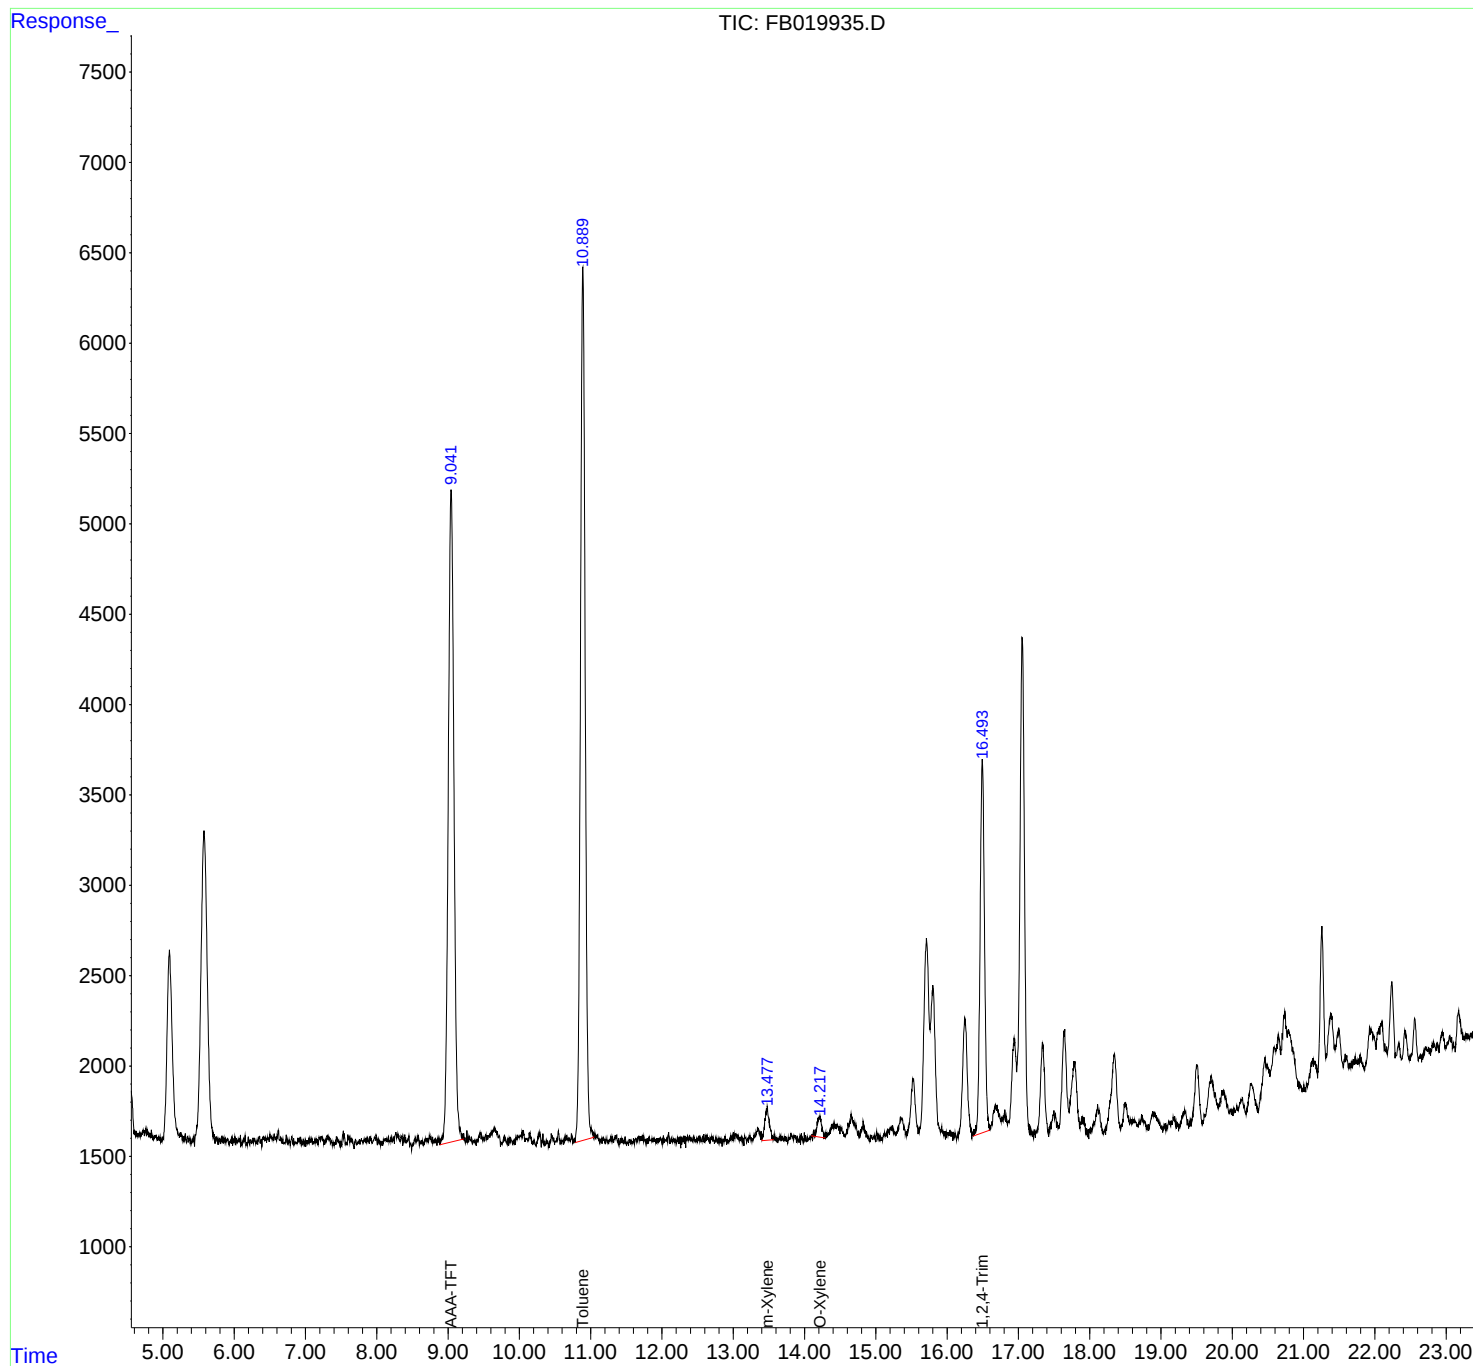

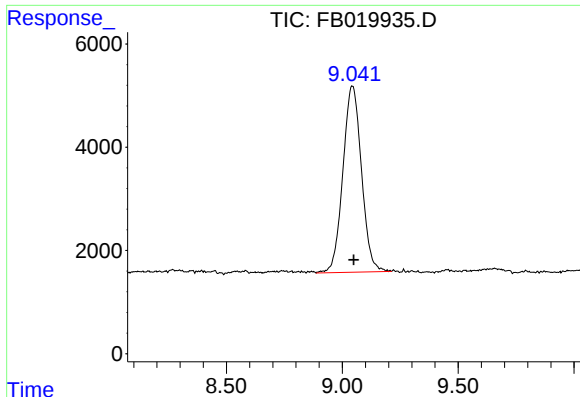


#5 AAA-TFT

R.T.: 9.043 min
Delta R.T.: -0.006 min
Response: 200814
Conc: 17.18 ng/ml

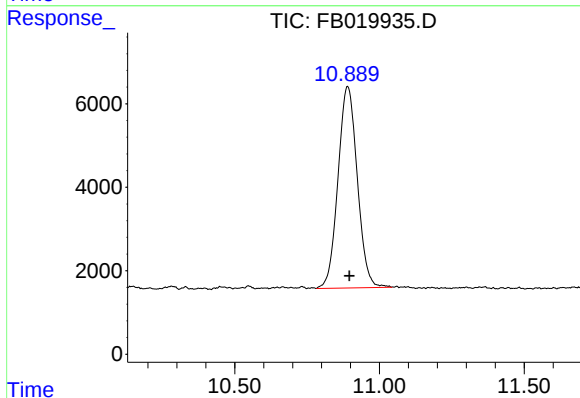


#6 Toluene

R.T.: 10.891 min
Delta R.T.: -0.006 min
Response: 223179
Conc: 12.76 ng/ml

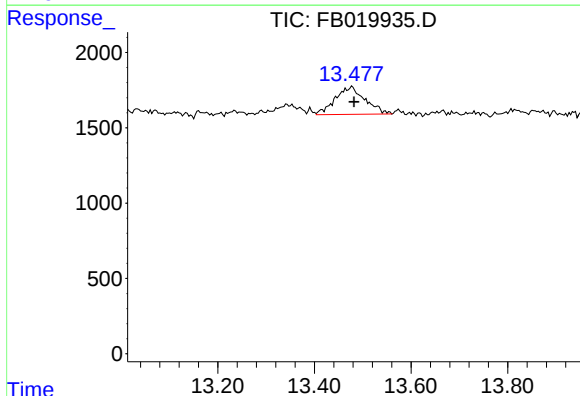


#8 m-Xylene

R.T.: 13.477 min
Delta R.T.: -0.005 min
Response: 7847
Conc: 0.34 ng/ml

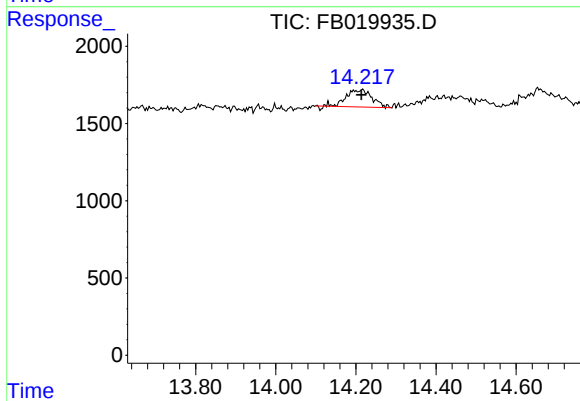

#9 O-Xylene

R.T.: 14.216 min
Delta R.T.: 0.002 min
Response: 4840
Conc: 0.22 ng/ml

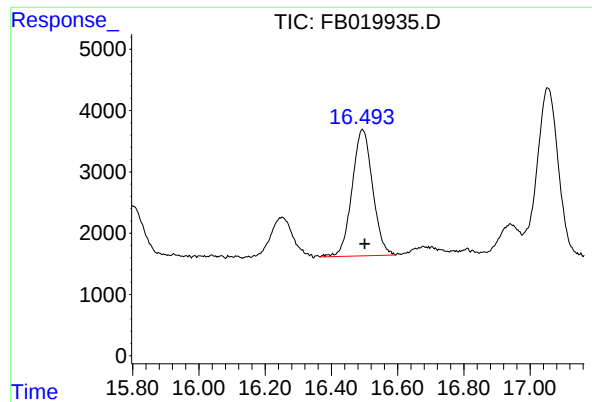

#10 1,2,4-Trimethylbenzene

R.T.: 16.495 min
Delta R.T.: -0.005 min
Response: 88589
Conc: 3.82 ng/ml