

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB022720\
 Data File : FB023738.D
 Signal(s) : FID2B.CH
 Acq On : 27 Feb 2020 13:14
 Operator : DD/AJ
 Sample : L1363-07MSD
 Misc : 5.05g/5.00ml DI WATER
 ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Feb 28 00:25:17 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB020620.M
 Quant Title :
 QLast Update : Thu Feb 06 11:13:47 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.799	391721	19.240 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.690	669089	22.236 ng/ml
2) t 2,2,4-Trimethylpentane	7.417	590144	18.085 ng/ml
3) t n-Heptane	7.757	64824	2.015 ng/ml
4) t Benzene	7.892	352623	8.621 ng/ml
6) t Toluene	10.631	958154	24.138 ng/ml
7) t Ethylbenzene	13.068	486536	13.088 ng/ml
8) t m-Xylene	13.203	171415	4.800 ng/ml
9) t O-Xylene	13.933	889851	25.801 ng/ml
10) t 1,2,4-Trimethylbenzene	16.216	194785	6.653 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB022720\
Data File : FB023738.D
Signal(s) : FID2B.CH
Acq On : 27 Feb 2020 13:14
Operator : DD/AJ
Sample : L1363-07MSD
Misc : 5.05g/5.00ml DI WATER
ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Feb 28 00:25:17 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB020620.M
Quant Title :
QLast Update : Thu Feb 06 11:13:47 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

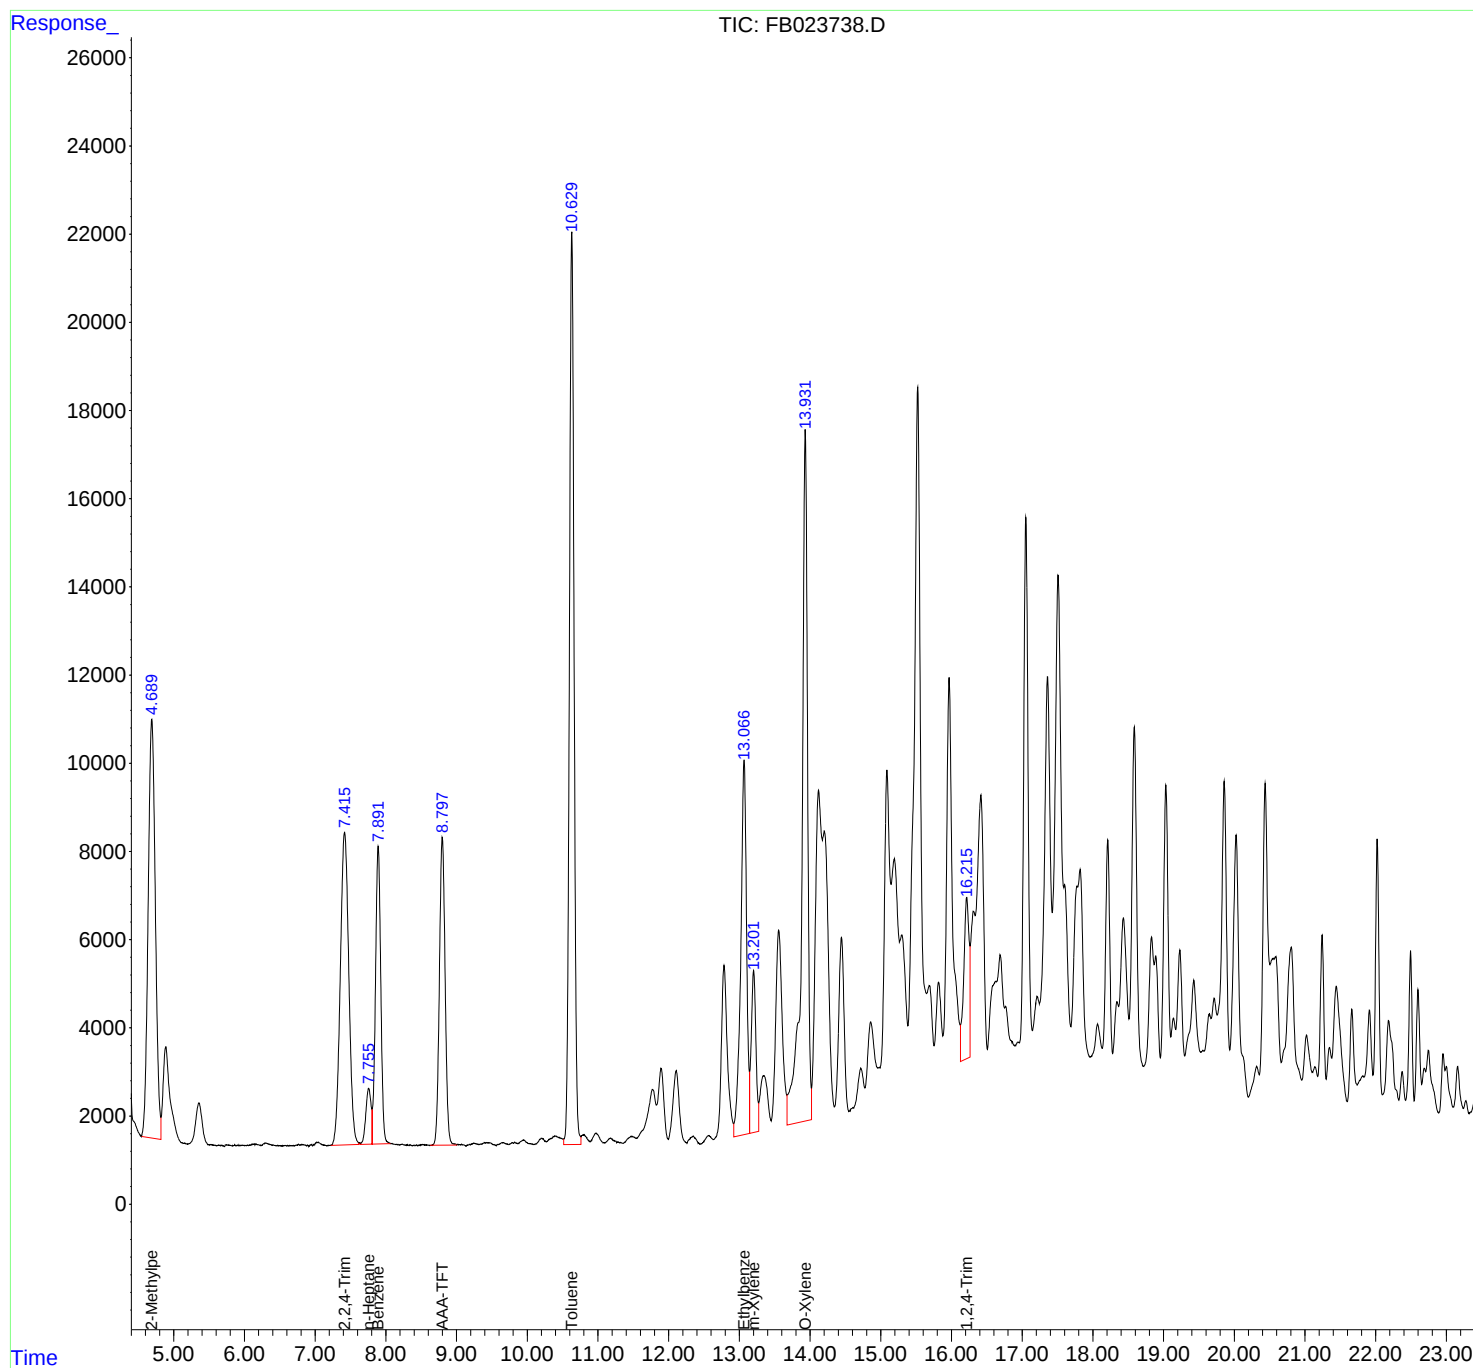

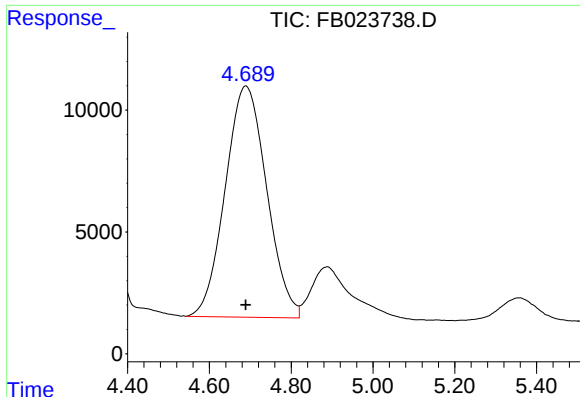


#1 2-Methylpentane

R.T.: 4.690 min
Delta R.T.: 0.000 min
Response: 669089
Conc: 22.24 ng/ml

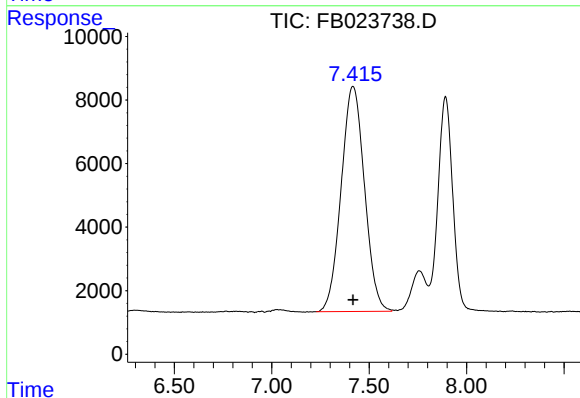


#2 2,2,4-Trimethylpentane

R.T.: 7.417 min
Delta R.T.: 0.000 min
Response: 590144
Conc: 18.09 ng/ml

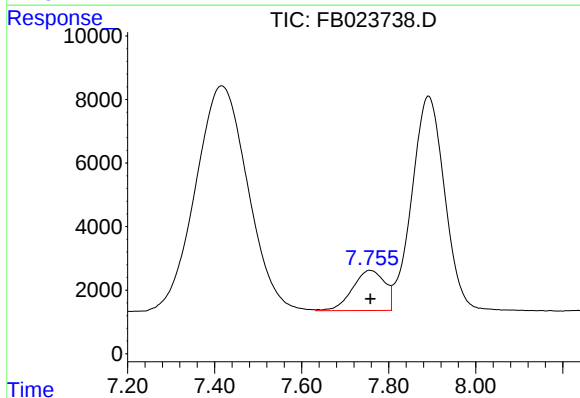


#3 n-Heptane

R.T.: 7.757 min
Delta R.T.: 0.000 min
Response: 64824
Conc: 2.01 ng/ml

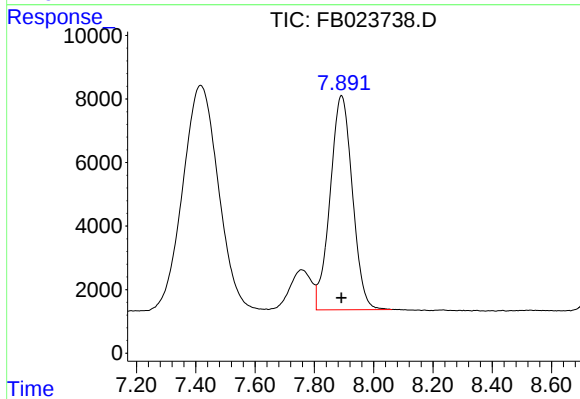


#4 Benzene

R.T.: 7.892 min
Delta R.T.: 0.000 min
Response: 352623
Conc: 8.62 ng/ml

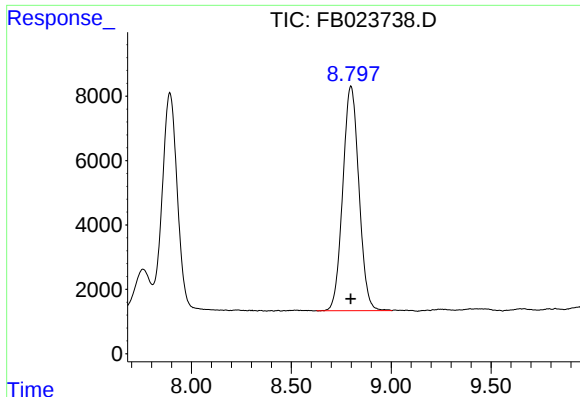


#5 AAA-TFT

R.T.: 8.799 min
Delta R.T.: 0.000 min
Response: 391721
Conc: 19.24 ng/ml

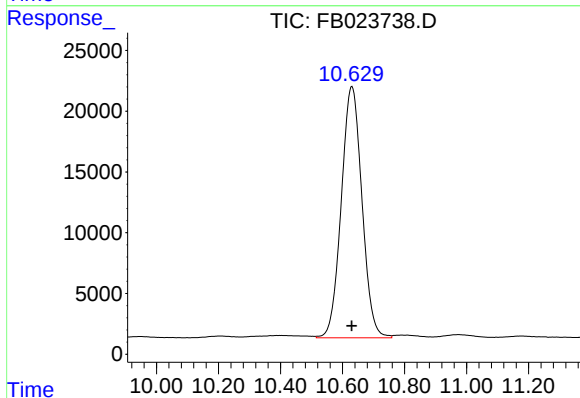


#6 Toluene

R.T.: 10.631 min
Delta R.T.: 0.000 min
Response: 958154
Conc: 24.14 ng/ml

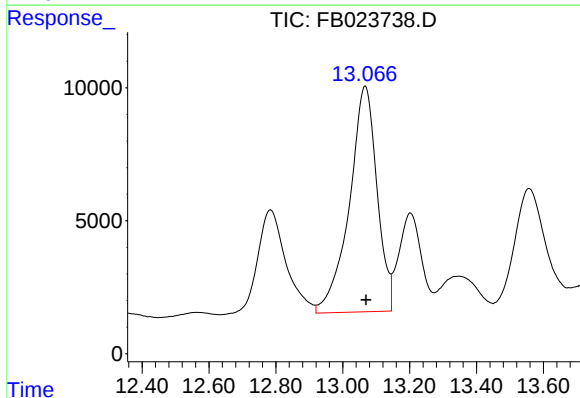


#7 Ethylbenzene

R.T.: 13.068 min
Delta R.T.: -0.003 min
Response: 486536
Conc: 13.09 ng/ml

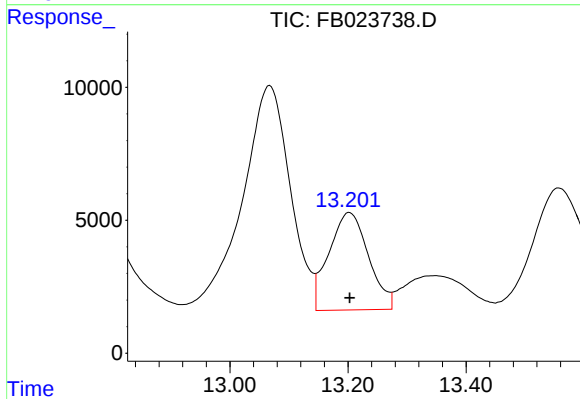


#8 m-Xylene

R.T.: 13.203 min
Delta R.T.: 0.000 min
Response: 171415
Conc: 4.80 ng/ml

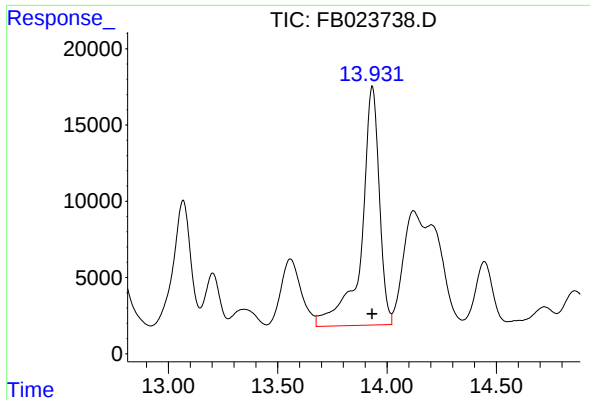

#9 O-Xylene

R.T.: 13.933 min
Delta R.T.: 0.002 min
Response: 889851
Conc: 25.80 ng/ml

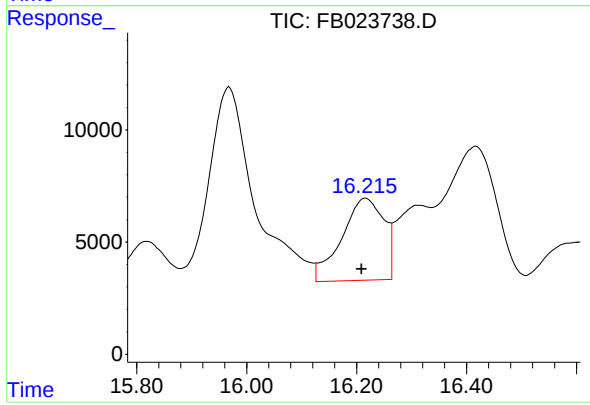

#10 1,2,4-Trimethylbenzene

R.T.: 16.216 min
Delta R.T.: 0.007 min
Response: 194785
Conc: 6.65 ng/ml