

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB022819\
 Data File : FB019947.D
 Signal(s) : FID2B.CH
 Acq On : 28 Feb 2019 9:44
 Operator : MJ/SJ
 Sample : BSF0228S1
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Mar 01 00:58:19 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB012919.M
 Quant Title :
 QLast Update : Tue Jan 29 12:07:12 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.039	222150	19.004 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.894	621529	35.899 ng/ml
2) t 2,2,4-Trimethylpentane	7.654	623016	37.569 ng/ml
3) t n-Heptane	7.994	190401	11.815 ng/ml
4) t Benzene	8.132	211762	11.227 ng/ml
6) t Toluene	10.886	549828	31.432 ng/ml
7) t Ethylbenzene	13.338	218657	9.964 ng/ml
8) t m-Xylene	13.471	458959	20.053 ng/ml
9) t O-Xylene	14.203	444080	19.883 ng/ml
10) t 1,2,4-Trimethylbenzene	16.489	459138	19.816 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB022819\
Data File : FB019947.D
Signal(s) : FID2B.CH
Acq On : 28 Feb 2019 9:44
Operator : MJ/SJ
Sample : BSF0228S1
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Mar 01 00:58:19 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB012919.M
Quant Title :
QLast Update : Tue Jan 29 12:07:12 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

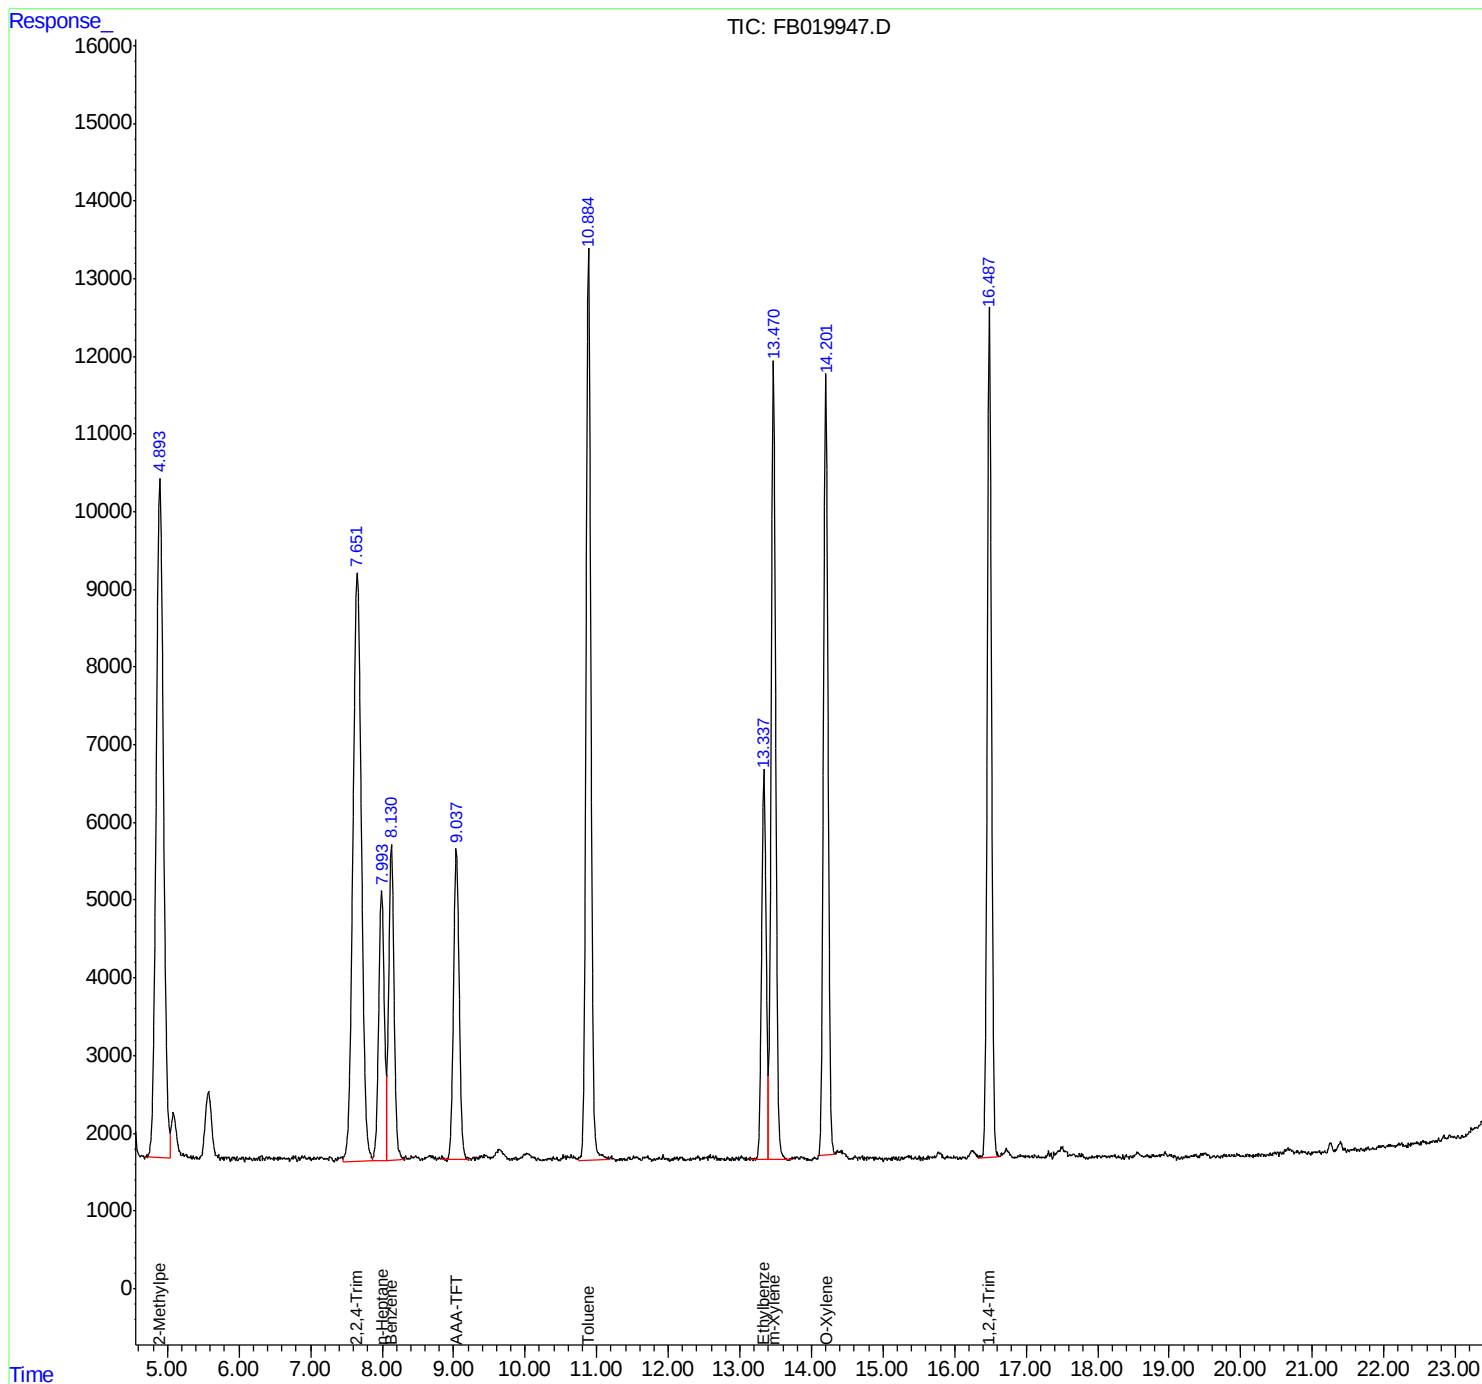

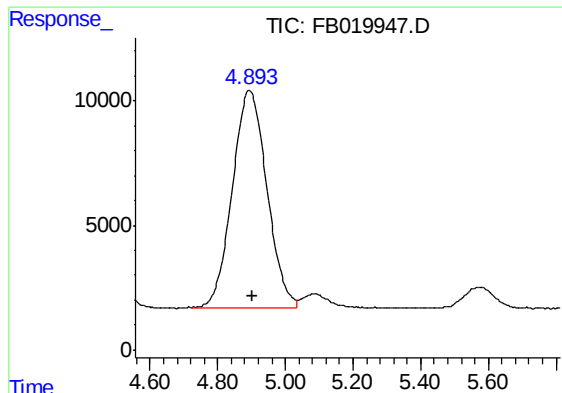


#1 2-Methylpentane

R.T.: 4.894 min
Delta R.T.: -0.008 min
Response: 621529
Conc: 35.90 ng/ml

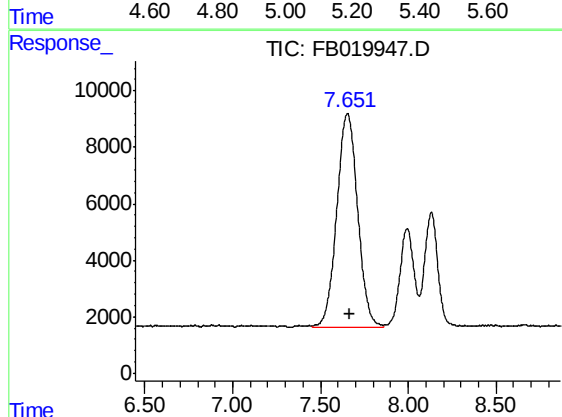


#2 2,2,4-Trimethylpentane

R.T.: 7.654 min
Delta R.T.: -0.011 min
Response: 623016
Conc: 37.57 ng/ml

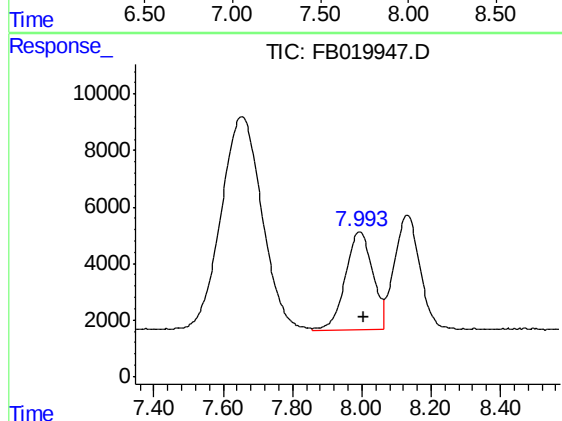


#3 n-Heptane

R.T.: 7.994 min
Delta R.T.: -0.010 min
Response: 190401
Conc: 11.82 ng/ml

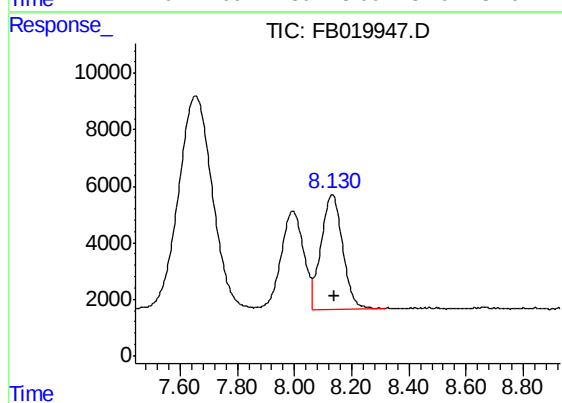


#4 Benzene

R.T.: 8.132 min
Delta R.T.: -0.010 min
Response: 211762
Conc: 11.23 ng/ml

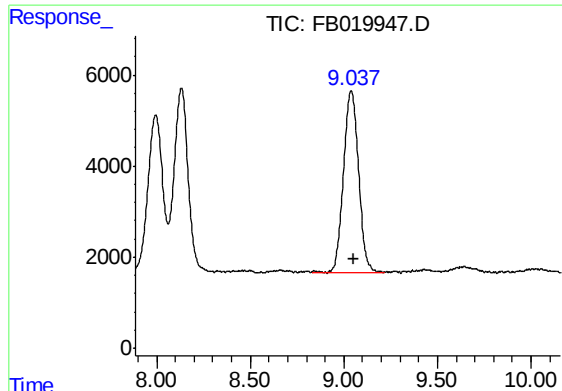


#5 AAA-TFT

R.T.: 9.039 min
Delta R.T.: -0.011 min
Response: 222150
Conc: 19.00 ng/ml

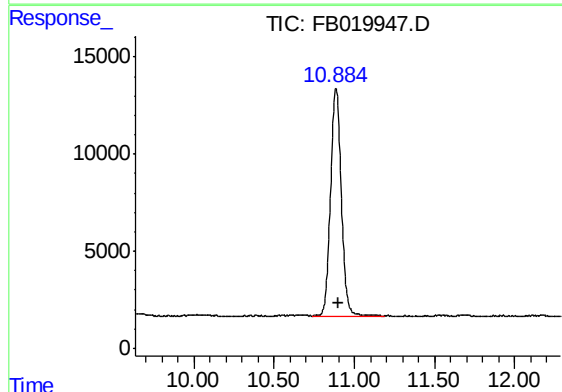


#6 Toluene

R.T.: 10.886 min
Delta R.T.: -0.011 min
Response: 549828
Conc: 31.43 ng/ml

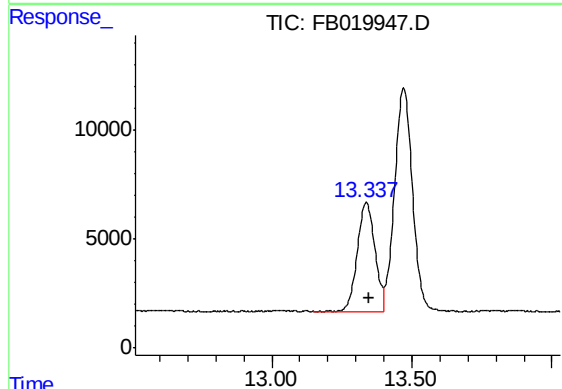


#7 Ethylbenzene

R.T.: 13.338 min
Delta R.T.: -0.011 min
Response: 218657
Conc: 9.96 ng/ml

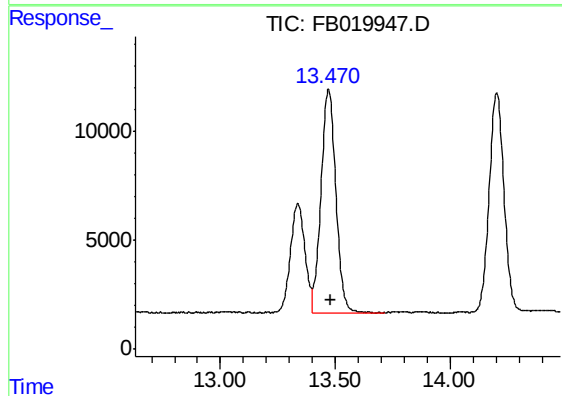


#8 m-Xylene

R.T.: 13.471 min
Delta R.T.: -0.011 min
Response: 458959
Conc: 20.05 ng/ml

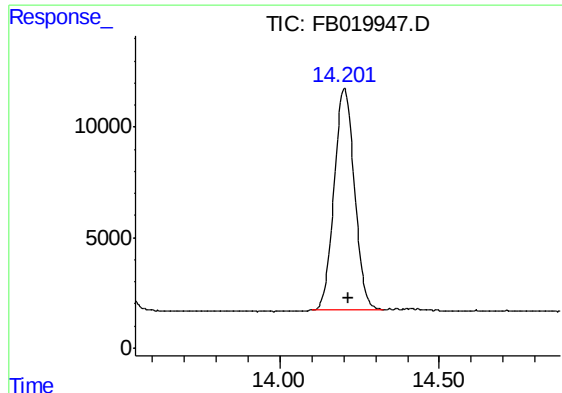

#9 O-Xylene

R.T.: 14.203 min
Delta R.T.: -0.011 min
Response: 444080
Conc: 19.88 ng/ml

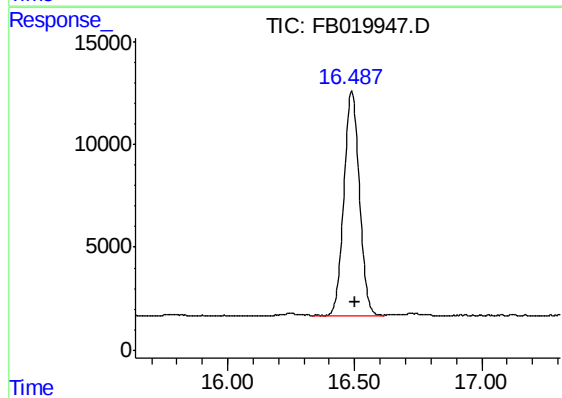

#10 1,2,4-Trimethylbenzene

R.T.: 16.489 min
Delta R.T.: -0.011 min
Response: 459138
Conc: 19.82 ng/ml