

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB022820\
 Data File : FB023741.D
 Signal(s) : FID2B.CH
 Acq On : 28 Feb 2020 10:37
 Operator : DD/AJ
 Sample : VBF0228S1
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Feb 28 22:53:26 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB020620.M
 Quant Title :
 QLast Update : Thu Feb 06 11:13:47 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.795	386778	18.997 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.681	16924	0.562 ng/ml
2) t 2,2,4-Trimethylpentane	7.414	2743	0.084 ng/ml
4) t Benzene	7.899	3655	0.089 ng/ml
6) t Toluene	10.631	18397	0.463 ng/ml
7) t Ethylbenzene	13.060	4480	0.121 ng/ml
8) t m-Xylene	13.203	10937	0.306 ng/ml
9) t O-Xylene	13.929	14433	0.418 ng/ml
10) t 1,2,4-Trimethylbenzene	16.207	12659	0.432 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB022820\
Data File : FB023741.D
Signal(s) : FID2B.CH
Acq On : 28 Feb 2020 10:37
Operator : DD/AJ
Sample : VBF0228S1
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Feb 28 22:53:26 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB020620.M
Quant Title :
QLast Update : Thu Feb 06 11:13:47 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

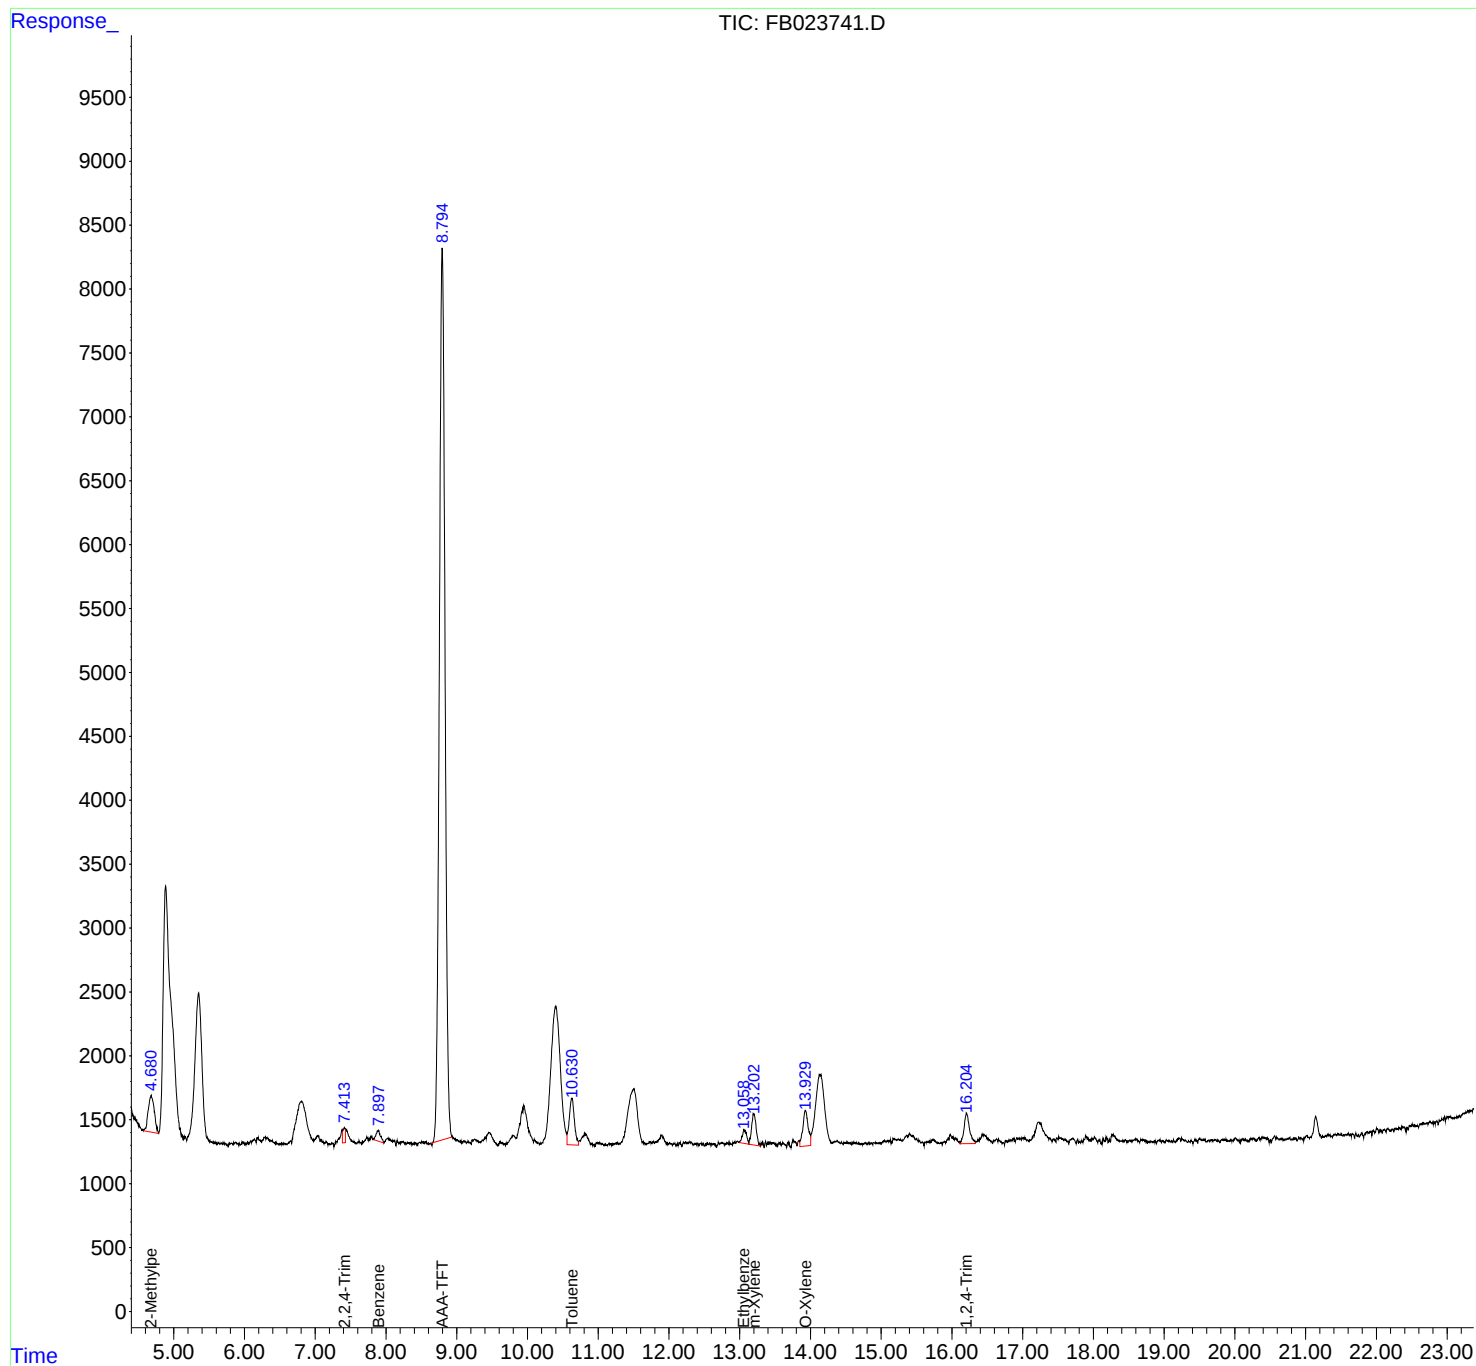


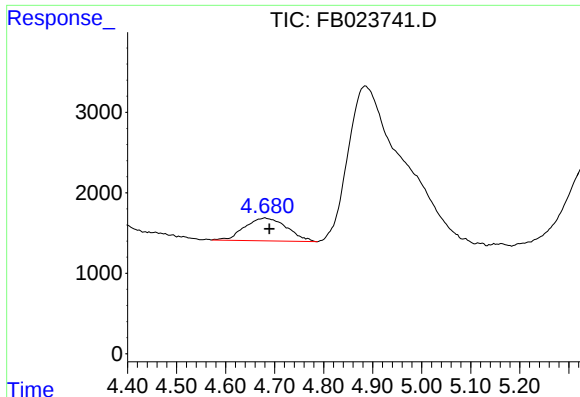

#1 2-Methylpentane


R.T.: 4.681 min
Delta R.T.: -0.008 min
Response: 16924
Conc: 0.56 ng/ml

Instrument :
FID_B
ClientSampleId :

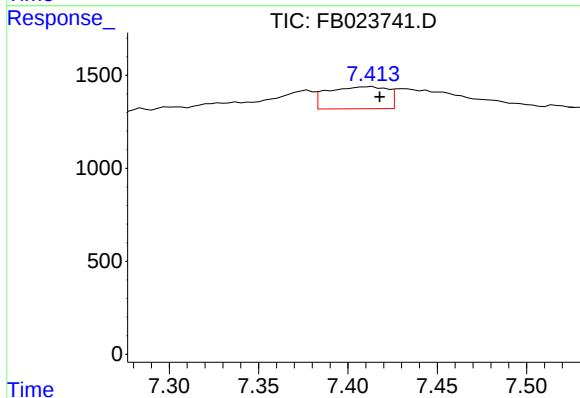


#2 2,2,4-Trimethylpentane

R.T.: 7.414 min
Delta R.T.: -0.004 min
Response: 2743
Conc: 0.08 ng/ml

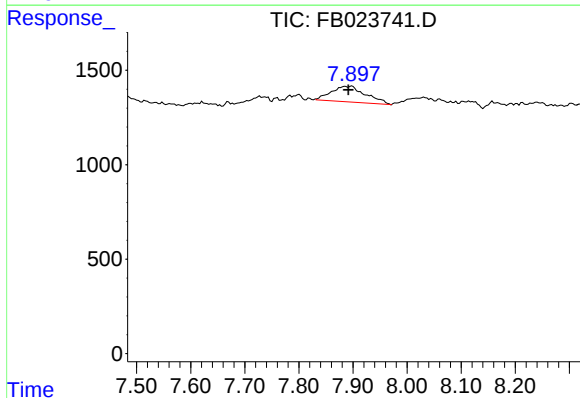


#4 Benzene

R.T.: 7.899 min
Delta R.T.: 0.007 min
Response: 3655
Conc: 0.09 ng/ml

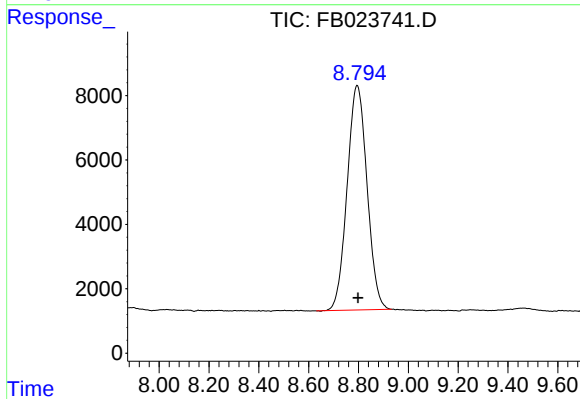

#5 AAA-TFT


R.T.: 8.795 min
Delta R.T.: -0.003 min
Response: 386778
Conc: 19.00 ng/ml

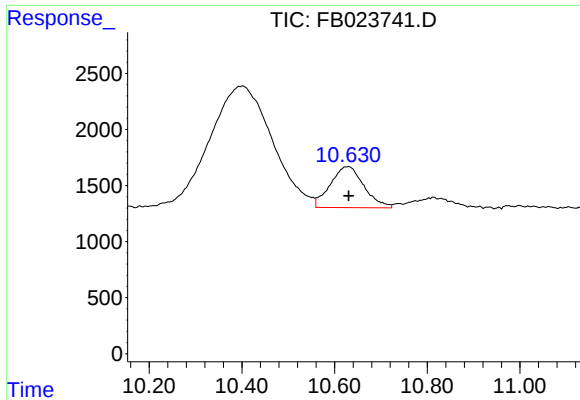

#6 Toluene


R.T.: 10.631 min
Delta R.T.: 0.000 min
Response: 18397
Conc: 0.46 ng/ml

Instrument :
FID_B
ClientSampleId :

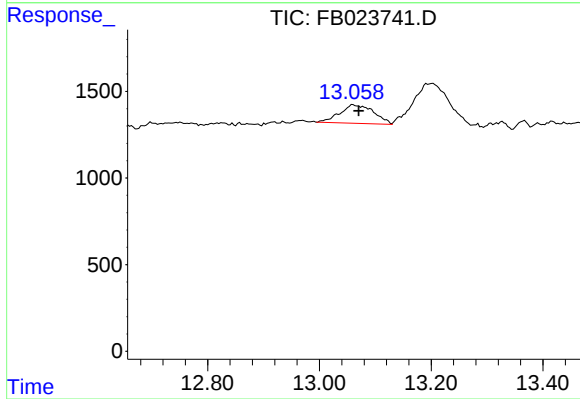


#7 Ethylbenzene

R.T.: 13.060 min
Delta R.T.: -0.010 min
Response: 4480
Conc: 0.12 ng/ml

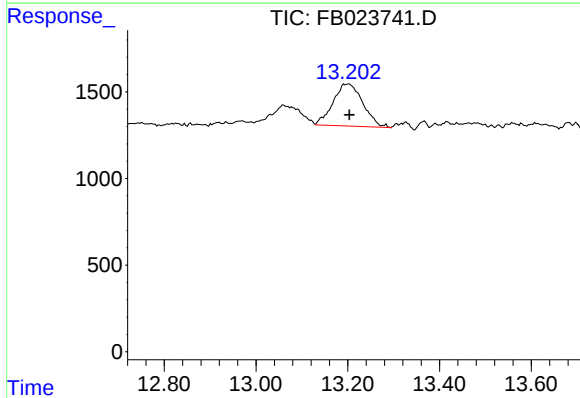


#8 m-Xylene

R.T.: 13.203 min
Delta R.T.: 0.000 min
Response: 10937
Conc: 0.31 ng/ml

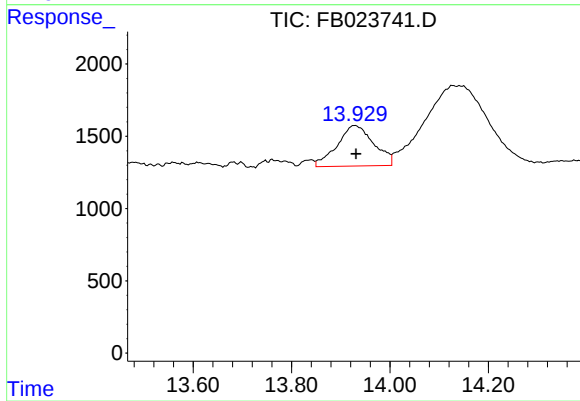

#9 O-Xylene

R.T.: 13.929 min
Delta R.T.: -0.002 min
Response: 14433
Conc: 0.42 ng/ml

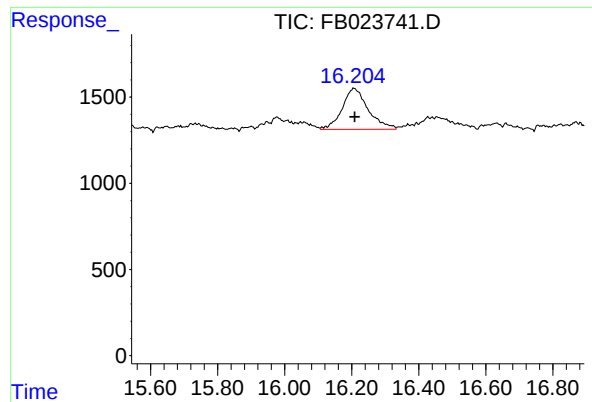

#10 1,2,4-Trimethylbenzene

R.T.: 16.207 min
Delta R.T.: -0.002 min
Response: 12659
Conc: 0.43 ng/ml

Instrument :
FID_B
ClientSampleId :