

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB022820\
 Data File : FB023743.D
 Signal(s) : FID2B.CH
 Acq On : 28 Feb 2020 11:37
 Operator : DD/AJ
 Sample : L1373-05
 Misc : 5.04g/5.00ml DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Feb 28 22:53:37 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB020620.M
 Quant Title :
 QLast Update : Thu Feb 06 11:13:47 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.798	438704	21.548 ng/ml
Target Compounds			
6) t Toluene	10.630	5478	0.138 ng/ml
8) t m-Xylene	13.203	698	0.020 ng/ml
9) t O-Xylene	13.931	1797	0.052 ng/ml
10) t 1,2,4-Trimethylbenzene	16.202	905	0.031 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB022820\
Data File : FB023743.D
Signal(s) : FID2B.CH
Acq On : 28 Feb 2020 11:37
Operator : DD/AJ
Sample : L1373-05
Misc : 5.04g/5.00ml DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Feb 28 22:53:37 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB020620.M
Quant Title :
QLast Update : Thu Feb 06 11:13:47 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

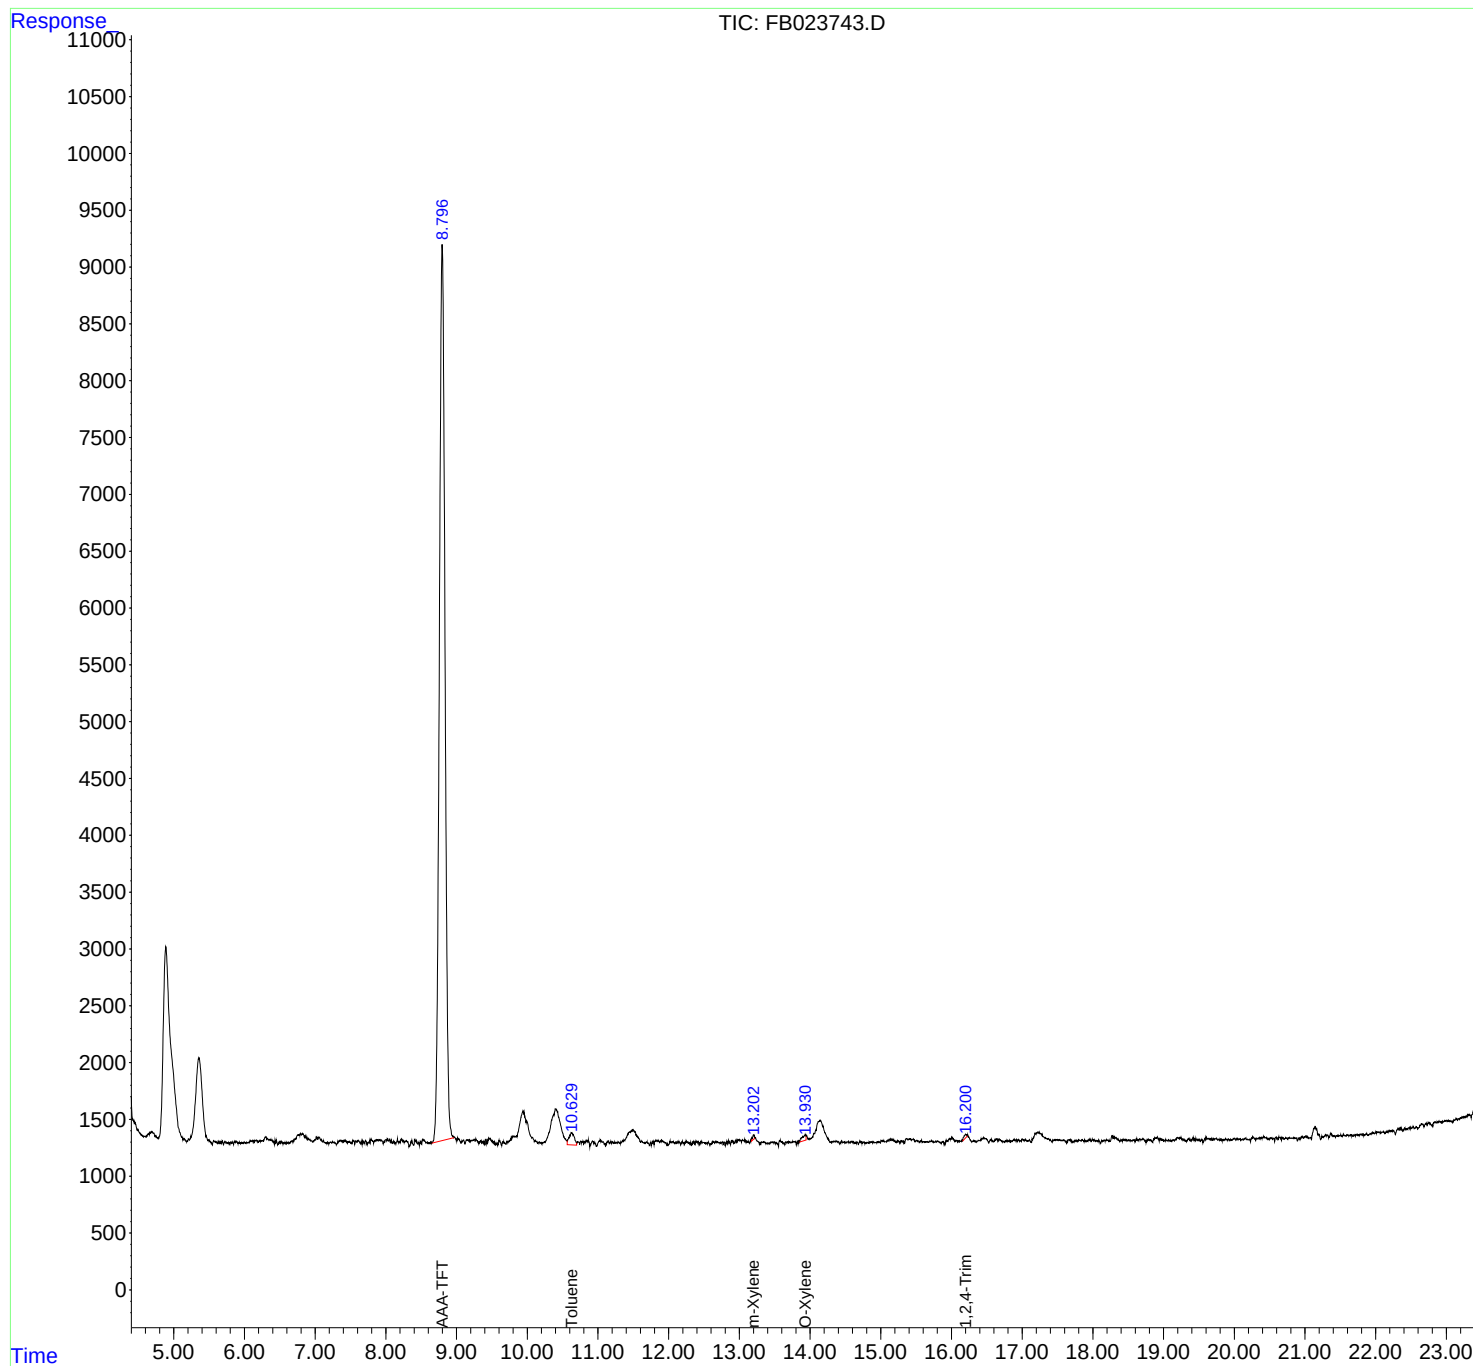


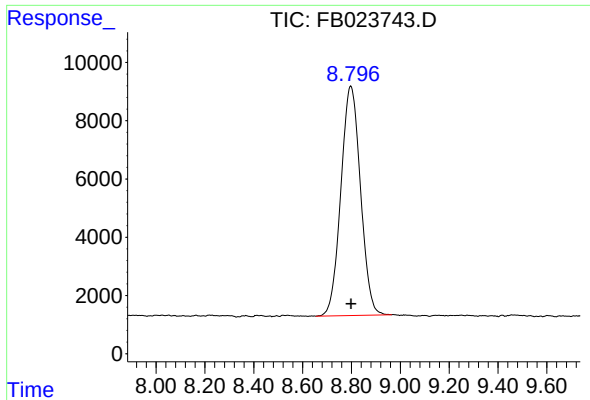

#5 AAA-TFT


R.T.: 8.798 min
Delta R.T.: 0.000 min
Response: 438704
Conc: 21.55 ng/ml

Instrument :
FID_B
ClientSampleId :

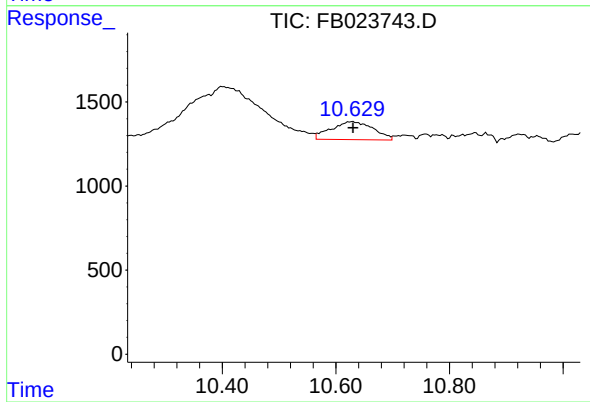


#6 Toluene

R.T.: 10.630 min
Delta R.T.: 0.000 min
Response: 5478
Conc: 0.14 ng/ml

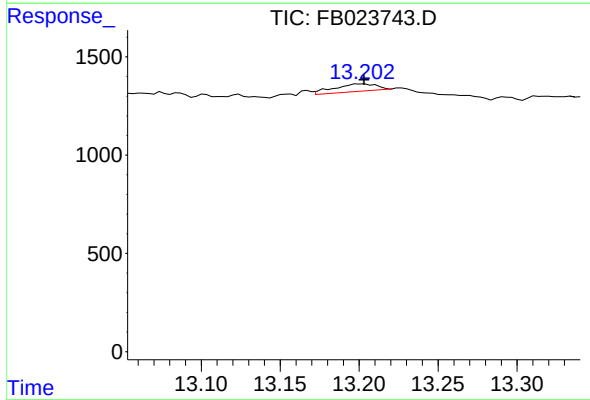


#8 m-Xylene

R.T.: 13.203 min
Delta R.T.: 0.000 min
Response: 698
Conc: 0.02 ng/ml

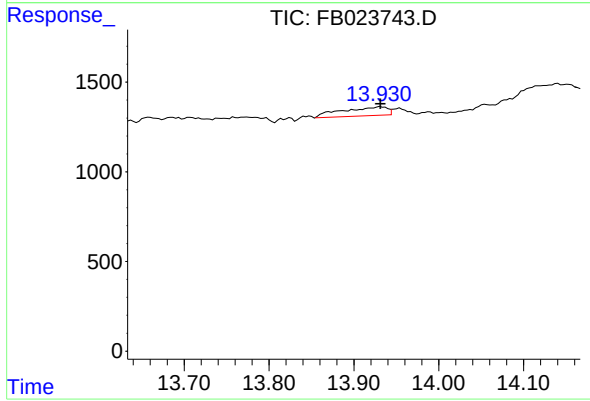

#9 O-Xylene

R.T.: 13.931 min
Delta R.T.: 0.000 min
Response: 1797
Conc: 0.05 ng/ml

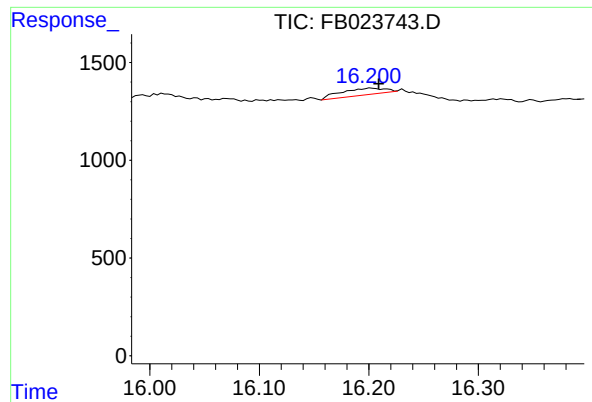

#10 1,2,4-Trimethylbenzene

R.T.: 16.202 min
Delta R.T.: -0.007 min
Response: 905
Conc: 0.03 ng/ml

Instrument :
FID_B
ClientSampleId :