

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB022820\
 Data File : FB023745.D
 Signal(s) : FID2B.CH
 Acq On : 28 Feb 2020 12:37
 Operator : DD/AJ
 Sample : L1373-05MSD
 Misc : 5.06g/5.00ml DI WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Feb 28 22:53:48 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB020620.M
 Quant Title :
 QLast Update : Thu Feb 06 11:13:47 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.798	432772	21.256 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.689	774235	25.731 ng/ml
2) t 2,2,4-Trimethylpentane	7.417	799228	24.493 ng/ml
3) t n-Heptane	7.757	255577	7.944 ng/ml
4) t Benzene	7.891	376787	9.212 ng/ml
6) t Toluene	10.629	1101180	27.741 ng/ml
7) t Ethylbenzene	13.070	333095	8.960 ng/ml
8) t m-Xylene	13.203	640132	17.925 ng/ml
9) t O-Xylene	13.931	617976	17.918 ng/ml
10) t 1,2,4-Trimethylbenzene	16.209	505742	17.273 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB022820\
Data File : FB023745.D
Signal(s) : FID2B.CH
Acq On : 28 Feb 2020 12:37
Operator : DD/AJ
Sample : L1373-05MSD
Misc : 5.06g/5.00ml DI WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Feb 28 22:53:48 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB020620.M
Quant Title :
QLast Update : Thu Feb 06 11:13:47 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

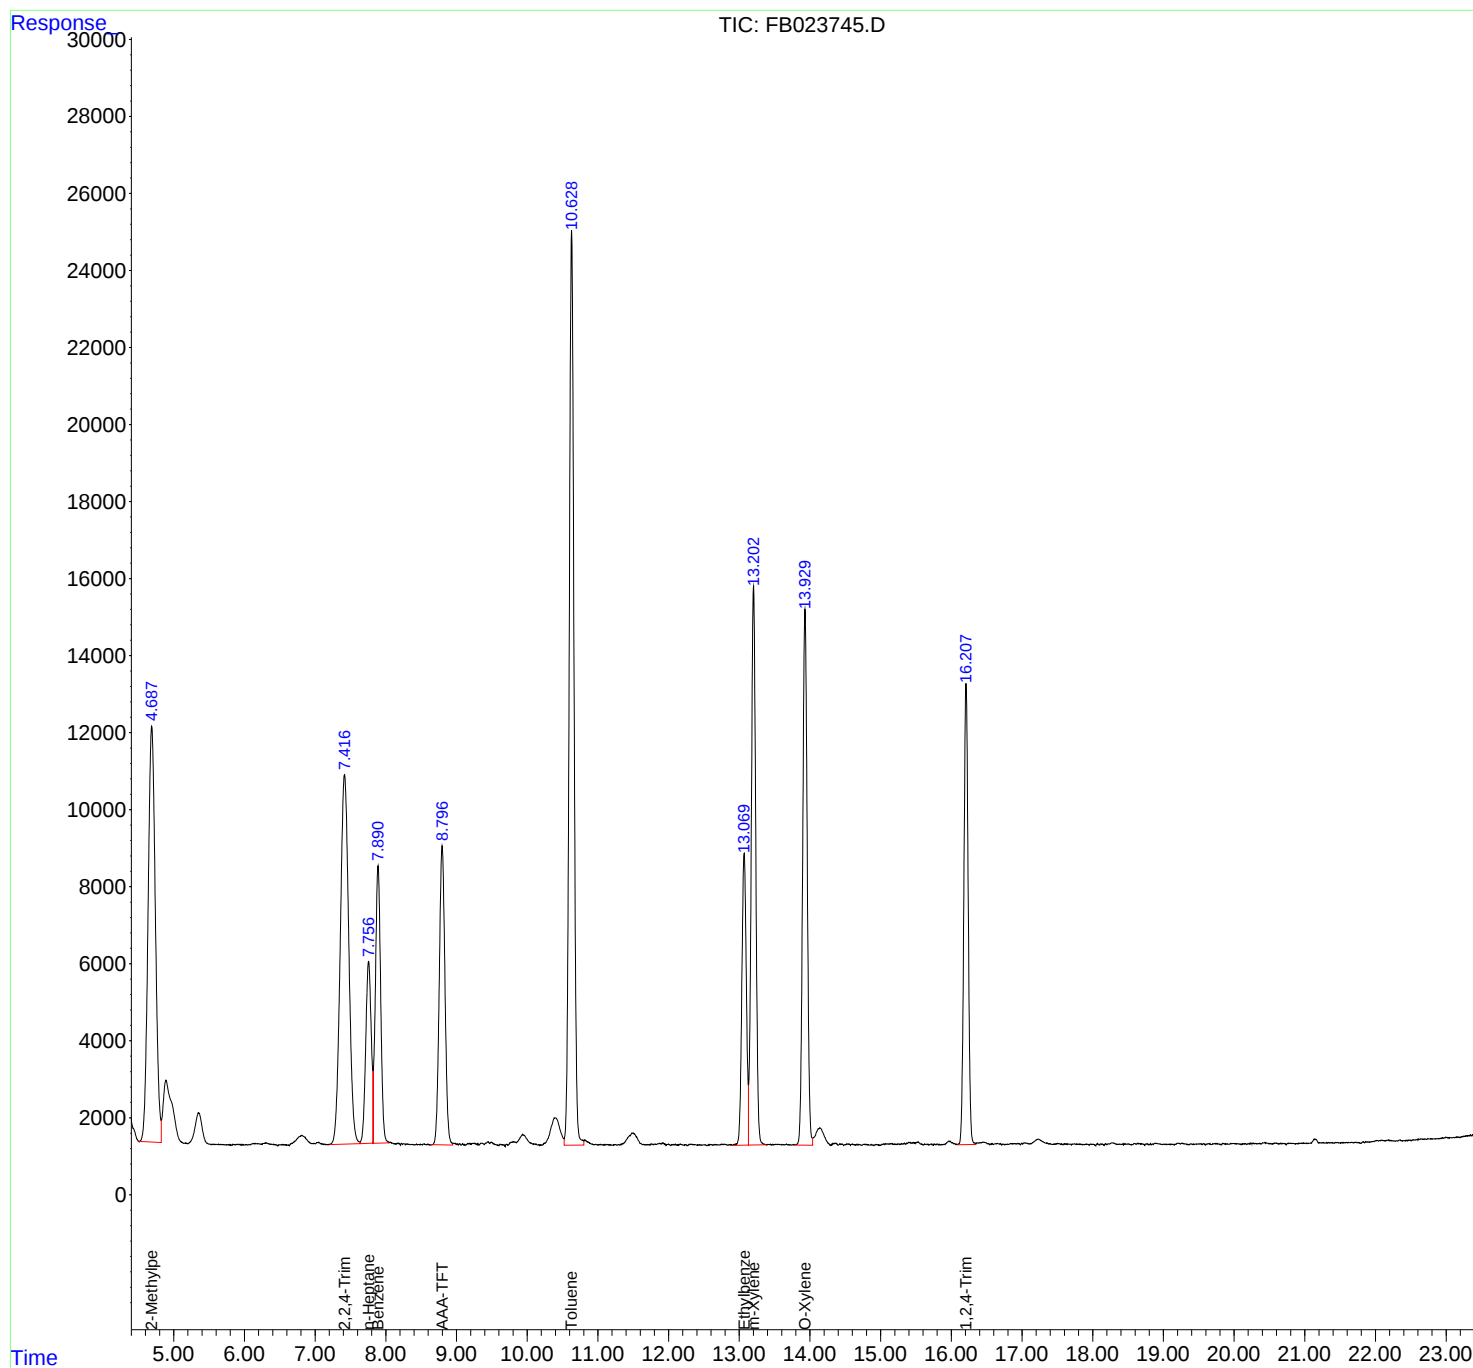


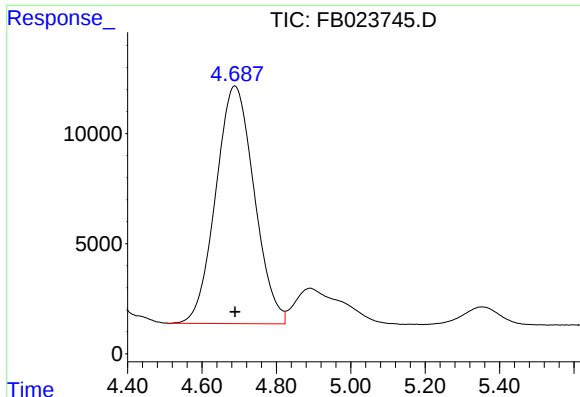

#1 2-Methylpentane


R.T.: 4.689 min
Delta R.T.: 0.000 min
Response: 774235
Conc: 25.73 ng/ml

Instrument :
FID_B
ClientSampleId :

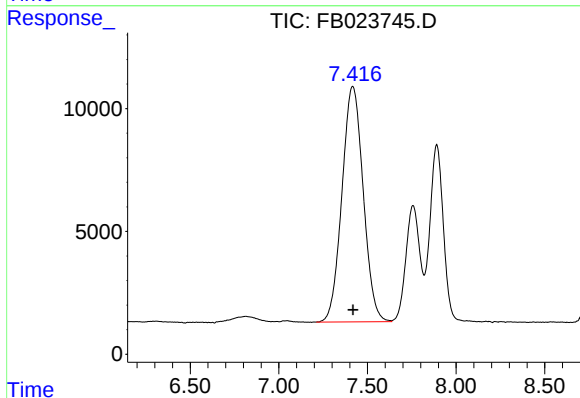


#2 2,2,4-Trimethylpentane

R.T.: 7.417 min
Delta R.T.: 0.000 min
Response: 799228
Conc: 24.49 ng/ml

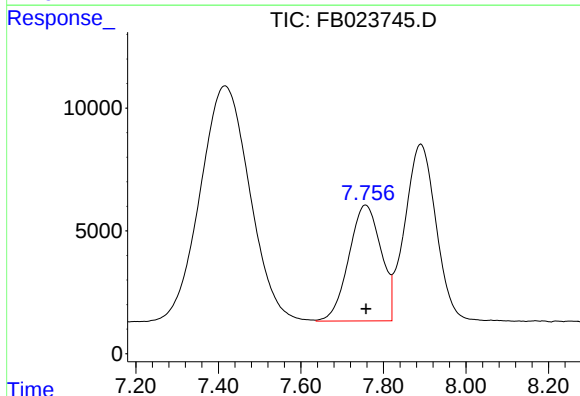


#3 n-Heptane

R.T.: 7.757 min
Delta R.T.: 0.000 min
Response: 255577
Conc: 7.94 ng/ml

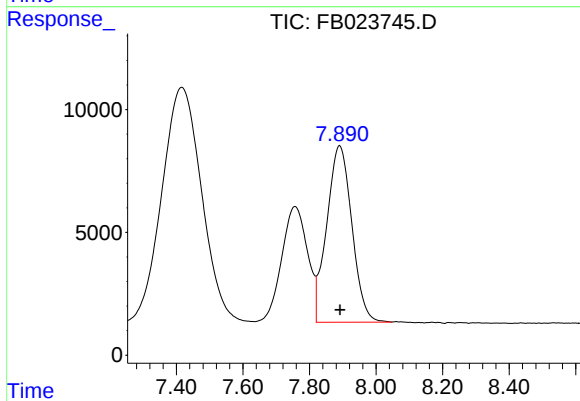

#4 Benzene


R.T.: 7.891 min
Delta R.T.: 0.000 min
Response: 376787
Conc: 9.21 ng/ml

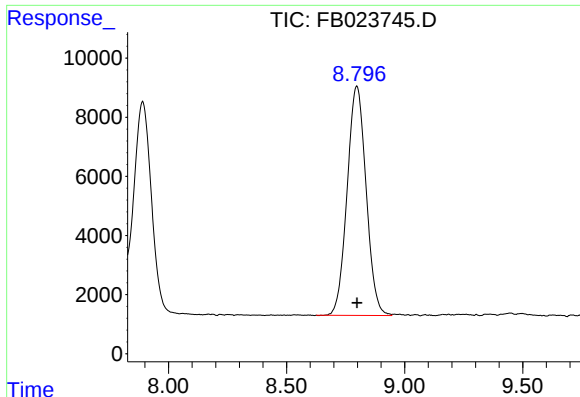

#5 AAA-TFT


R.T.: 8.798 min
Delta R.T.: 0.000 min
Response: 432772
Conc: 21.26 ng/ml

Instrument :
FID_B
ClientSampleId :

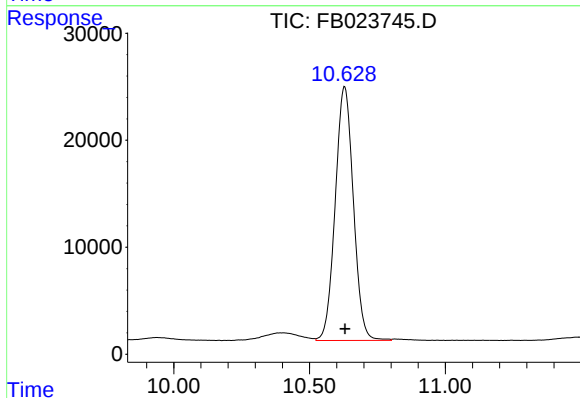


#6 Toluene

R.T.: 10.629 min
Delta R.T.: 0.000 min
Response: 1101180
Conc: 27.74 ng/ml

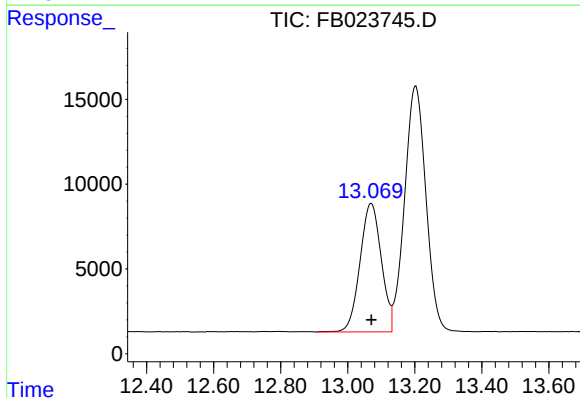


#7 Ethylbenzene

R.T.: 13.070 min
Delta R.T.: 0.000 min
Response: 333095
Conc: 8.96 ng/ml

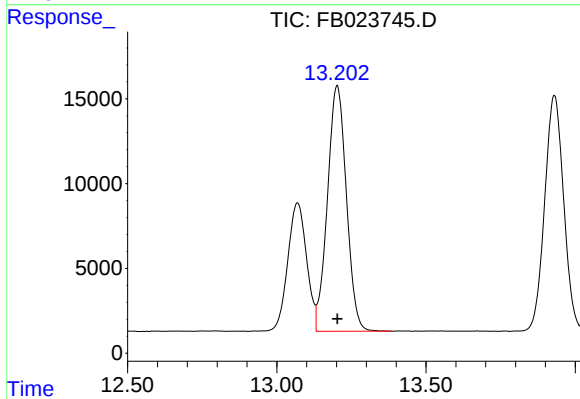

#8 m-Xylene

R.T.: 13.203 min
Delta R.T.: 0.000 min
Response: 640132
Conc: 17.92 ng/ml

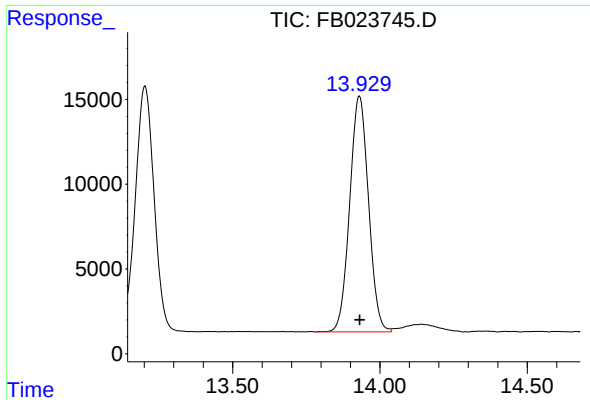

#9 O-Xylene


R.T.: 13.931 min

Delta R.T.: 0.000 min

Response: 617976

Conc: 17.92 ng/ml

Instrument :
FID_B
ClientSampleId :

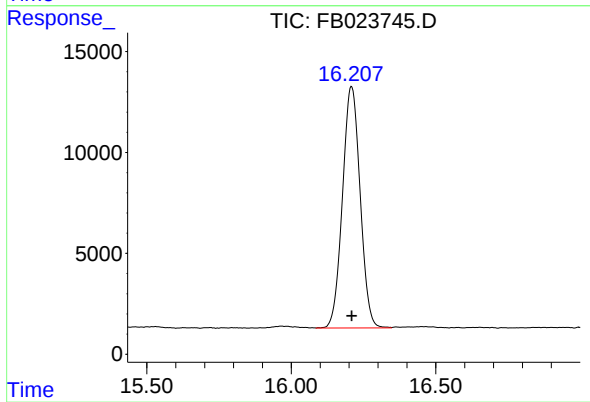

#10 1,2,4-Trimethylbenzene

R.T.: 16.209 min

Delta R.T.: 0.000 min

Response: 505742

Conc: 17.27 ng/ml