

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB022820\  
 Data File : FB023747.D  
 Signal(s) : FID2B.CH  
 Acq On : 28 Feb 2020 16:39  
 Operator : DD/AJ  
 Sample : L1743-02  
 Misc : 5.02g/5.00ml DI WATER  
 ALS Vial : 8 Sample Multiplier: 1

Instrument :  
 FID\_B  
 ClientSampleId :

Integration File: Calibration.e  
 Quant Time: Feb 28 22:54:00 2020  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB020620.M  
 Quant Title :  
 QLast Update : Thu Feb 06 11:13:47 2020  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 5 g/ml  
 Signal Phase : RTX-502.2  
 Signal Info : 60mx0.53mmx3.00um

| Compound                    | R.T.   | Response | Conc Units   |
|-----------------------------|--------|----------|--------------|
| -----                       |        |          |              |
| System Monitoring Compounds |        |          |              |
| 5) s AAA-TFT                | 8.794  | 405233   | 19.904 ng/ml |
| Target Compounds            |        |          |              |
| 6) t Toluene                | 10.624 | 3991     | 0.101 ng/ml  |
| 9) t O-Xylene               | 13.912 | 2106     | 0.061 ng/ml  |
| -----                       |        |          |              |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB022820\  
Data File : FB023747.D  
Signal(s) : FID2B.CH  
Acq On : 28 Feb 2020 16:39  
Operator : DD/AJ  
Sample : L1743-02  
Misc : 5.02g/5.00ml DI WATER  
ALS Vial : 8 Sample Multiplier: 1

Instrument :  
FID\_B  
ClientSampleId :

Integration File: Calibration.e  
Quant Time: Feb 28 22:54:00 2020  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB020620.M  
Quant Title :  
QLast Update : Thu Feb 06 11:13:47 2020  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 5 g/ml  
Signal Phase : RTX-502.2  
Signal Info : 60mx0.53mmx3.00um

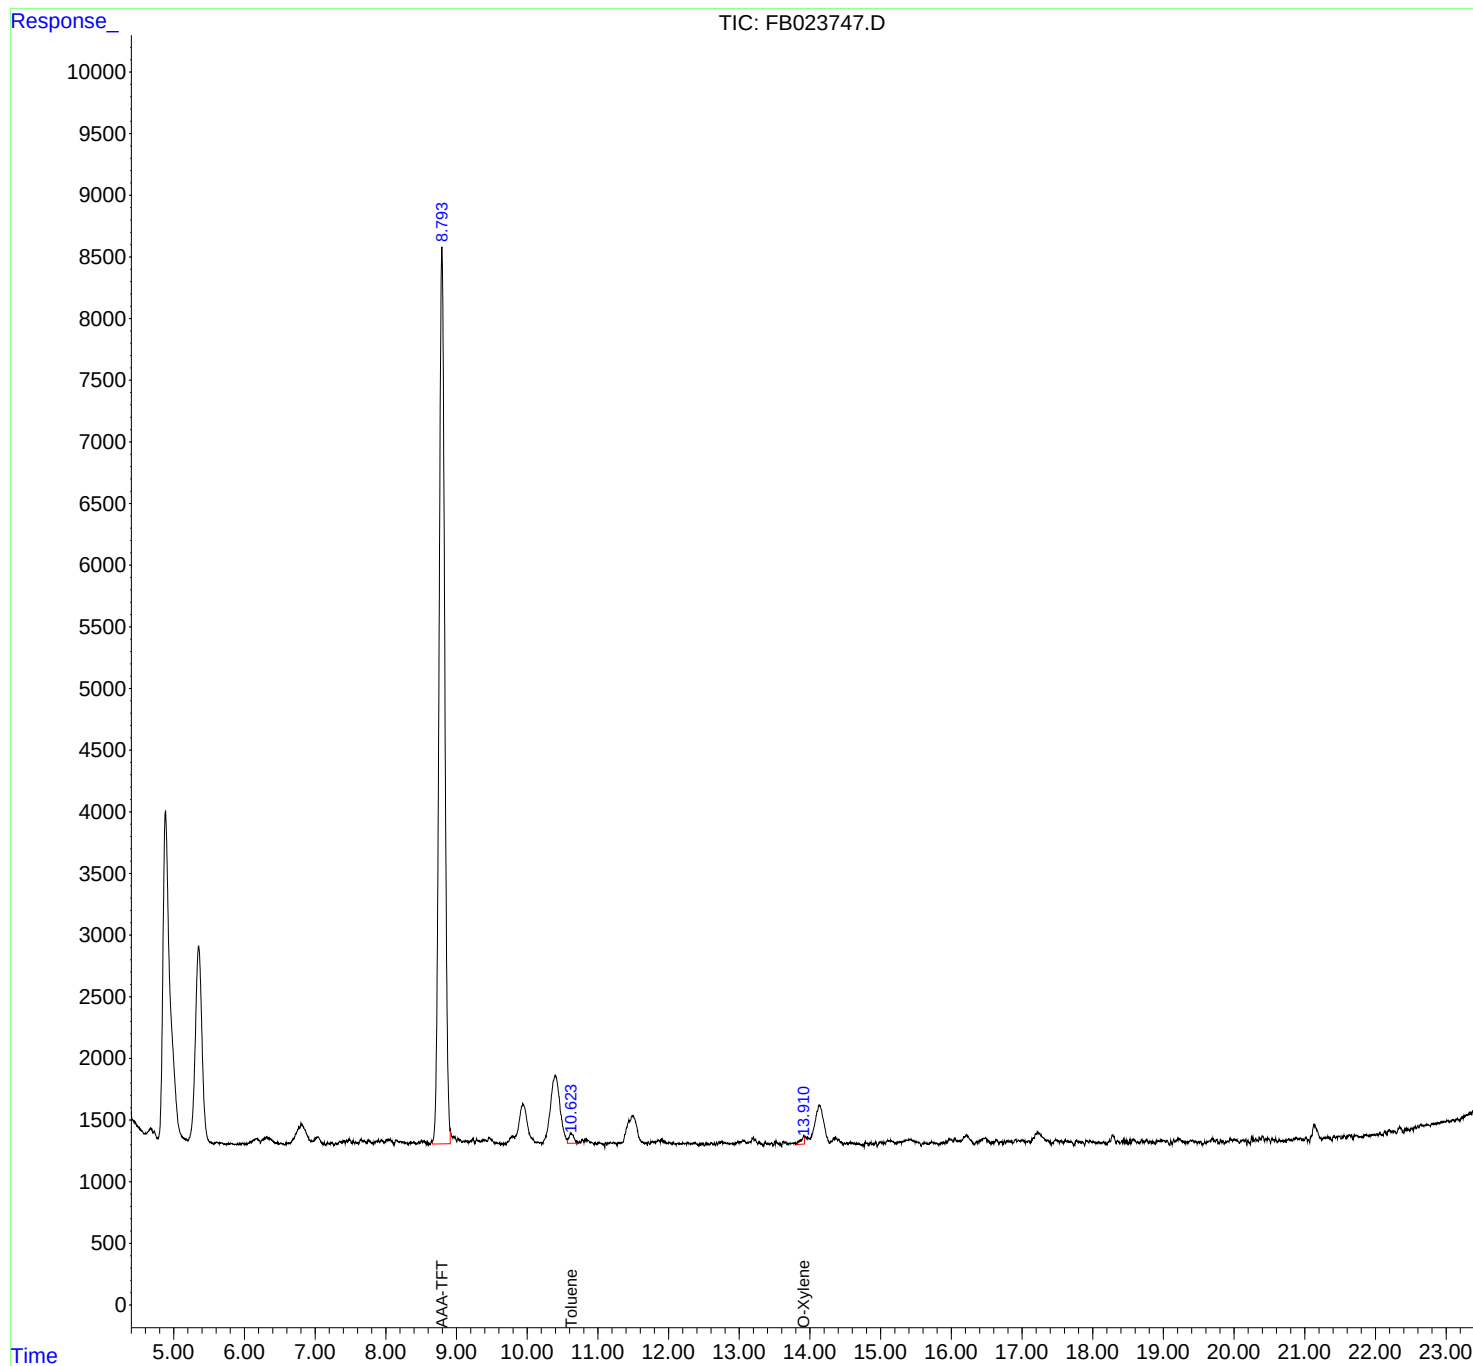


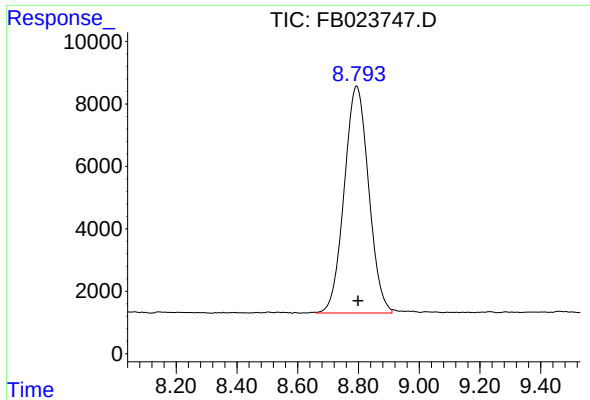

#5 AAA-TFT


R.T.: 8.794 min  
Delta R.T.: -0.004 min  
Response: 405233  
Conc: 19.90 ng/ml

Instrument :  
FID\_B  
ClientSampleId :

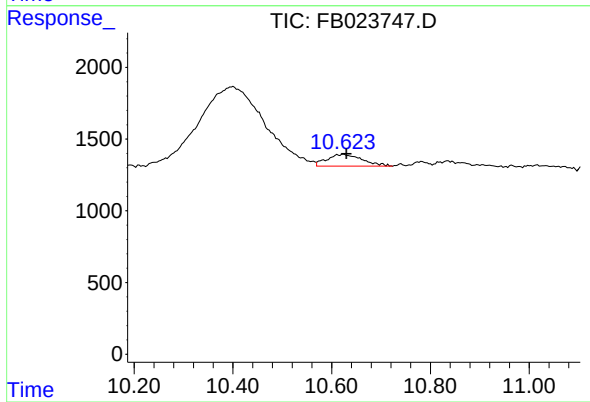

#6 Toluene

R.T.: 10.624 min  
Delta R.T.: -0.006 min  
Response: 3991  
Conc: 0.10 ng/ml

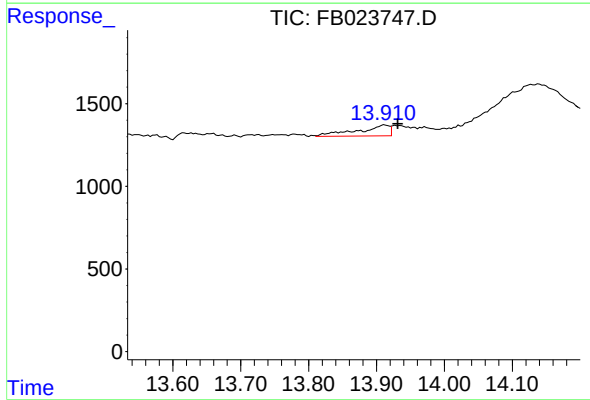

#9 O-Xylene

R.T.: 13.912 min  
Delta R.T.: -0.019 min  
Response: 2106  
Conc: 0.06 ng/ml