

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB022820\
 Data File : FB023742.D
 Signal(s) : FID2B.CH
 Acq On : 28 Feb 2020 11:07
 Operator : DD/AJ
 Sample : BSF0228S1
 Misc : 5.00g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0228S1

Integration File: Calibration.e
 Quant Time: Feb 28 22:53:31 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB020620.M
 Quant Title :
 QLast Update : Thu Feb 06 11:13:47 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.797	404678	19.876 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.688	842004	27.983 ng/ml
2) t 2,2,4-Trimethylpentane	7.414	968024	29.666 ng/ml
3) t n-Heptane	7.755	306014	9.511 ng/ml
4) t Benzene	7.889	382900	9.362 ng/ml
6) t Toluene	10.628	1130426	28.478 ng/ml
7) t Ethylbenzene	13.068	356055	9.578 ng/ml
8) t m-Xylene	13.202	683661	19.144 ng/ml
9) t O-Xylene	13.929	657044	19.051 ng/ml
10) t 1,2,4-Trimethylbenzene	16.208	559800	19.120 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB022820\
Data File : FB023742.D
Signal(s) : FID2B.CH
Acq On : 28 Feb 2020 11:07
Operator : DD/AJ
Sample : BSF0228S1
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0228S1

Integration File: Calibration.e
Quant Time: Feb 28 22:53:31 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB020620.M
Quant Title :
QLast Update : Thu Feb 06 11:13:47 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

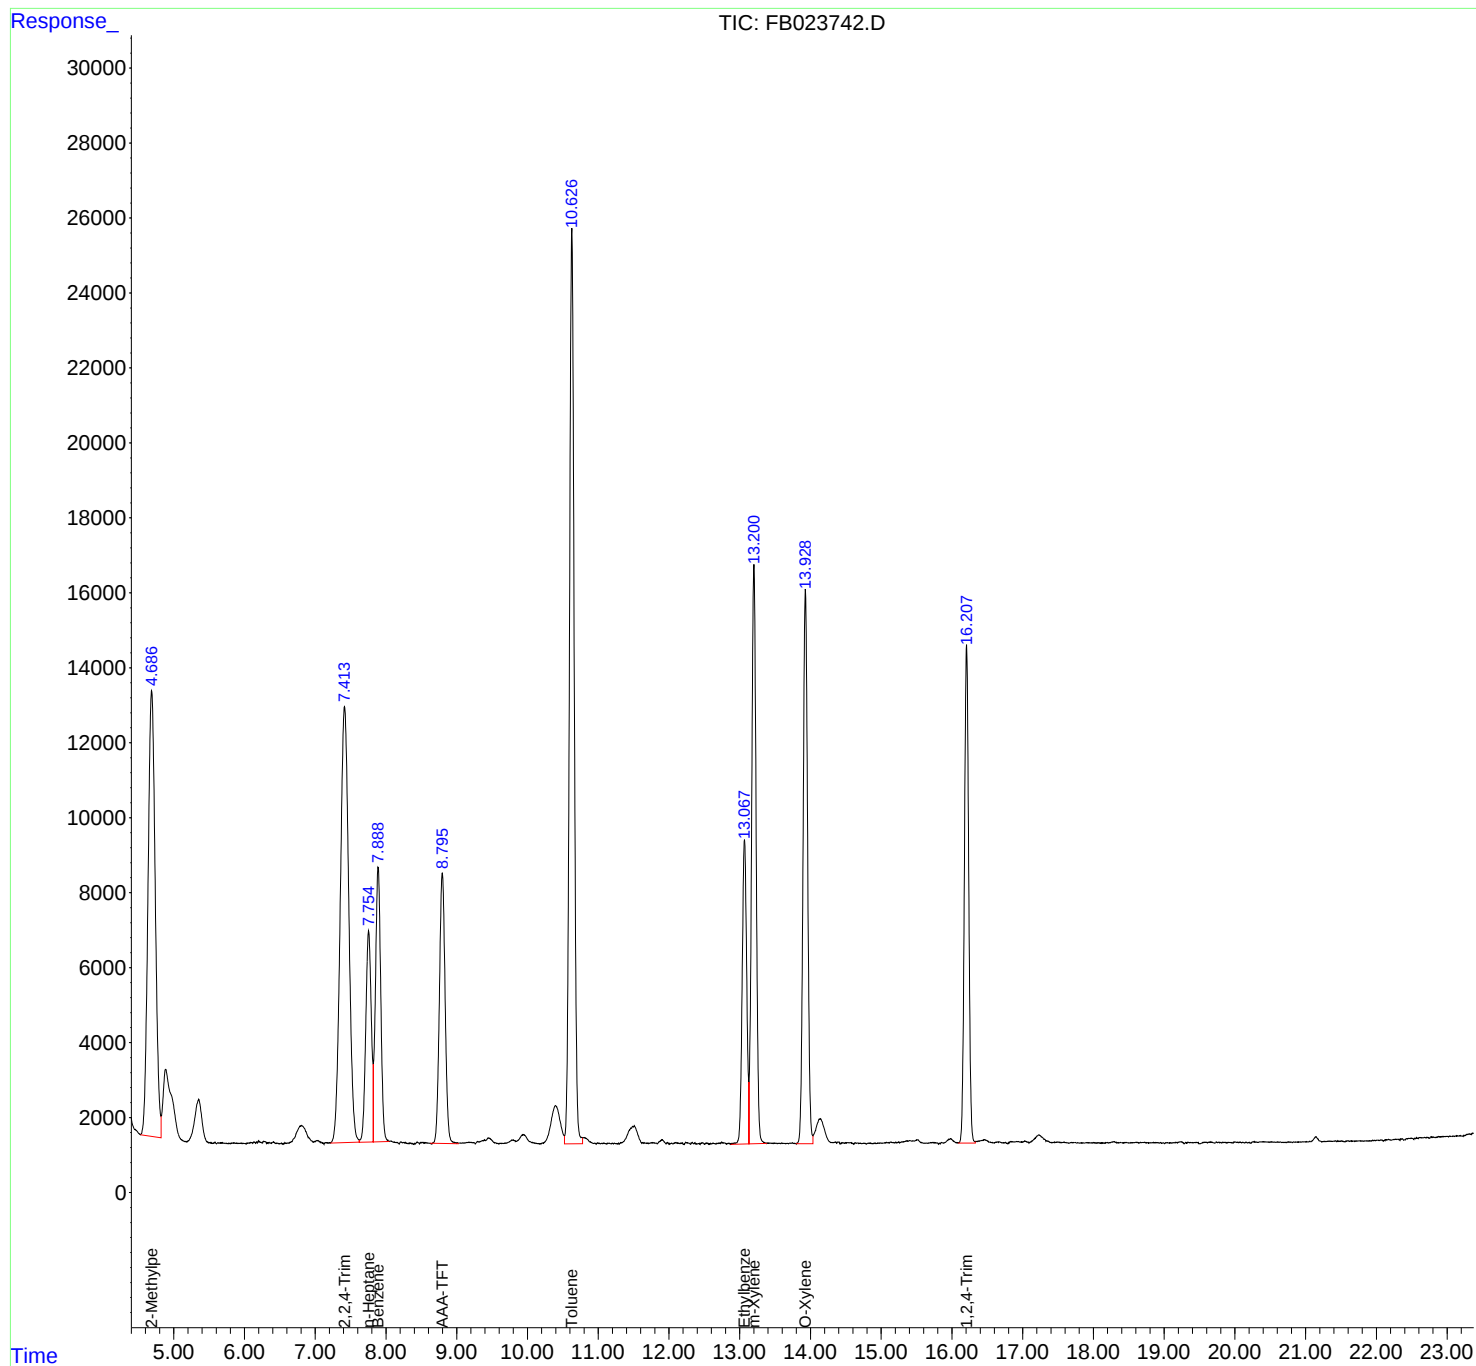


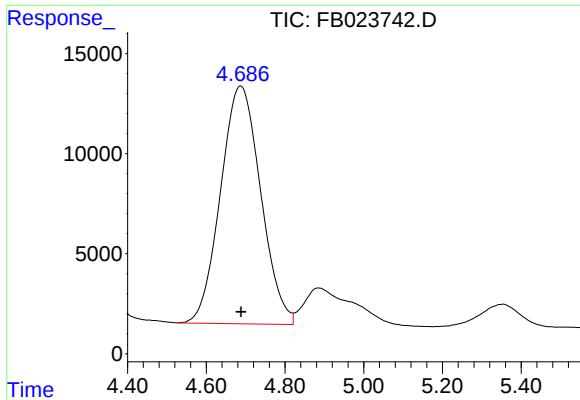

#1 2-Methylpentane


R.T.: 4.688 min
Delta R.T.: -0.001 min
Response: 842004
Conc: 27.98 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0228S1

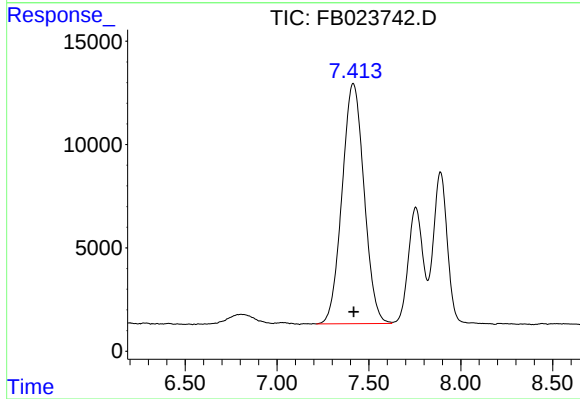


#2 2,2,4-Trimethylpentane

R.T.: 7.414 min
Delta R.T.: -0.004 min
Response: 968024
Conc: 29.67 ng/ml

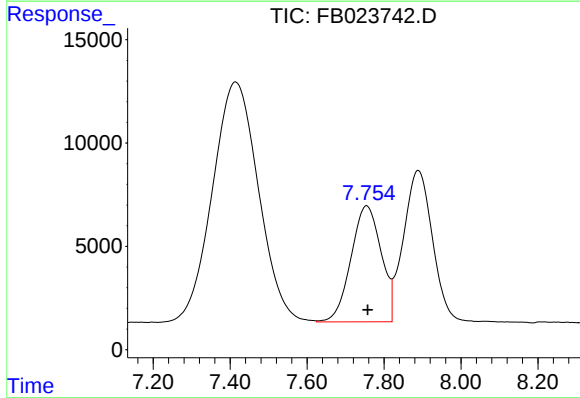


#3 n-Heptane

R.T.: 7.755 min
Delta R.T.: -0.003 min
Response: 306014
Conc: 9.51 ng/ml

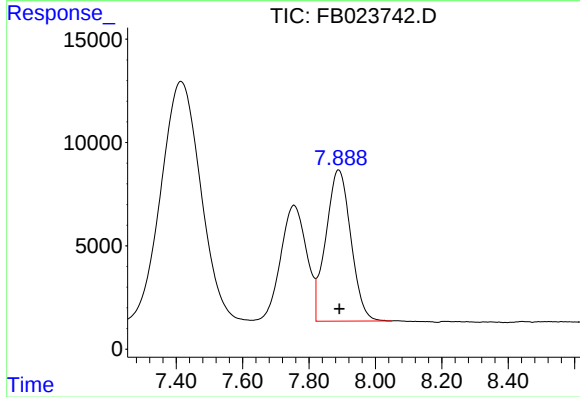

#4 Benzene


R.T.: 7.889 min
Delta R.T.: -0.002 min
Response: 382900
Conc: 9.36 ng/ml

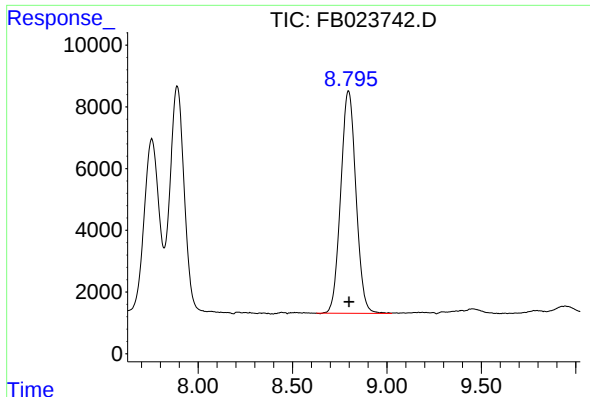

#5 AAA-TFT


R.T.: 8.797 min
Delta R.T.: -0.002 min
Response: 404678
Conc: 19.88 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0228S1

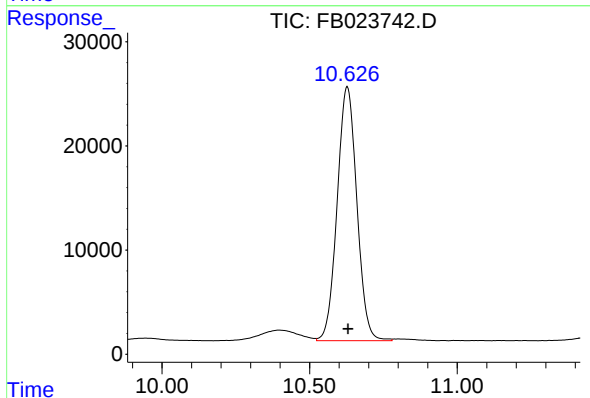


#6 Toluene

R.T.: 10.628 min
Delta R.T.: -0.002 min
Response: 1130426
Conc: 28.48 ng/ml

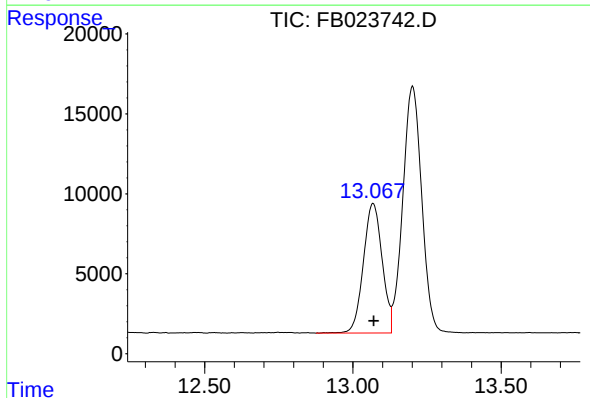


#7 Ethylbenzene

R.T.: 13.068 min
Delta R.T.: -0.002 min
Response: 356055
Conc: 9.58 ng/ml

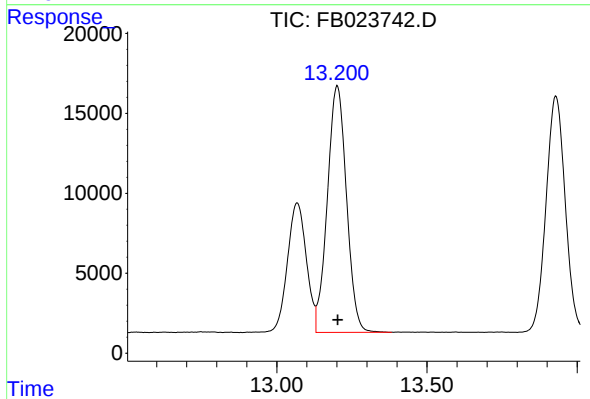

#8 m-Xylene


R.T.: 13.202 min
Delta R.T.: -0.002 min
Response: 683661
Conc: 19.14 ng/ml

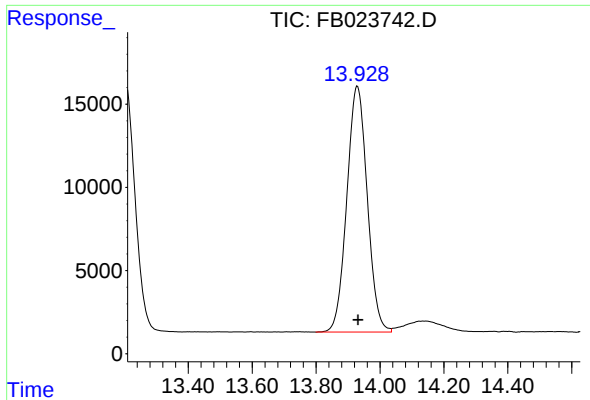

#9 O-Xylene

R.T.: 13.929 min
Delta R.T.: -0.002 min
Response: 657044
Conc: 19.05 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0228S1

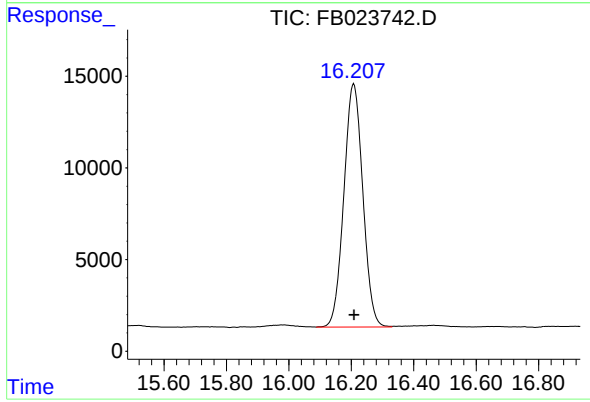

#10 1,2,4-Trimethylbenzene

R.T.: 16.208 min
Delta R.T.: -0.001 min
Response: 559800
Conc: 19.12 ng/ml