

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB022820\
 Data File : FB023744.D
 Signal(s) : FID2B.CH
 Acq On : 28 Feb 2020 12:07
 Operator : DD/AJ
 Sample : L1373-05MS
 Misc : 5.06g/5.00ml DI WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 TR-06-022720MS

Integration File: Calibration.e
 Quant Time: Feb 28 22:53:42 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB020620.M
 Quant Title :
 QLast Update : Thu Feb 06 11:13:47 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.797	439368	21.580 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.691	800567	26.606 ng/ml
2) t 2,2,4-Trimethylpentane	7.416	875500	26.830 ng/ml
3) t n-Heptane	7.756	277184	8.615 ng/ml
4) t Benzene	7.891	395621	9.673 ng/ml
6) t Toluene	10.629	1162307	29.281 ng/ml
7) t Ethylbenzene	13.069	361191	9.716 ng/ml
8) t m-Xylene	13.202	694453	19.446 ng/ml
9) t O-Xylene	13.930	665534	19.297 ng/ml
10) t 1,2,4-Trimethylbenzene	16.209	546592	18.669 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB022820\
Data File : FB023744.D
Signal(s) : FID2B.CH
Acq On : 28 Feb 2020 12:07
Operator : DD/AJ
Sample : L1373-05MS
Misc : 5.06g/5.00ml DI WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
TR-06-022720MS

Integration File: Calibration.e
Quant Time: Feb 28 22:53:42 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB020620.M
Quant Title :
QLast Update : Thu Feb 06 11:13:47 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

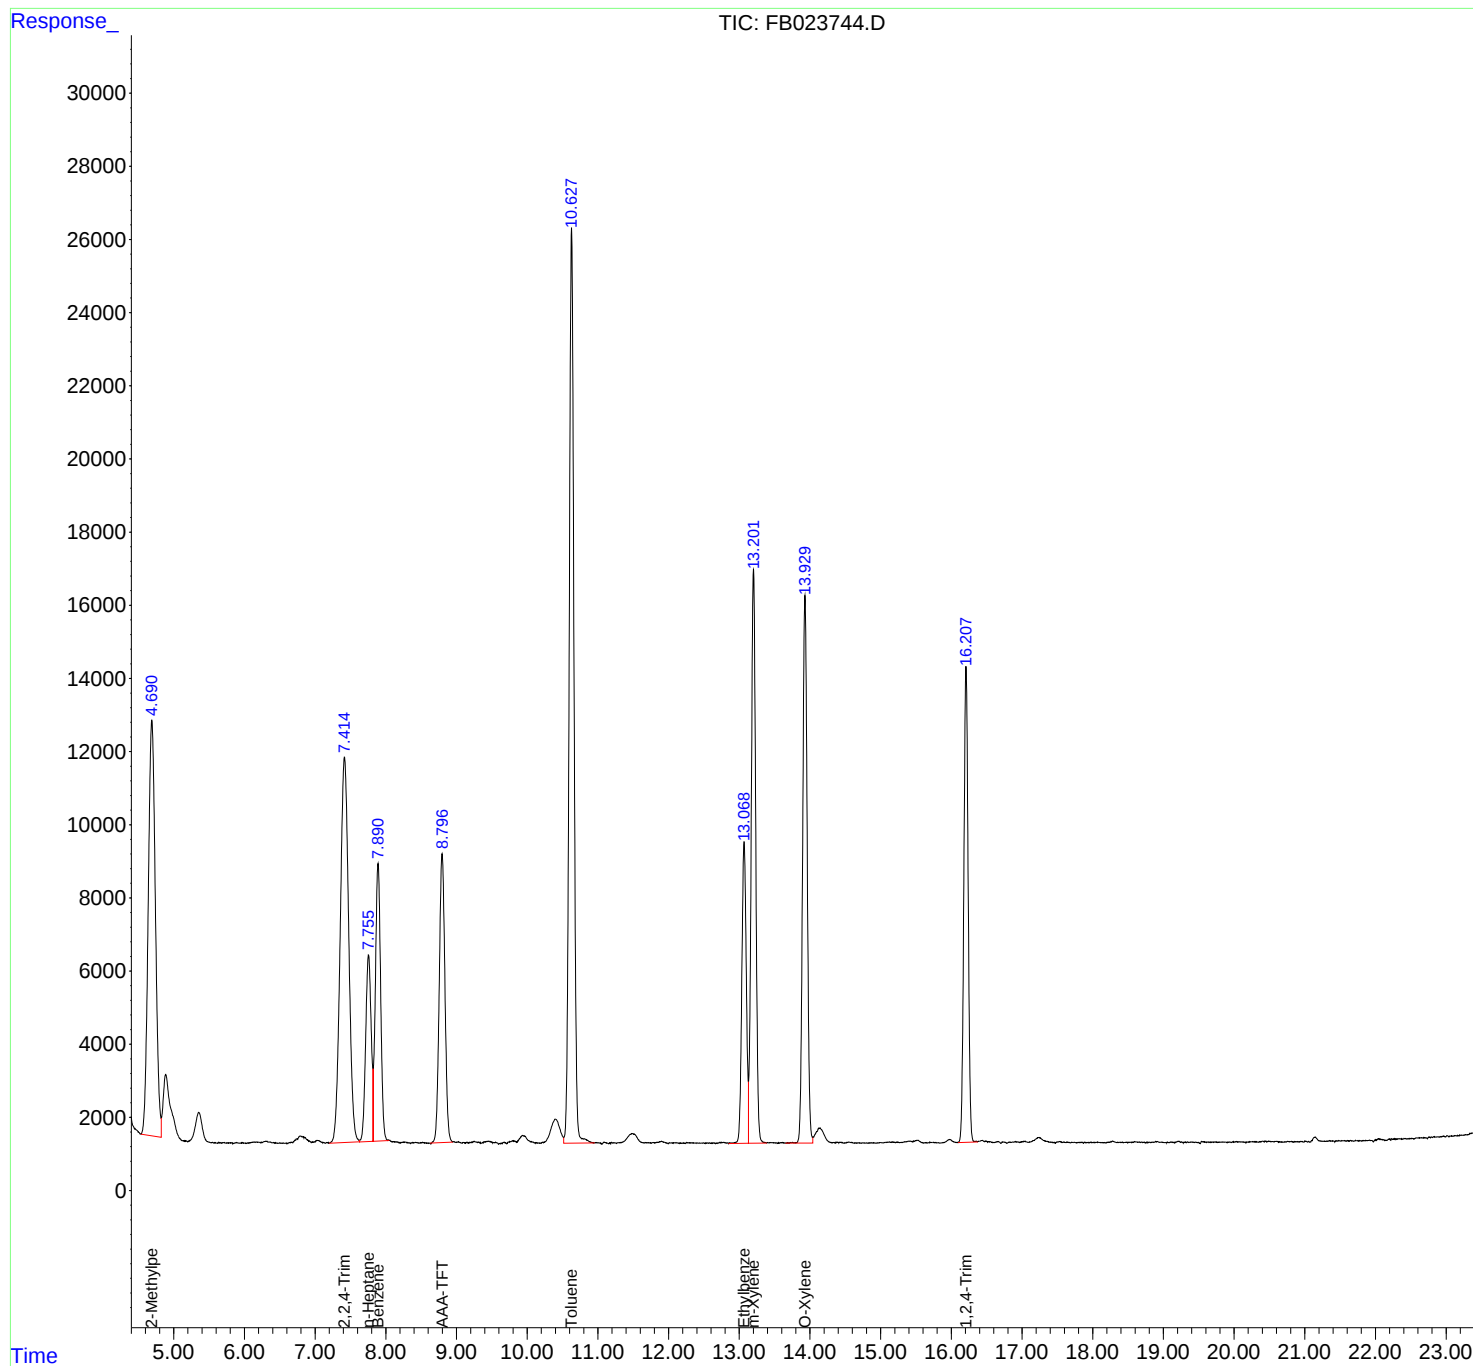


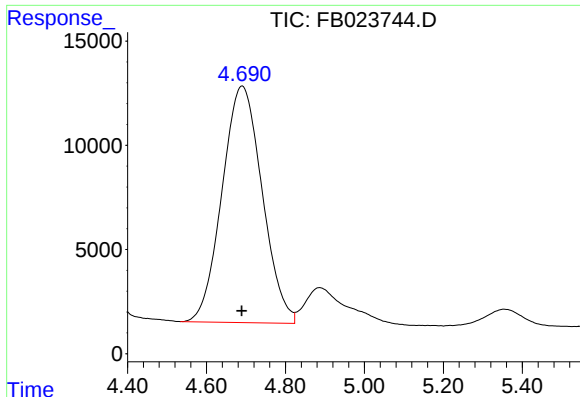

#1 2-Methylpentane


R.T.: 4.691 min
Delta R.T.: 0.002 min
Response: 800567
Conc: 26.61 ng/ml

Instrument :
FID_B
ClientSampleId :
TR-06-022720MS

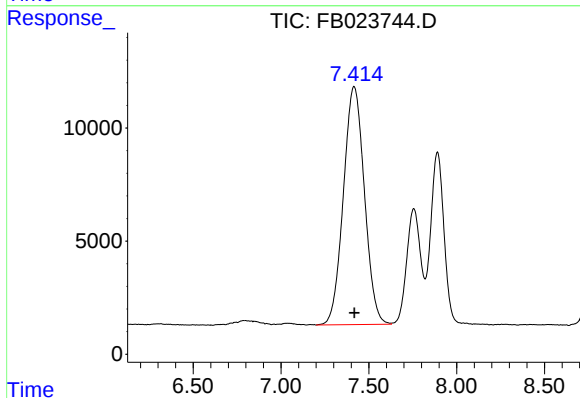


#2 2,2,4-Trimethylpentane

R.T.: 7.416 min
Delta R.T.: -0.002 min
Response: 875500
Conc: 26.83 ng/ml

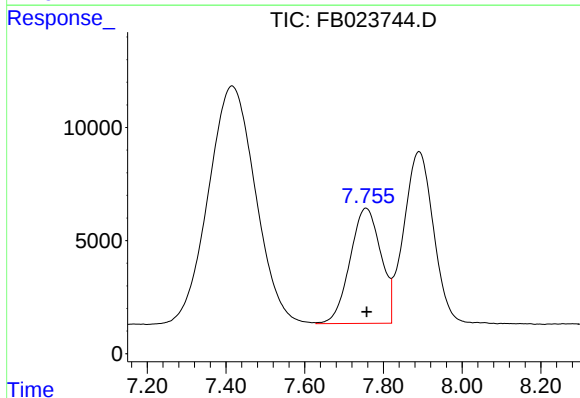


#3 n-Heptane

R.T.: 7.756 min
Delta R.T.: -0.002 min
Response: 277184
Conc: 8.62 ng/ml

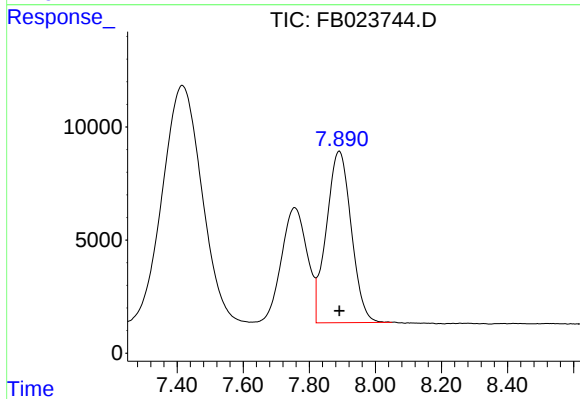

#4 Benzene


R.T.: 7.891 min
Delta R.T.: 0.000 min
Response: 395621
Conc: 9.67 ng/ml

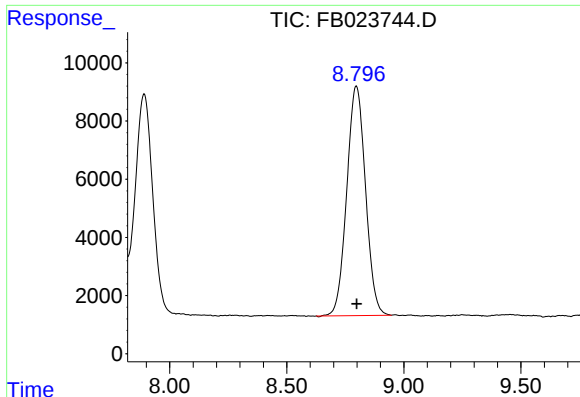

#5 AAA-TFT


R.T.: 8.797 min
Delta R.T.: -0.001 min
Response: 439368
Conc: 21.58 ng/ml

Instrument :
FID_B
ClientSampleId :
TR-06-022720MS

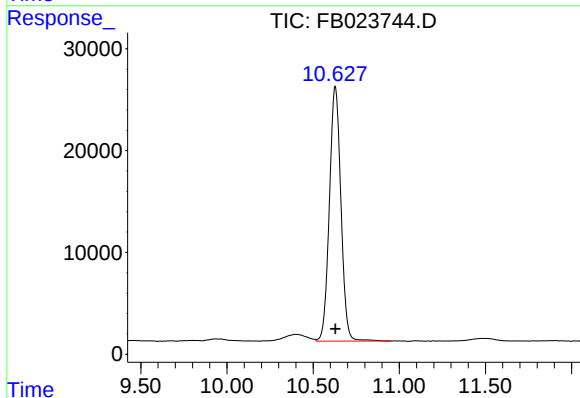


#6 Toluene

R.T.: 10.629 min
Delta R.T.: -0.001 min
Response: 1162307
Conc: 29.28 ng/ml

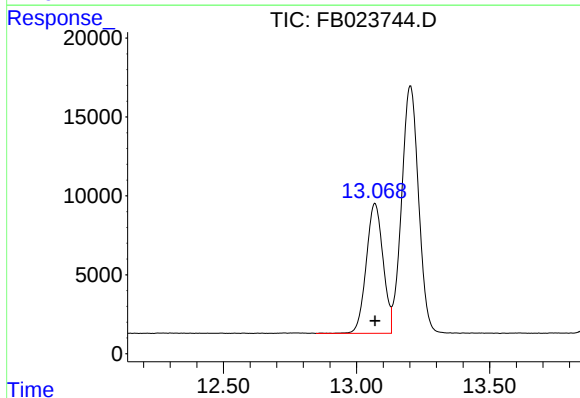


#7 Ethylbenzene

R.T.: 13.069 min
Delta R.T.: 0.000 min
Response: 361191
Conc: 9.72 ng/ml

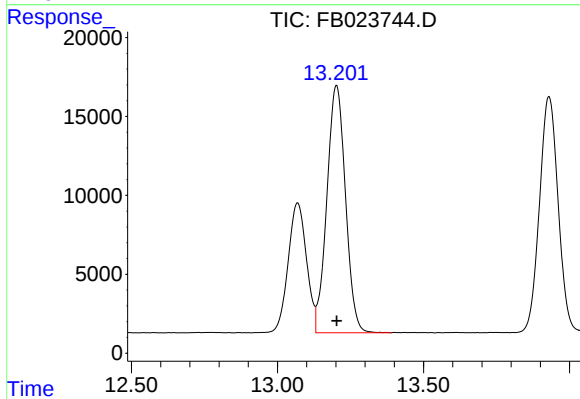

#8 m-Xylene


R.T.: 13.202 min
Delta R.T.: 0.000 min
Response: 694453
Conc: 19.45 ng/ml

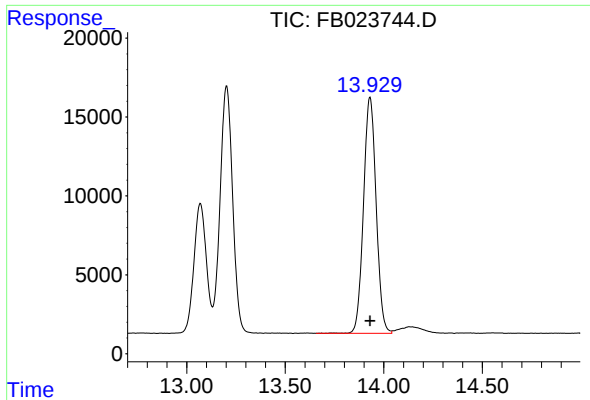

#9 O-Xylene

R.T.: 13.930 min
Delta R.T.: -0.001 min
Response: 665534
Conc: 19.30 ng/ml

Instrument :
FID_B
ClientSampleId :
TR-06-022720MS

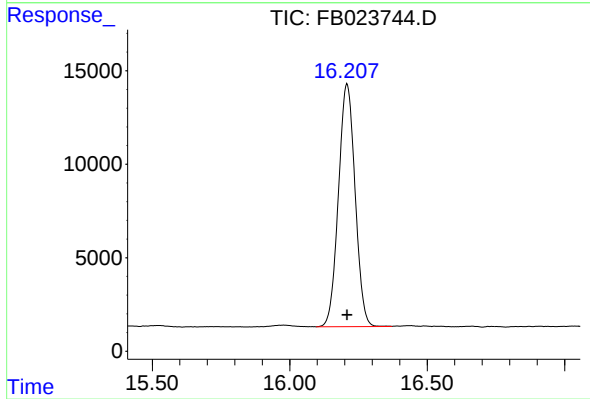

#10 1,2,4-Trimethylbenzene

R.T.: 16.209 min
Delta R.T.: 0.000 min
Response: 546592
Conc: 18.67 ng/ml