

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB030119\
 Data File : FB019996.D
 Signal(s) : FID2B.CH
 Acq On : 1 Mar 2019 15:55
 Operator : MJ/SJ
 Sample : K1665-03MSD
 Misc : 5.03g/5.00ml DI WATER
 ALS Vial : 11 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Mar 02 03:14:05 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030119.M
 Quant Title :
 QLast Update : Fri Mar 01 06:28:25 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.039	227901	20.337 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.895	528356	25.394 ng/ml
2) t 2,2,4-Trimethylpentane	7.653	485745	24.127 ng/ml
3) t n-Heptane	7.994	149291	8.004 ng/ml
4) t Benzene	8.133	195767	9.339 ng/ml
6) t Toluene	10.886	535027	28.231 ng/ml
7) t Ethylbenzene	13.338	209063	9.205 ng/ml
8) t m-Xylene	13.471	433368	18.482 ng/ml
9) t O-Xylene	14.203	425863	18.290 ng/ml
10) t 1,2,4-Trimethylbenzene	16.490	421092	18.289 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB030119\
Data File : FB019996.D
Signal(s) : FID2B.CH
Acq On : 1 Mar 2019 15:55
Operator : MJ/SJ
Sample : K1665-03MSD
Misc : 5.03g/5.00ml DI WATER
ALS Vial : 11 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Mar 02 03:14:05 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030119.M
Quant Title :
QLast Update : Fri Mar 01 06:28:25 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

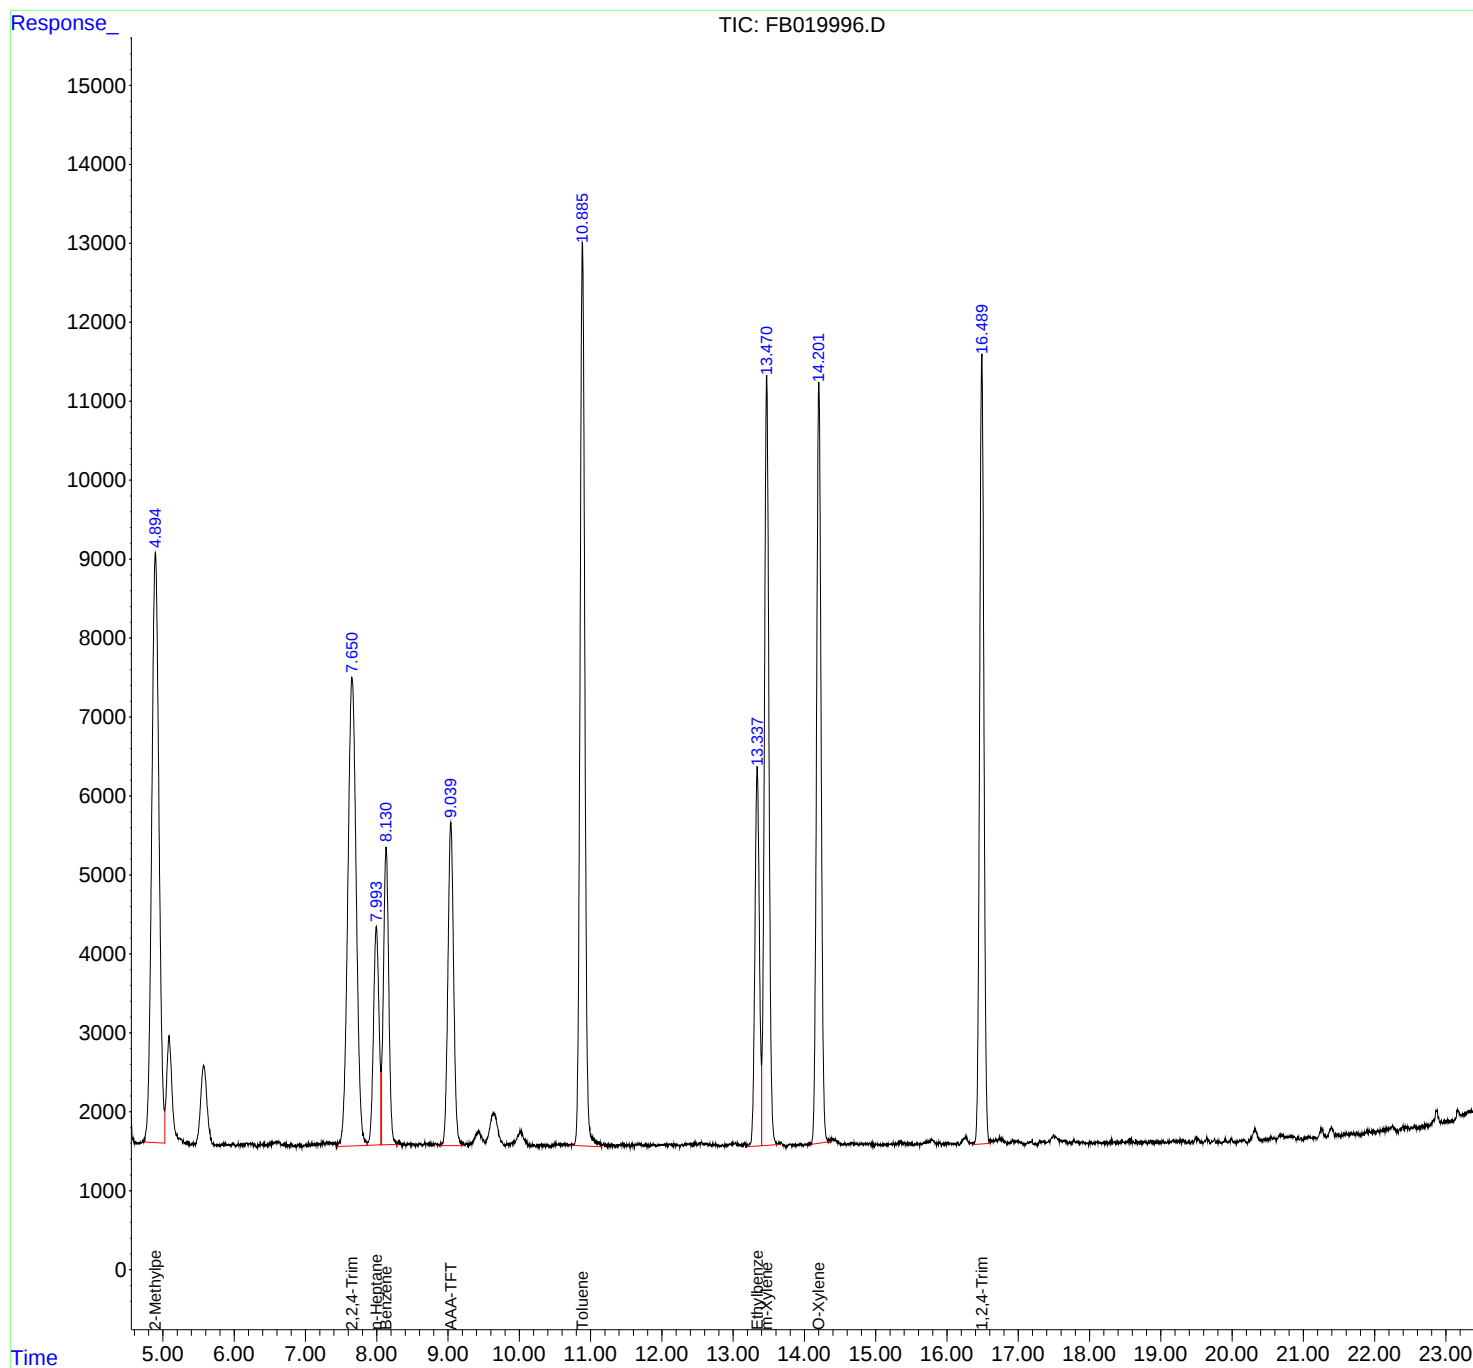

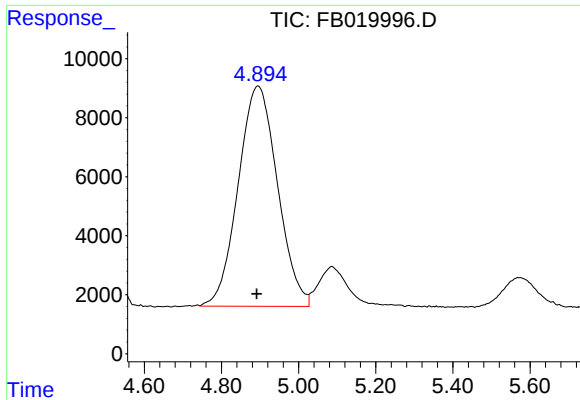


#1 2-Methylpentane

R.T.: 4.895 min
Delta R.T.: 0.004 min
Response: 528356
Conc: 25.39 ng/ml

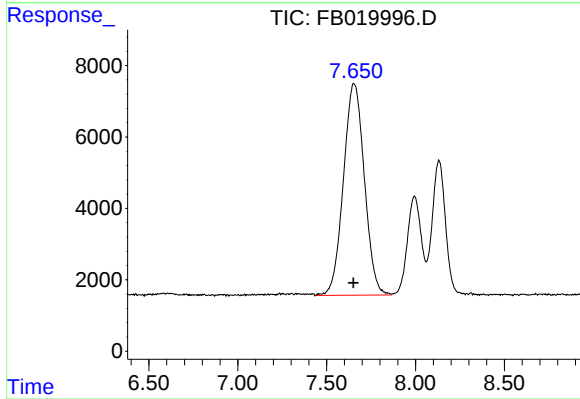


#2 2,2,4-Trimethylpentane

R.T.: 7.653 min
Delta R.T.: 0.002 min
Response: 485745
Conc: 24.13 ng/ml

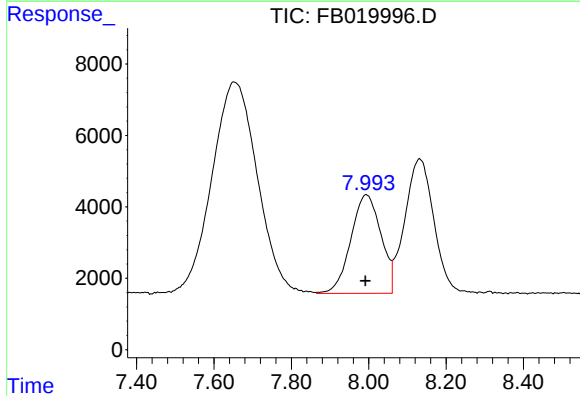


#3 n-Heptane

R.T.: 7.994 min
Delta R.T.: 0.003 min
Response: 149291
Conc: 8.00 ng/ml

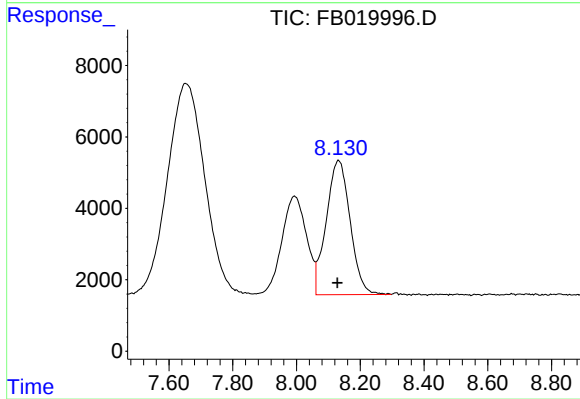


#4 Benzene

R.T.: 8.133 min
Delta R.T.: 0.004 min
Response: 195767
Conc: 9.34 ng/ml

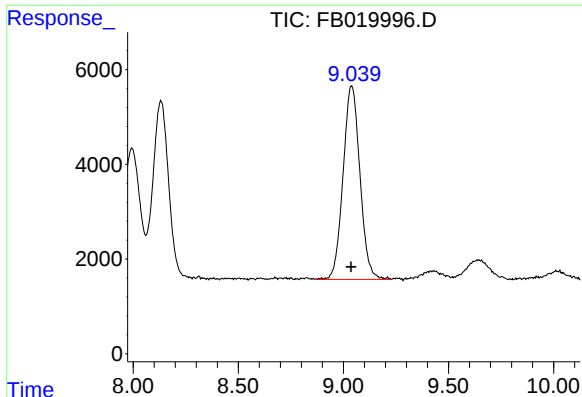


#5 AAA-TFT

R.T.: 9.039 min
Delta R.T.: 0.003 min
Response: 227901
Conc: 20.34 ng/ml

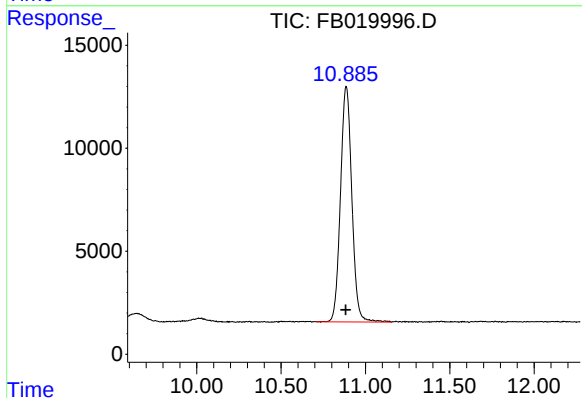


#6 Toluene

R.T.: 10.886 min
Delta R.T.: 0.003 min
Response: 535027
Conc: 28.23 ng/ml

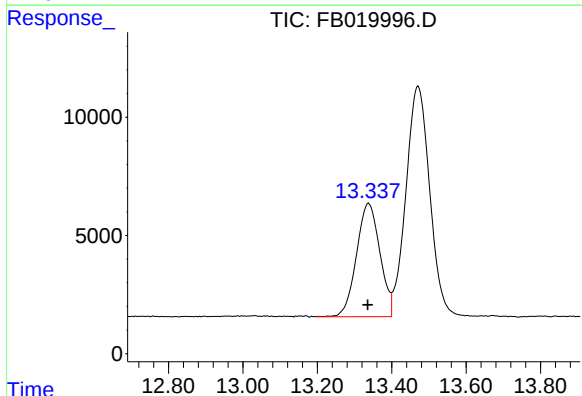


#7 Ethylbenzene

R.T.: 13.338 min
Delta R.T.: 0.002 min
Response: 209063
Conc: 9.20 ng/ml

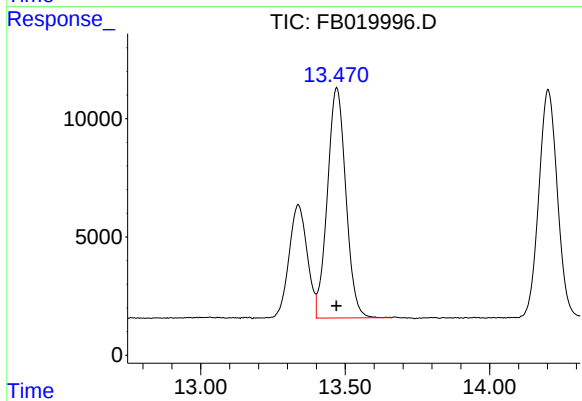


#8 m-Xylene

R.T.: 13.471 min
Delta R.T.: 0.002 min
Response: 433368
Conc: 18.48 ng/ml

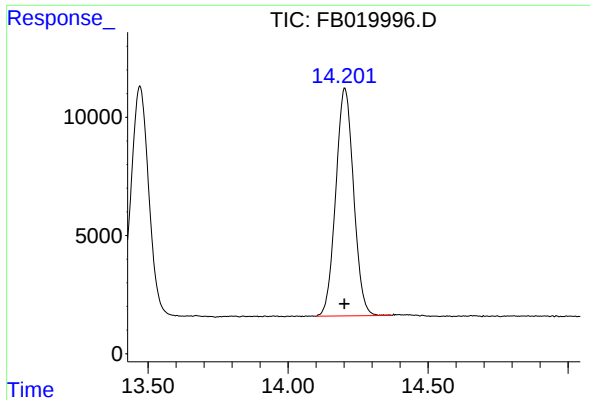

#9 O-Xylene

R.T.: 14.203 min
Delta R.T.: 0.002 min
Response: 425863
Conc: 18.29 ng/ml

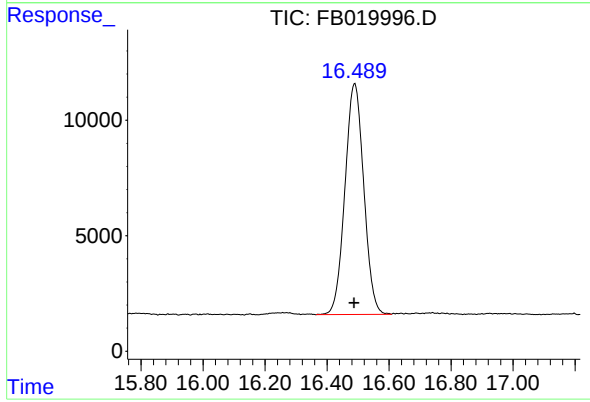

#10 1,2,4-Trimethylbenzene

R.T.: 16.490 min
Delta R.T.: 0.002 min
Response: 421092
Conc: 18.29 ng/ml