

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB030119\
 Data File : FB019985.D
 Signal(s) : FID2B.CH
 Acq On : 1 Mar 2019 6:39
 Operator : MJ/SJ
 Sample : FB030119GROICV
 Misc : 5.00g/5.00ml DI WATER
 ALS Vial : 42 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Mar 01 07:11:02 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030119.M
 Quant Title :
 QLast Update : Fri Mar 01 06:28:25 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.038	230701	20.587 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.894	630079	30.283 ng/ml
2) t 2,2,4-Trimethylpentane	7.652	608383	30.219 ng/ml
3) t n-Heptane	7.993	186985	10.025 ng/ml
4) t Benzene	8.131	206889	9.869 ng/ml
6) t Toluene	10.885	556692	29.374 ng/ml
7) t Ethylbenzene	13.337	221825	9.767 ng/ml
8) t m-Xylene	13.470	463705	19.776 ng/ml
9) t O-Xylene	14.202	455268	19.553 ng/ml
10) t 1,2,4-Trimethylbenzene	16.488	455042	19.764 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB030119\
Data File : FB019985.D
Signal(s) : FID2B.CH
Acq On : 1 Mar 2019 6:39
Operator : MJ/SJ
Sample : FB030119GROICV
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 42 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Mar 01 07:11:02 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030119.M
Quant Title :
QLast Update : Fri Mar 01 06:28:25 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

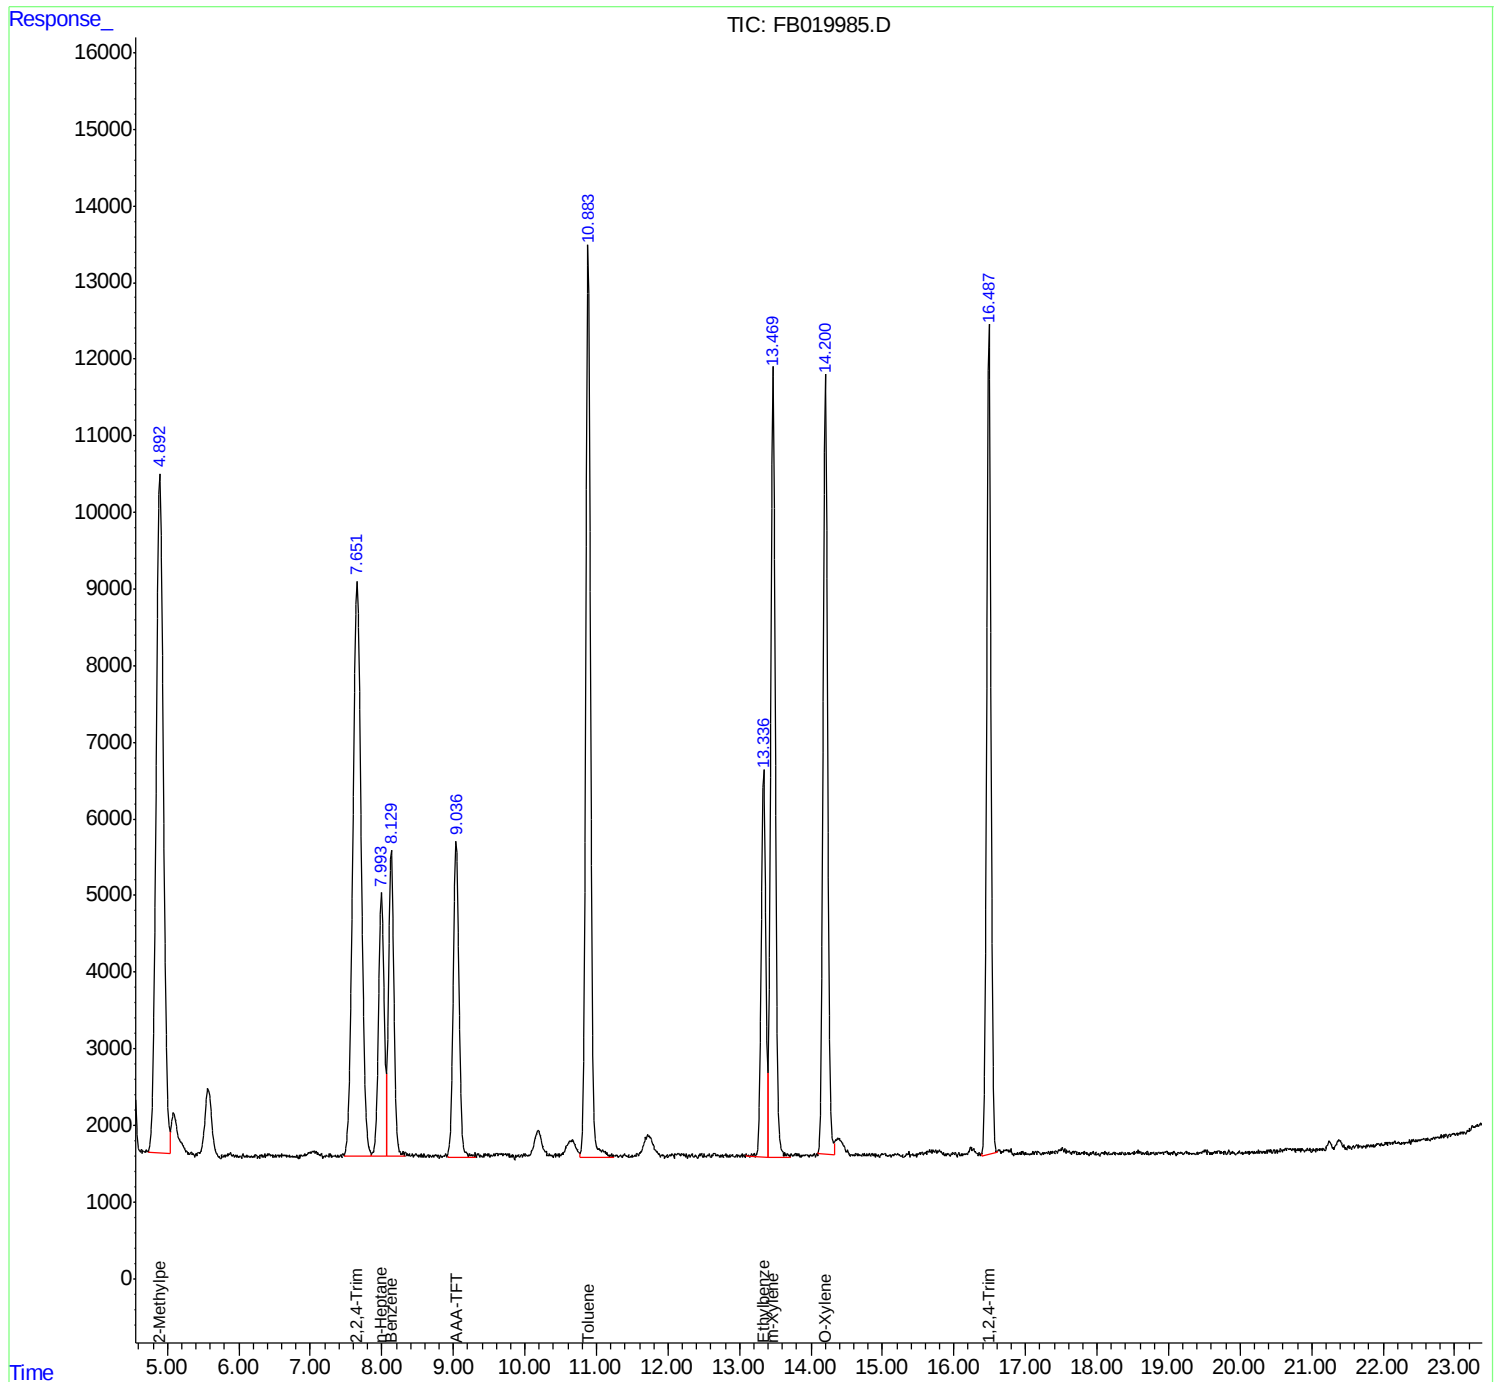

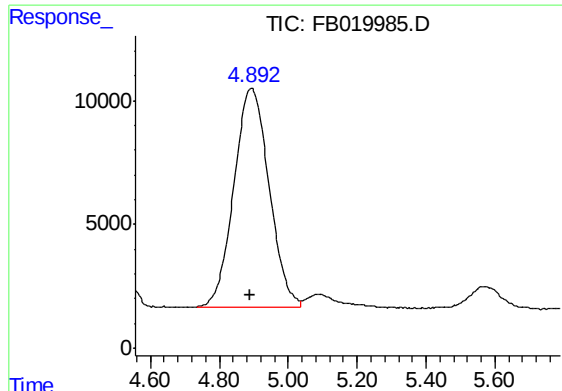


#1 2-Methylpentane

R.T.: 4.894 min
Delta R.T.: 0.003 min
Response: 630079
Conc: 30.28 ng/ml

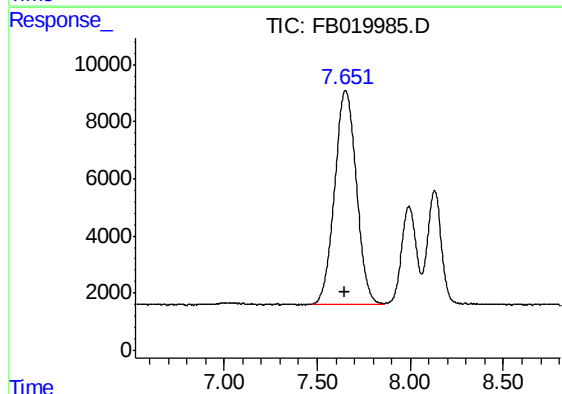


#2 2,2,4-Trimethylpentane

R.T.: 7.652 min
Delta R.T.: 0.000 min
Response: 608383
Conc: 30.22 ng/ml

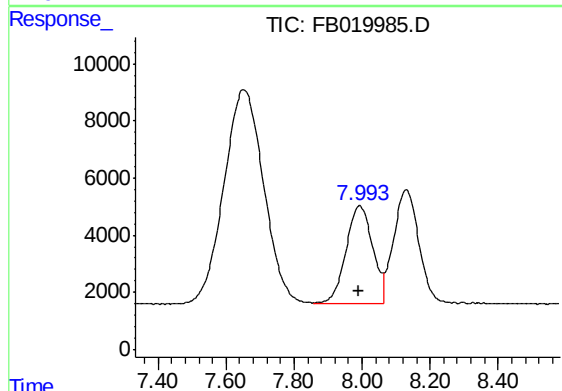


#3 n-Heptane

R.T.: 7.993 min
Delta R.T.: 0.002 min
Response: 186985
Conc: 10.03 ng/ml

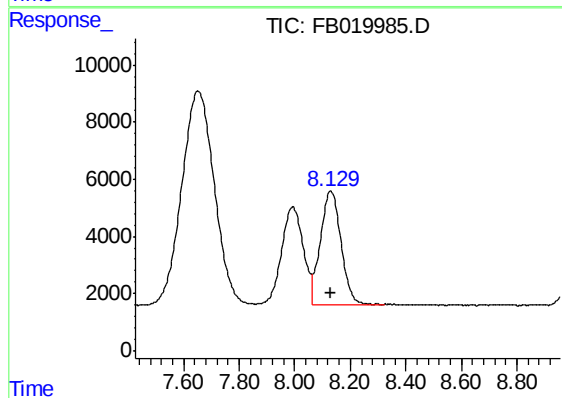


#4 Benzene

R.T.: 8.131 min
Delta R.T.: 0.002 min
Response: 206889
Conc: 9.87 ng/ml

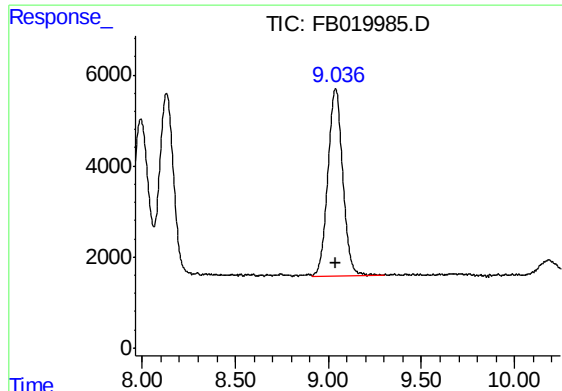


#5 AAA-TFT

R.T.: 9.038 min
Delta R.T.: 0.001 min
Response: 230701
Conc: 20.59 ng/ml

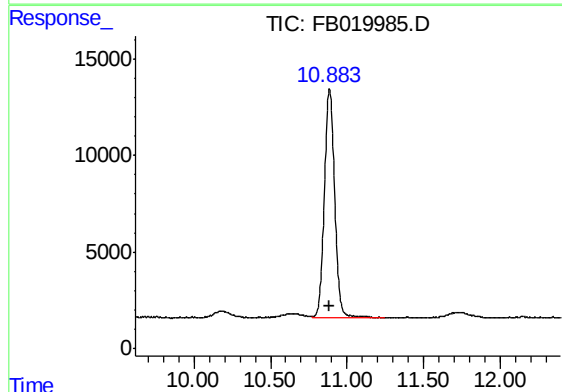


#6 Toluene

R.T.: 10.885 min
Delta R.T.: 0.000 min
Response: 556692
Conc: 29.37 ng/ml

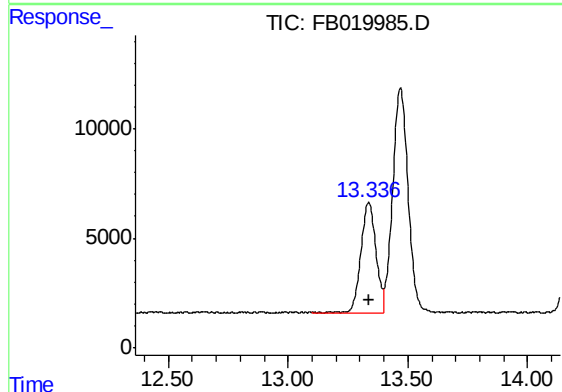


#7 Ethylbenzene

R.T.: 13.337 min
Delta R.T.: 0.001 min
Response: 221825
Conc: 9.77 ng/ml

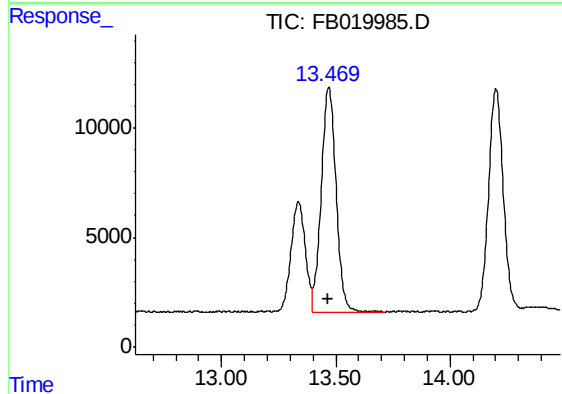


#8 m-Xylene

R.T.: 13.470 min
Delta R.T.: 0.000 min
Response: 463705
Conc: 19.78 ng/ml

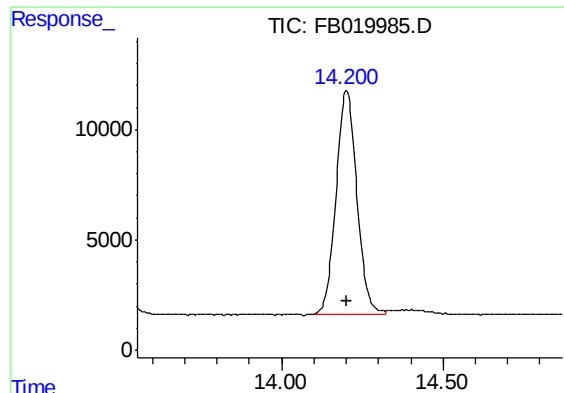

#9 O-Xylene

R.T.: 14.202 min
Delta R.T.: 0.000 min
Response: 455268
Conc: 19.55 ng/ml

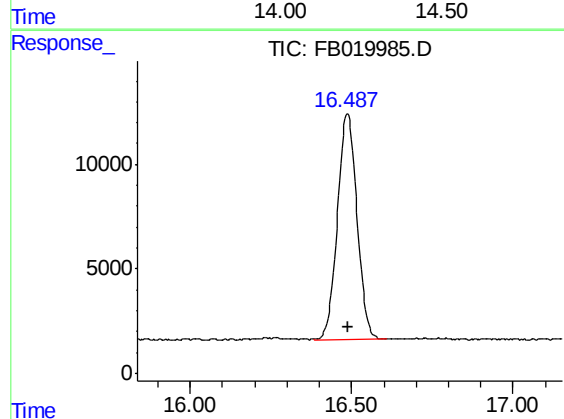

#10 1,2,4-Trimethylbenzene

R.T.: 16.488 min
Delta R.T.: 0.000 min
Response: 455042
Conc: 19.76 ng/ml