

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB030119\
 Data File : FB019990.D
 Signal(s) : FID2B.CH
 Acq On : 1 Mar 2019 12:42
 Operator : MJ/SJ
 Sample : K1560-01
 Misc : 5.00g/5.00ml DI WATER(1 PPB LOD)
 ALS Vial : 5 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Mar 02 04:02:22 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030119.M
 Quant Title :
 QLast Update : Fri Mar 01 06:28:25 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.039	219082	19.550 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.902	21463	1.032 ng/ml
2) t 2,2,4-Trimethylpentane	7.660	25672	1.275 ng/ml
3) t n-Heptane	7.994	7842	0.420 ng/ml
4) t Benzene	8.135	9274	0.442 ng/ml
6) t Toluene	10.890	29373	1.550 ng/ml
7) t Ethylbenzene	13.334	10140	0.446 ng/ml
8) t m-Xylene	13.473	21294	0.908 ng/ml
9) t O-Xylene	14.200	18423	0.791 ng/ml
10) t 1,2,4-Trimethylbenzene	16.489	22340	0.970 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB030119\
Data File : FB019990.D
Signal(s) : FID2B.CH
Acq On : 1 Mar 2019 12:42
Operator : MJ/SJ
Sample : K1560-01
Misc : 5.00g/5.00ml DI WATER(1 PPB LOD)
ALS Vial : 5 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Mar 02 04:02:22 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030119.M
Quant Title :
QLast Update : Fri Mar 01 06:28:25 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

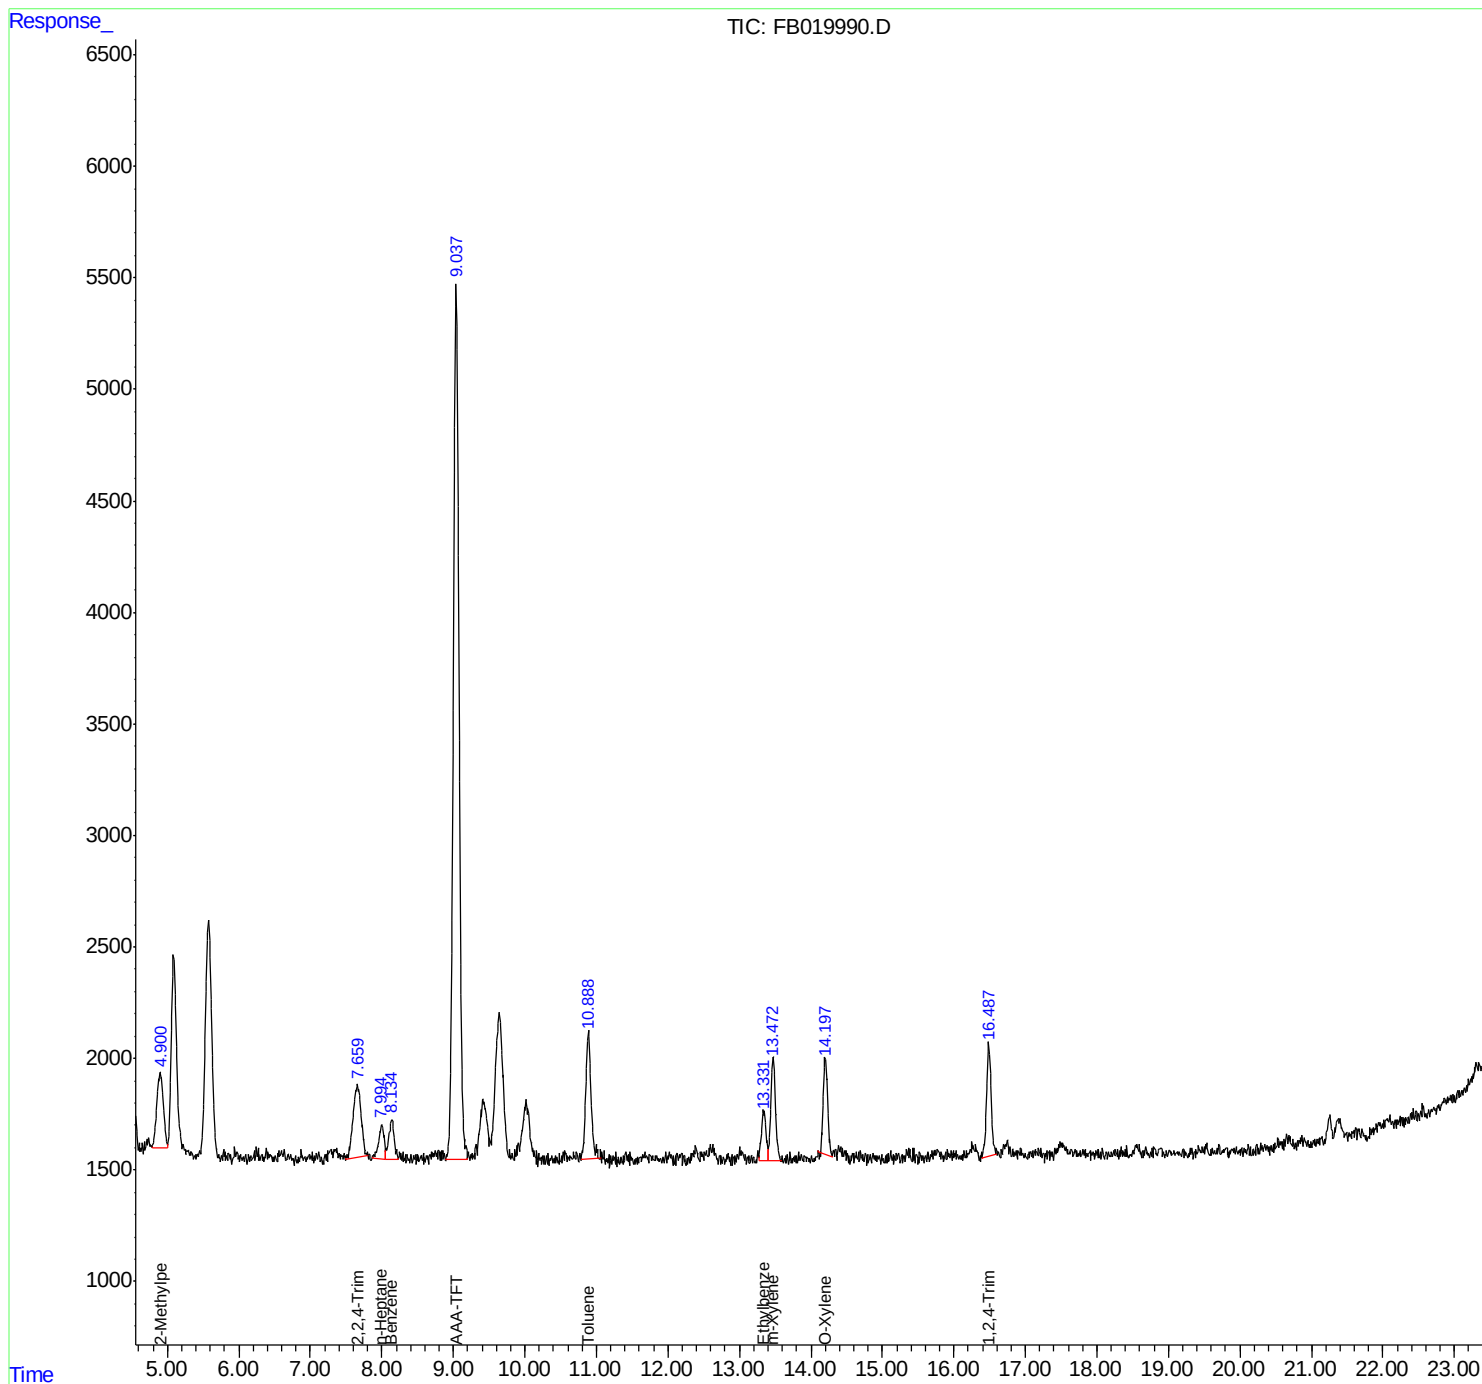

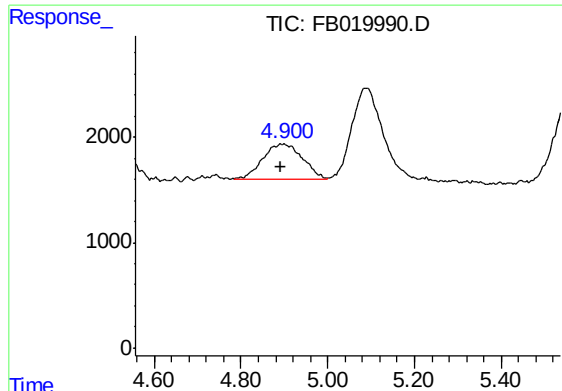


#1 2-Methylpentane

R.T.: 4.902 min
Delta R.T.: 0.011 min
Response: 21463
Conc: 1.03 ng/ml

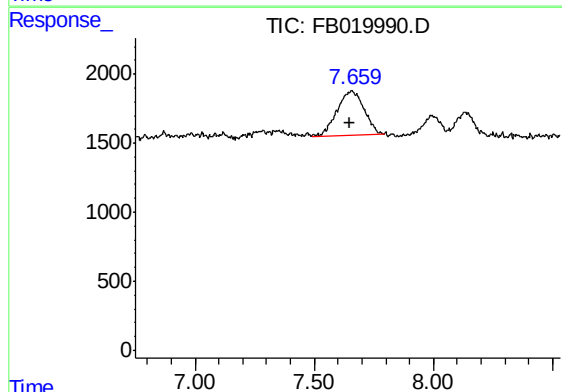


#2 2,2,4-Trimethylpentane

R.T.: 7.660 min
Delta R.T.: 0.009 min
Response: 25672
Conc: 1.28 ng/ml

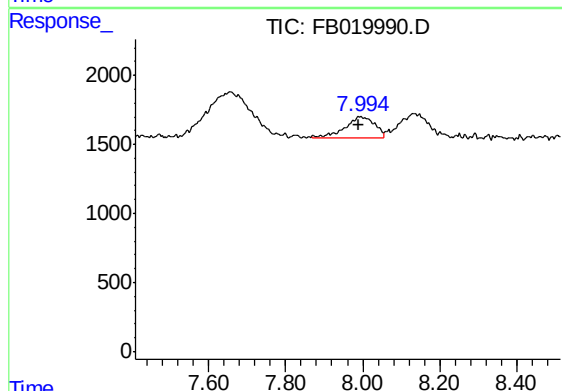


#3 n-Heptane

R.T.: 7.994 min
Delta R.T.: 0.003 min
Response: 7842
Conc: 0.42 ng/ml

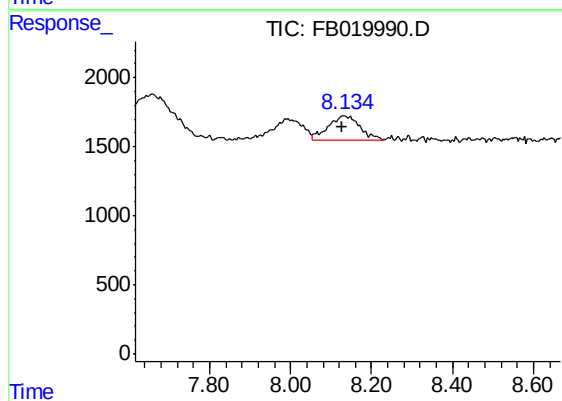


#4 Benzene

R.T.: 8.135 min
Delta R.T.: 0.006 min
Response: 9274
Conc: 0.44 ng/ml

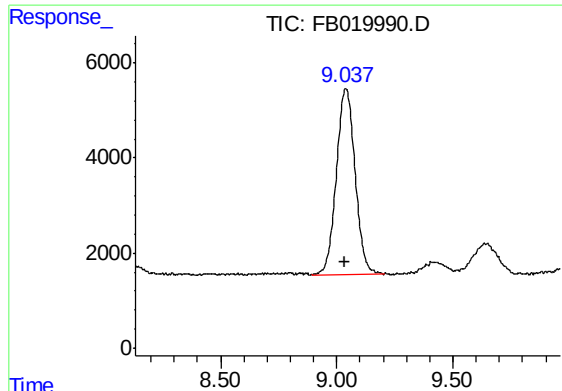


#5 AAA-TFT

R.T.: 9.039 min
Delta R.T.: 0.002 min
Response: 219082
Conc: 19.55 ng/ml

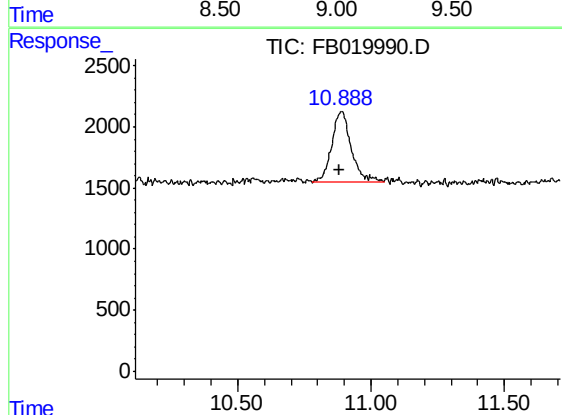


#6 Toluene

R.T.: 10.890 min
Delta R.T.: 0.006 min
Response: 29373
Conc: 1.55 ng/ml

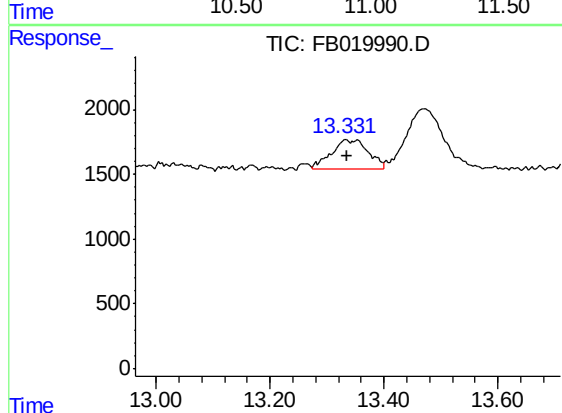


#7 Ethylbenzene

R.T.: 13.334 min
Delta R.T.: -0.002 min
Response: 10140
Conc: 0.45 ng/ml

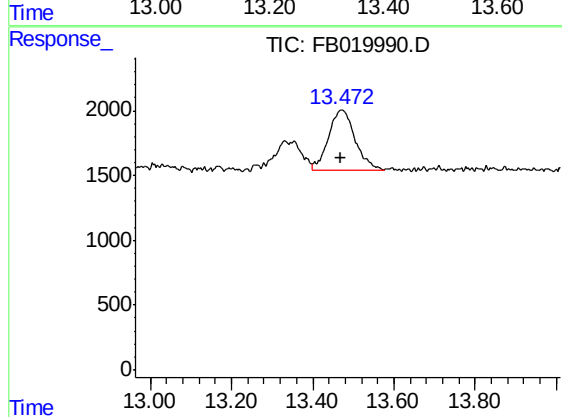


#8 m-Xylene

R.T.: 13.473 min
Delta R.T.: 0.004 min
Response: 21294
Conc: 0.91 ng/ml

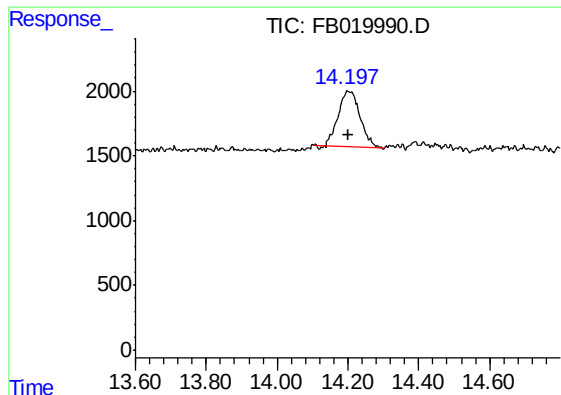

#9 O-Xylene

R.T.: 14.200 min
Delta R.T.: 0.000 min
Response: 18423
Conc: 0.79 ng/ml

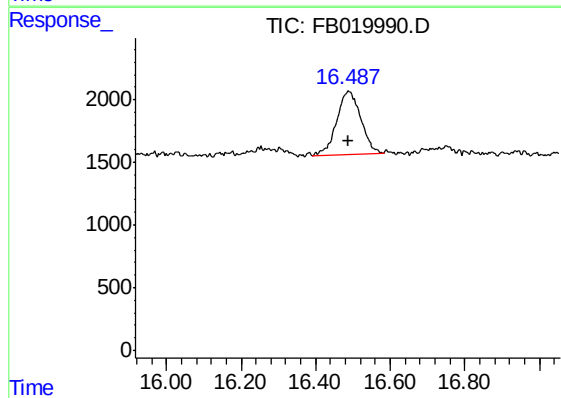

#10 1,2,4-Trimethylbenzene

R.T.: 16.489 min
Delta R.T.: 0.002 min
Response: 22340
Conc: 0.97 ng/ml