

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB030220\
 Data File : FB023759.D
 Signal(s) : FID2B.CH
 Acq On : 2 Mar 2020 9:24
 Operator : DD/AJ
 Sample : VBF0302S1
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Mar 03 00:41:43 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB020620.M
 Quant Title :
 QLast Update : Thu Feb 06 11:13:47 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.795	407439	20.012 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.681	14095	0.468 ng/ml
2) t 2,2,4-Trimethylpentane	7.413	5646	0.173 ng/ml
3) t n-Heptane	7.751	2106	0.065 ng/ml
4) t Benzene	7.885	4287	0.105 ng/ml
6) t Toluene	10.618	13062	0.329 ng/ml
7) t Ethylbenzene	13.056	1965	0.053 ng/ml
8) t m-Xylene	13.203	7437	0.208 ng/ml
9) t O-Xylene	13.925	12774	0.370 ng/ml
10) t 1,2,4-Trimethylbenzene	16.208	9620	0.329 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB030220\
Data File : FB023759.D
Signal(s) : FID2B.CH
Acq On : 2 Mar 2020 9:24
Operator : DD/AJ
Sample : VBF0302S1
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Mar 03 00:41:43 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB020620.M
Quant Title :
QLast Update : Thu Feb 06 11:13:47 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

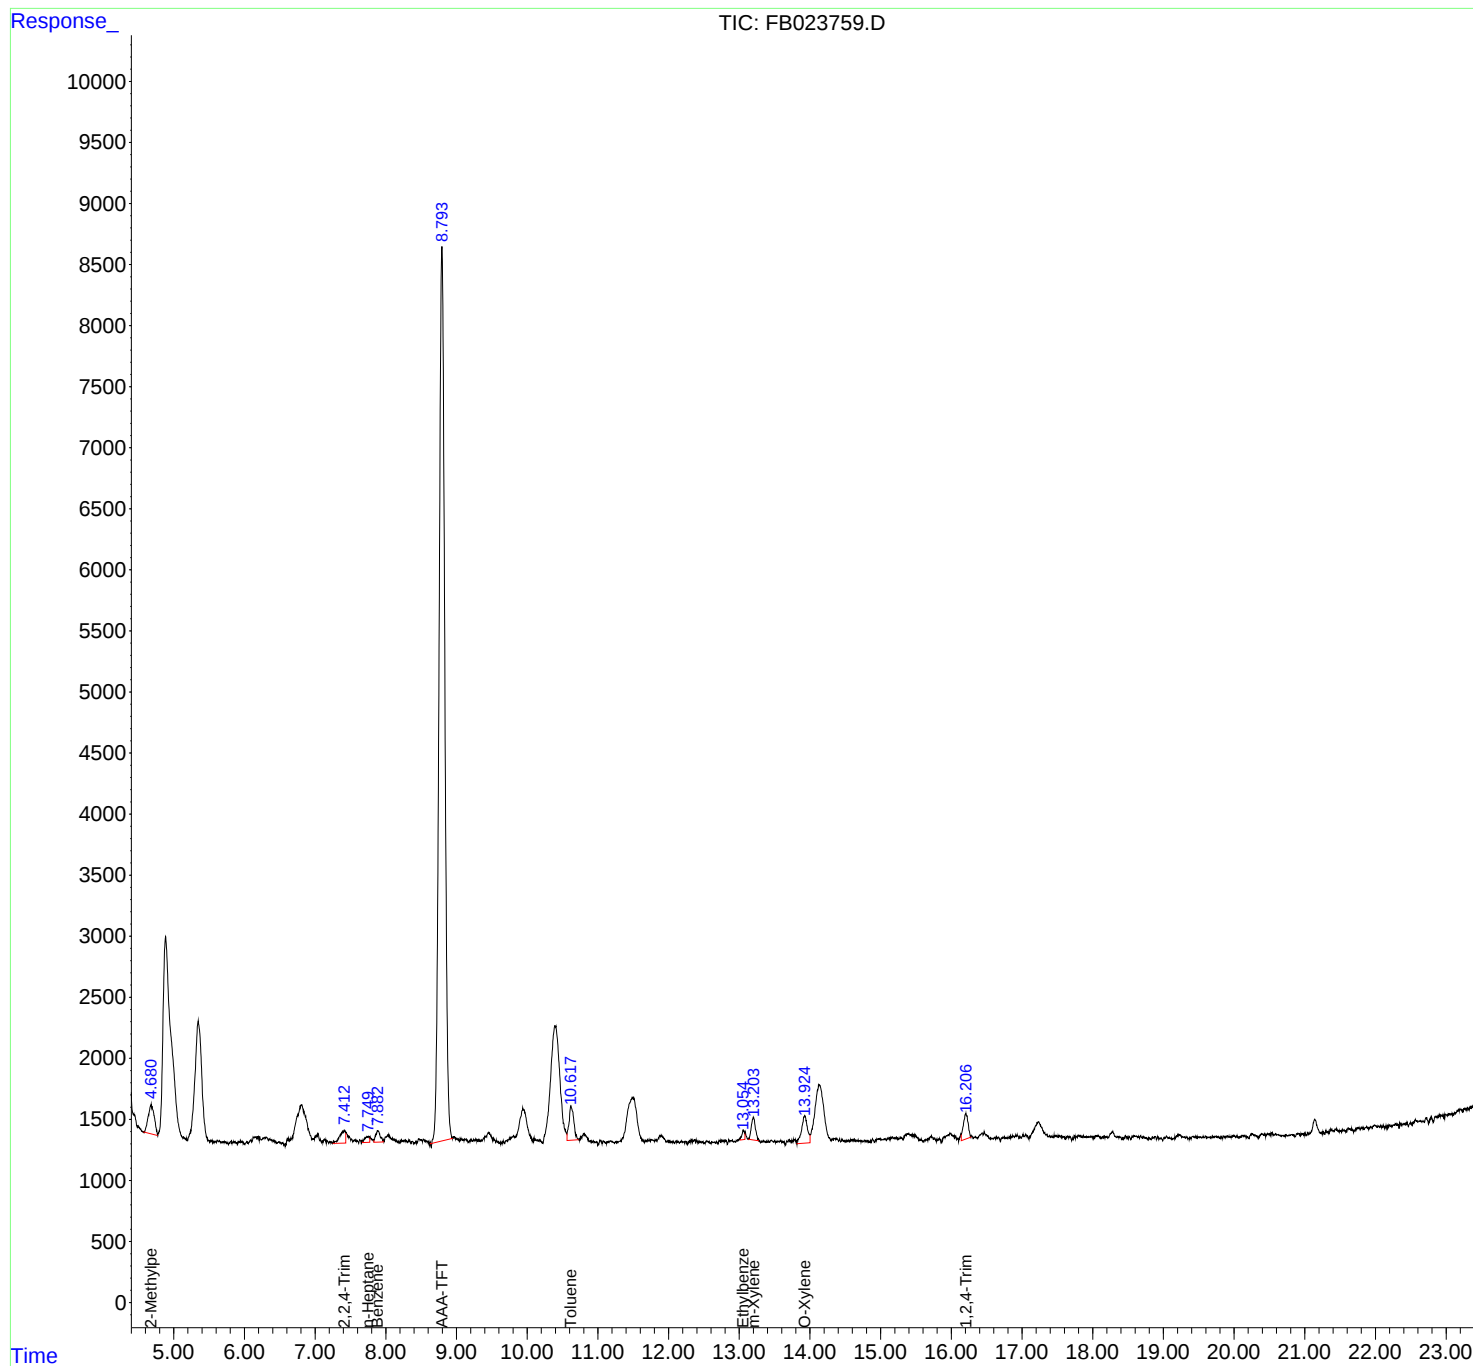


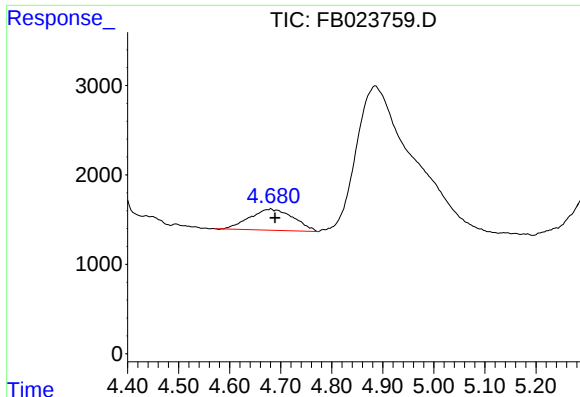

#1 2-Methylpentane


R.T.: 4.681 min
Delta R.T.: -0.008 min
Response: 14095
Conc: 0.47 ng/ml

Instrument :
FID_B
ClientSampleId :

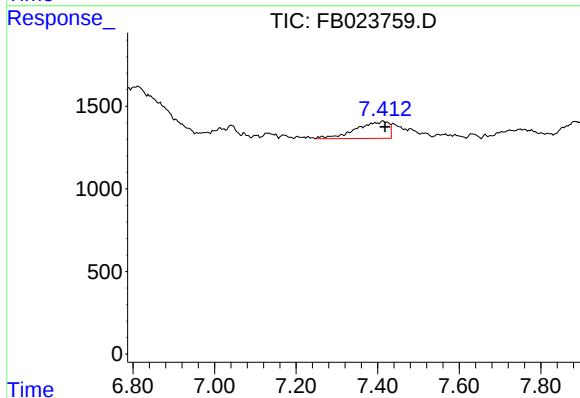


#2 2,2,4-Trimethylpentane

R.T.: 7.413 min
Delta R.T.: -0.004 min
Response: 5646
Conc: 0.17 ng/ml

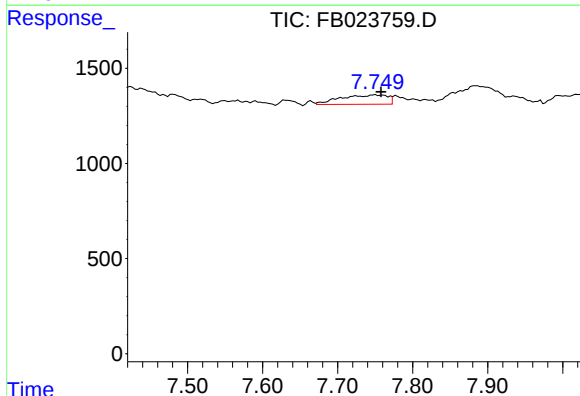


#3 n-Heptane

R.T.: 7.751 min
Delta R.T.: -0.007 min
Response: 2106
Conc: 0.07 ng/ml

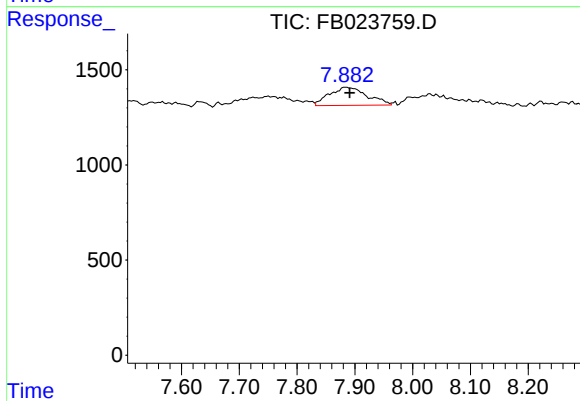

#4 Benzene


R.T.: 7.885 min
Delta R.T.: -0.007 min
Response: 4287
Conc: 0.10 ng/ml

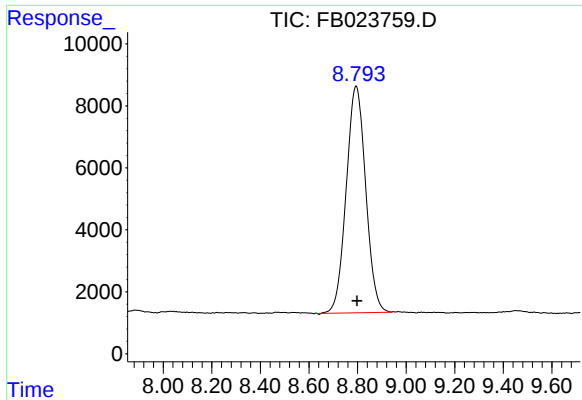

#5 AAA-TFT


R.T.: 8.795 min
Delta R.T.: -0.004 min
Response: 407439
Conc: 20.01 ng/ml

Instrument :
FID_B
ClientSampleId :

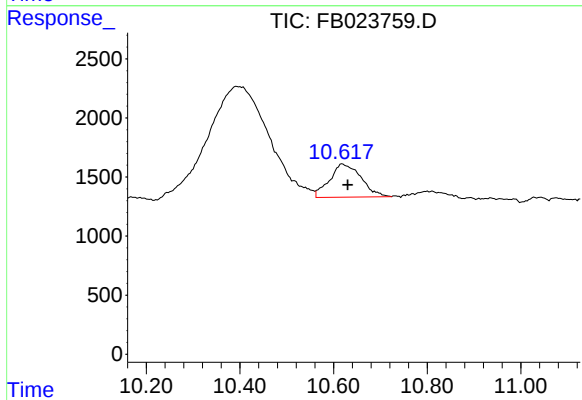


#6 Toluene

R.T.: 10.618 min
Delta R.T.: -0.012 min
Response: 13062
Conc: 0.33 ng/ml

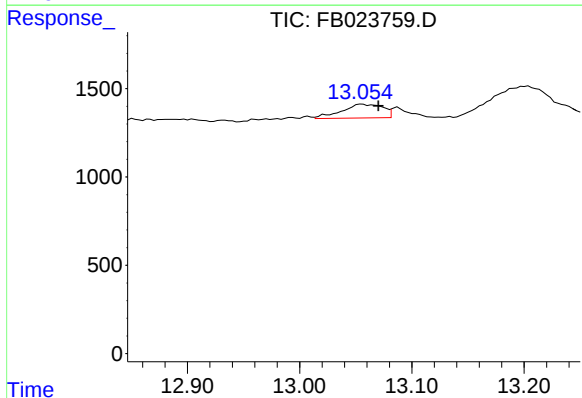


#7 Ethylbenzene

R.T.: 13.056 min
Delta R.T.: -0.014 min
Response: 1965
Conc: 0.05 ng/ml

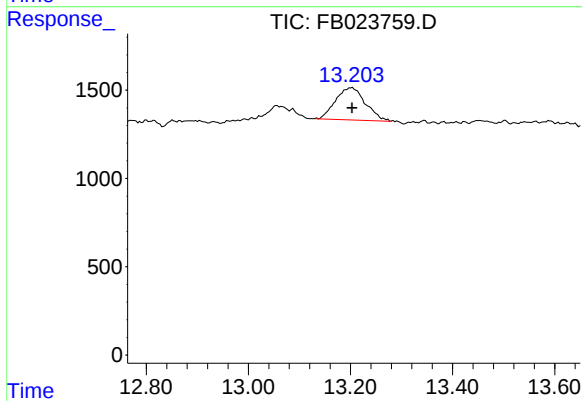

#8 m-Xylene


R.T.: 13.203 min
Delta R.T.: 0.000 min
Response: 7437
Conc: 0.21 ng/ml

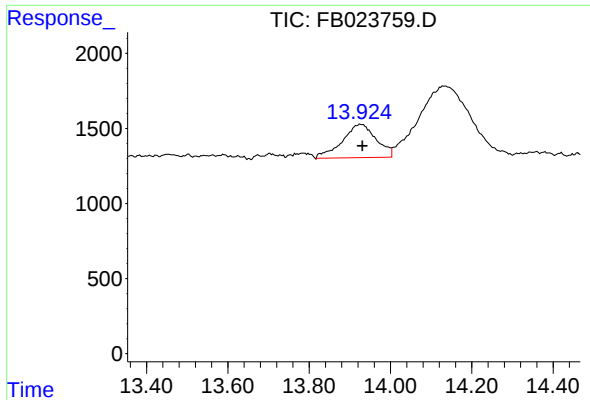

#9 O-Xylene

R.T.: 13.925 min
Delta R.T.: -0.006 min
Response: 12774
Conc: 0.37 ng/ml

Instrument :
FID_B
ClientSampleId :

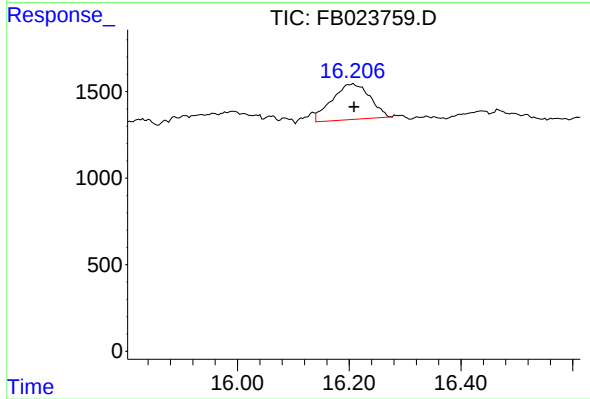

#10 1,2,4-Trimethylbenzene

R.T.: 16.208 min
Delta R.T.: -0.001 min
Response: 9620
Conc: 0.33 ng/ml