

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB030220\
 Data File : FB023761.D
 Signal(s) : FID2B.CH
 Acq On : 2 Mar 2020 10:44
 Operator : DD/AJ
 Sample : L1369-02
 Misc : 5.04g/5.00ml DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Mar 03 00:41:54 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB020620.M
 Quant Title :
 QLast Update : Thu Feb 06 11:13:47 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.795	415908	20.428 ng/ml
Target Compounds				
6) t	Toluene	10.617	1956	0.049 ng/ml
7) t	Ethylbenzene	13.069	3399	0.091 ng/ml
8) t	m-Xylene	13.196	7344	0.206 ng/ml
9) t	O-Xylene	13.932	10633	0.308 ng/ml
10) t	1,2,4-Trimethylbenzene	16.208	24599	0.840 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB030220\
Data File : FB023761.D
Signal(s) : FID2B.CH
Acq On : 2 Mar 2020 10:44
Operator : DD/AJ
Sample : L1369-02
Misc : 5.04g/5.00ml DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Mar 03 00:41:54 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB020620.M
Quant Title :
QLast Update : Thu Feb 06 11:13:47 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

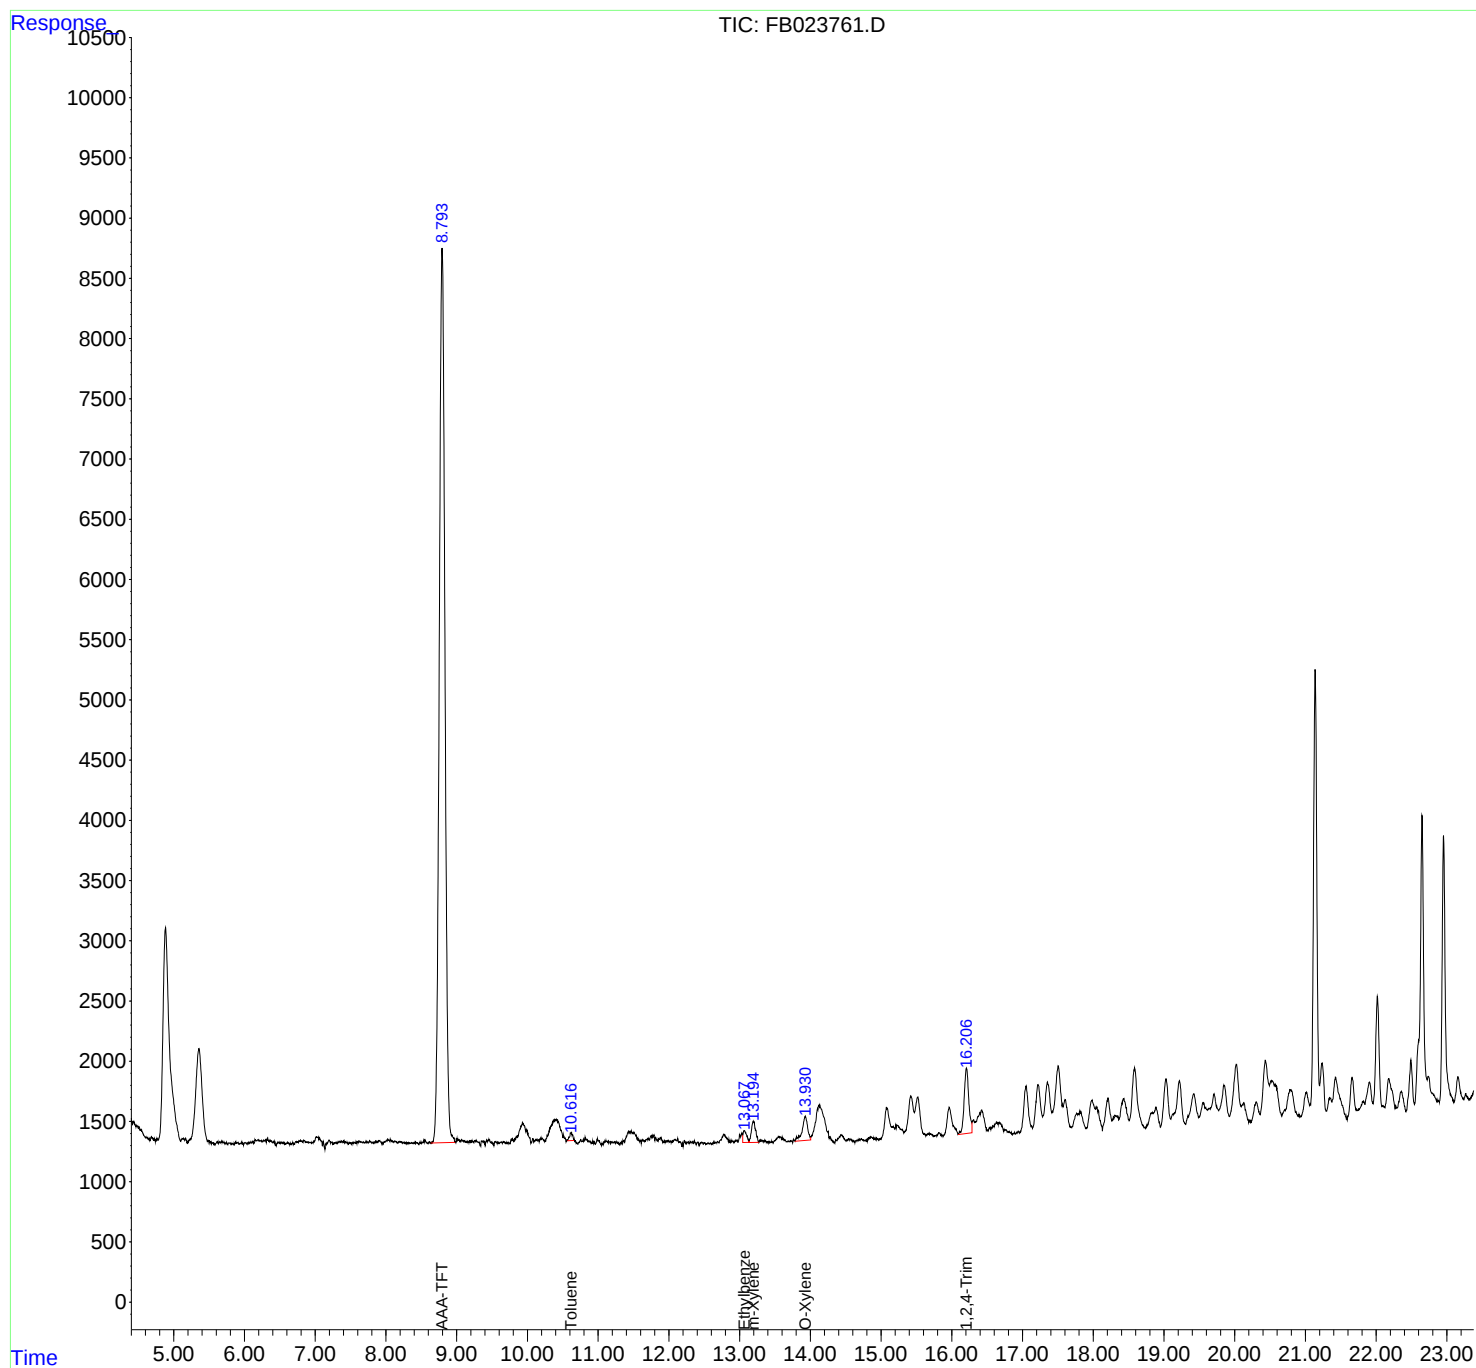


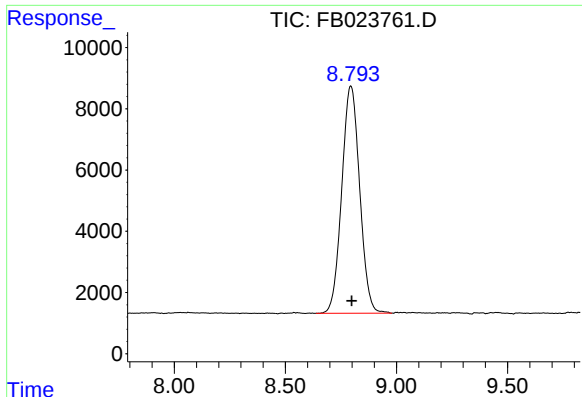

#5 AAA-TFT


R.T.: 8.795 min
Delta R.T.: -0.004 min
Response: 415908
Conc: 20.43 ng/ml

Instrument :
FID_B
ClientSampleId :

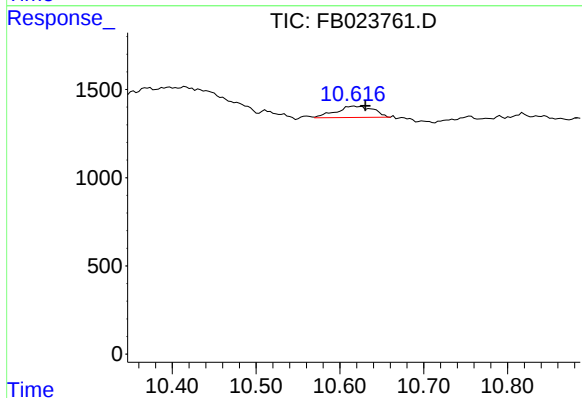


#6 Toluene

R.T.: 10.617 min
Delta R.T.: -0.013 min
Response: 1956
Conc: 0.05 ng/ml

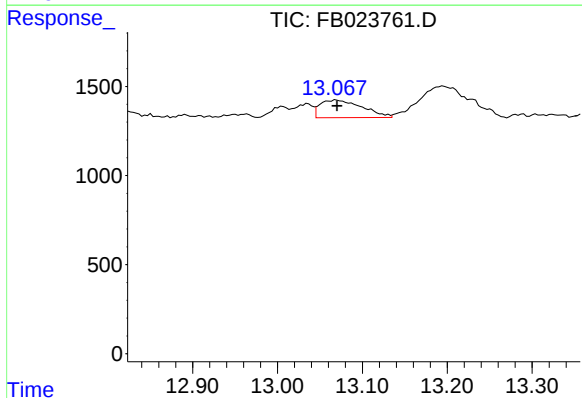


#7 Ethylbenzene

R.T.: 13.069 min
Delta R.T.: -0.001 min
Response: 3399
Conc: 0.09 ng/ml

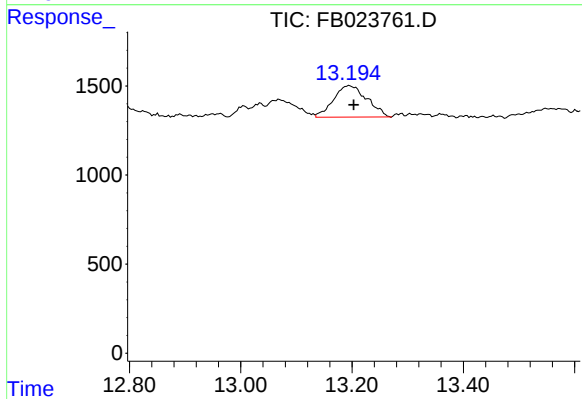

#8 m-Xylene


R.T.: 13.196 min
Delta R.T.: -0.008 min
Response: 7344
Conc: 0.21 ng/ml

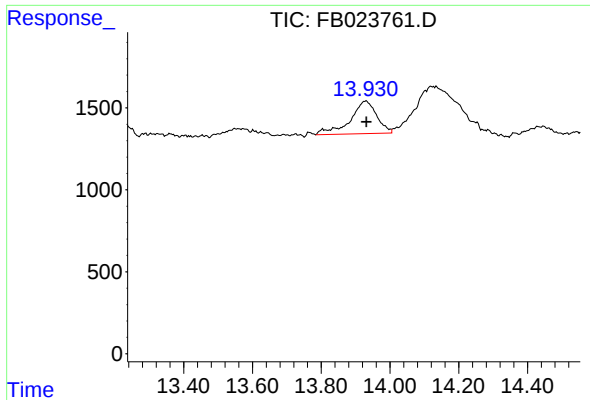

#9 O-Xylene

R.T.: 13.932 min
Delta R.T.: 0.000 min
Response: 10633
Conc: 0.31 ng/ml

Instrument :
FID_B
ClientSampleId :

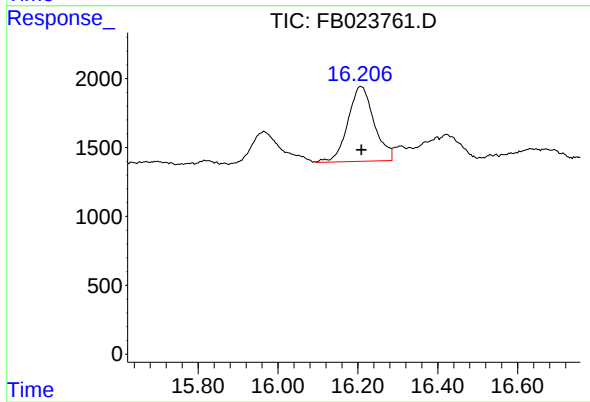

#10 1,2,4-Trimethylbenzene

R.T.: 16.208 min
Delta R.T.: -0.001 min
Response: 24599
Conc: 0.84 ng/ml