

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB030220\
 Data File : FB023764.D
 Signal(s) : FID2B.CH
 Acq On : 2 Mar 2020 12:14
 Operator : DD/AJ
 Sample : L1372-07MS
 Misc : 5.06g/5.00ml DI WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Mar 03 00:42:09 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB020620.M
 Quant Title :
 QLast Update : Thu Feb 06 11:13:47 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.798	448876	22.047 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.691	789034	26.222 ng/ml
2) t 2,2,4-Trimethylpentane	7.417	890159	27.279 ng/ml
3) t n-Heptane	7.757	277073	8.612 ng/ml
4) t Benzene	7.893	405569	9.916 ng/ml
6) t Toluene	10.630	1141526	28.758 ng/ml
7) t Ethylbenzene	13.070	350079	9.417 ng/ml
8) t m-Xylene	13.203	663386	18.576 ng/ml
9) t O-Xylene	13.931	650211	18.852 ng/ml
10) t 1,2,4-Trimethylbenzene	16.209	527587	18.020 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB030220\
Data File : FB023764.D
Signal(s) : FID2B.CH
Acq On : 2 Mar 2020 12:14
Operator : DD/AJ
Sample : L1372-07MS
Misc : 5.06g/5.00ml DI WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Mar 03 00:42:09 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB020620.M
Quant Title :
QLast Update : Thu Feb 06 11:13:47 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

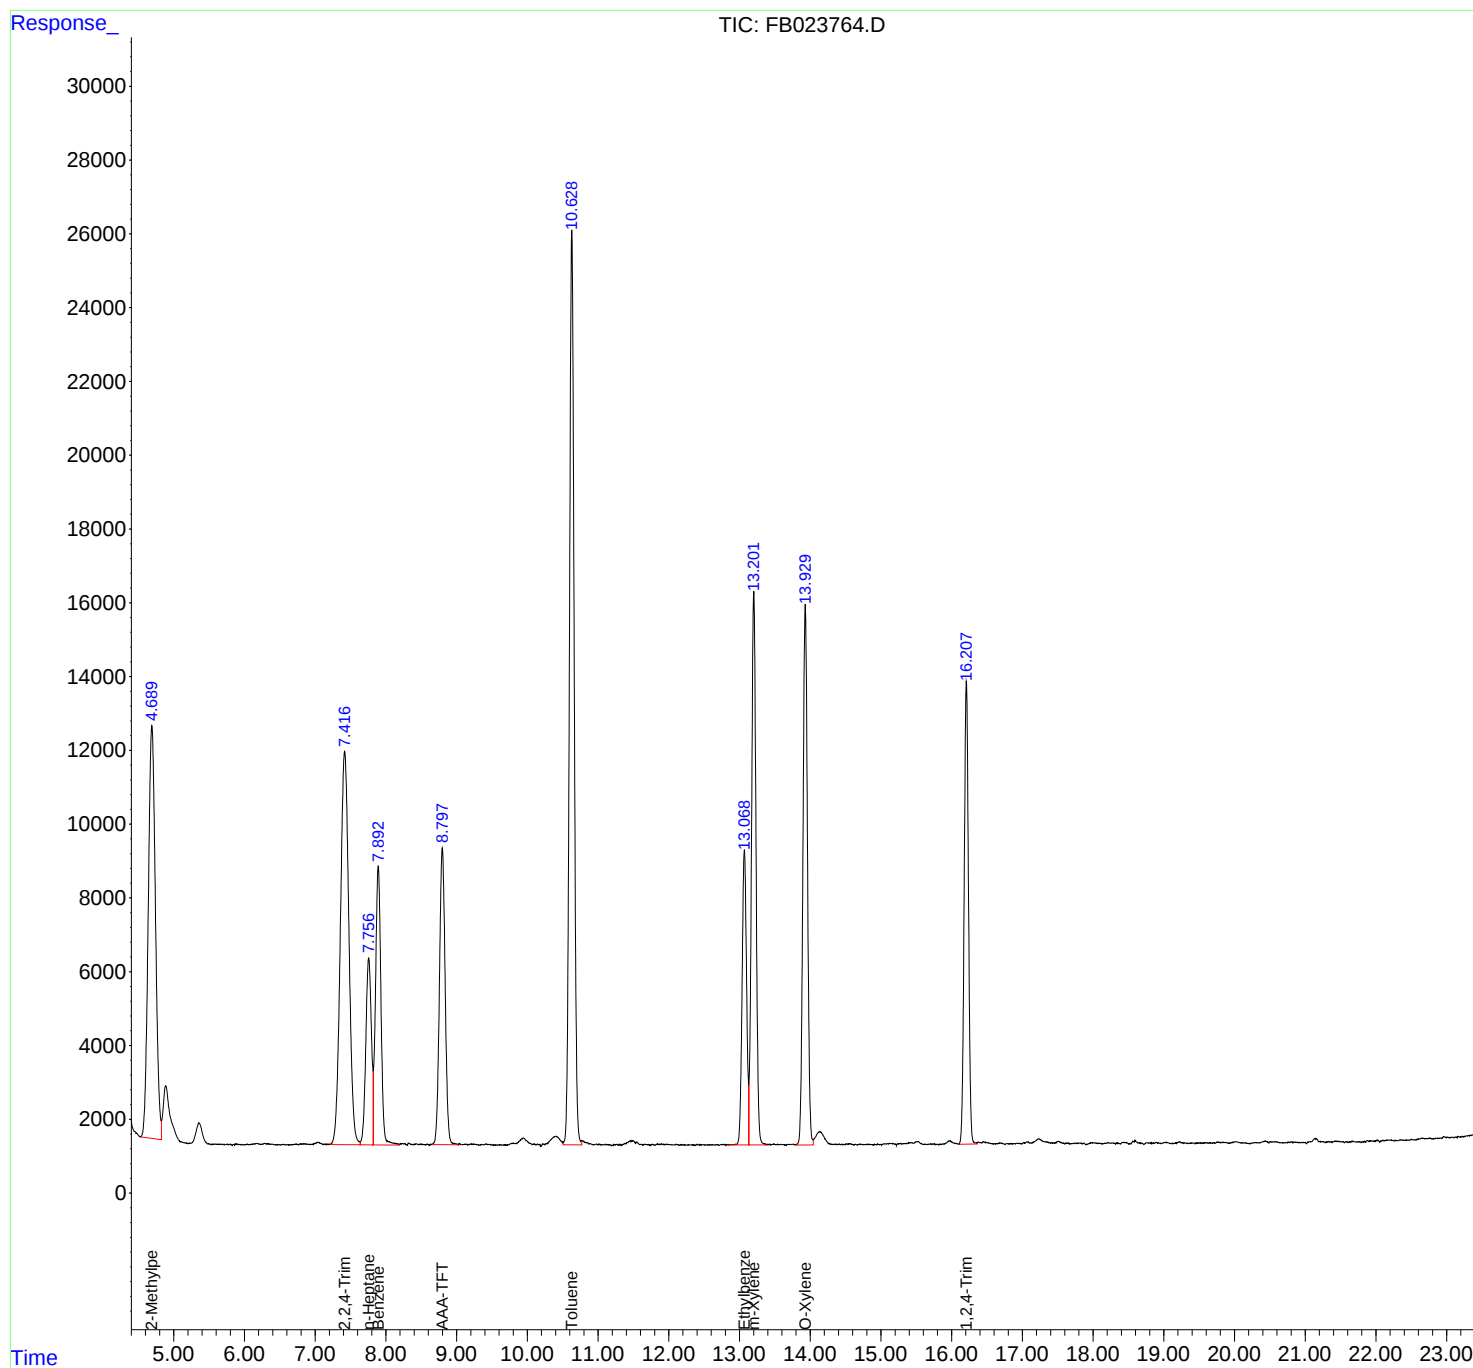


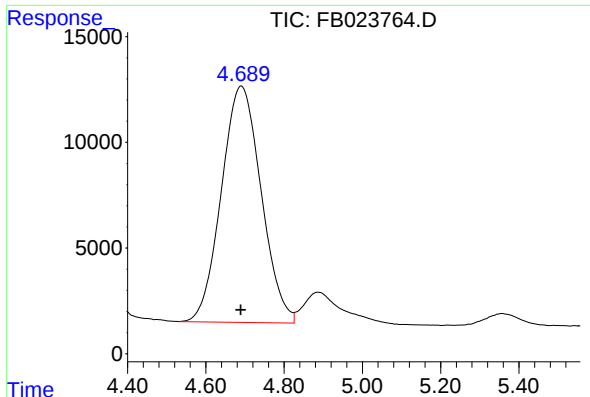

#1 2-Methylpentane


R.T.: 4.691 min
Delta R.T.: 0.002 min
Response: 789034
Conc: 26.22 ng/ml

Instrument :
FID_B
ClientSampleId :

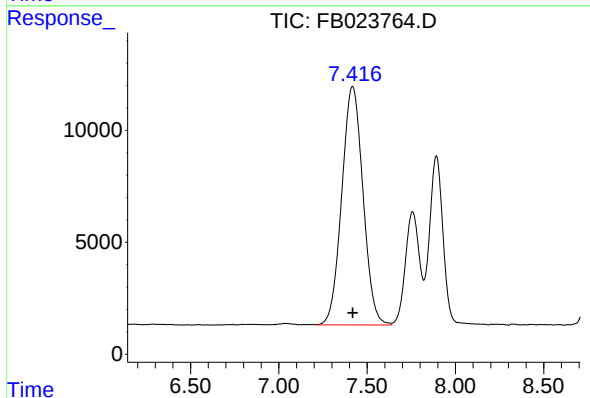


#2 2,2,4-Trimethylpentane

R.T.: 7.417 min
Delta R.T.: 0.000 min
Response: 890159
Conc: 27.28 ng/ml

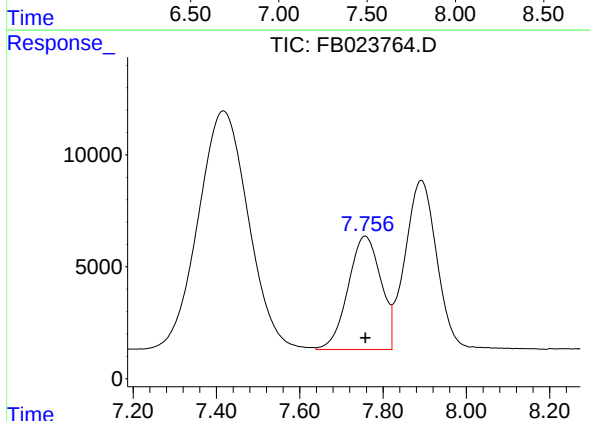


#3 n-Heptane

R.T.: 7.757 min
Delta R.T.: 0.000 min
Response: 277073
Conc: 8.61 ng/ml

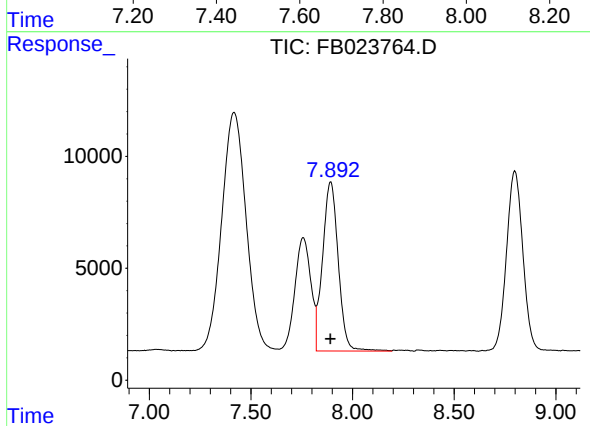

#4 Benzene


R.T.: 7.893 min
Delta R.T.: 0.001 min
Response: 405569
Conc: 9.92 ng/ml

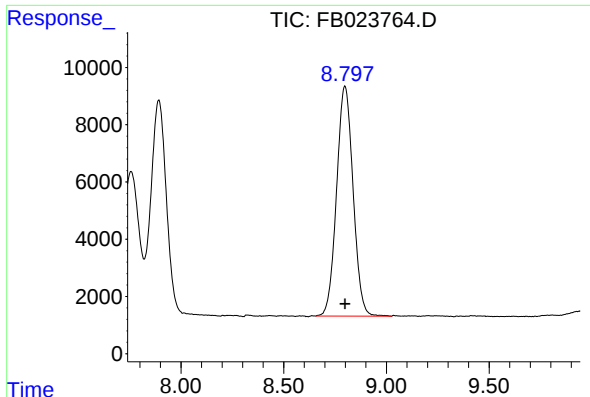

#5 AAA-TFT


R.T.: 8.798 min
Delta R.T.: 0.000 min
Response: 448876
Conc: 22.05 ng/ml

Instrument :
FID_B
ClientSampleId :

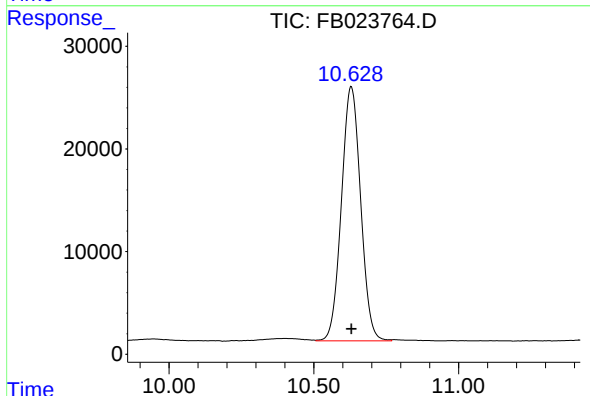


#6 Toluene

R.T.: 10.630 min
Delta R.T.: 0.000 min
Response: 1141526
Conc: 28.76 ng/ml

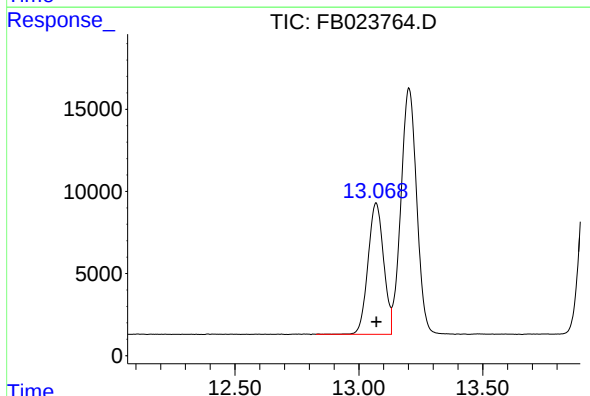


#7 Ethylbenzene

R.T.: 13.070 min
Delta R.T.: 0.000 min
Response: 350079
Conc: 9.42 ng/ml

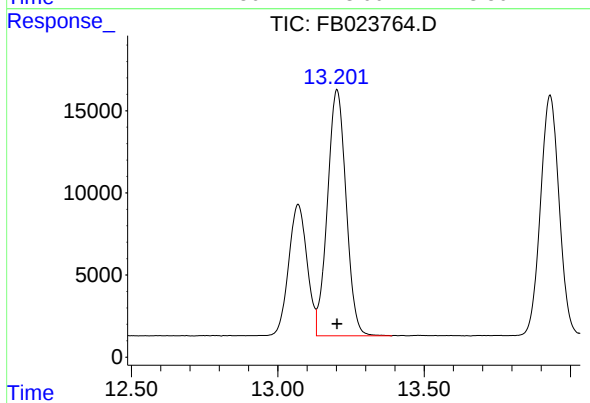

#8 m-Xylene


R.T.: 13.203 min
Delta R.T.: 0.000 min
Response: 663386
Conc: 18.58 ng/ml

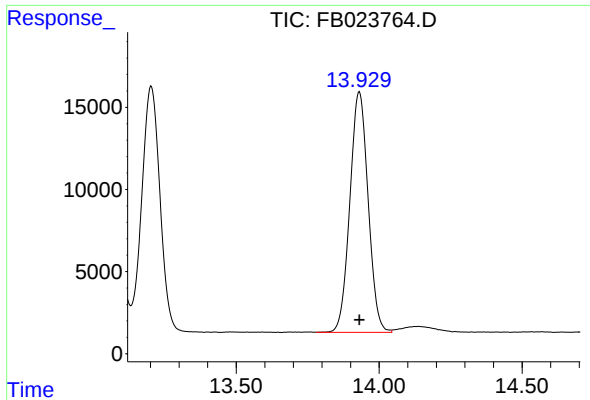

#9 O-Xylene

R.T.: 13.931 min
Delta R.T.: 0.000 min
Response: 650211
Conc: 18.85 ng/ml

Instrument :
FID_B
ClientSampleId :

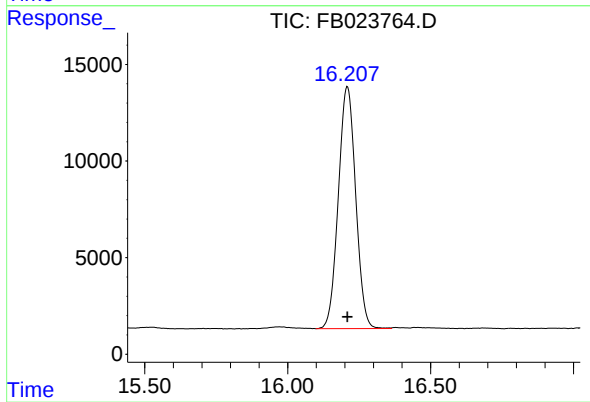

#10 1,2,4-Trimethylbenzene

R.T.: 16.209 min
Delta R.T.: 0.000 min
Response: 527587
Conc: 18.02 ng/ml