

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB030220\
 Data File : FB023760.D
 Signal(s) : FID2B.CH
 Acq On : 2 Mar 2020 9:54
 Operator : DD/AJ
 Sample : BSF0302S1
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0302S1

Integration File: SAMPLE.e
 Quant Time: Mar 03 00:41:49 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB020620.M
 Quant Title :
 QLast Update : Thu Feb 06 11:13:47 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.795	417897	20.526 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.687	850907	28.279 ng/ml
2) t 2,2,4-Trimethylpentane	7.414	994663	30.482 ng/ml
3) t n-Heptane	7.754	313553	9.746 ng/ml
4) t Benzene	7.888	394747	9.651 ng/ml
6) t Toluene	10.626	1160865	29.245 ng/ml
7) t Ethylbenzene	13.067	358260	9.637 ng/ml
8) t m-Xylene	13.200	691678	19.368 ng/ml
9) t O-Xylene	13.928	668232	19.375 ng/ml
10) t 1,2,4-Trimethylbenzene	16.206	573756	19.597 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB030220\
Data File : FB023760.D
Signal(s) : FID2B.CH
Acq On : 2 Mar 2020 9:54
Operator : DD/AJ
Sample : BSF0302S1
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0302S1

Integration File: SAMPLE.e
Quant Time: Mar 03 00:41:49 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB020620.M
Quant Title :
QLast Update : Thu Feb 06 11:13:47 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

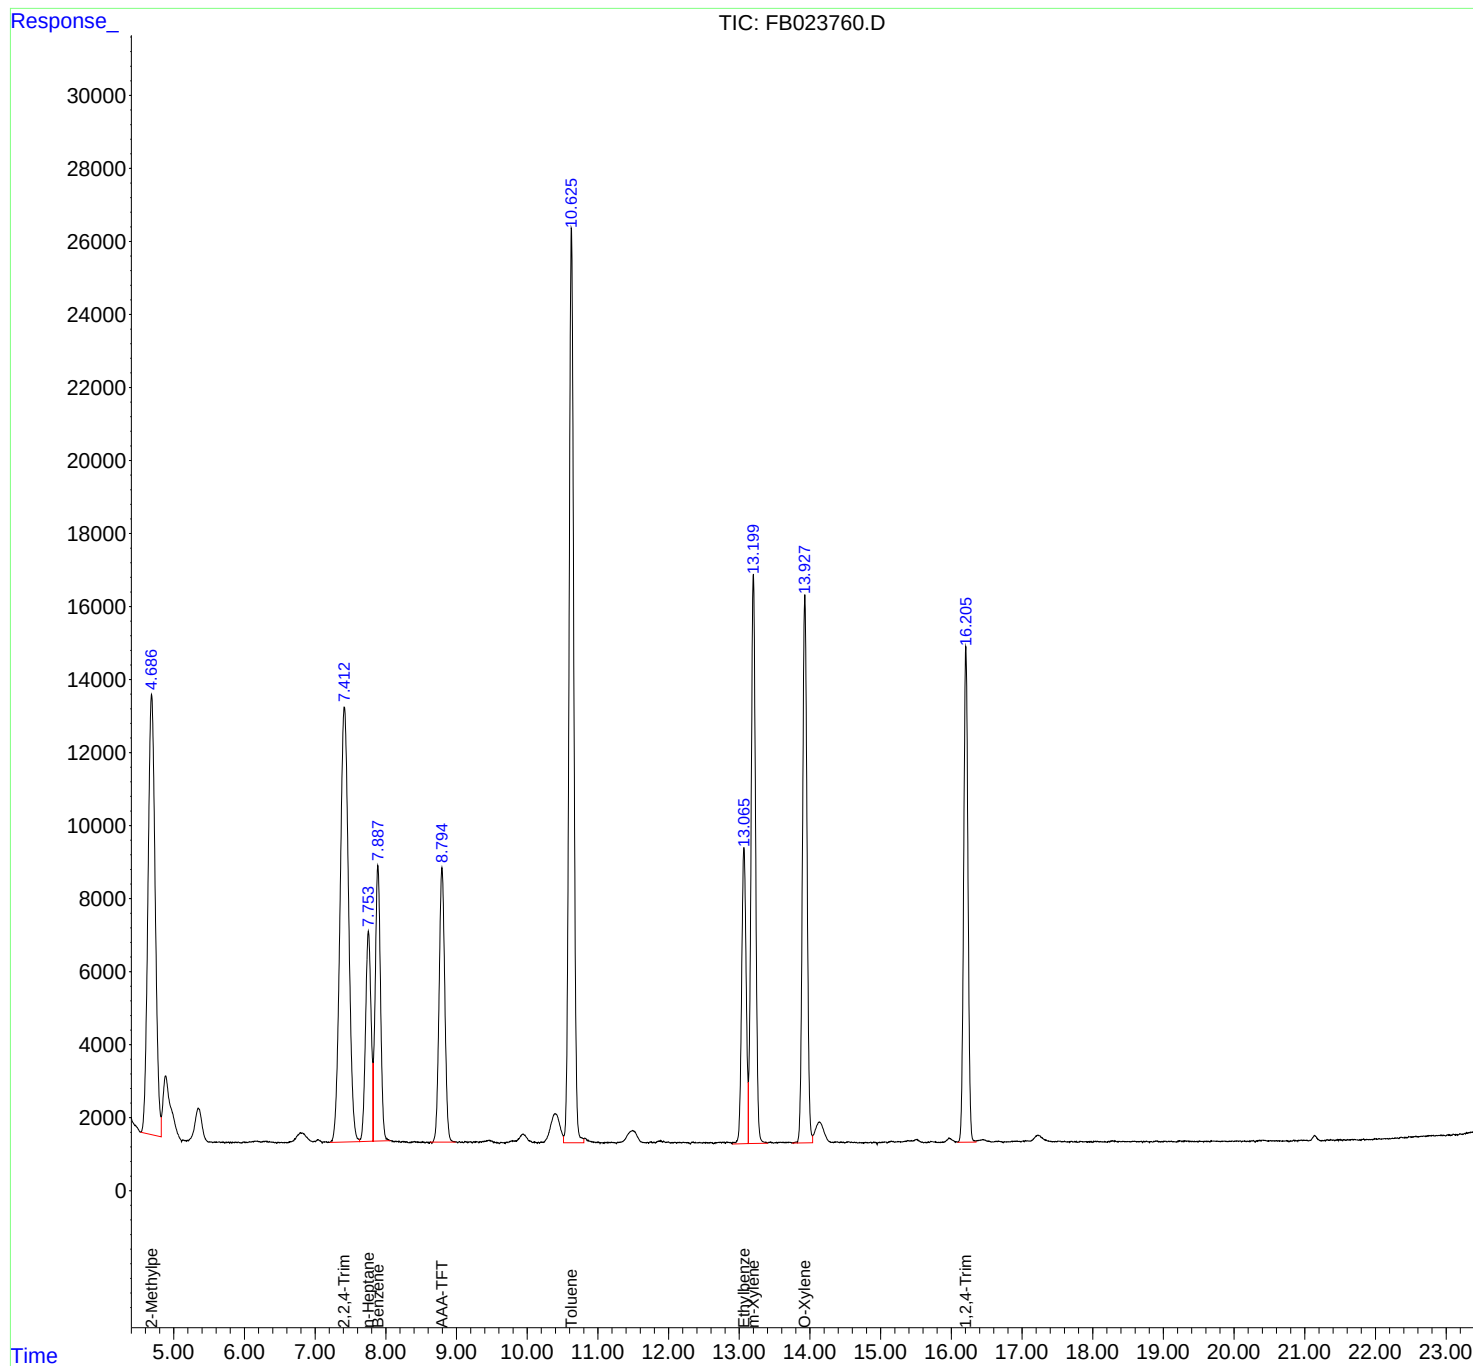


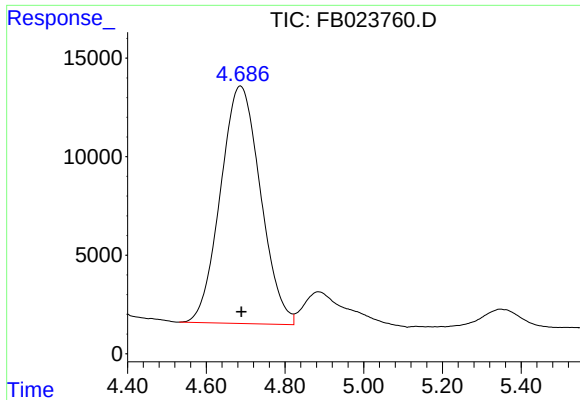

#1 2-Methylpentane


R.T.: 4.687 min
Delta R.T.: -0.002 min
Response: 850907
Conc: 28.28 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0302S1

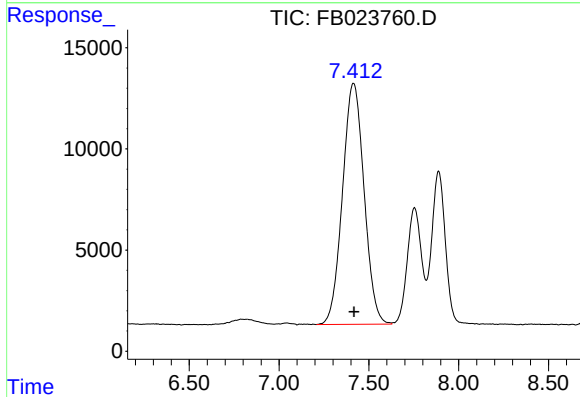


#2 2,2,4-Trimethylpentane

R.T.: 7.414 min
Delta R.T.: -0.004 min
Response: 994663
Conc: 30.48 ng/ml

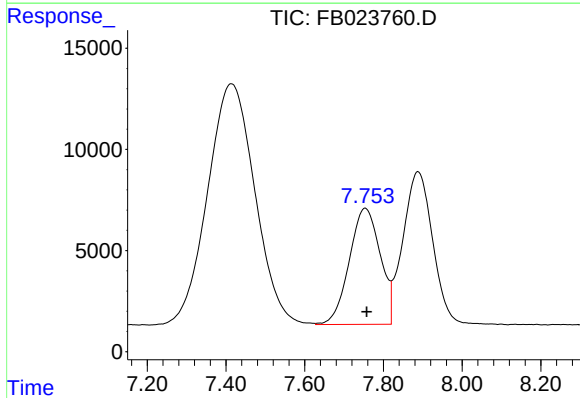


#3 n-Heptane

R.T.: 7.754 min
Delta R.T.: -0.004 min
Response: 313553
Conc: 9.75 ng/ml

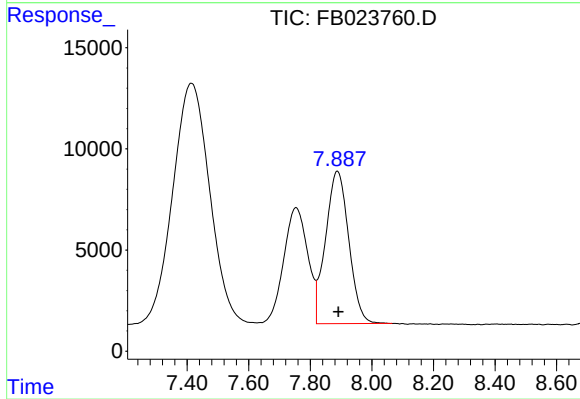

#4 Benzene


R.T.: 7.888 min
Delta R.T.: -0.003 min
Response: 394747
Conc: 9.65 ng/ml

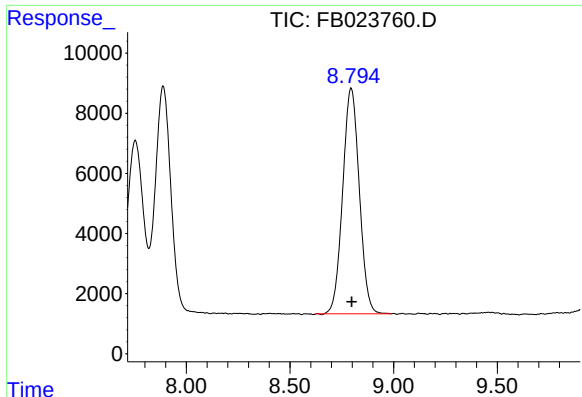

#5 AAA-TFT


R.T.: 8.795 min
Delta R.T.: -0.003 min
Response: 417897
Conc: 20.53 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0302S1

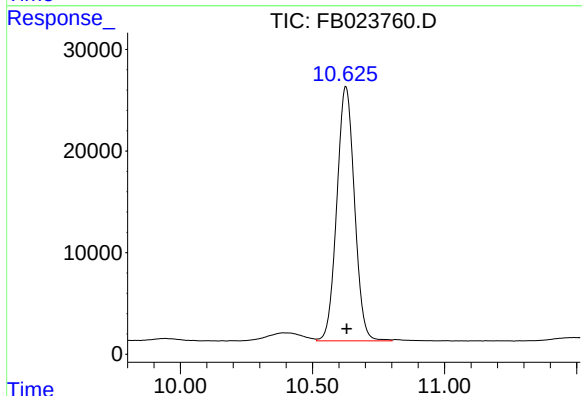


#6 Toluene

R.T.: 10.626 min
Delta R.T.: -0.004 min
Response: 1160865
Conc: 29.24 ng/ml

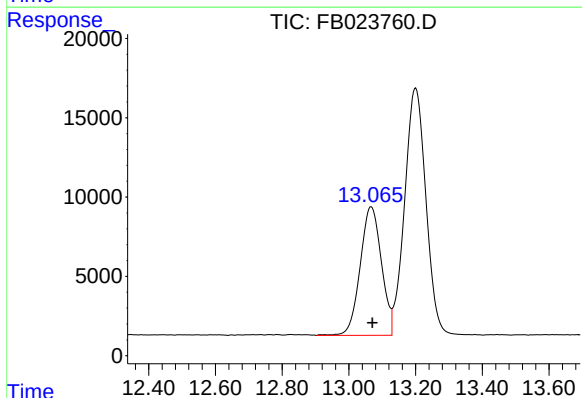


#7 Ethylbenzene

R.T.: 13.067 min
Delta R.T.: -0.003 min
Response: 358260
Conc: 9.64 ng/ml

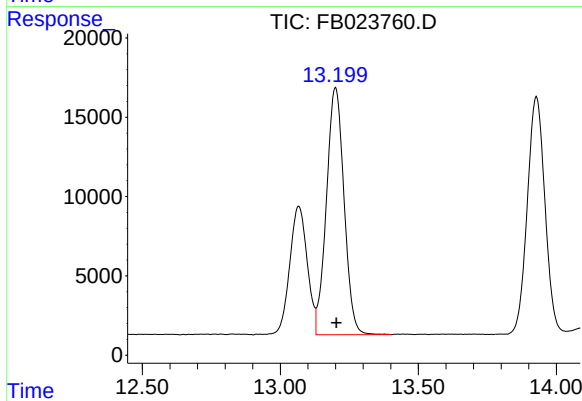

#8 m-Xylene


R.T.: 13.200 min
Delta R.T.: -0.003 min
Response: 691678
Conc: 19.37 ng/ml

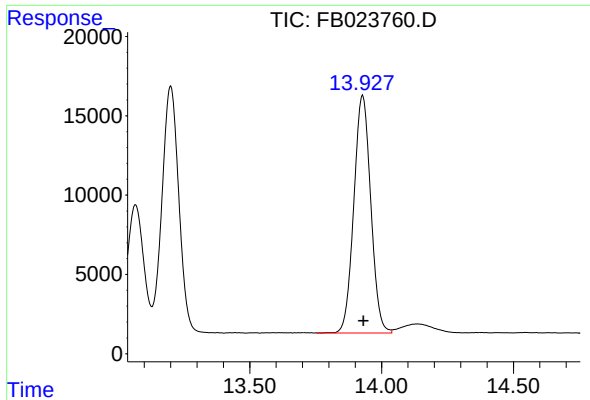

#9 O-Xylene

R.T.: 13.928 min
Delta R.T.: -0.003 min
Response: 668232
Conc: 19.37 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0302S1

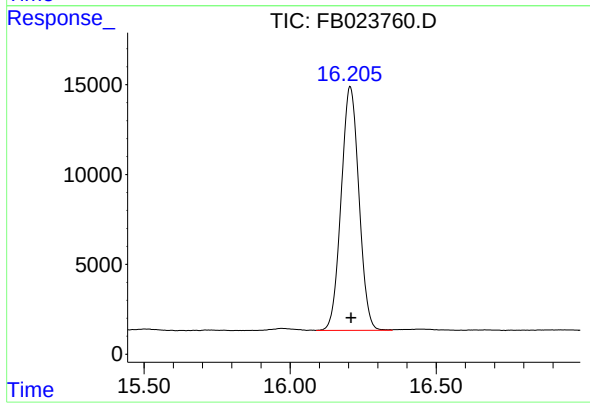

#10 1,2,4-Trimethylbenzene

R.T.: 16.206 min
Delta R.T.: -0.003 min
Response: 573756
Conc: 19.60 ng/ml