

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB030220\
 Data File : FB023765.D
 Signal(s) : FID2B.CH
 Acq On : 2 Mar 2020 12:44
 Operator : DD/AJ
 Sample : L1372-07MSD
 Misc : 5.03g/5.00ml DI WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 SU-03-022820MSD

Integration File: SAMPLE.e
 Quant Time: Mar 03 00:42:14 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB020620.M
 Quant Title :
 QLast Update : Thu Feb 06 11:13:47 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.798	450148	22.110 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.689	772499	25.673 ng/ml
2) t 2,2,4-Trimethylpentane	7.417	812851	24.910 ng/ml
3) t n-Heptane	7.756	246742	7.669 ng/ml
4) t Benzene	7.891	395603	9.672 ng/ml
6) t Toluene	10.629	1135153	28.597 ng/ml
7) t Ethylbenzene	13.069	343221	9.233 ng/ml
8) t m-Xylene	13.202	647846	18.141 ng/ml
9) t O-Xylene	13.930	637734	18.491 ng/ml
10) t 1,2,4-Trimethylbenzene	16.209	507205	17.323 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB030220\
Data File : FB023765.D
Signal(s) : FID2B.CH
Acq On : 2 Mar 2020 12:44
Operator : DD/AJ
Sample : L1372-07MSD
Misc : 5.03g/5.00ml DI WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
SU-03-022820MSD

Integration File: SAMPLE.e
Quant Time: Mar 03 00:42:14 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB020620.M
Quant Title :
QLast Update : Thu Feb 06 11:13:47 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

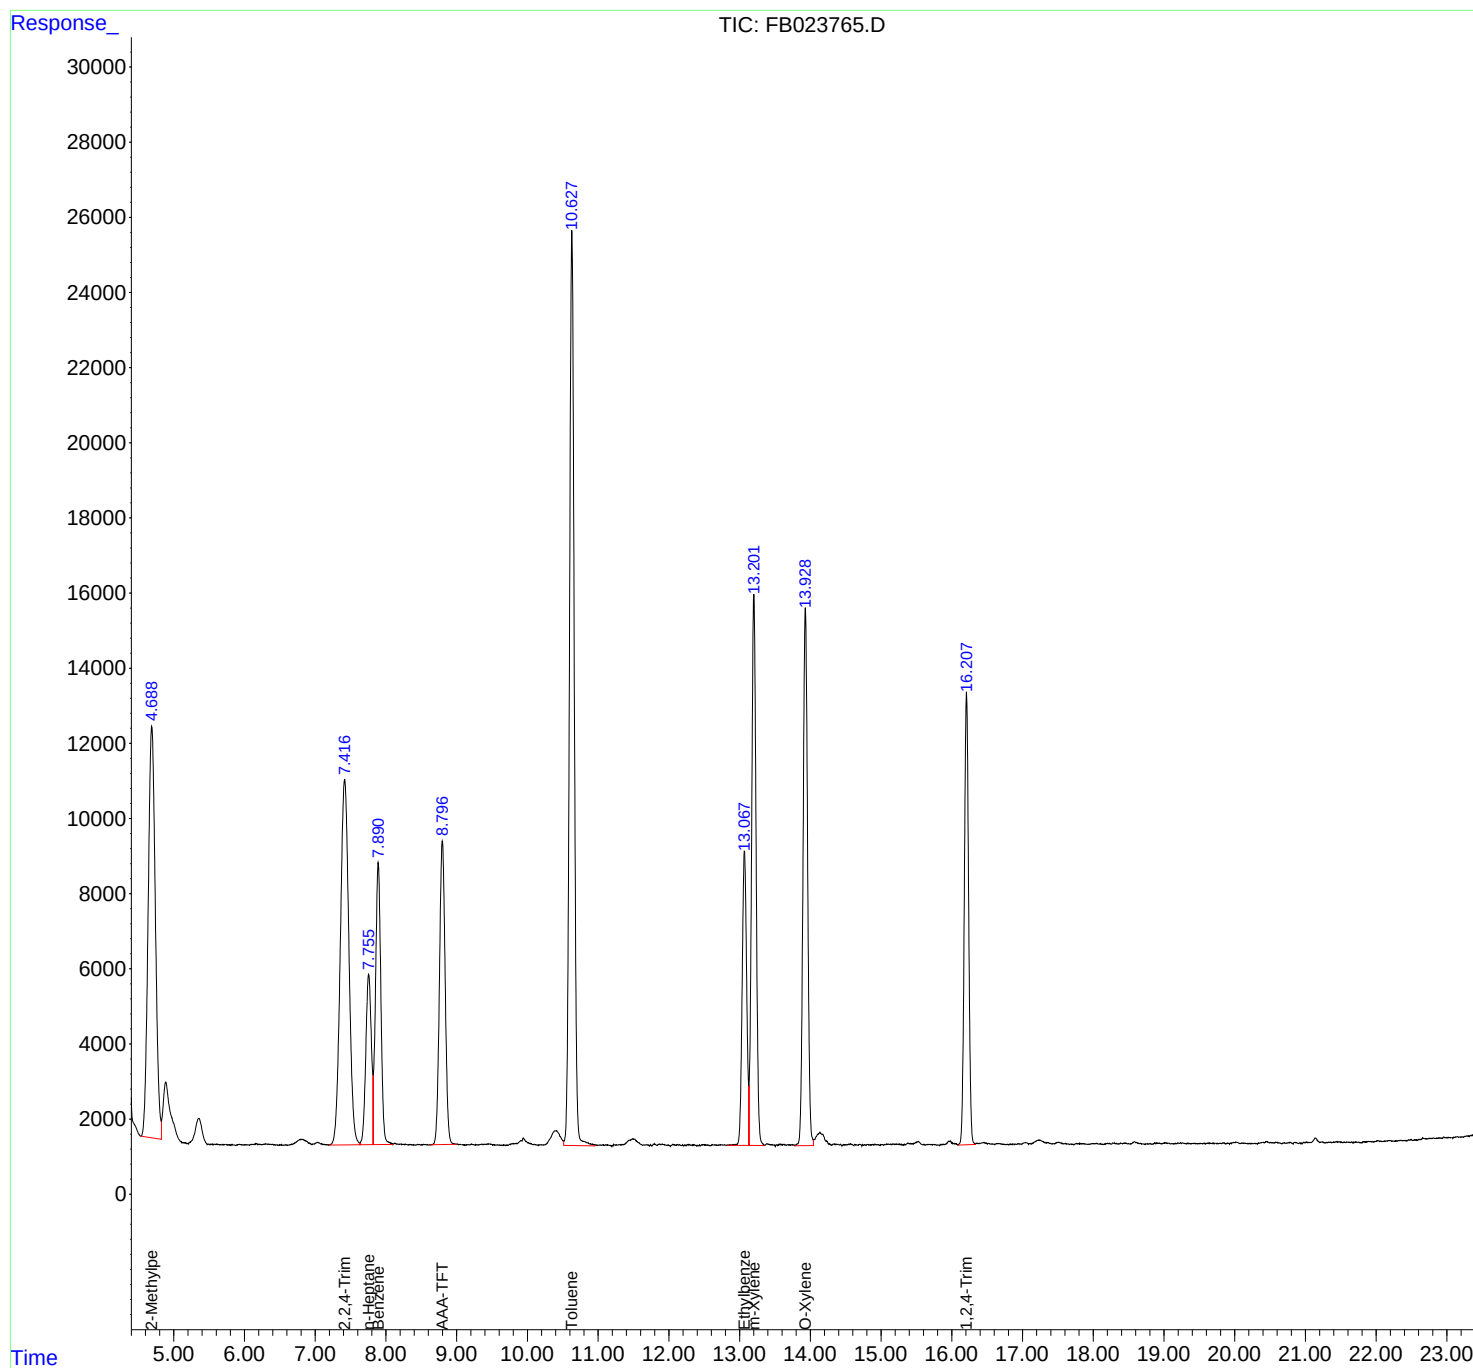


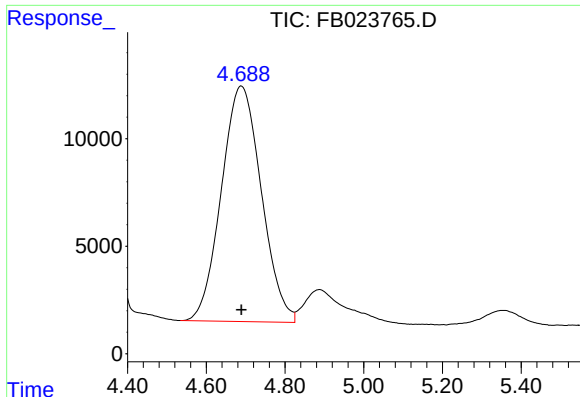

#1 2-Methylpentane


R.T.: 4.689 min
Delta R.T.: 0.000 min
Response: 772499
Conc: 25.67 ng/ml

Instrument :
FID_B
ClientSampleId :
SU-03-022820MSD

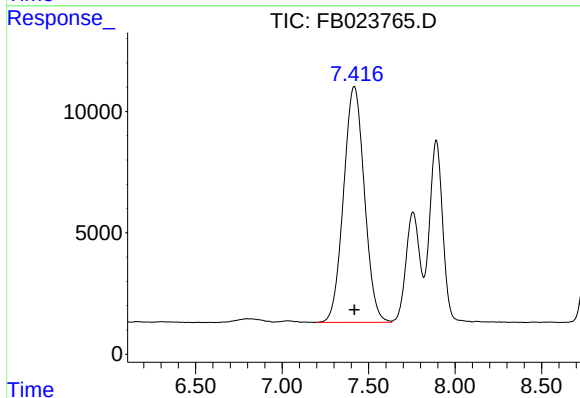


#2 2,2,4-Trimethylpentane

R.T.: 7.417 min
Delta R.T.: 0.000 min
Response: 812851
Conc: 24.91 ng/ml

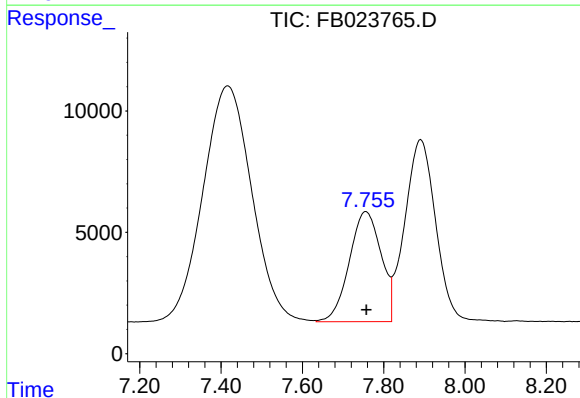


#3 n-Heptane

R.T.: 7.756 min
Delta R.T.: -0.002 min
Response: 246742
Conc: 7.67 ng/ml

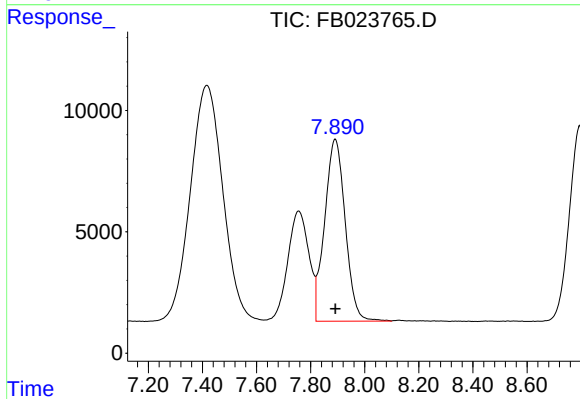

#4 Benzene


R.T.: 7.891 min
Delta R.T.: 0.000 min
Response: 395603
Conc: 9.67 ng/ml

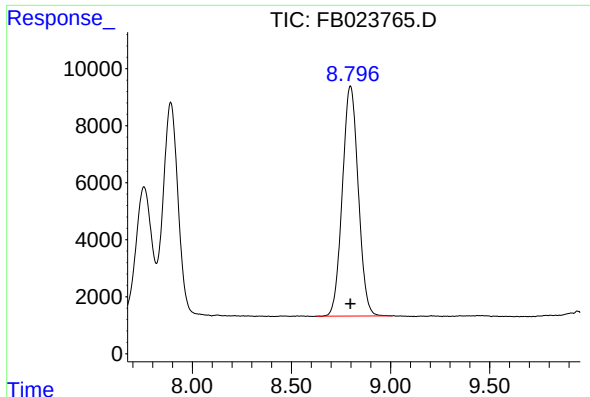

#5 AAA-TFT


R.T.: 8.798 min
Delta R.T.: 0.000 min
Response: 450148
Conc: 22.11 ng/ml

Instrument :
FID_B
ClientSampleId :
SU-03-022820MSD

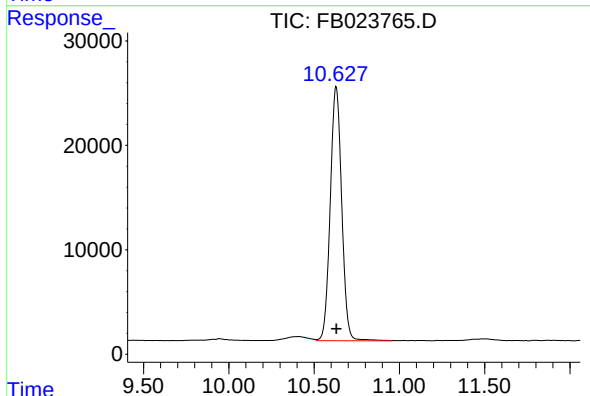


#6 Toluene

R.T.: 10.629 min
Delta R.T.: -0.001 min
Response: 1135153
Conc: 28.60 ng/ml

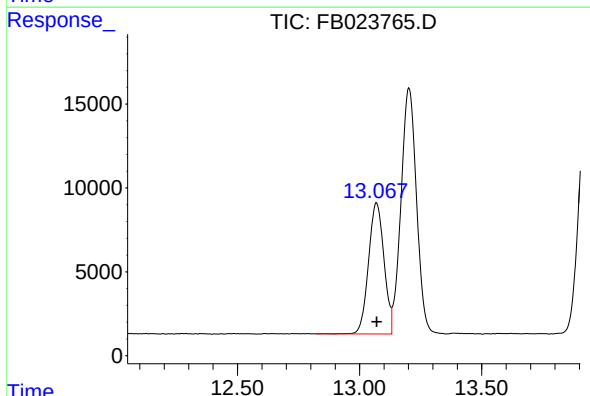


#7 Ethylbenzene

R.T.: 13.069 min
Delta R.T.: -0.001 min
Response: 343221
Conc: 9.23 ng/ml

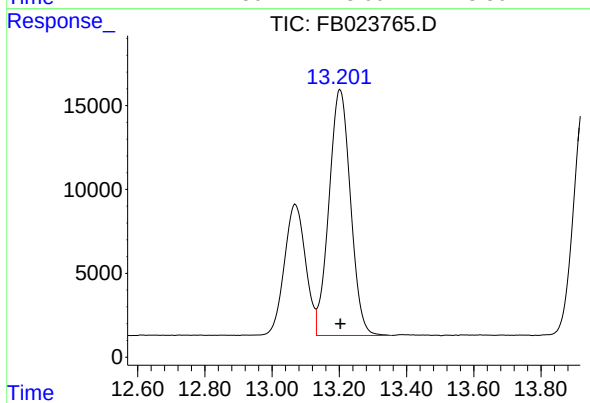

#8 m-Xylene


R.T.: 13.202 min
Delta R.T.: 0.000 min
Response: 647846
Conc: 18.14 ng/ml

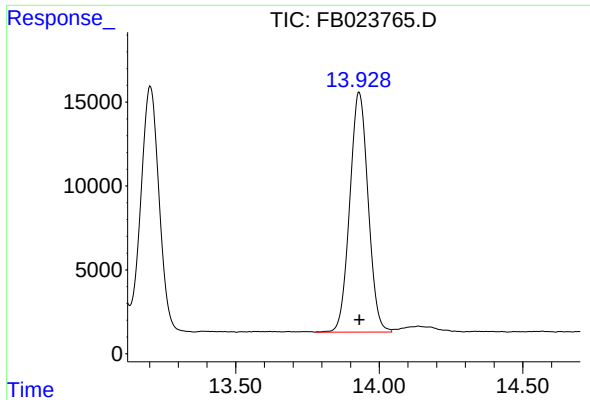

#9 O-Xylene

R.T.: 13.930 min
Delta R.T.: -0.001 min
Response: 637734
Conc: 18.49 ng/ml

Instrument :
FID_B
ClientSampleId :
SU-03-022820MSD

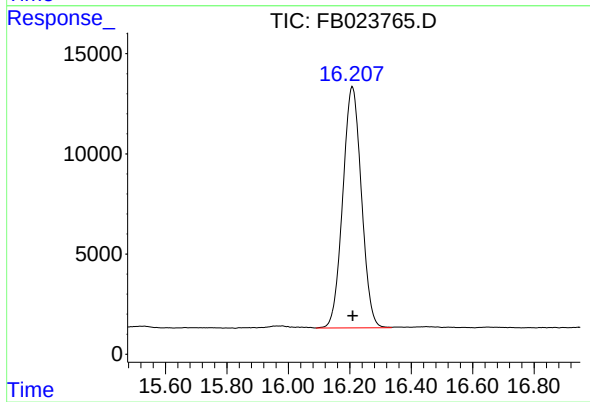

#10 1,2,4-Trimethylbenzene

R.T.: 16.209 min
Delta R.T.: 0.000 min
Response: 507205
Conc: 17.32 ng/ml