

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB030221\
 Data File : FB025478.D
 Signal(s) : FID2B.CH
 Acq On : 2 Mar 2021 9:44
 Operator : DD/AJ
 Sample : BSF0302S1
 Misc : 5.00g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0302S1

Integration File: Calibration.e
 Quant Time: Mar 03 00:27:24 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB021921.M
 Quant Title :
 QLast Update : Mon Feb 22 11:51:04 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.798	547302	21.577 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.688	1000313	28.382 ng/ml
2) t 2,2,4-Trimethylpentane	7.415	1117217	30.088 ng/ml
3) t n-Heptane	7.757	362540	10.015 ng/ml
4) t Benzene	7.891	443876	9.609 ng/ml
6) t Toluene	10.629	1284981	28.741 ng/ml
7) t Ethylbenzene	13.069	393276	9.744 ng/ml
8) t m-Xylene	13.202	789812	19.633 ng/ml
9) t O-Xylene	13.930	756376	19.541 ng/ml
10) t 1,2,4-Trimethylbenzene	16.208	662641	19.740 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB030221\
Data File : FB025478.D
Signal(s) : FID2B.CH
Acq On : 2 Mar 2021 9:44
Operator : DD/AJ
Sample : BSF0302S1
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0302S1

Integration File: Calibration.e
Quant Time: Mar 03 00:27:24 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB021921.M
Quant Title :
QLast Update : Mon Feb 22 11:51:04 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

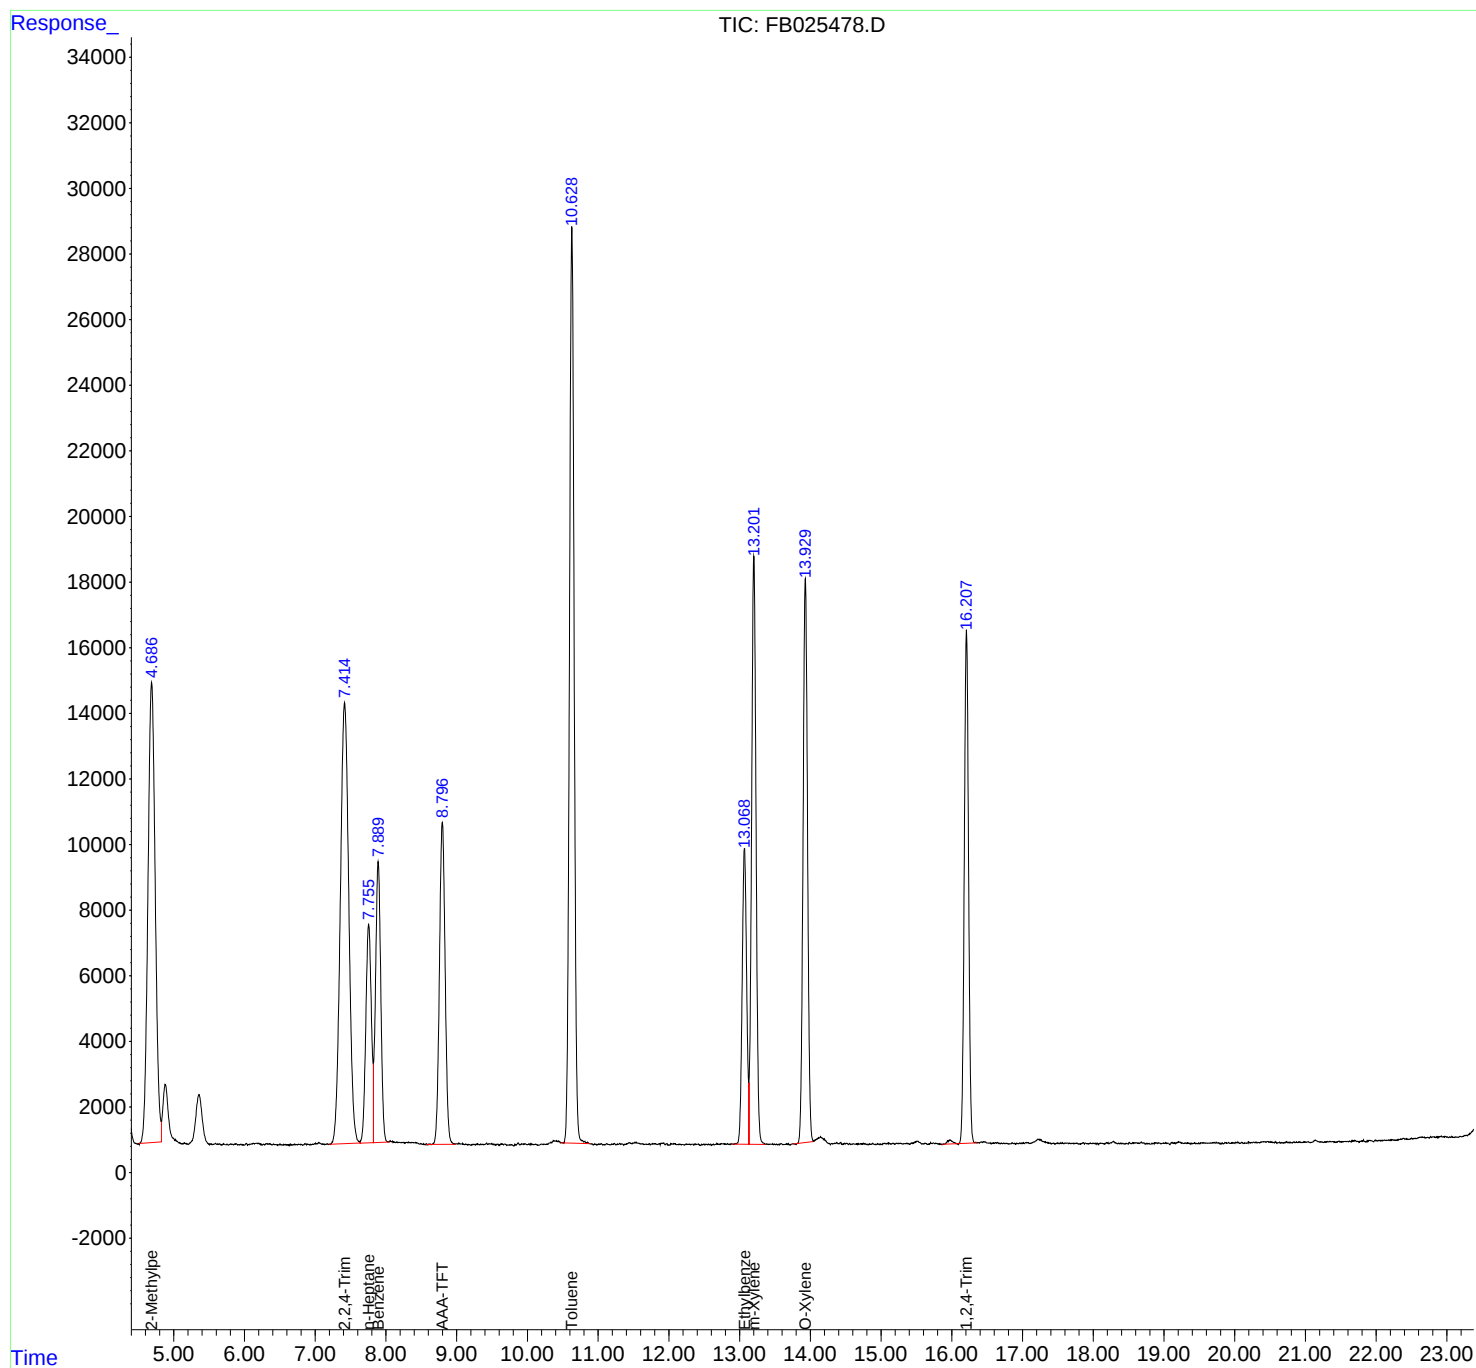


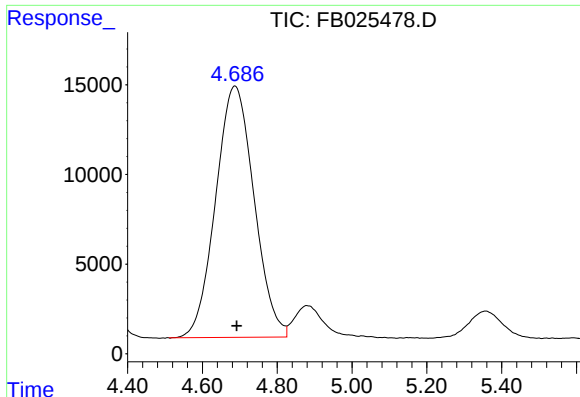

#1 2-Methylpentane


R.T.: 4.688 min
Delta R.T.: -0.004 min
Response: 1000313
Conc: 28.38 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0302S1

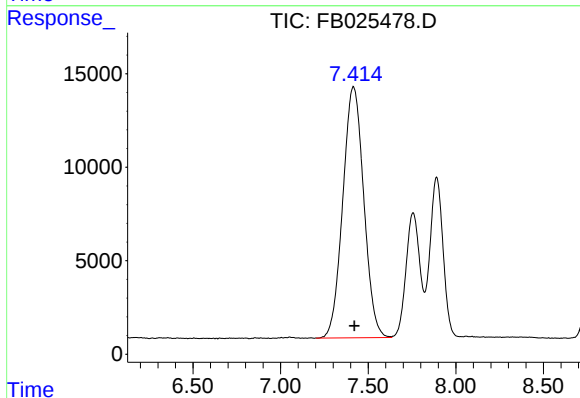


#2 2,2,4-Trimethylpentane

R.T.: 7.415 min
Delta R.T.: -0.006 min
Response: 1117217
Conc: 30.09 ng/ml

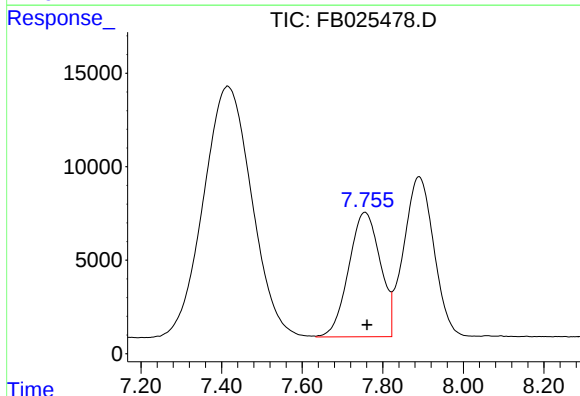


#3 n-Heptane

R.T.: 7.757 min
Delta R.T.: -0.005 min
Response: 362540
Conc: 10.01 ng/ml

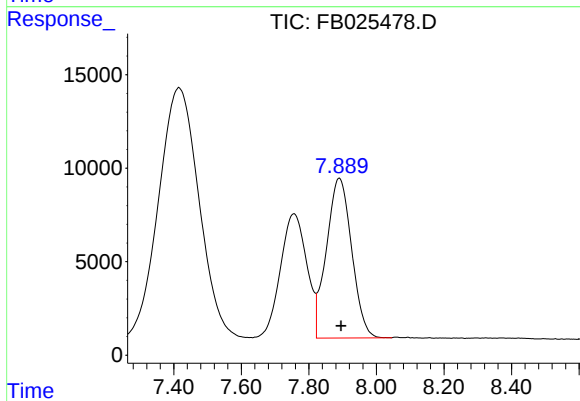

#4 Benzene


R.T.: 7.891 min
Delta R.T.: -0.005 min
Response: 443876
Conc: 9.61 ng/ml

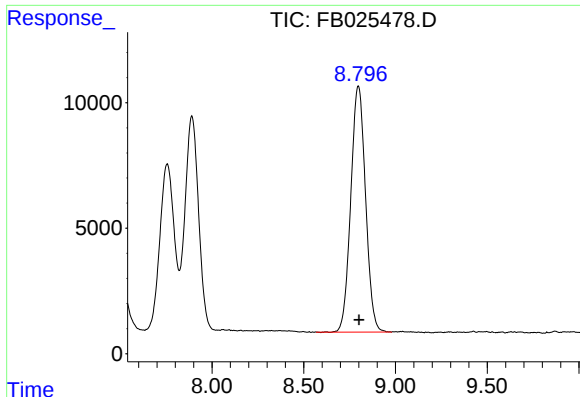

#5 AAA-TFT


R.T.: 8.798 min
Delta R.T.: -0.004 min
Response: 547302
Conc: 21.58 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0302S1

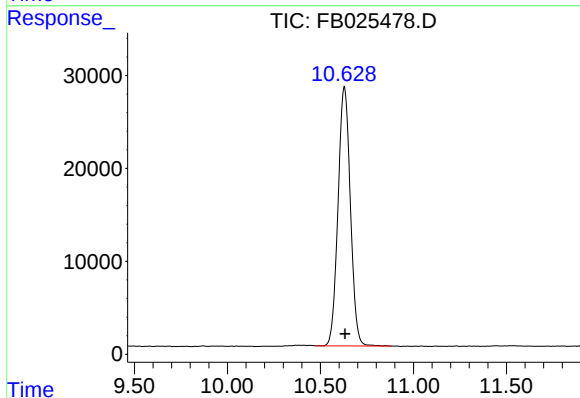


#6 Toluene

R.T.: 10.629 min
Delta R.T.: -0.005 min
Response: 1284981
Conc: 28.74 ng/ml

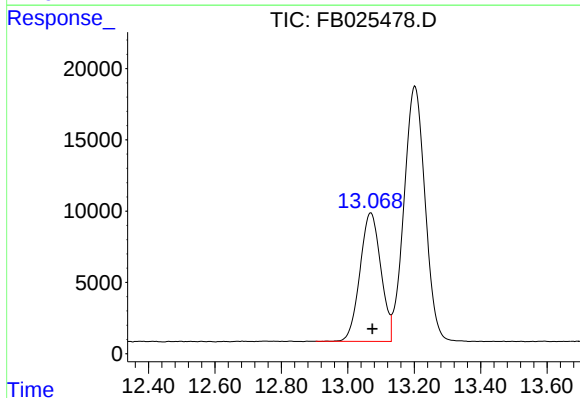


#7 Ethylbenzene

R.T.: 13.069 min
Delta R.T.: -0.005 min
Response: 393276
Conc: 9.74 ng/ml

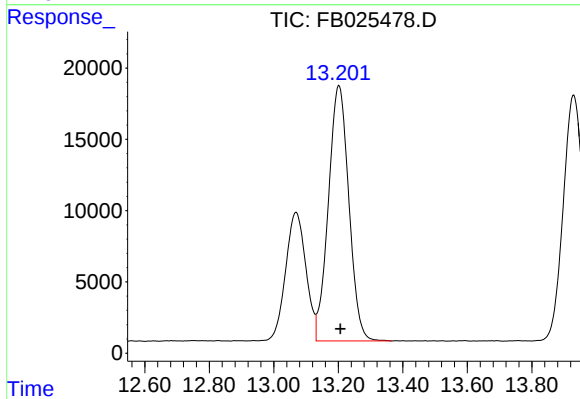

#8 m-Xylene


R.T.: 13.202 min
Delta R.T.: -0.004 min
Response: 789812
Conc: 19.63 ng/ml

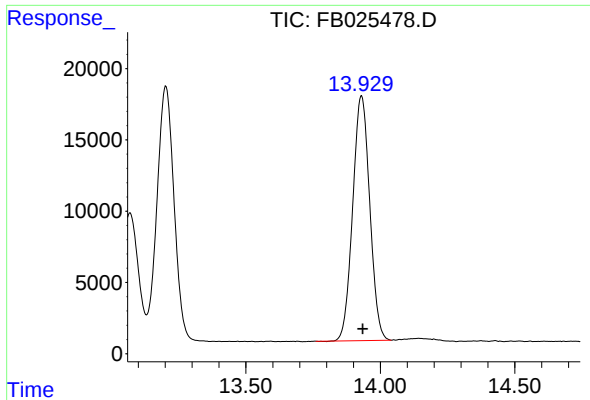

#9 O-Xylene

R.T.: 13.930 min
Delta R.T.: -0.004 min
Response: 756376
Conc: 19.54 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0302S1

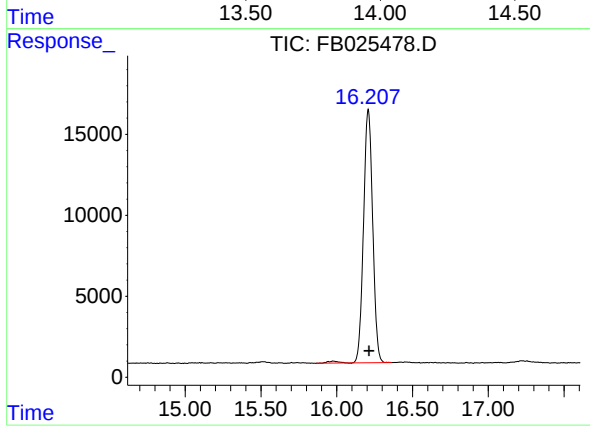

#10 1,2,4-Trimethylbenzene

R.T.: 16.208 min
Delta R.T.: -0.004 min
Response: 662641
Conc: 19.74 ng/ml