

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB030221\
 Data File : FB025481.D
 Signal(s) : FID2B.CH
 Acq On : 2 Mar 2021 11:45
 Operator : DD/AJ
 Sample : M1509-01MS
 Misc : 5.03g/5.00ml DI WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BU-02-022621MS

Integration File: Calibration.e
 Quant Time: Mar 03 00:27:46 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB021921.M
 Quant Title :
 QLast Update : Mon Feb 22 11:51:04 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.799	500888	19.747 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.687	862200	24.463 ng/ml
2) t 2,2,4-Trimethylpentane	7.417	867537	23.364 ng/ml
3) t n-Heptane	7.758	280769	7.756 ng/ml
4) t Benzene	7.893	417204	9.031 ng/ml
6) t Toluene	10.631	1191336	26.646 ng/ml
7) t Ethylbenzene	13.072	360878	8.941 ng/ml
8) t m-Xylene	13.205	716912	17.821 ng/ml
9) t O-Xylene	13.933	691960	17.876 ng/ml
10) t 1,2,4-Trimethylbenzene	16.211	574923	17.127 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB030221\
Data File : FB025481.D
Signal(s) : FID2B.CH
Acq On : 2 Mar 2021 11:45
Operator : DD/AJ
Sample : M1509-01MS
Misc : 5.03g/5.00ml DI WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BU-02-022621MS

Integration File: Calibration.e
Quant Time: Mar 03 00:27:46 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB021921.M
Quant Title :
QLast Update : Mon Feb 22 11:51:04 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

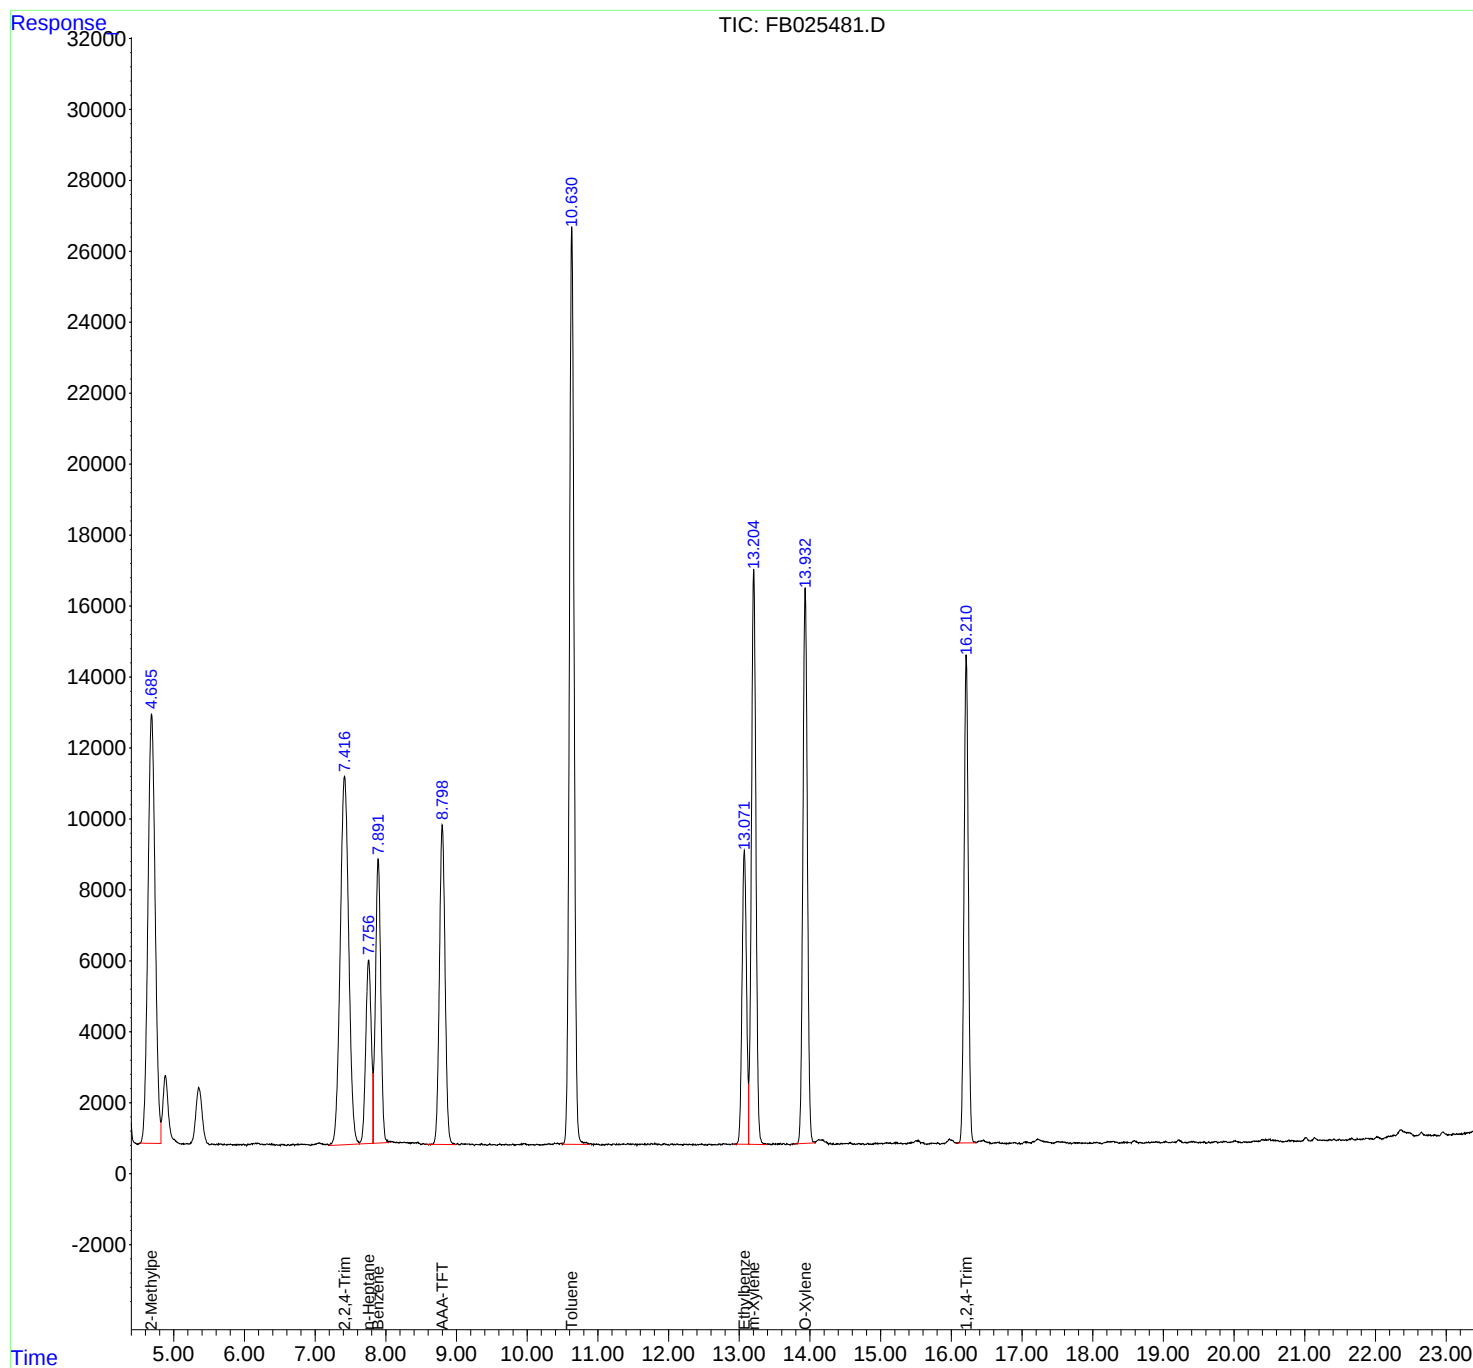


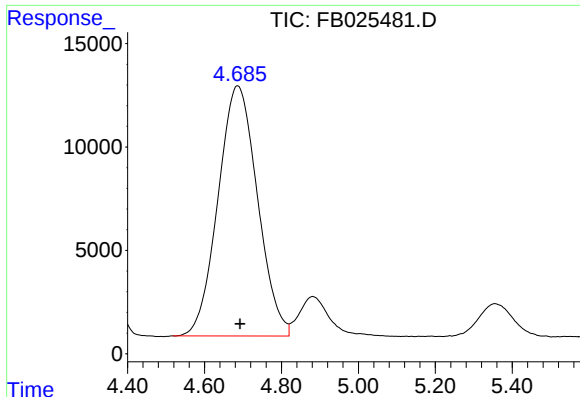

#1 2-Methylpentane


R.T.: 4.687 min
Delta R.T.: -0.005 min
Response: 862200
Conc: 24.46 ng/ml

Instrument :
FID_B
ClientSampleId :
BU-02-022621MS

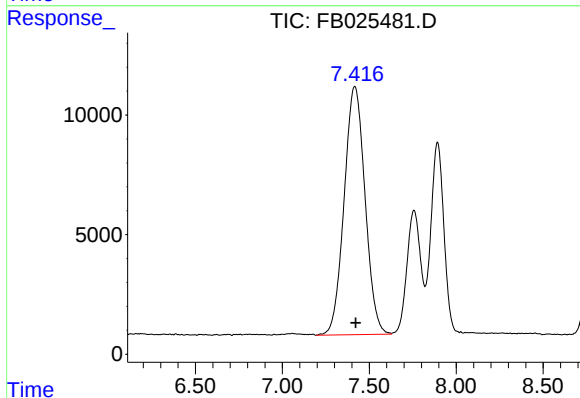


#2 2,2,4-Trimethylpentane

R.T.: 7.417 min
Delta R.T.: -0.005 min
Response: 867537
Conc: 23.36 ng/ml

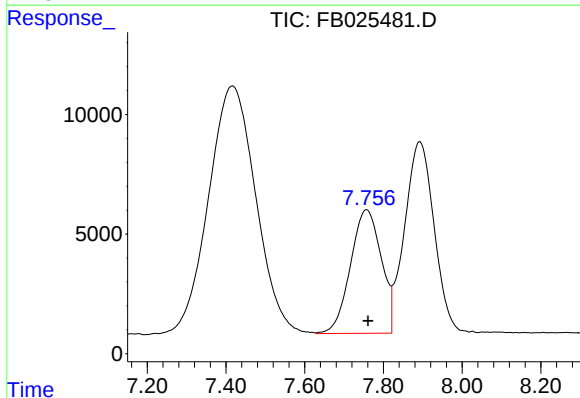


#3 n-Heptane

R.T.: 7.758 min
Delta R.T.: -0.004 min
Response: 280769
Conc: 7.76 ng/ml

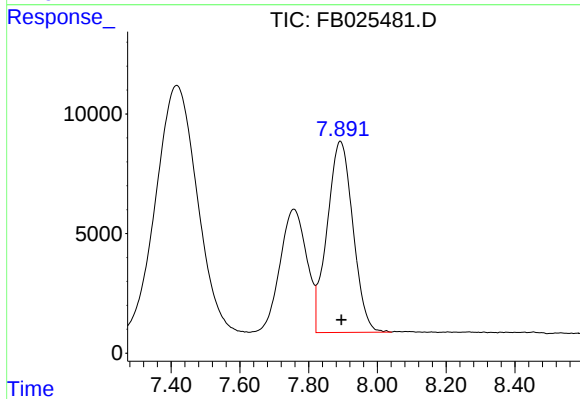

#4 Benzene


R.T.: 7.893 min
Delta R.T.: -0.003 min
Response: 417204
Conc: 9.03 ng/ml

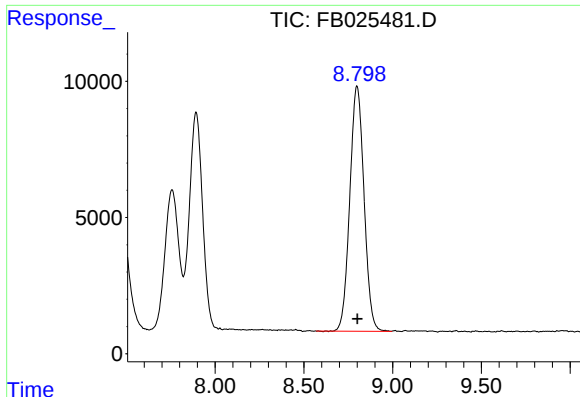

#5 AAA-TFT


R.T.: 8.799 min
Delta R.T.: -0.003 min
Response: 500888
Conc: 19.75 ng/ml

Instrument :
FID_B
ClientSampleId :
BU-02-022621MS

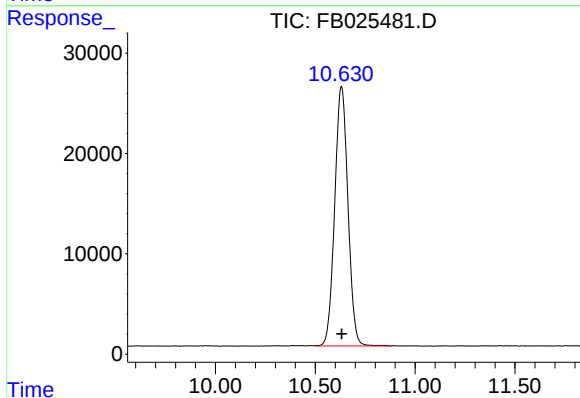


#6 Toluene

R.T.: 10.631 min
Delta R.T.: -0.002 min
Response: 1191336
Conc: 26.65 ng/ml

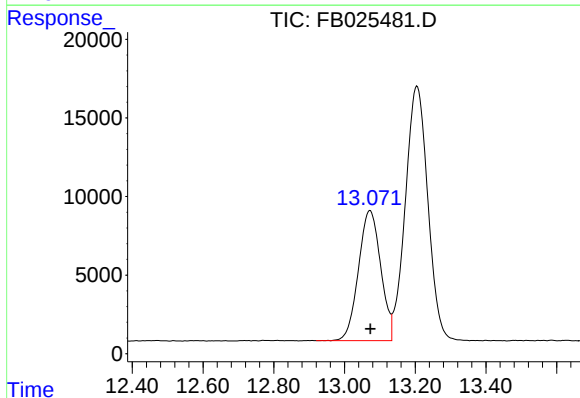


#7 Ethylbenzene

R.T.: 13.072 min
Delta R.T.: -0.002 min
Response: 360878
Conc: 8.94 ng/ml

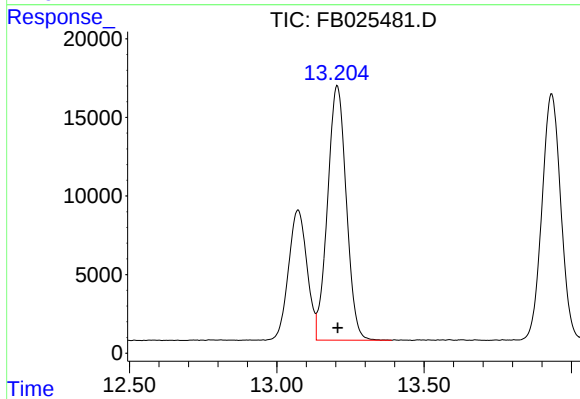

#8 m-Xylene


R.T.: 13.205 min
Delta R.T.: -0.001 min
Response: 716912
Conc: 17.82 ng/ml

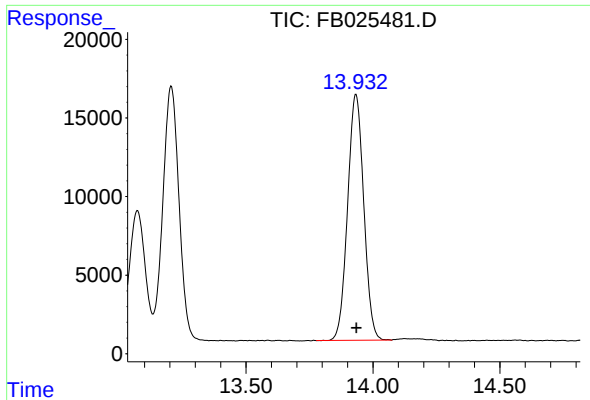

#9 O-Xylene

R.T.: 13.933 min
Delta R.T.: -0.001 min
Response: 691960
Conc: 17.88 ng/ml

Instrument :
FID_B
ClientSampleId :
BU-02-022621MS

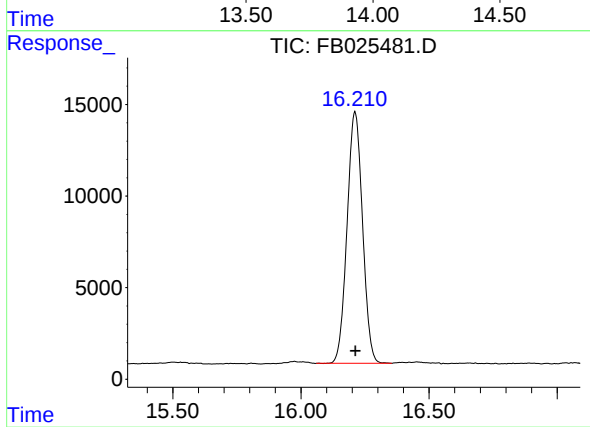

#10 1,2,4-Trimethylbenzene

R.T.: 16.211 min
Delta R.T.: 0.000 min
Response: 574923
Conc: 17.13 ng/ml