

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB030223\
Data File : FB029400.D
Signal(s) : FID2B.CH
Acq On : 2 Mar 2023 13:43
Operator : YP/AJ
Sample : 01767-11
Misc : 7.71G/5.00 ML DI WATER
ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Mar 02 23:39:11 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030123.M
Quant Title :
QLast Update : Wed Mar 01 12:30:24 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.793	168885	13.939 ng/ml
Target Compounds			
6) t Toluene	10.630	7137	0.362 ng/ml
9) t O-Xylene	13.921	3816	0.207 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB030223\
Data File : FB029400.D
Signal(s) : FID2B.CH
Acq On : 2 Mar 2023 13:43
Operator : YP/AJ
Sample : 01767-11
Misc : 7.71G/5.00 ML DI WATER
ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Mar 02 23:39:11 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030123.M
Quant Title :
QLast Update : Wed Mar 01 12:30:24 2023
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

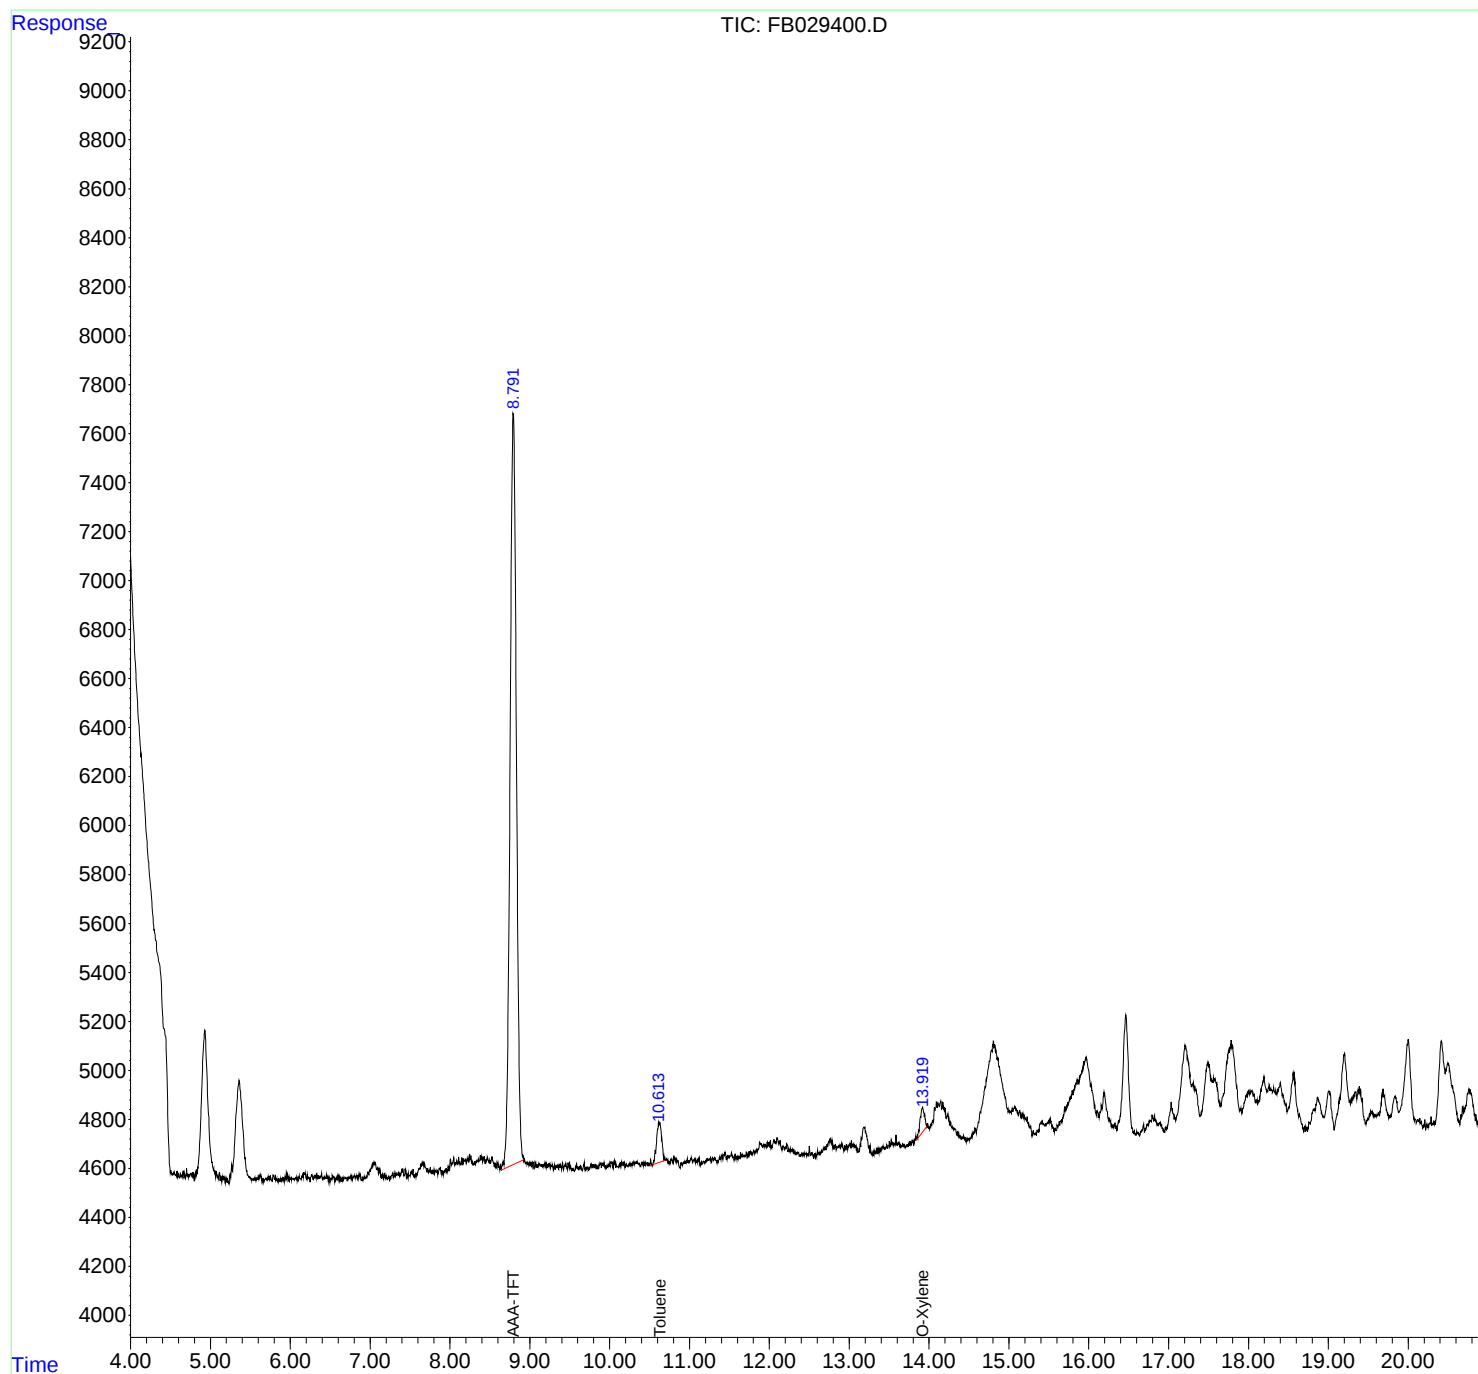

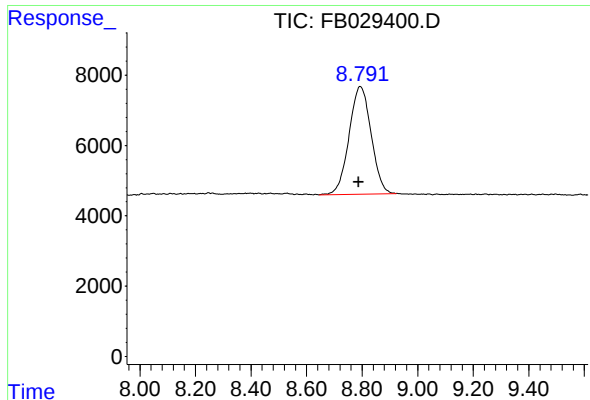


#5 AAA-TFT

R.T.: 8.793 min
Delta R.T.: 0.006 min
Response: 168885
Conc: 13.94 ng/ml

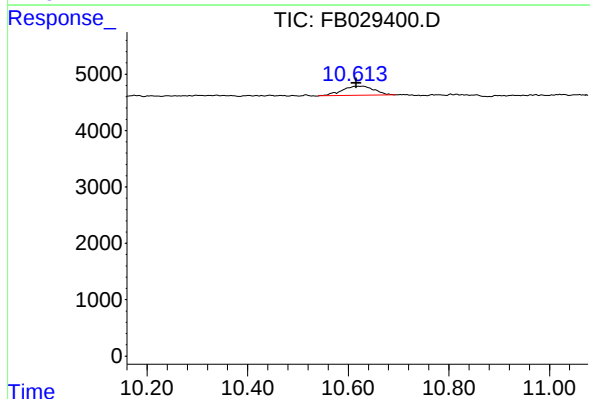

#6 Toluene

R.T.: 10.630 min
Delta R.T.: 0.014 min
Response: 7137
Conc: 0.36 ng/ml

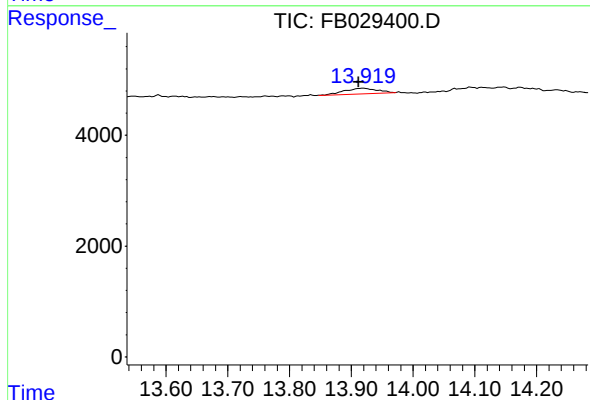

#9 O-Xylene

R.T.: 13.921 min
Delta R.T.: 0.009 min
Response: 3816
Conc: 0.21 ng/ml