

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB030223\
 Data File : FB029404.D
 Signal(s) : FID2B.CH
 Acq On : 2 Mar 2023 16:12
 Operator : YP/AJ
 Sample : BSF0302S2
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 11 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Mar 02 23:39:36 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030123.M
 Quant Title :
 QLast Update : Wed Mar 01 12:30:24 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.793	248325	20.496 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.710	463752	30.223 ng/ml
2) t	2,2,4-Trimethylpentane	7.418	535589	31.796 ng/ml
3) t	n-Heptane	7.752	166266	9.613 ng/ml
4) t	Benzene	7.888	196633	9.687 ng/ml
6) t	Toluene	10.622	563792	28.562 ng/ml
7) t	Ethylbenzene	13.058	181372	9.742 ng/ml
8) t	m-Xylene	13.191	362814	19.502 ng/ml
9) t	O-Xylene	13.918	359083	19.501 ng/ml
10) t	1,2,4-Trimethylbenzene	16.193	372404	19.994 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB030223\
Data File : FB029404.D
Signal(s) : FID2B.CH
Acq On : 2 Mar 2023 16:12
Operator : YP/AJ
Sample : BSF0302S2
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 11 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Mar 02 23:39:36 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030123.M
Quant Title :
QLast Update : Wed Mar 01 12:30:24 2023
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

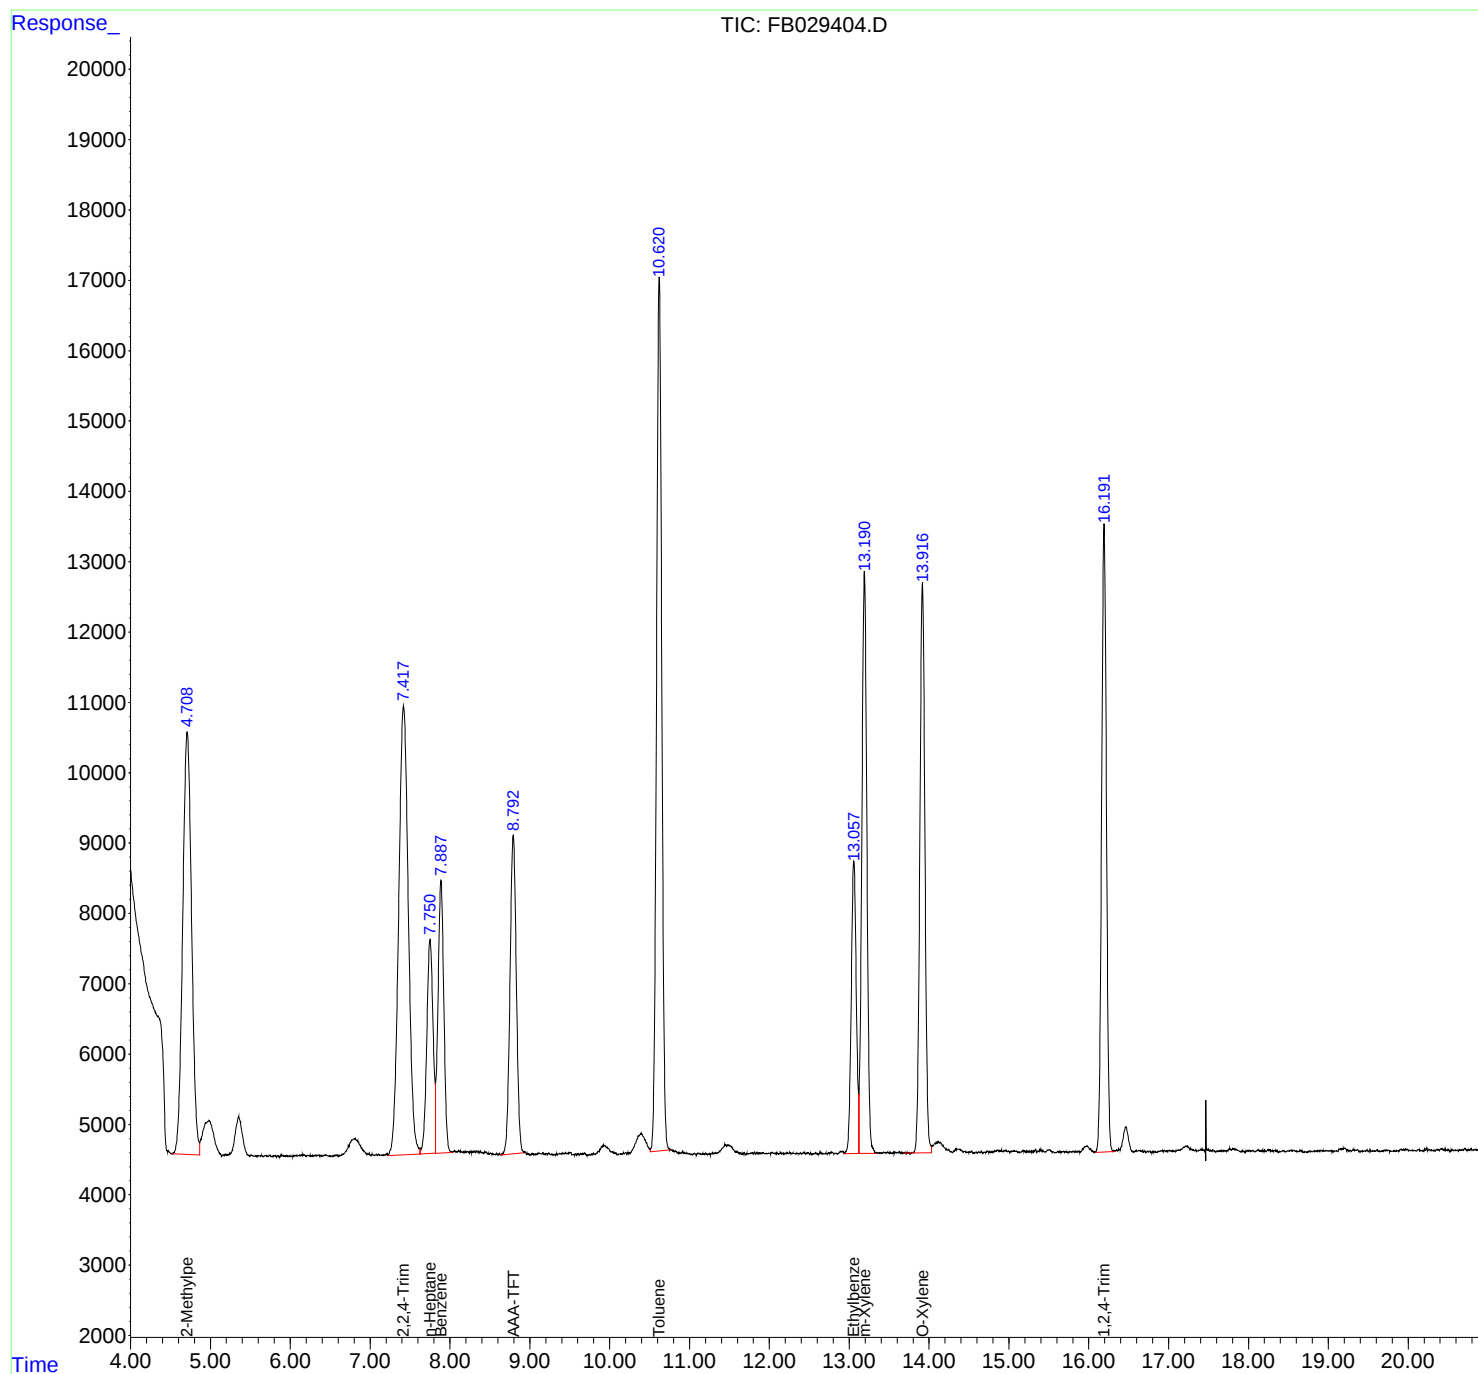

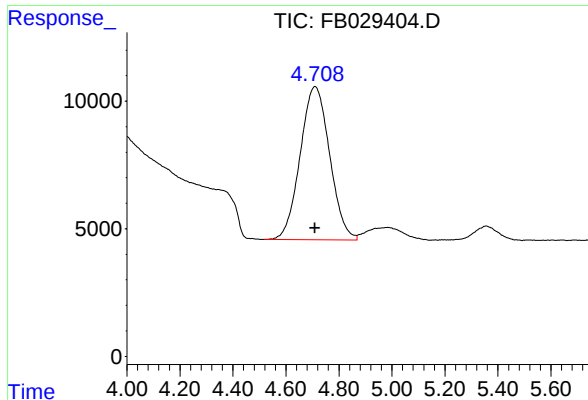


#1 2-Methylpentane

R.T.: 4.710 min
Delta R.T.: 0.000 min
Response: 463752
Conc: 30.22 ng/ml

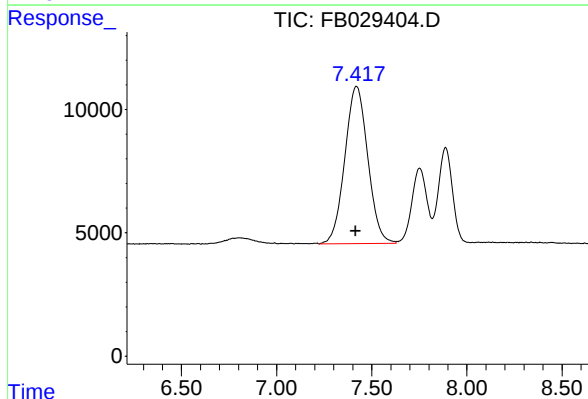


#2 2,2,4-Trimethylpentane

R.T.: 7.418 min
Delta R.T.: 0.003 min
Response: 535589
Conc: 31.80 ng/ml

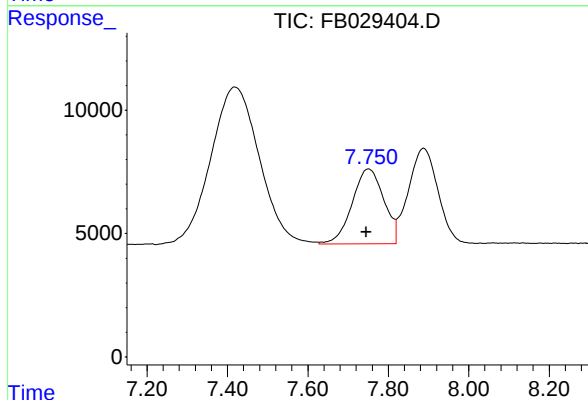


#3 n-Heptane

R.T.: 7.752 min
Delta R.T.: 0.006 min
Response: 166266
Conc: 9.61 ng/ml

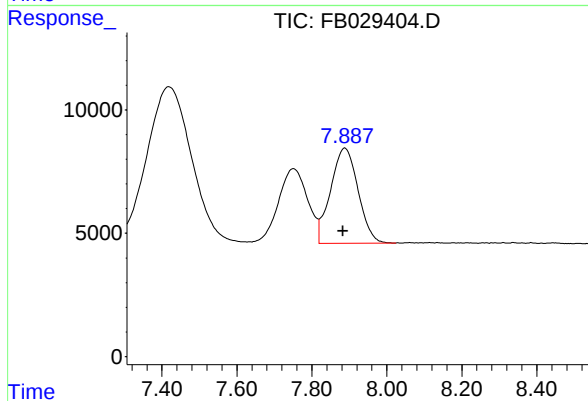


#4 Benzene

R.T.: 7.888 min
Delta R.T.: 0.005 min
Response: 196633
Conc: 9.69 ng/ml

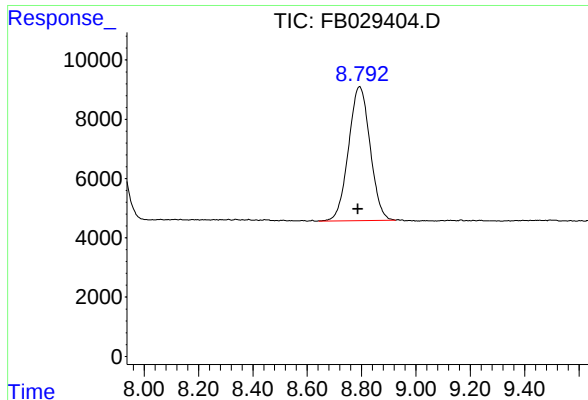


#5 AAA-TFT

R.T.: 8.793 min
Delta R.T.: 0.006 min
Response: 248325
Conc: 20.50 ng/ml

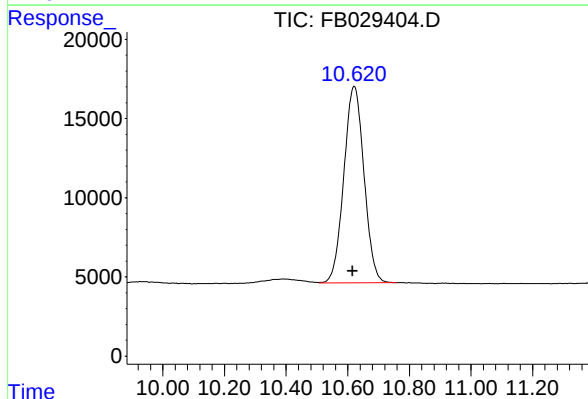


#6 Toluene

R.T.: 10.622 min
Delta R.T.: 0.006 min
Response: 563792
Conc: 28.56 ng/ml

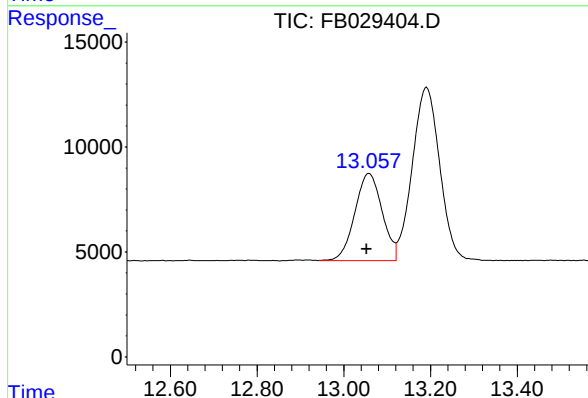


#7 Ethylbenzene

R.T.: 13.058 min
Delta R.T.: 0.006 min
Response: 181372
Conc: 9.74 ng/ml

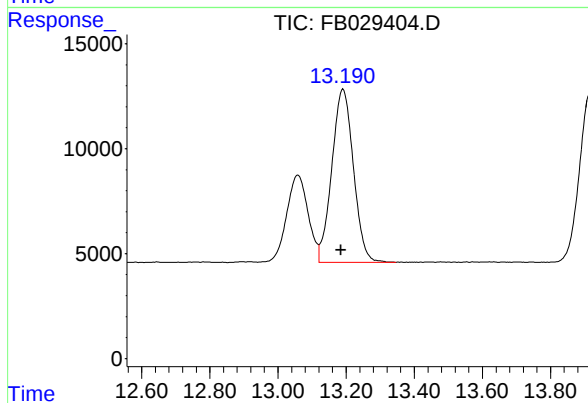


#8 m-Xylene

R.T.: 13.191 min
Delta R.T.: 0.006 min
Response: 362814
Conc: 19.50 ng/ml

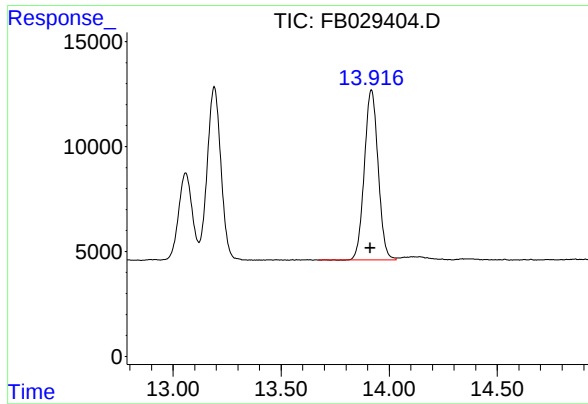

#9 O-Xylene

R.T.: 13.918 min
Delta R.T.: 0.006 min
Response: 359083
Conc: 19.50 ng/ml

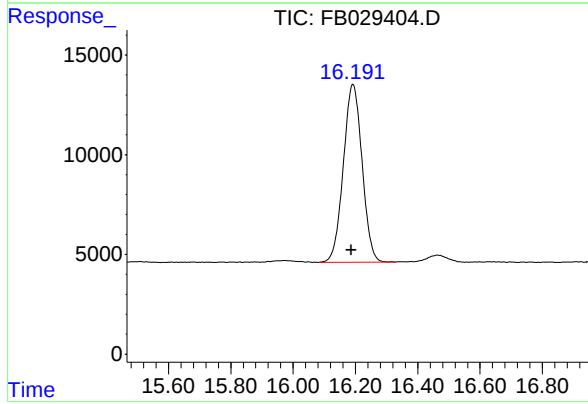

#10 1,2,4-Trimethylbenzene

R.T.: 16.193 min
Delta R.T.: 0.006 min
Response: 372404
Conc: 19.99 ng/ml