

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB030223\
 Data File : FB029397.D
 Signal(s) : FID2B.CH
 Acq On : 2 Mar 2023 11:51
 Operator : YP/AJ
 Sample : BSF0302S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Mar 02 23:38:52 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030123.M
 Quant Title :
 QLast Update : Wed Mar 01 12:30:24 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.794	274401	22.649 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.713	483824	31.532 ng/ml
2) t 2,2,4-Trimethylpentane	7.423	549419	32.616 ng/ml
3) t n-Heptane	7.752	184857	10.688 ng/ml
4) t Benzene	7.889	219101	10.794 ng/ml
6) t Toluene	10.622	639260	32.386 ng/ml
7) t Ethylbenzene	13.058	196805	10.571 ng/ml
8) t m-Xylene	13.191	388954	20.908 ng/ml
9) t O-Xylene	13.918	382759	20.787 ng/ml
10) t 1,2,4-Trimethylbenzene	16.193	375437	20.157 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB030223\
Data File : FB029397.D
Signal(s) : FID2B.CH
Acq On : 2 Mar 2023 11:51
Operator : YP/AJ
Sample : BSF0302S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Mar 02 23:38:52 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030123.M
Quant Title :
QLast Update : Wed Mar 01 12:30:24 2023
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

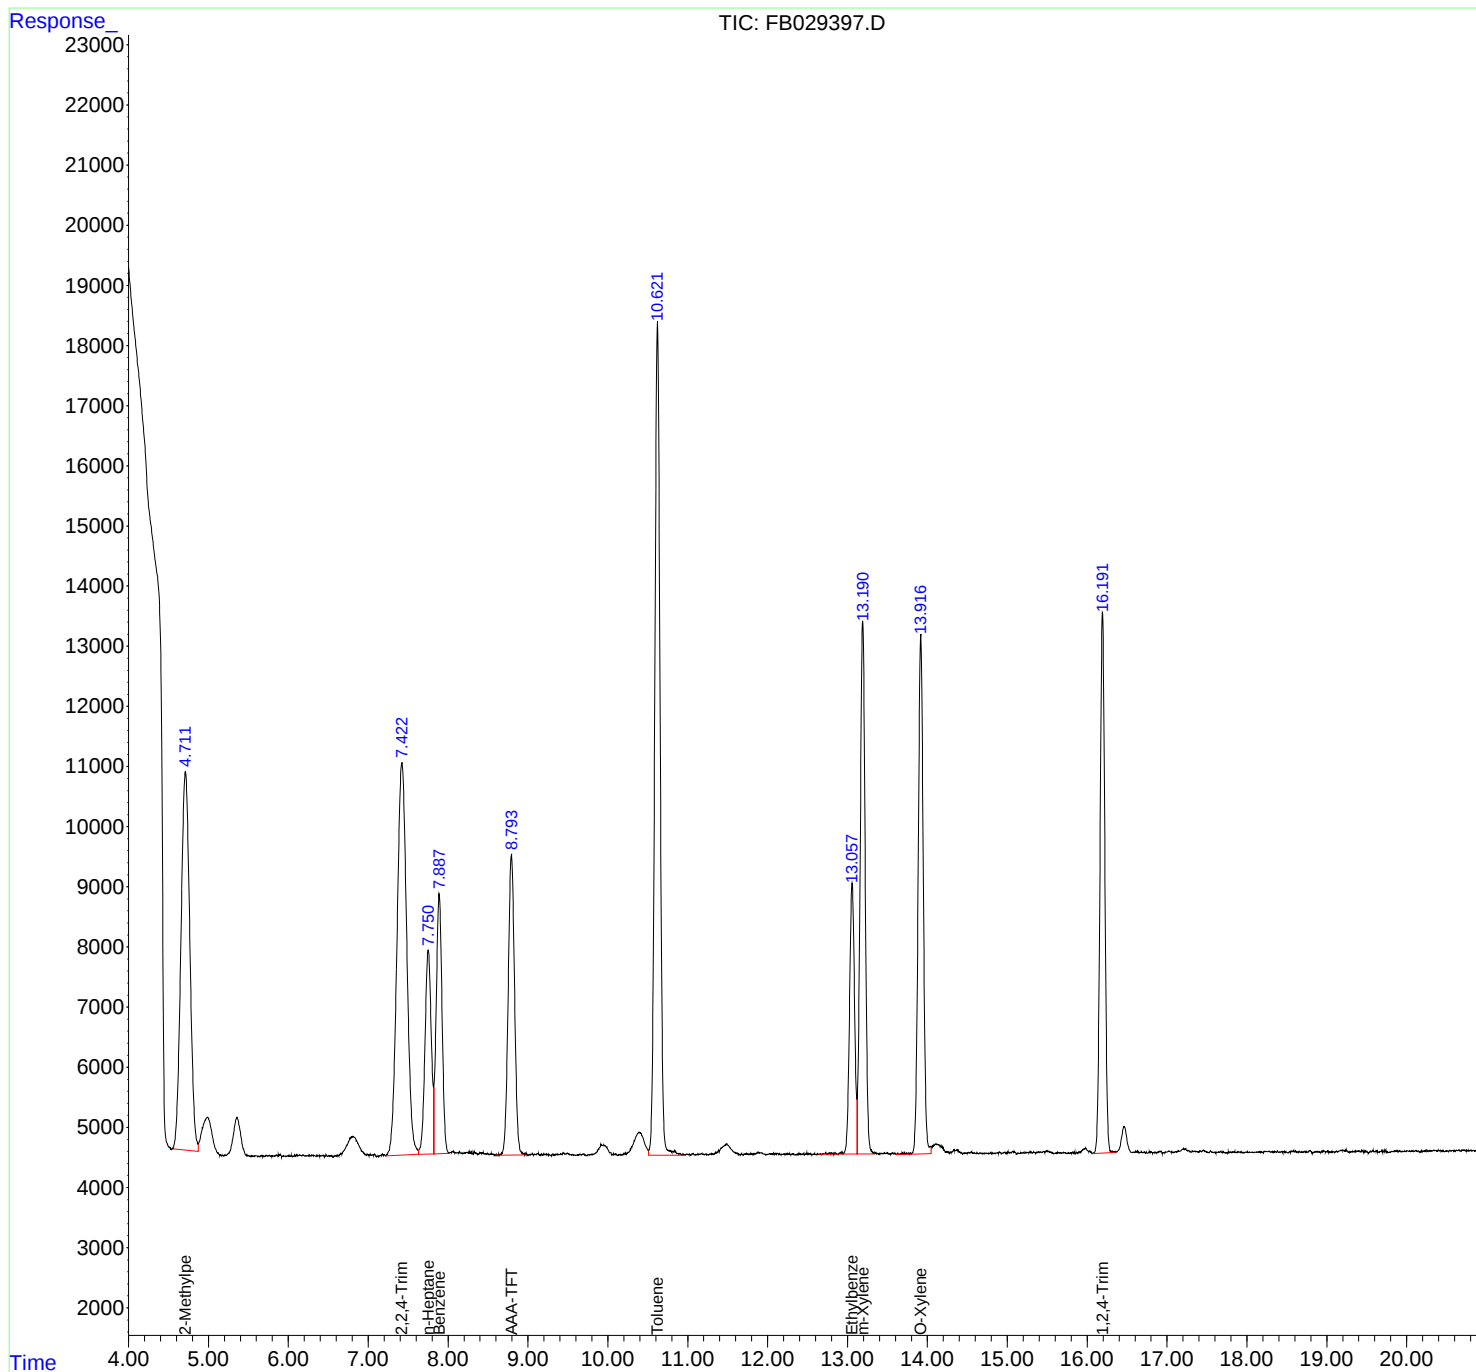

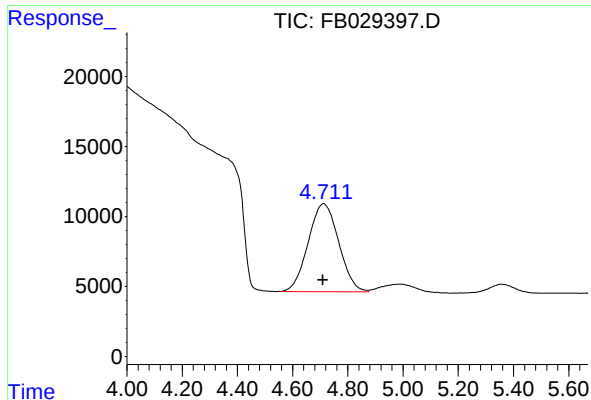


#1 2-Methylpentane

R.T.: 4.713 min
Delta R.T.: 0.003 min
Response: 483824
Conc: 31.53 ng/ml

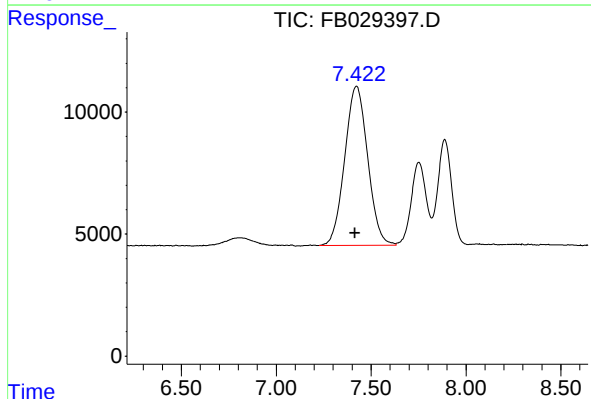


#2 2,2,4-Trimethylpentane

R.T.: 7.423 min
Delta R.T.: 0.007 min
Response: 549419
Conc: 32.62 ng/ml

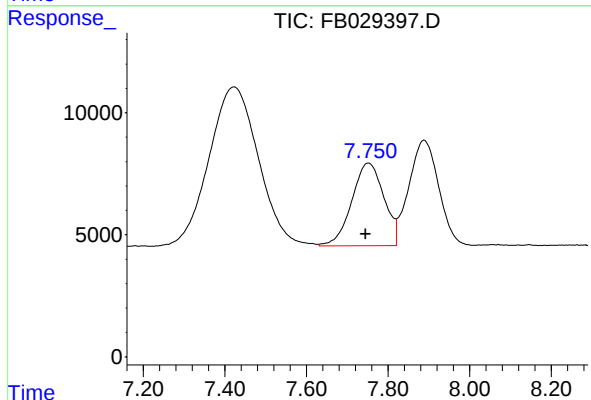


#3 n-Heptane

R.T.: 7.752 min
Delta R.T.: 0.006 min
Response: 184857
Conc: 10.69 ng/ml

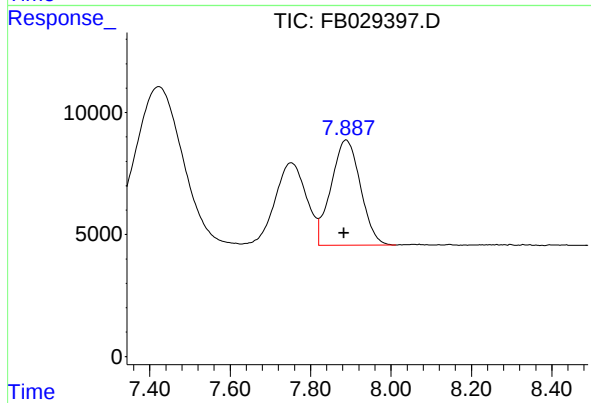


#4 Benzene

R.T.: 7.889 min
Delta R.T.: 0.006 min
Response: 219101
Conc: 10.79 ng/ml

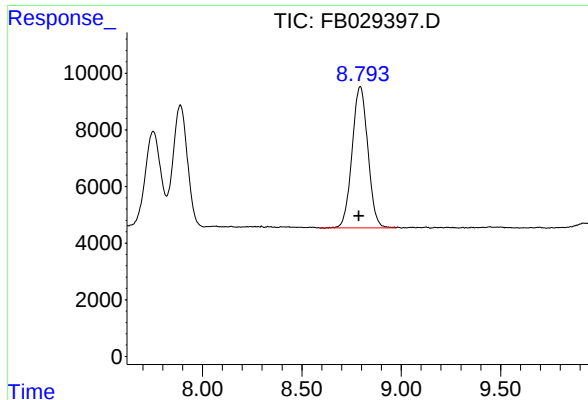


#5 AAA-TFT

R.T.: 8.794 min
Delta R.T.: 0.006 min
Response: 274401
Conc: 22.65 ng/ml

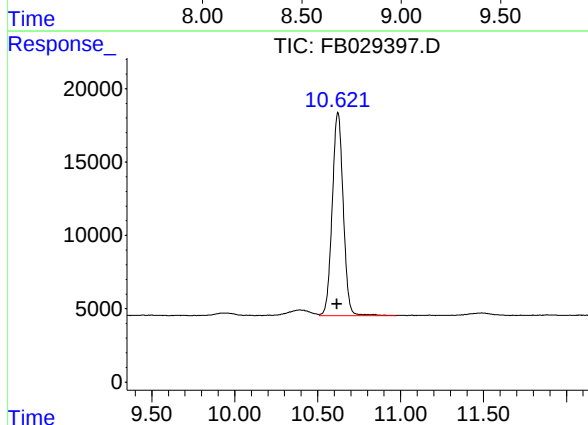


#6 Toluene

R.T.: 10.622 min
Delta R.T.: 0.006 min
Response: 639260
Conc: 32.39 ng/ml

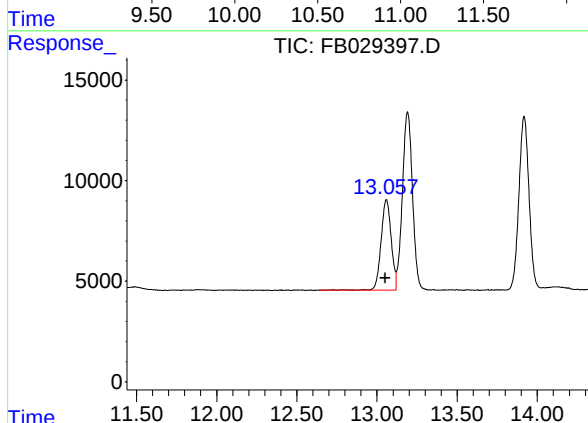


#7 Ethylbenzene

R.T.: 13.058 min
Delta R.T.: 0.006 min
Response: 196805
Conc: 10.57 ng/ml

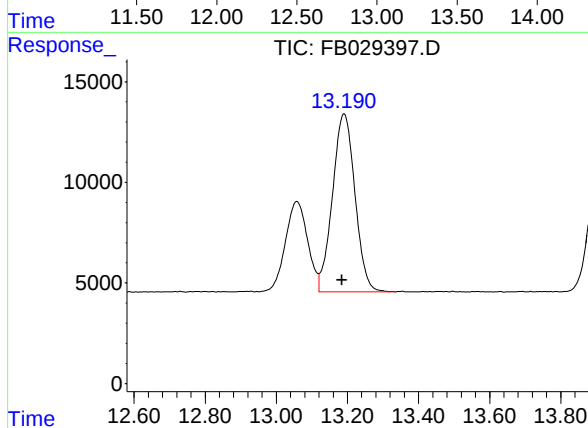


#8 m-Xylene

R.T.: 13.191 min
Delta R.T.: 0.006 min
Response: 388954
Conc: 20.91 ng/ml

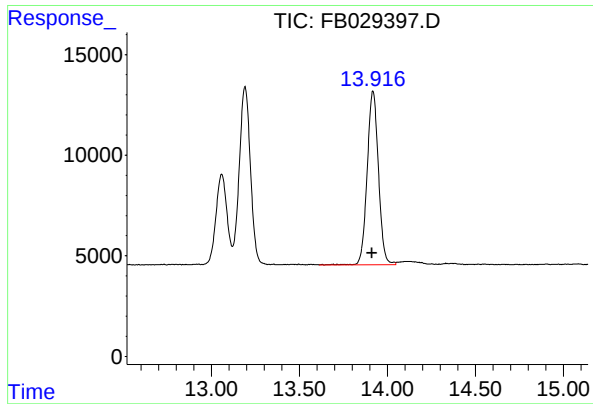

#9 O-Xylene

R.T.: 13.918 min
Delta R.T.: 0.006 min
Response: 382759
Conc: 20.79 ng/ml

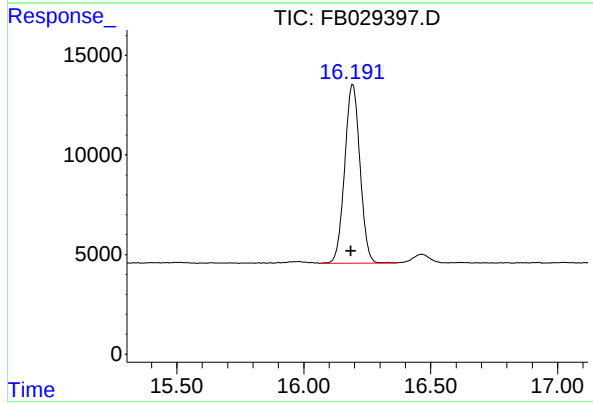

#10 1,2,4-Trimethylbenzene

R.T.: 16.193 min
Delta R.T.: 0.006 min
Response: 375437
Conc: 20.16 ng/ml