

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB030321\
 Data File : FB025490.D
 Signal(s) : FID2B.CH
 Acq On : 3 Mar 2021 11:47
 Operator : DD/AJ
 Sample : M1537-01MS
 Misc : 5.08g/5.00ml DI WATER
 ALS Vial : 5 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Mar 04 00:01:08 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB021921.M
 Quant Title :
 QLast Update : Mon Feb 22 11:51:04 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.802	507341	20.001 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.691	925680	26.264 ng/ml
2) t	2,2,4-Trimethylpentane	7.420	961734	25.900 ng/ml
3) t	n-Heptane	7.760	309940	8.562 ng/ml
4) t	Benzene	7.896	434816	9.412 ng/ml
6) t	Toluene	10.634	1238228	27.695 ng/ml
7) t	Ethylbenzene	13.074	371704	9.210 ng/ml
8) t	m-Xylene	13.207	738971	18.369 ng/ml
9) t	O-Xylene	13.934	716415	18.508 ng/ml
10) t	1,2,4-Trimethylbenzene	16.213	590769	17.599 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB030321\
Data File : FB025490.D
Signal(s) : FID2B.CH
Acq On : 3 Mar 2021 11:47
Operator : DD/AJ
Sample : M1537-01MS
Misc : 5.08g/5.00ml DI WATER
ALS Vial : 5 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Mar 04 00:01:08 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB021921.M
Quant Title :
QLast Update : Mon Feb 22 11:51:04 2021
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

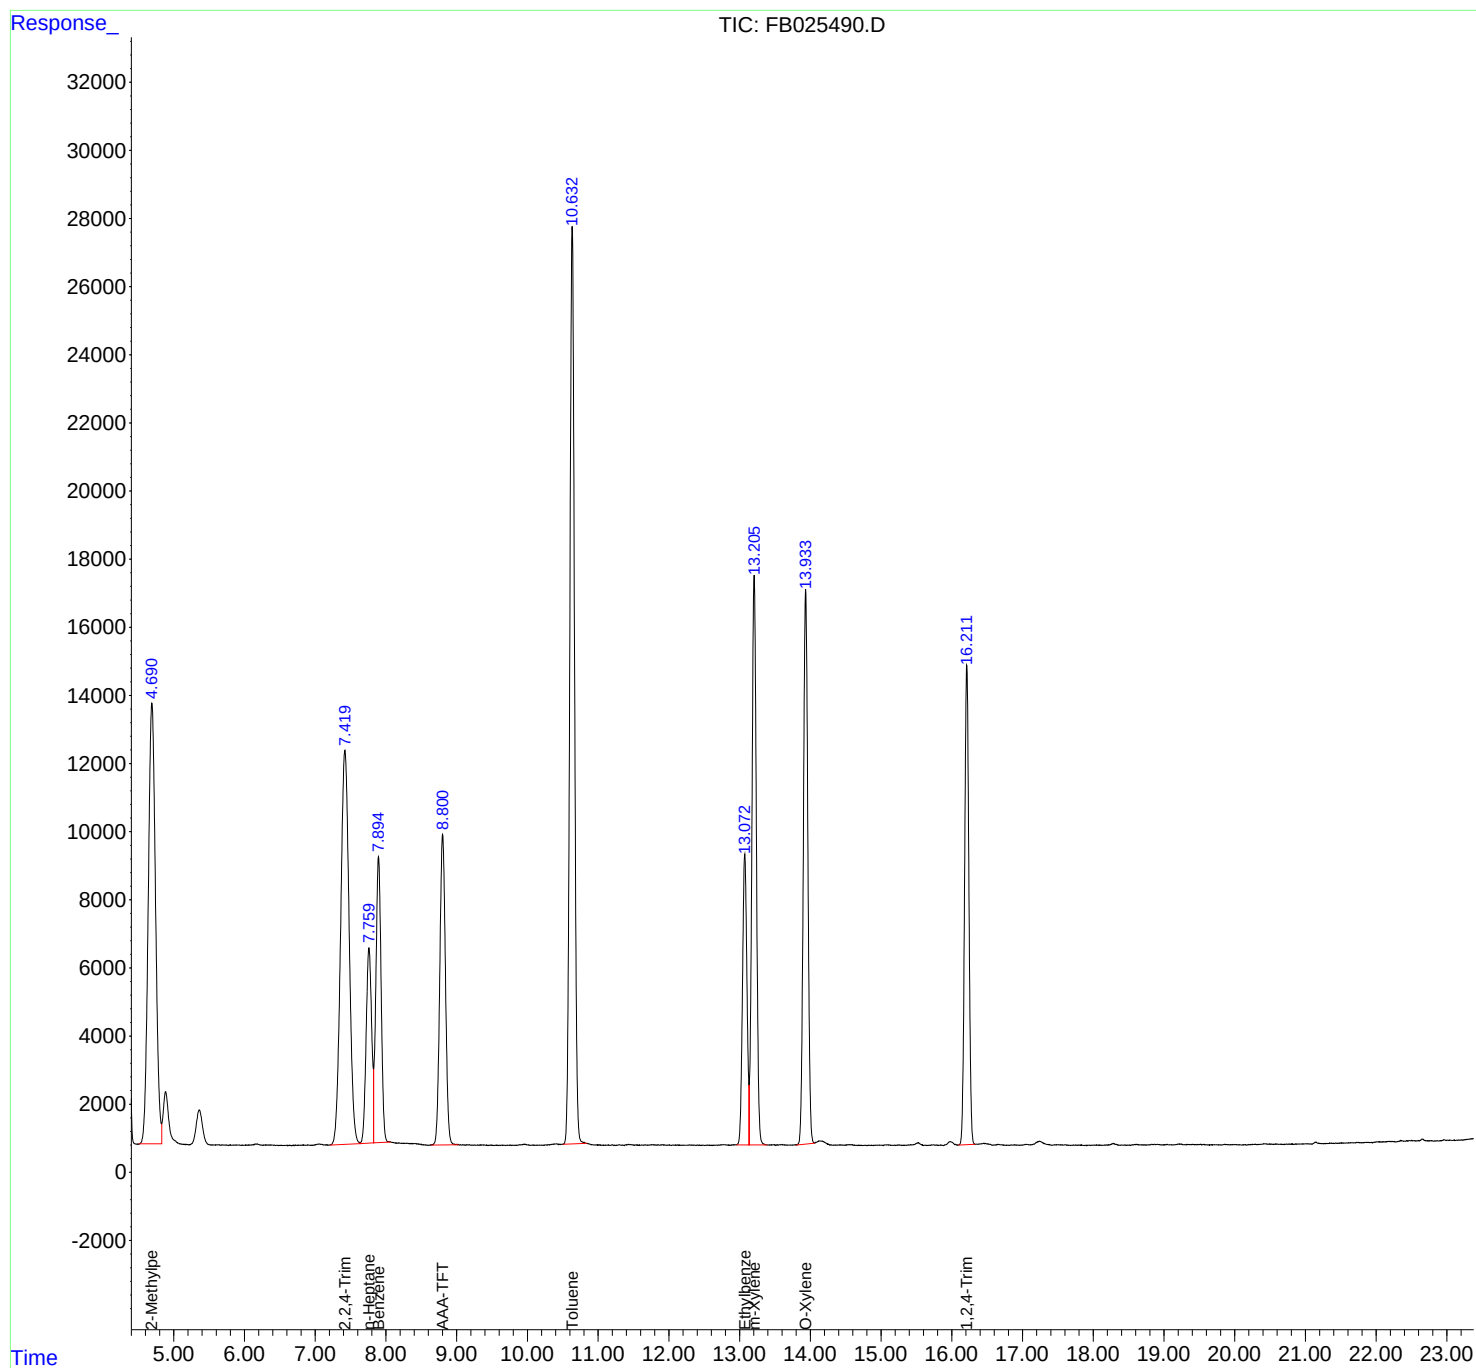

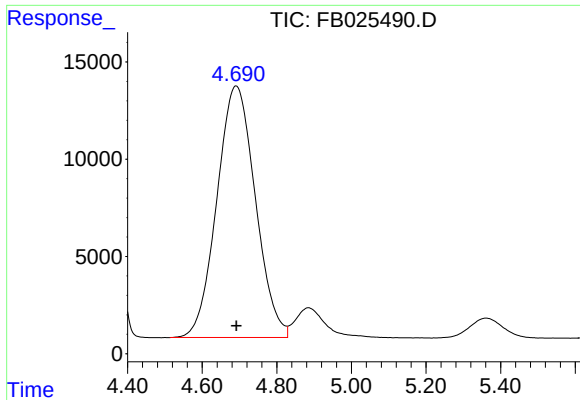


#1 2-Methylpentane

R.T.: 4.691 min
Delta R.T.: 0.000 min
Response: 925680
Conc: 26.26 ng/ml

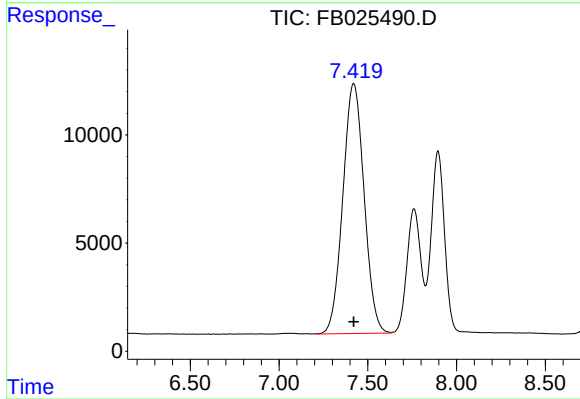


#2 2,2,4-Trimethylpentane

R.T.: 7.420 min
Delta R.T.: -0.001 min
Response: 961734
Conc: 25.90 ng/ml

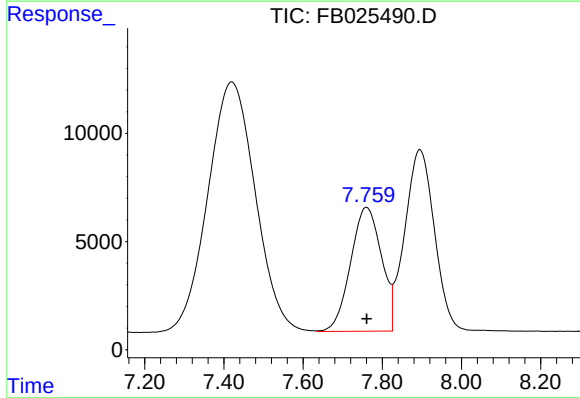


#3 n-Heptane

R.T.: 7.760 min
Delta R.T.: 0.000 min
Response: 309940
Conc: 8.56 ng/ml

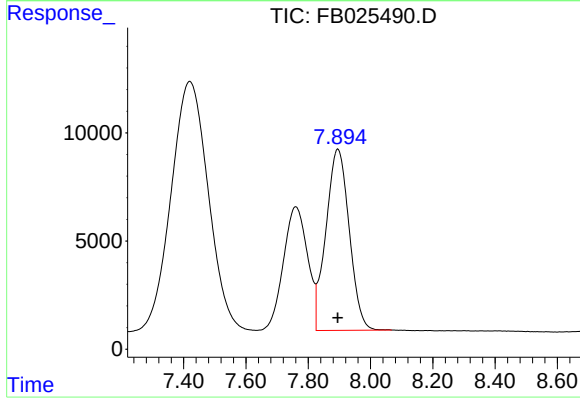


#4 Benzene

R.T.: 7.896 min
Delta R.T.: 0.000 min
Response: 434816
Conc: 9.41 ng/ml

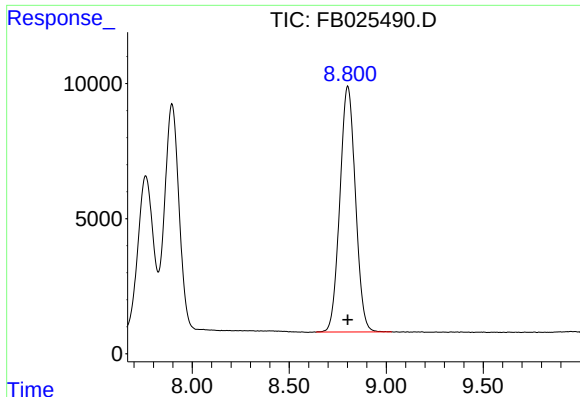


#5 AAA-TFT

R.T.: 8.802 min
Delta R.T.: 0.000 min
Response: 507341
Conc: 20.00 ng/ml

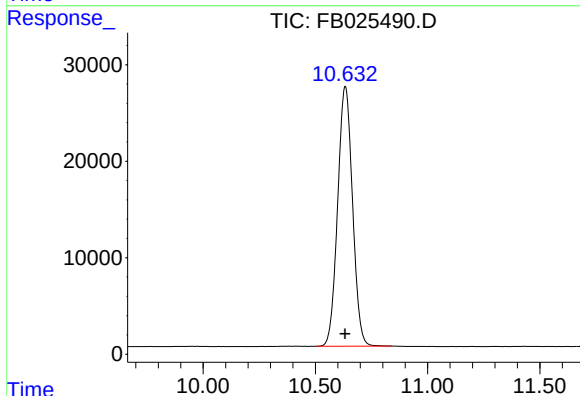


#6 Toluene

R.T.: 10.634 min
Delta R.T.: 0.000 min
Response: 1238228
Conc: 27.70 ng/ml

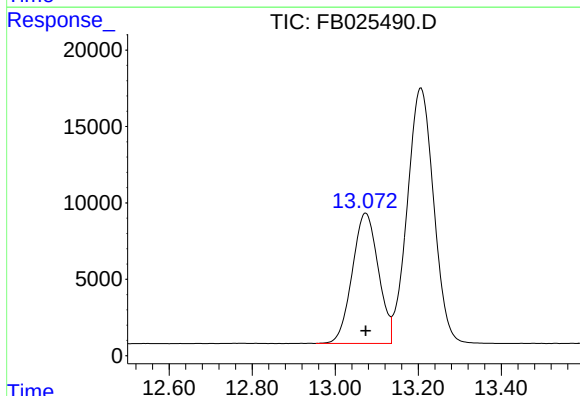


#7 Ethylbenzene

R.T.: 13.074 min
Delta R.T.: 0.000 min
Response: 371704
Conc: 9.21 ng/ml

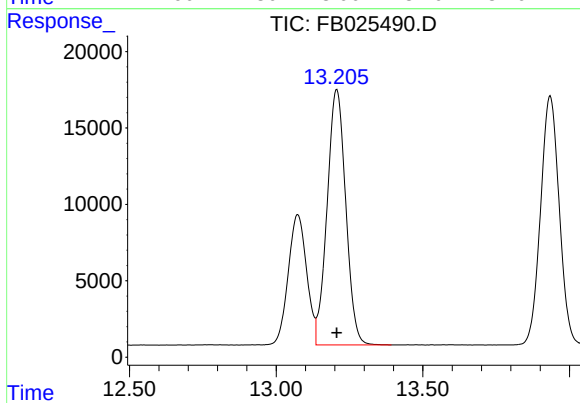


#8 m-Xylene

R.T.: 13.207 min
Delta R.T.: 0.000 min
Response: 738971
Conc: 18.37 ng/ml

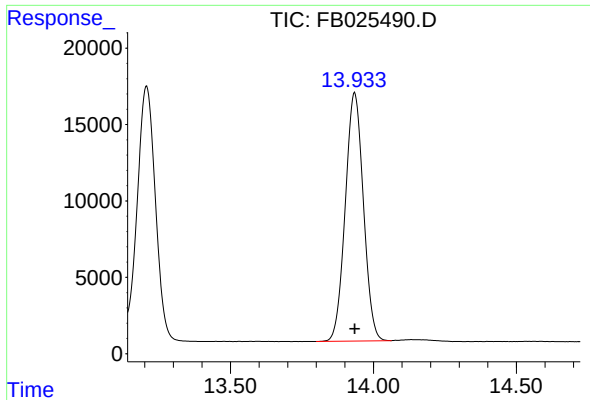

#9 O-Xylene

R.T.: 13.934 min
Delta R.T.: 0.000 min
Response: 716415
Conc: 18.51 ng/ml

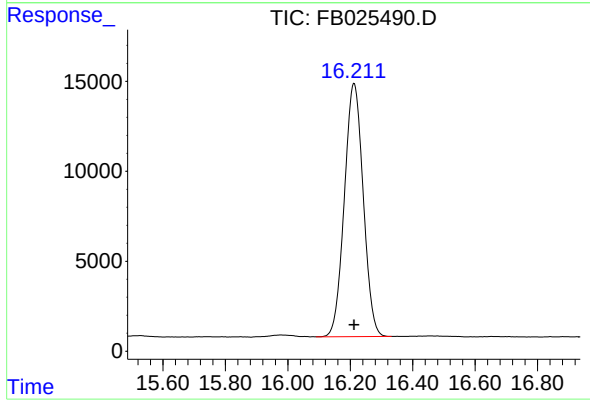

#10 1,2,4-Trimethylbenzene

R.T.: 16.213 min
Delta R.T.: 0.000 min
Response: 590769
Conc: 17.60 ng/ml