

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB030321\
 Data File : FB025491.D
 Signal(s) : FID2B.CH
 Acq On : 3 Mar 2021 12:18
 Operator : DD/AJ
 Sample : M1537-01MSD
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Mar 04 00:01:19 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB021921.M
 Quant Title :
 QLast Update : Mon Feb 22 11:51:04 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.802	511974	20.184 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.689	883502	25.068 ng/ml
2) t 2,2,4-Trimethylpentane	7.420	899459	24.223 ng/ml
3) t n-Heptane	7.760	292317	8.075 ng/ml
4) t Benzene	7.895	421774	9.130 ng/ml
6) t Toluene	10.634	1194304	26.713 ng/ml
7) t Ethylbenzene	13.074	362818	8.989 ng/ml
8) t m-Xylene	13.207	720322	17.906 ng/ml
9) t O-Xylene	13.935	692819	17.899 ng/ml
10) t 1,2,4-Trimethylbenzene	16.213	574177	17.105 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB030321\
Data File : FB025491.D
Signal(s) : FID2B.CH
Acq On : 3 Mar 2021 12:18
Operator : DD/AJ
Sample : M1537-01MSD
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Mar 04 00:01:19 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB021921.M
Quant Title :
QLast Update : Mon Feb 22 11:51:04 2021
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

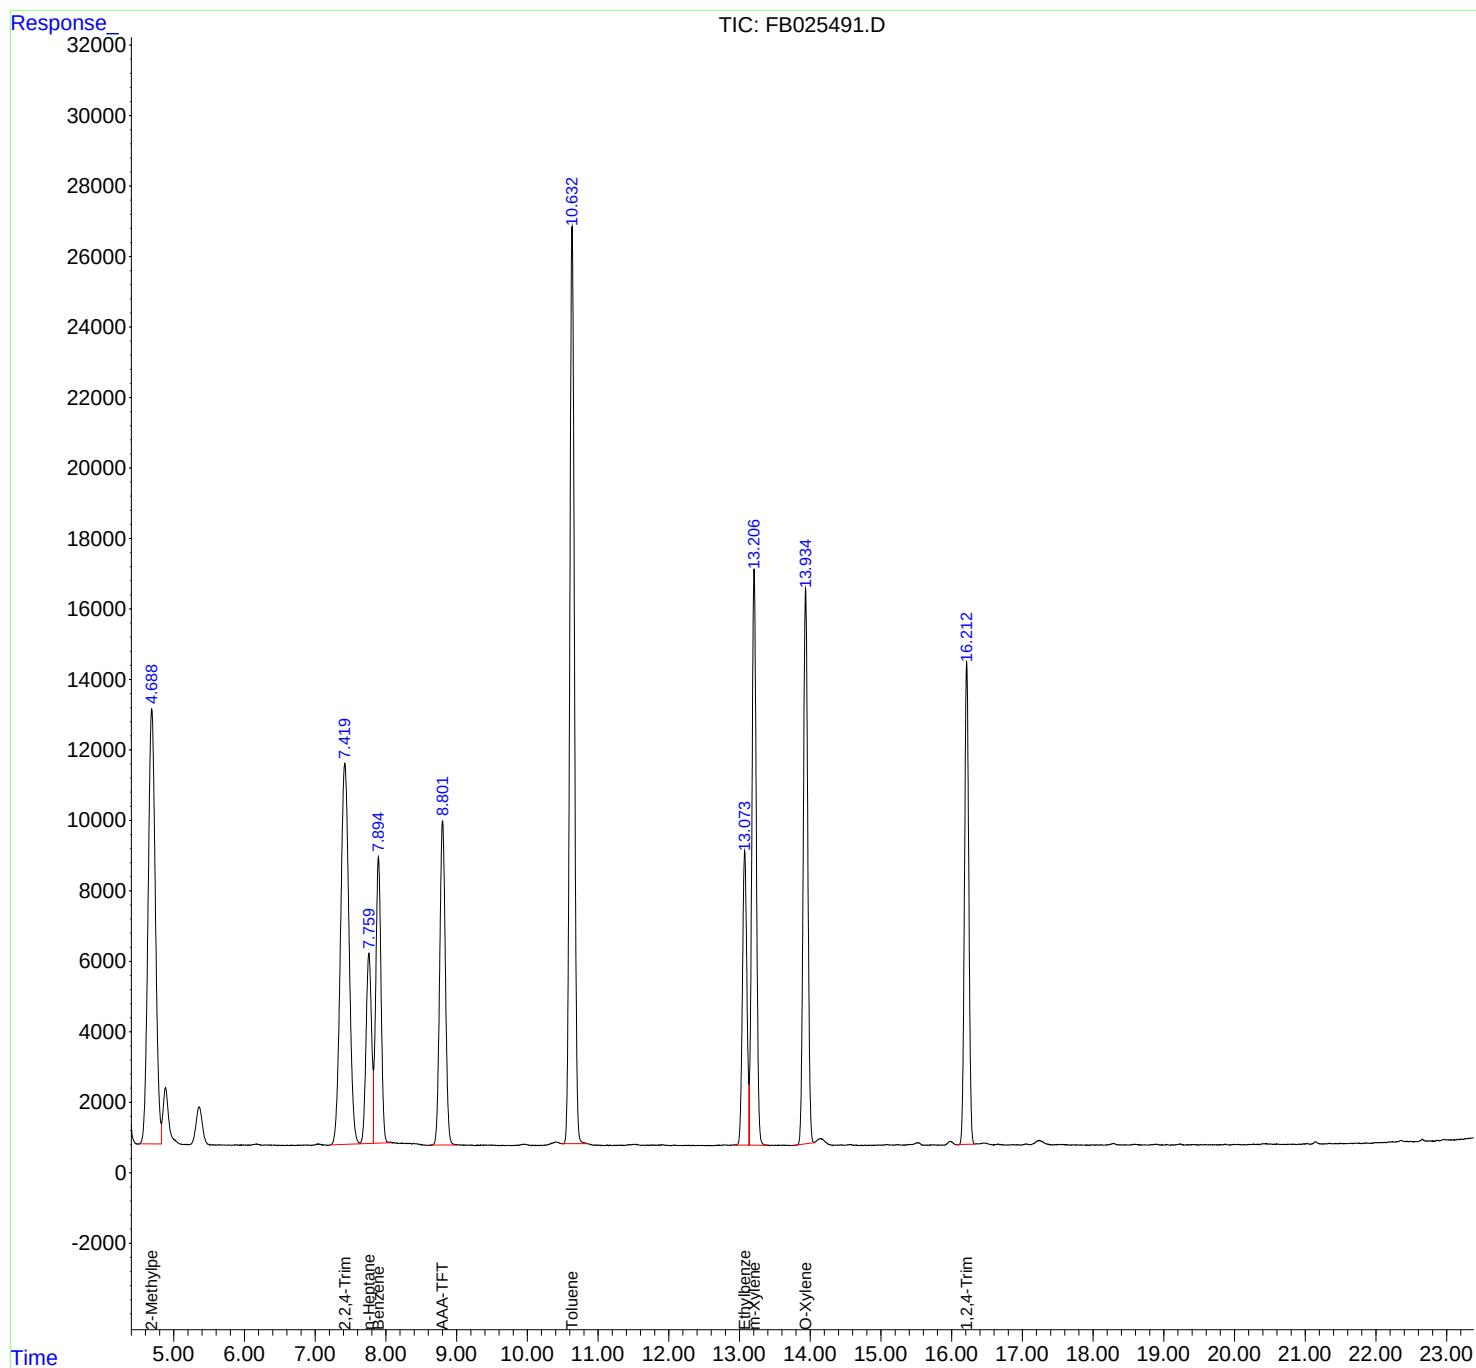

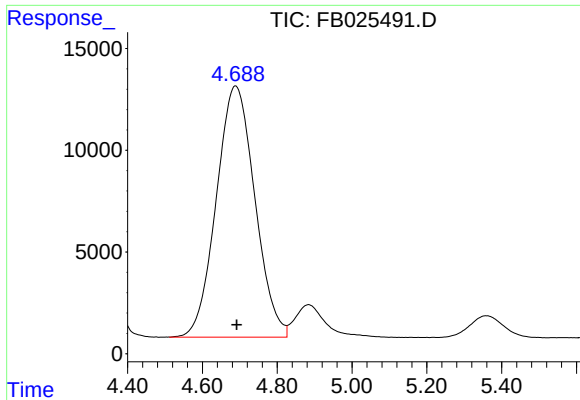


#1 2-Methylpentane

R.T.: 4.689 min
Delta R.T.: -0.003 min
Response: 883502
Conc: 25.07 ng/ml

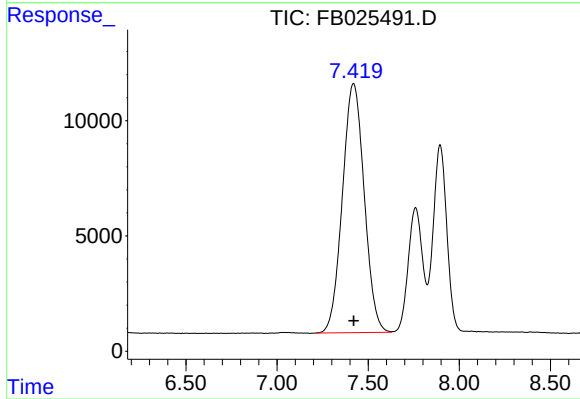


#2 2,2,4-Trimethylpentane

R.T.: 7.420 min
Delta R.T.: -0.002 min
Response: 899459
Conc: 24.22 ng/ml

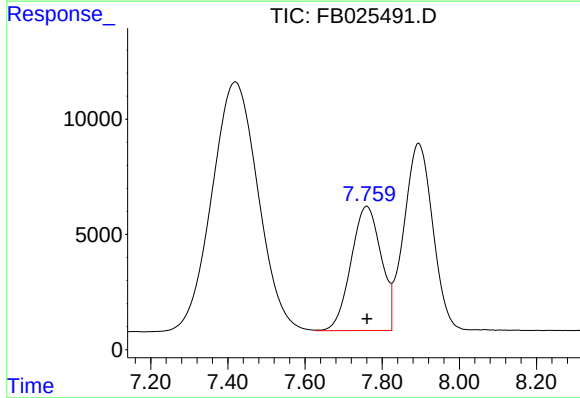


#3 n-Heptane

R.T.: 7.760 min
Delta R.T.: 0.000 min
Response: 292317
Conc: 8.07 ng/ml

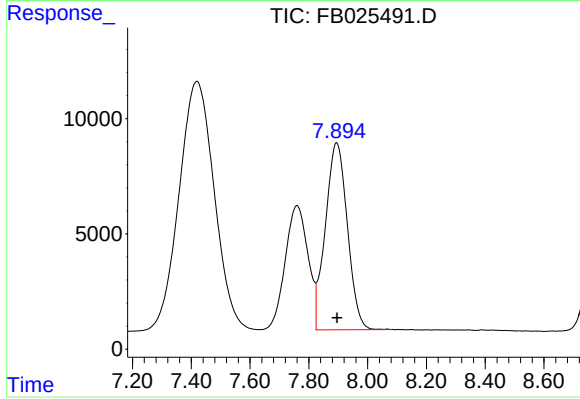


#4 Benzene

R.T.: 7.895 min
Delta R.T.: 0.000 min
Response: 421774
Conc: 9.13 ng/ml

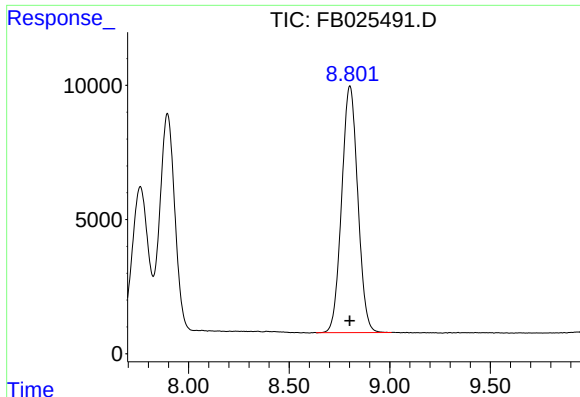


#5 AAA-TFT

R.T.: 8.802 min
Delta R.T.: 0.000 min
Response: 511974
Conc: 20.18 ng/ml

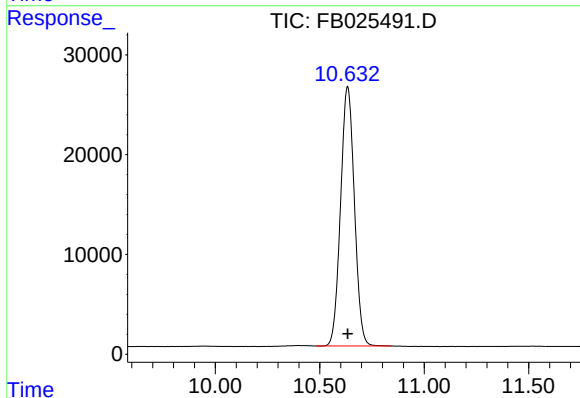


#6 Toluene

R.T.: 10.634 min
Delta R.T.: 0.000 min
Response: 1194304
Conc: 26.71 ng/ml

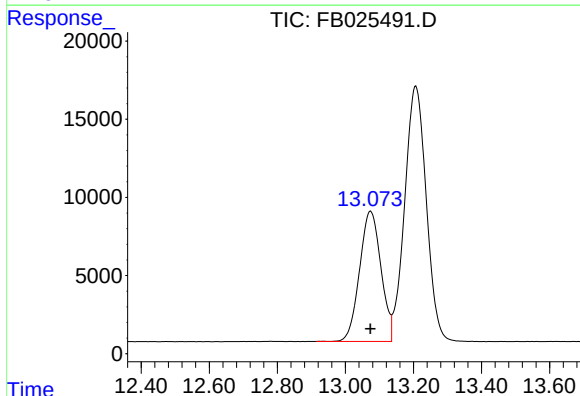


#7 Ethylbenzene

R.T.: 13.074 min
Delta R.T.: 0.000 min
Response: 362818
Conc: 8.99 ng/ml

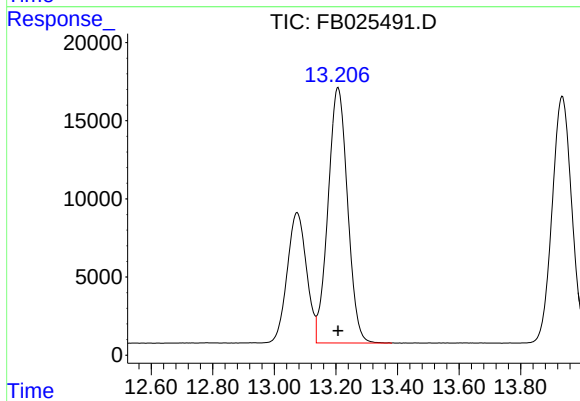


#8 m-Xylene

R.T.: 13.207 min
Delta R.T.: 0.000 min
Response: 720322
Conc: 17.91 ng/ml

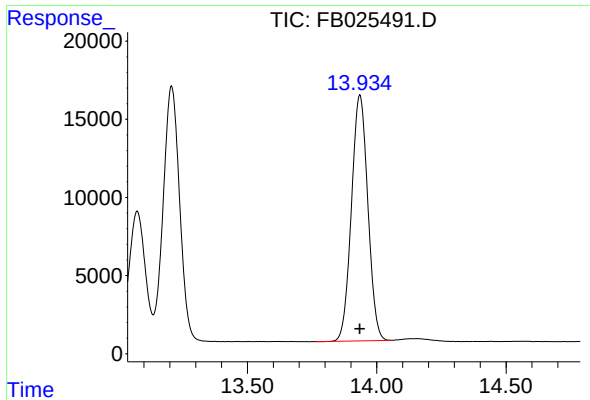

#9 O-Xylene

R.T.: 13.935 min
Delta R.T.: 0.000 min
Response: 692819
Conc: 17.90 ng/ml

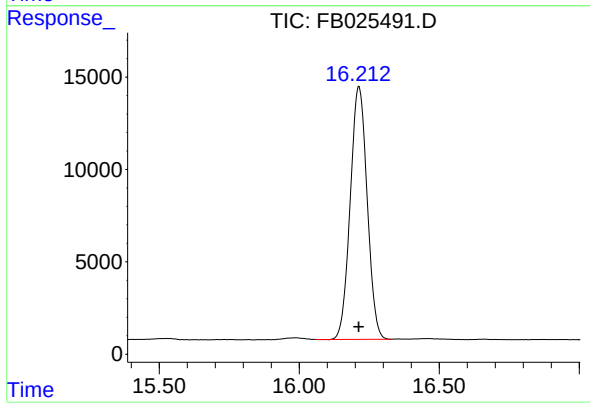

#10 1,2,4-Trimethylbenzene

R.T.: 16.213 min
Delta R.T.: 0.001 min
Response: 574177
Conc: 17.10 ng/ml