

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB030321\
 Data File : FB025488.D
 Signal(s) : FID2B.CH
 Acq On : 3 Mar 2021 10:43
 Operator : DD/AJ
 Sample : BSF0303S1
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: SAMPLE.e
 Quant Time: Mar 04 00:00:52 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB021921.M
 Quant Title :
 QLast Update : Mon Feb 22 11:51:04 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.802	558524	22.019 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.691	997060	28.289 ng/ml
2) t	2,2,4-Trimethylpentane	7.421	1121001	30.190 ng/ml
3) t	n-Heptane	7.760	365210	10.088 ng/ml
4) t	Benzene	7.895	449016	9.720 ng/ml
6) t	Toluene	10.633	1285681	28.757 ng/ml
7) t	Ethylbenzene	13.074	392804	9.732 ng/ml
8) t	m-Xylene	13.206	790929	19.661 ng/ml
9) t	O-Xylene	13.935	760040	19.635 ng/ml
10) t	1,2,4-Trimethylbenzene	16.212	659557	19.648 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB030321\
Data File : FB025488.D
Signal(s) : FID2B.CH
Acq On : 3 Mar 2021 10:43
Operator : DD/AJ
Sample : BSF0303S1
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: SAMPLE.e
Quant Time: Mar 04 00:00:52 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB021921.M
Quant Title :
QLast Update : Mon Feb 22 11:51:04 2021
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

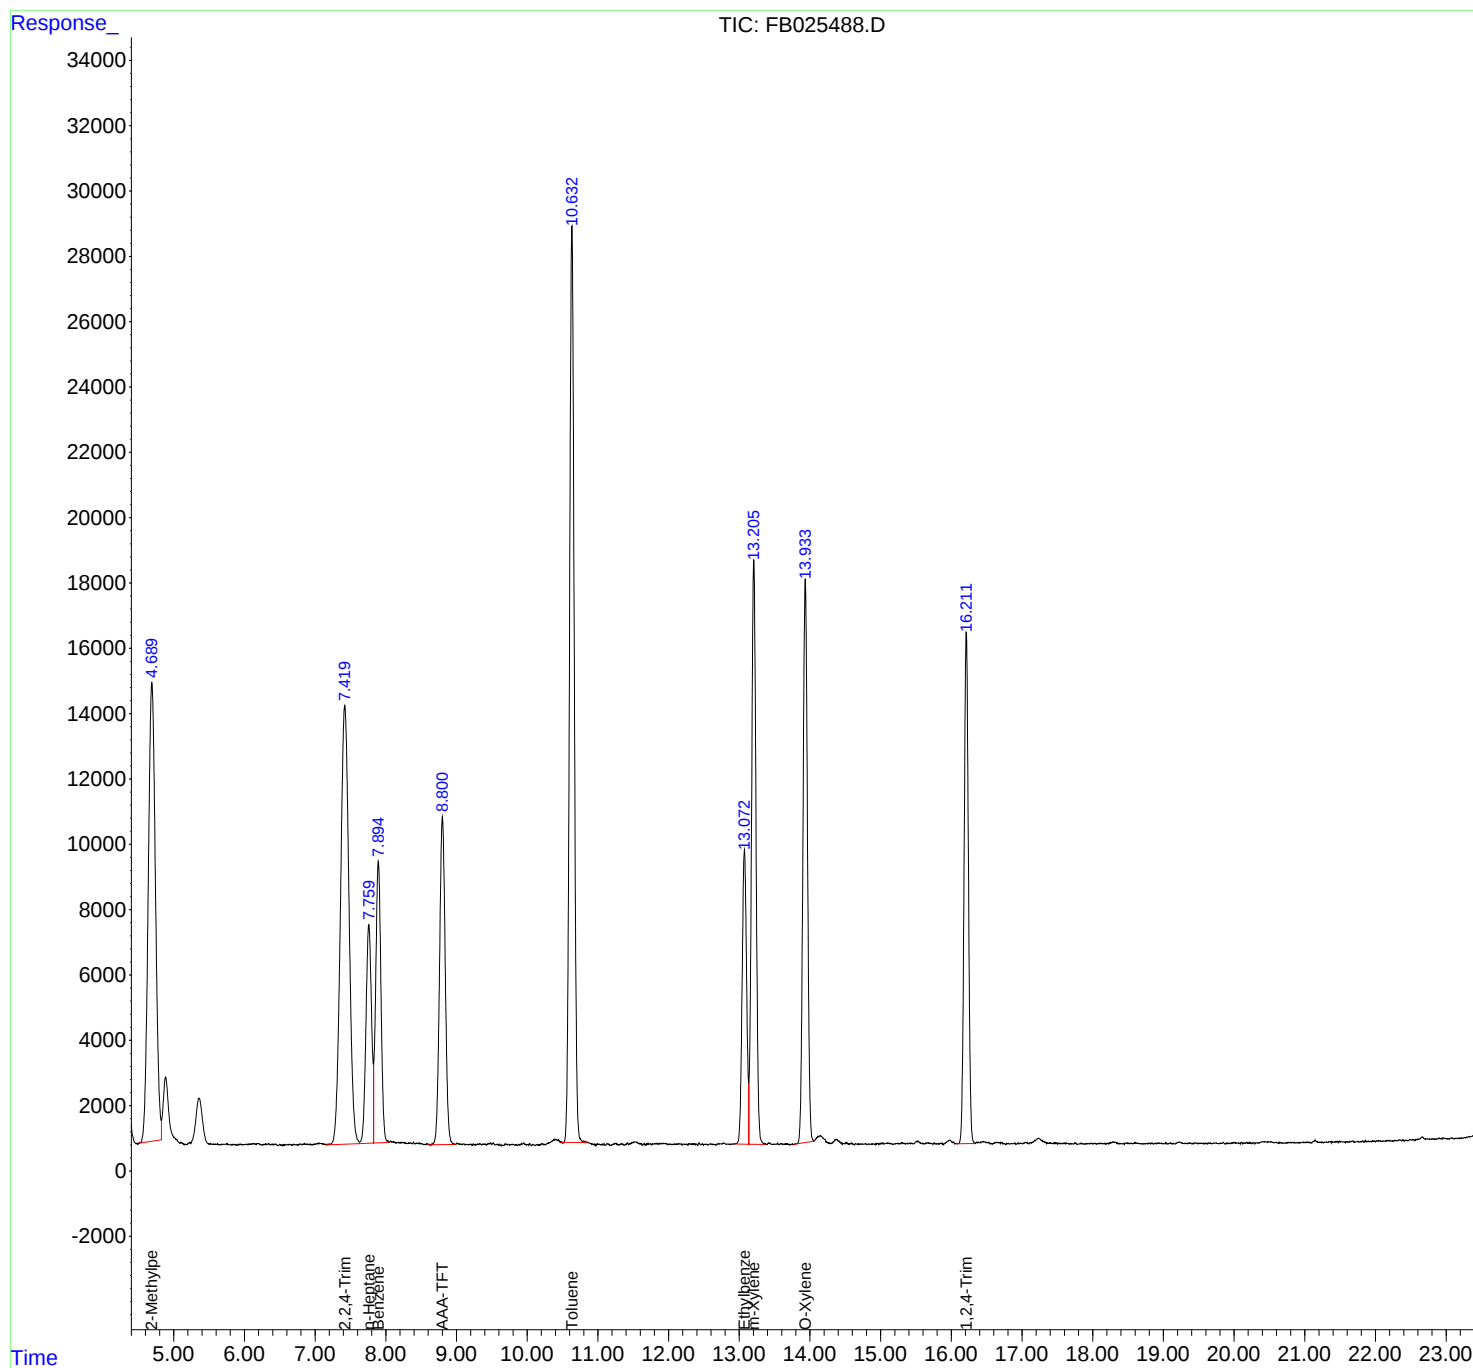

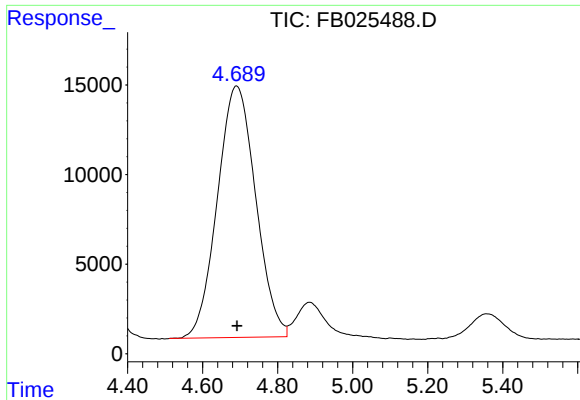


#1 2-Methylpentane

R.T.: 4.691 min
Delta R.T.: -0.001 min
Response: 997060
Conc: 28.29 ng/ml

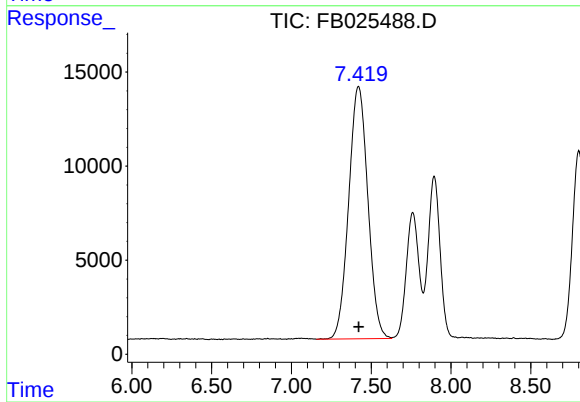


#2 2,2,4-Trimethylpentane

R.T.: 7.421 min
Delta R.T.: 0.000 min
Response: 1121001
Conc: 30.19 ng/ml

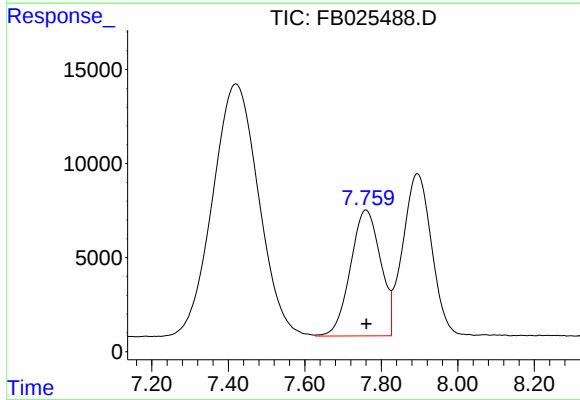


#3 n-Heptane

R.T.: 7.760 min
Delta R.T.: 0.000 min
Response: 365210
Conc: 10.09 ng/ml

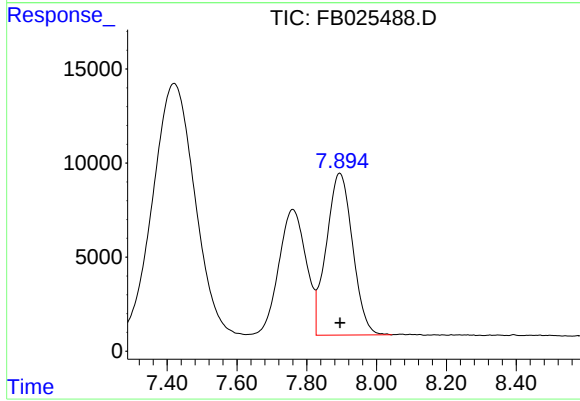


#4 Benzene

R.T.: 7.895 min
Delta R.T.: 0.000 min
Response: 449016
Conc: 9.72 ng/ml

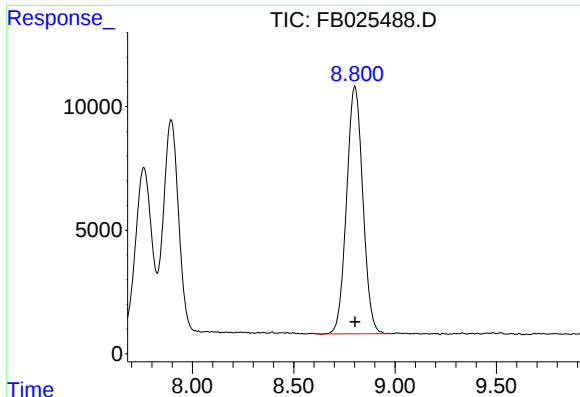


#5 AAA-TFT

R.T.: 8.802 min
Delta R.T.: 0.000 min
Response: 558524
Conc: 22.02 ng/ml

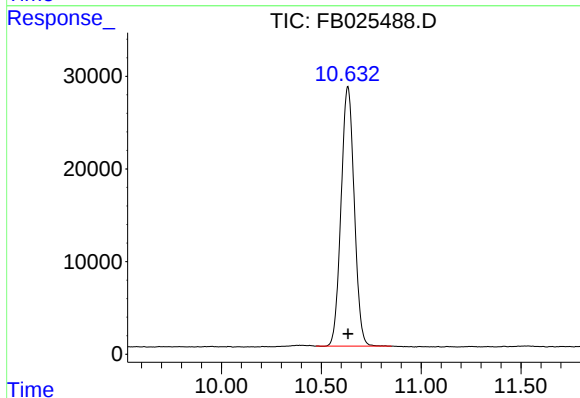


#6 Toluene

R.T.: 10.633 min
Delta R.T.: 0.000 min
Response: 1285681
Conc: 28.76 ng/ml

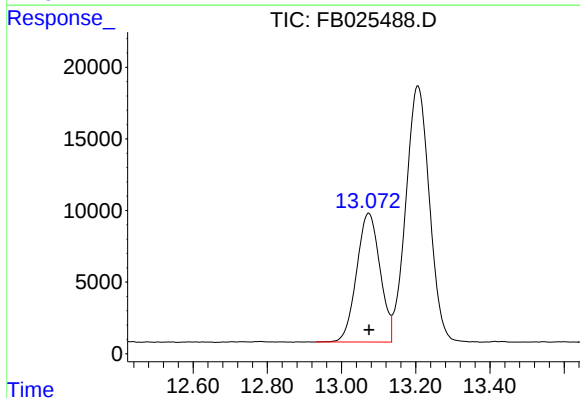


#7 Ethylbenzene

R.T.: 13.074 min
Delta R.T.: 0.000 min
Response: 392804
Conc: 9.73 ng/ml

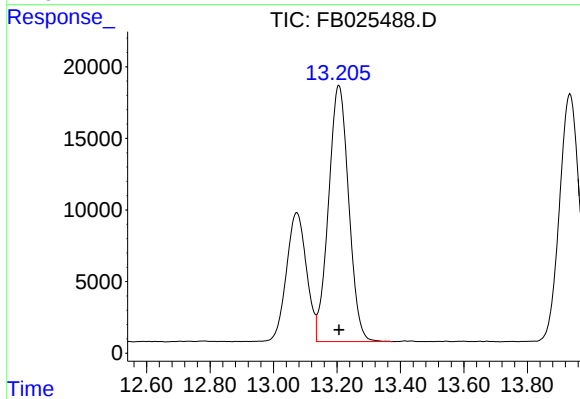


#8 m-Xylene

R.T.: 13.206 min
Delta R.T.: 0.000 min
Response: 790929
Conc: 19.66 ng/ml

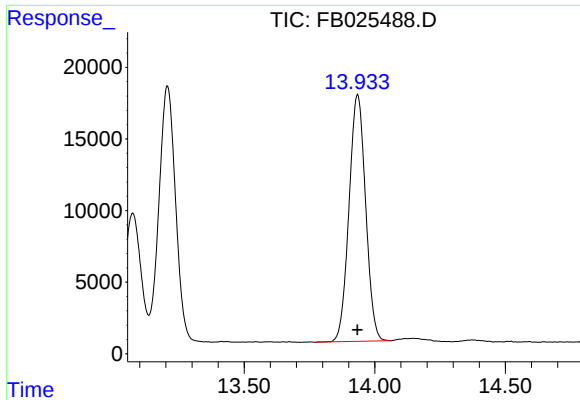

#9 O-Xylene

R.T.: 13.935 min
Delta R.T.: 0.000 min
Response: 760040
Conc: 19.64 ng/ml

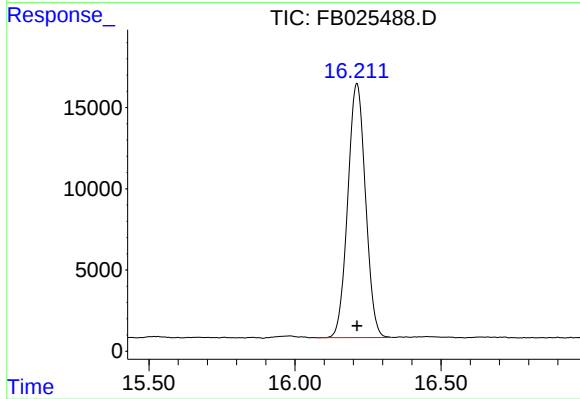

#10 1,2,4-Trimethylbenzene

R.T.: 16.212 min
Delta R.T.: 0.000 min
Response: 659557
Conc: 19.65 ng/ml