

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB030325\
 Data File : FB031527.D
 Signal(s) : FID2B.CH
 Acq On : 3 Mar 2025 12:02
 Operator : YP/AJ
 Sample : BSF0303S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0303S1

Integration File: SAMPLE.e
 Quant Time: Mar 04 00:18:53 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB021125.M
 Quant Title :
 QLast Update : Tue Feb 11 12:33:57 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.791	504773	21.471 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.722	749742	23.471 ng/ml
2) t 2,2,4-Trimethylpentane	7.422	981150	25.216 ng/ml
3) t n-Heptane	7.753	290497	8.434 ng/ml
4) t Benzene	7.893	406179	9.149 ng/ml
6) t Toluene	10.619	1147791	27.942 ng/ml
7) t Ethylbenzene	13.057	338939	9.336 ng/ml
8) t m-Xylene	13.190	742697	18.901 ng/ml
9) t O-Xylene	13.918	706790	18.896 ng/ml
10) t 1,2,4-Trimethylbenzene	16.194	547036	18.460 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB030325\
Data File : FB031527.D
Signal(s) : FID2B.CH
Acq On : 3 Mar 2025 12:02
Operator : YP/AJ
Sample : BSF0303S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0303S1

Integration File: SAMPLE.e
Quant Time: Mar 04 00:18:53 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB021125.M
Quant Title :
QLast Update : Tue Feb 11 12:33:57 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

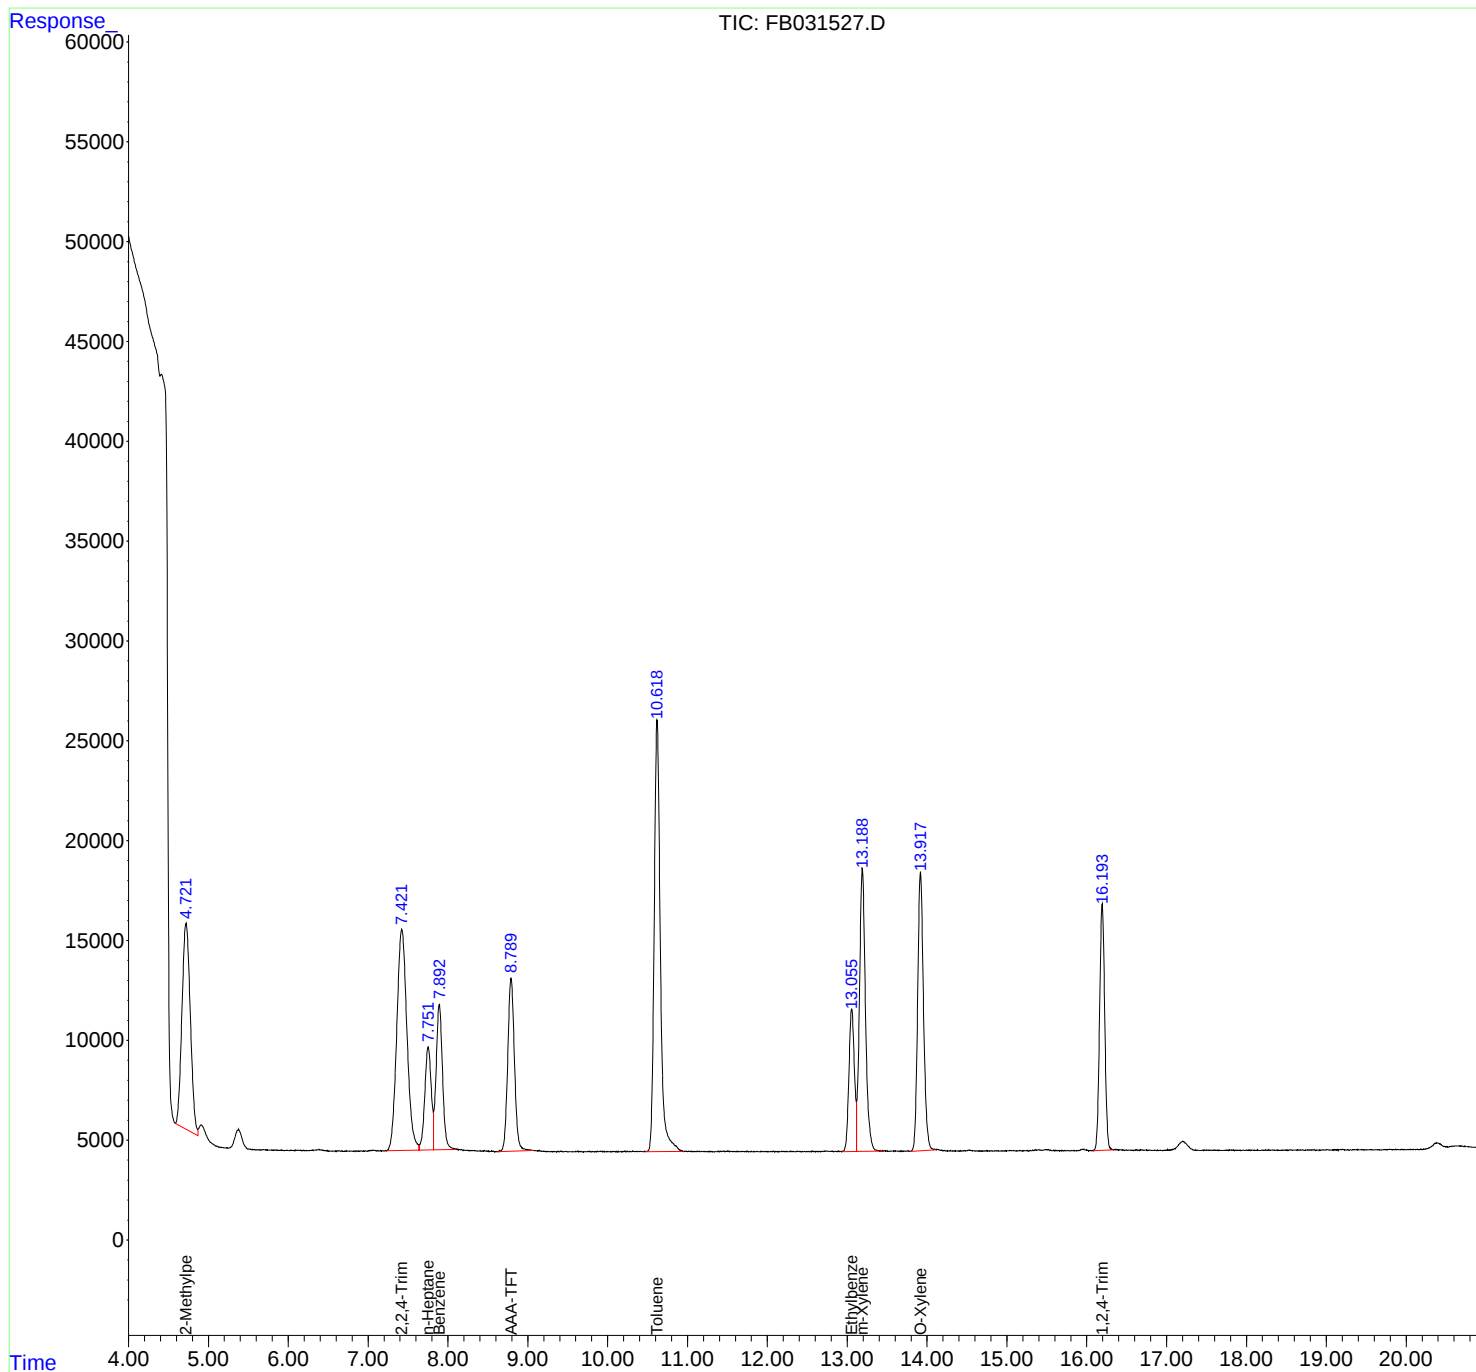


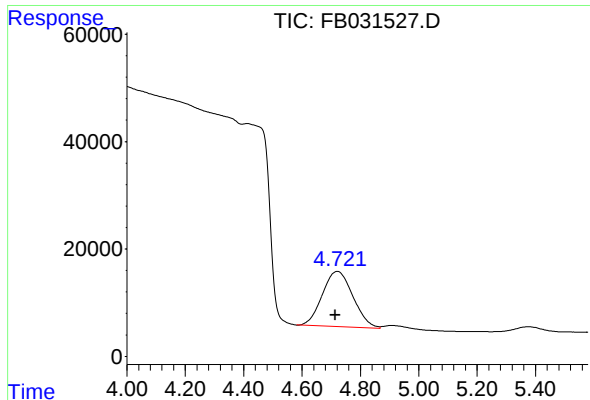

#1 2-Methylpentane


R.T.: 4.722 min
Delta R.T.: 0.008 min
Response: 749742
Conc: 23.47 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0303S1

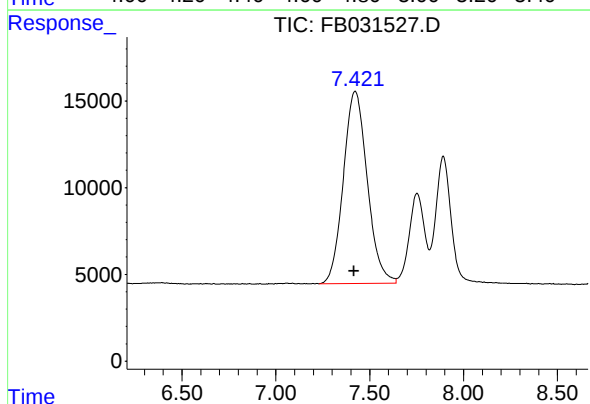


#2 2,2,4-Trimethylpentane

R.T.: 7.422 min
Delta R.T.: 0.006 min
Response: 981150
Conc: 25.22 ng/ml

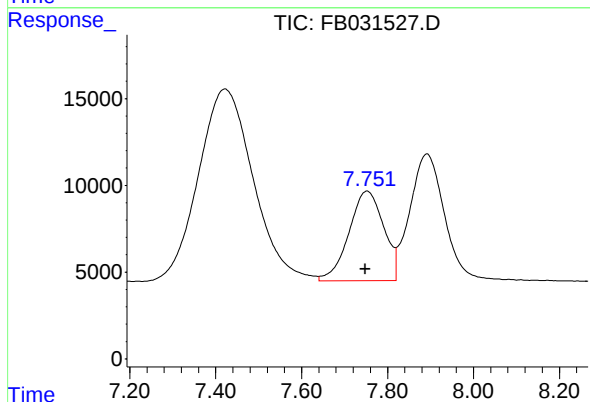


#3 n-Heptane

R.T.: 7.753 min
Delta R.T.: 0.005 min
Response: 290497
Conc: 8.43 ng/ml

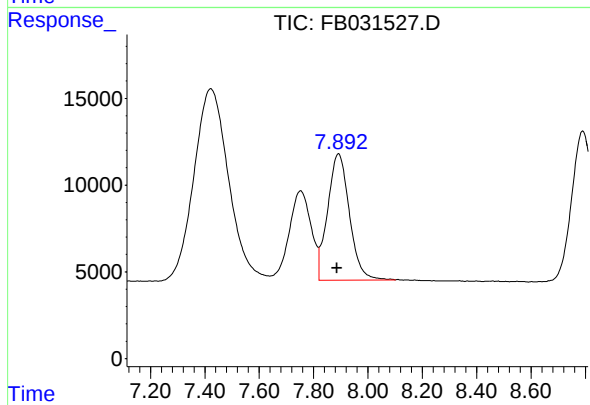

#4 Benzene


R.T.: 7.893 min
Delta R.T.: 0.007 min
Response: 406179
Conc: 9.15 ng/ml

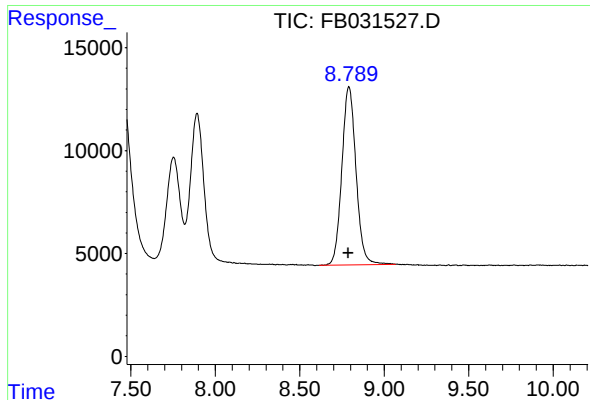

#5 AAA-TFT


R.T.: 8.791 min
Delta R.T.: 0.004 min
Response: 504773
Conc: 21.47 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0303S1

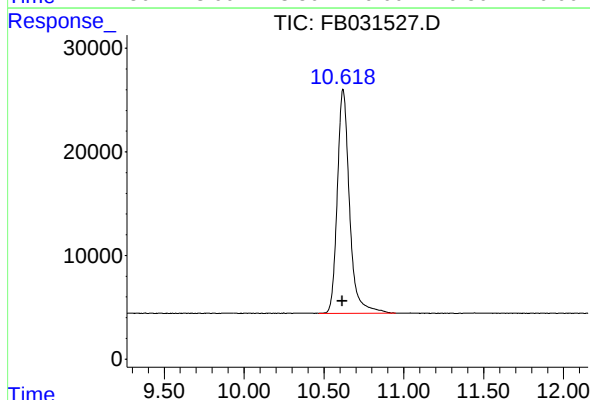


#6 Toluene

R.T.: 10.619 min
Delta R.T.: 0.004 min
Response: 1147791
Conc: 27.94 ng/ml

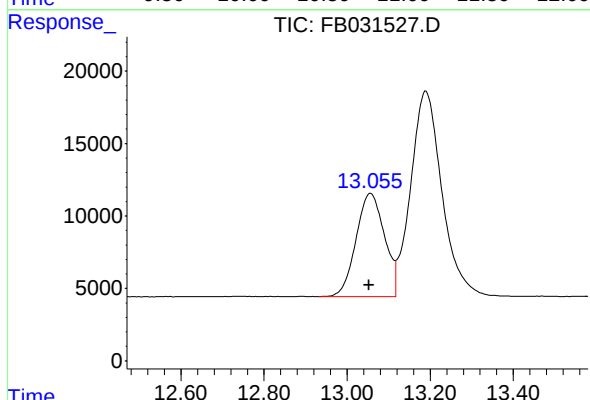


#7 Ethylbenzene

R.T.: 13.057 min
Delta R.T.: 0.004 min
Response: 338939
Conc: 9.34 ng/ml

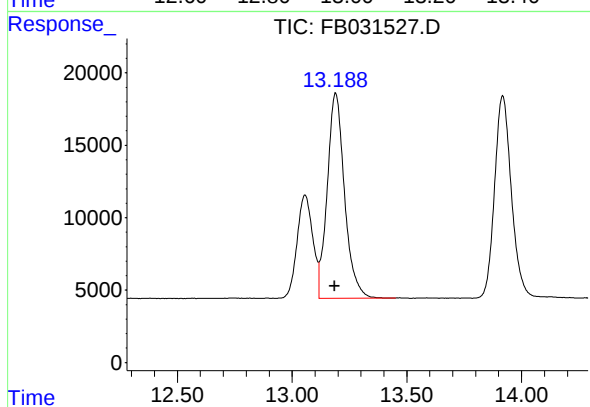

#8 m-Xylene


R.T.: 13.190 min
Delta R.T.: 0.004 min
Response: 742697
Conc: 18.90 ng/ml

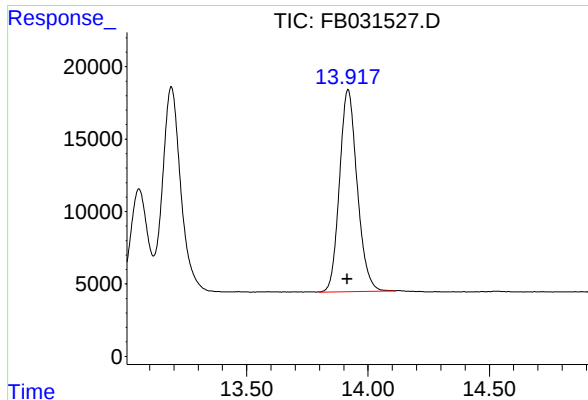

#9 O-Xylene

R.T.: 13.918 min
Delta R.T.: 0.004 min
Response: 706790
Conc: 18.90 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0303S1

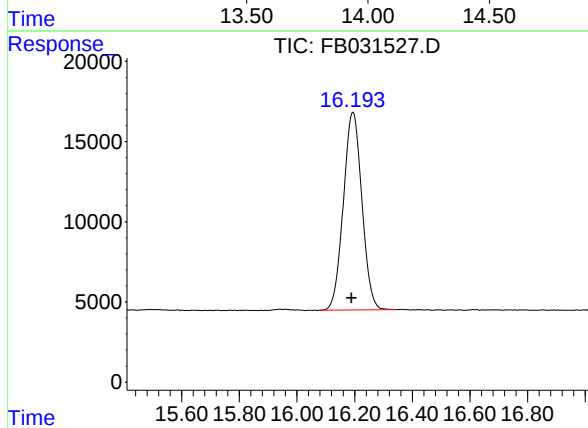

#10 1,2,4-Trimethylbenzene

R.T.: 16.194 min
Delta R.T.: 0.004 min
Response: 547036
Conc: 18.46 ng/ml