

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB030325\
 Data File : FB031538.D
 Signal(s) : FID2B.CH
 Acq On : 3 Mar 2025 19:29
 Operator : YP/AJ
 Sample : BSF0303S3
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0303S3

Integration File: SAMPLE.e
 Quant Time: Mar 04 00:21:30 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB021125.M
 Quant Title :
 QLast Update : Tue Feb 11 12:33:57 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.789	387937	16.501 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.717	1028200	32.188 ng/ml
2) t 2,2,4-Trimethylpentane	7.419	1227630	31.551 ng/ml
3) t n-Heptane	7.751	358871	10.419 ng/ml
4) t Benzene	7.890	466653	10.511 ng/ml
6) t Toluene	10.619	1307172	31.822 ng/ml
7) t Ethylbenzene	13.056	378319	10.420 ng/ml
8) t m-Xylene	13.189	825321	21.004 ng/ml
9) t O-Xylene	13.918	792185	21.179 ng/ml
10) t 1,2,4-Trimethylbenzene	16.194	588806	19.869 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB030325\
Data File : FB031538.D
Signal(s) : FID2B.CH
Acq On : 3 Mar 2025 19:29
Operator : YP/AJ
Sample : BSF0303S3
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0303S3

Integration File: SAMPLE.e
Quant Time: Mar 04 00:21:30 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB021125.M
Quant Title :
QLast Update : Tue Feb 11 12:33:57 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

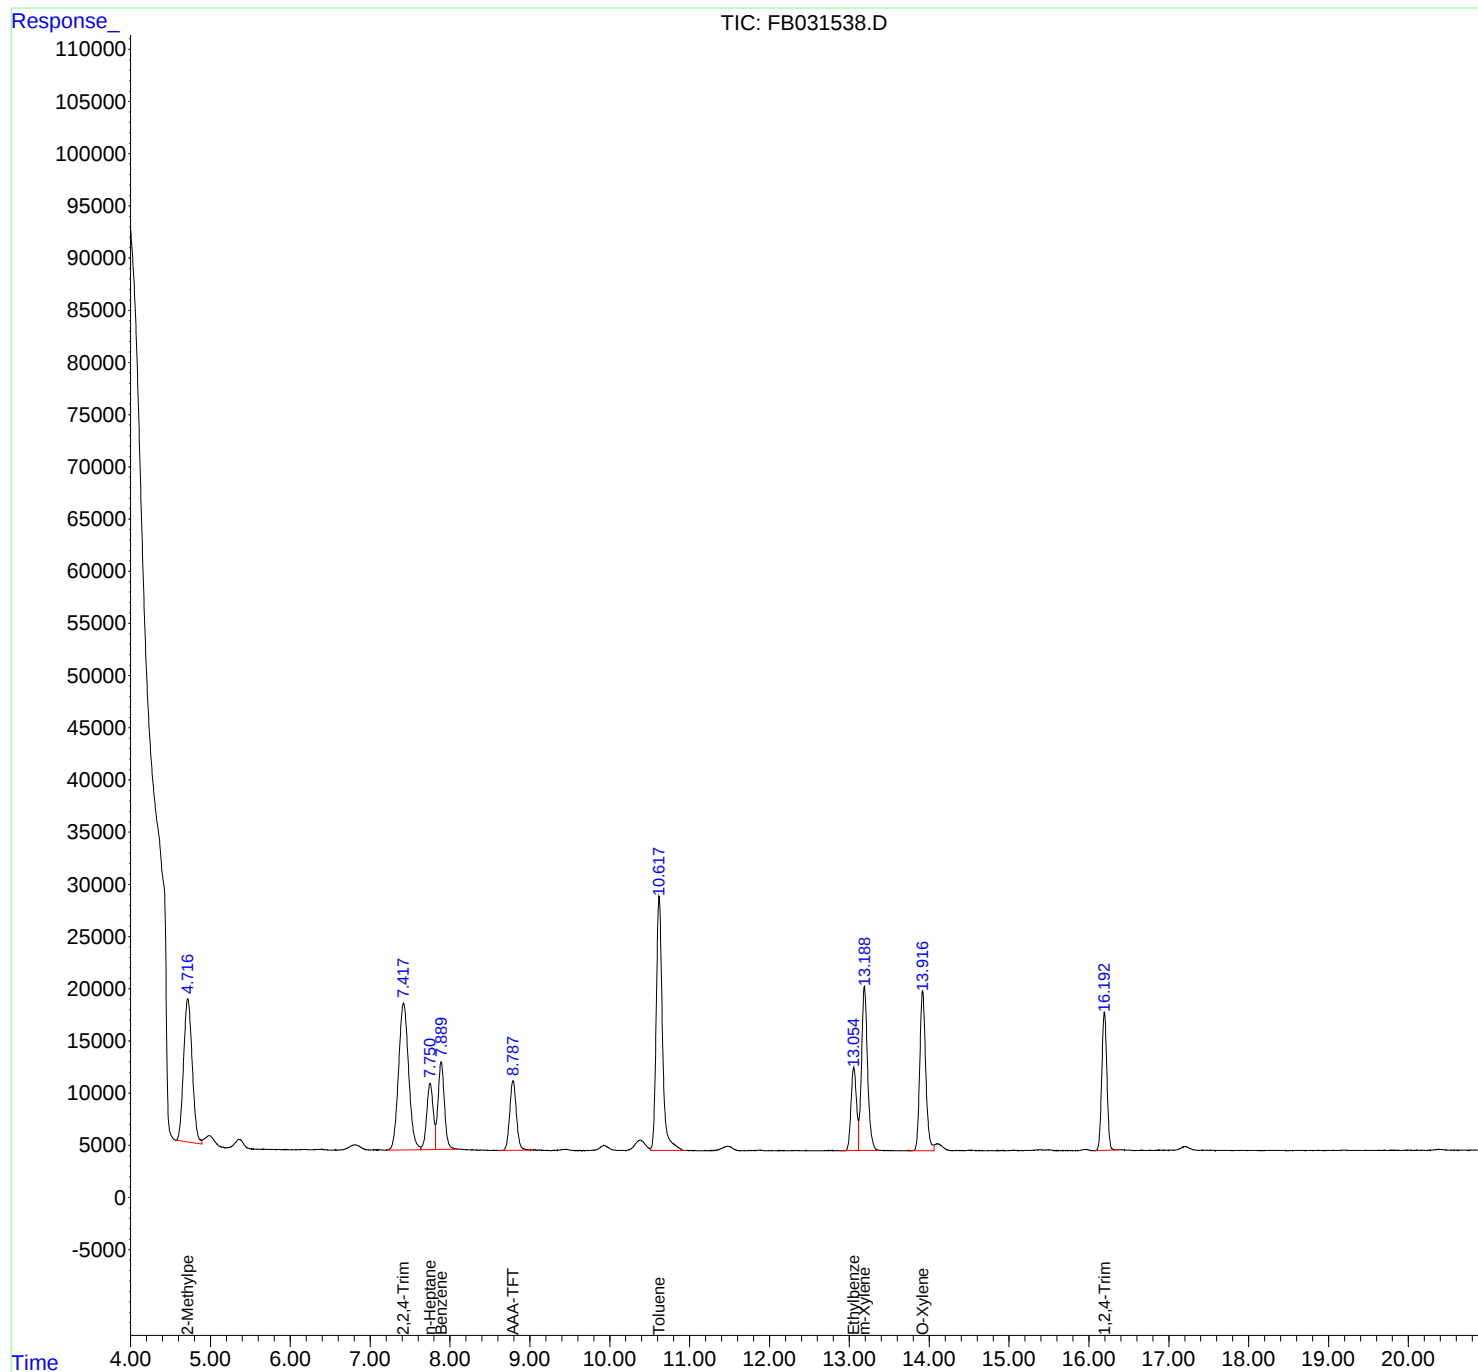


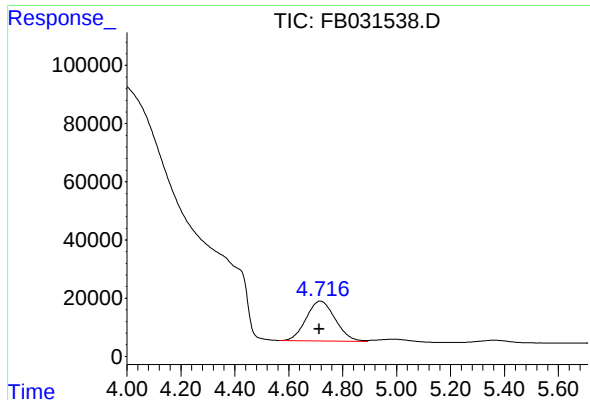

#1 2-Methylpentane


R.T.: 4.717 min
Delta R.T.: 0.003 min
Response: 1028200
Conc: 32.19 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0303S3

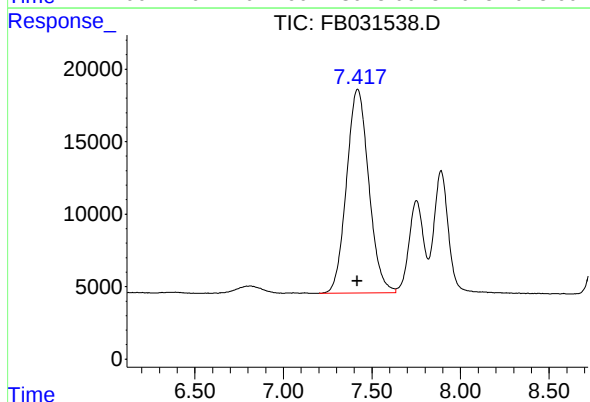


#2 2,2,4-Trimethylpentane

R.T.: 7.419 min
Delta R.T.: 0.003 min
Response: 1227630
Conc: 31.55 ng/ml

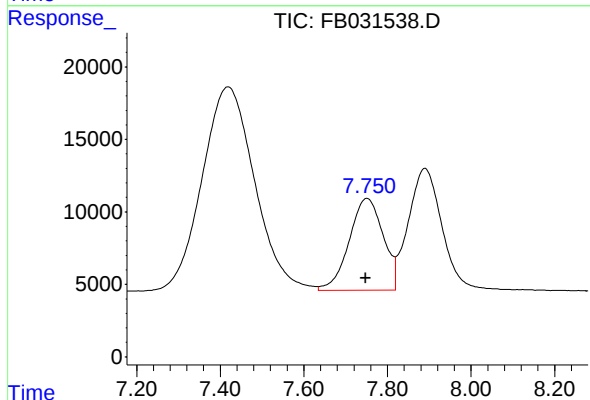


#3 n-Heptane

R.T.: 7.751 min
Delta R.T.: 0.004 min
Response: 358871
Conc: 10.42 ng/ml

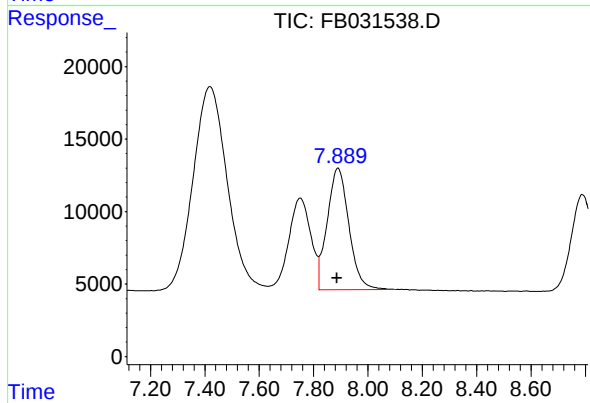

#4 Benzene


R.T.: 7.890 min
Delta R.T.: 0.005 min
Response: 466653
Conc: 10.51 ng/ml

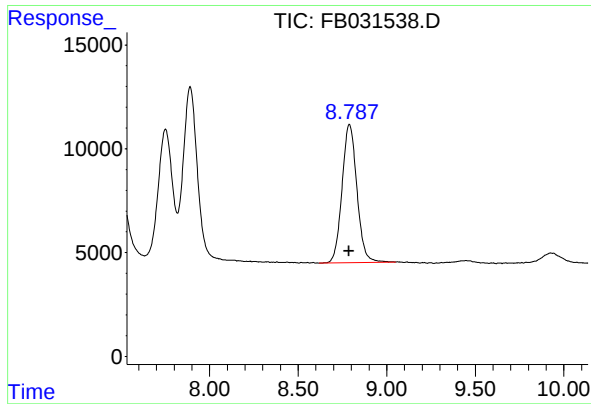

#5 AAA-TFT


R.T.: 8.789 min
Delta R.T.: 0.003 min
Response: 387937
Conc: 16.50 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0303S3

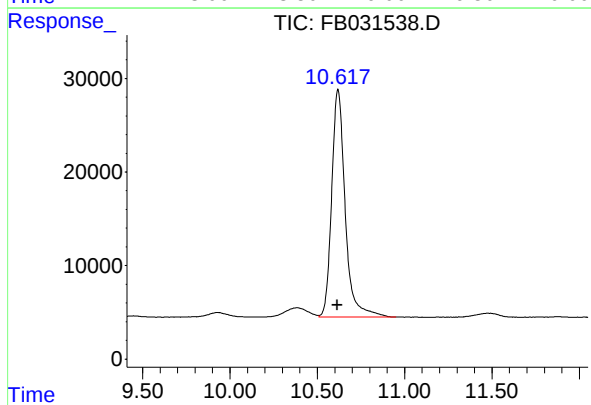


#6 Toluene

R.T.: 10.619 min
Delta R.T.: 0.004 min
Response: 1307172
Conc: 31.82 ng/ml

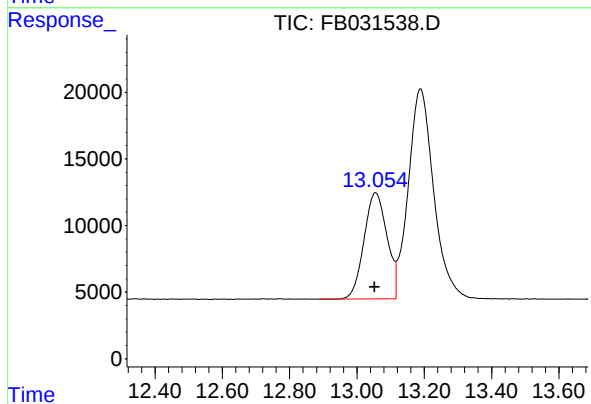


#7 Ethylbenzene

R.T.: 13.056 min
Delta R.T.: 0.003 min
Response: 378319
Conc: 10.42 ng/ml

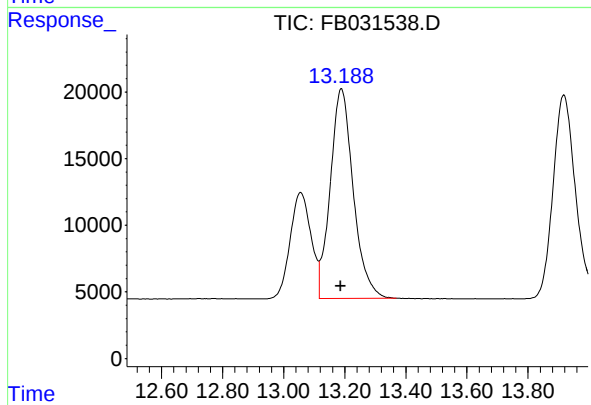

#8 m-Xylene


R.T.: 13.189 min
Delta R.T.: 0.003 min
Response: 825321
Conc: 21.00 ng/ml

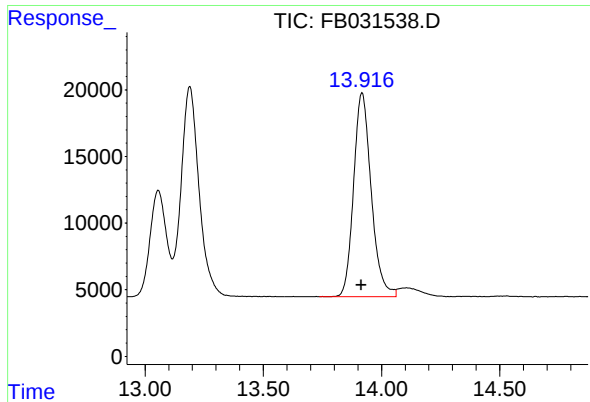

#9 O-Xylene

R.T.: 13.918 min
Delta R.T.: 0.004 min
Response: 792185
Conc: 21.18 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0303S3

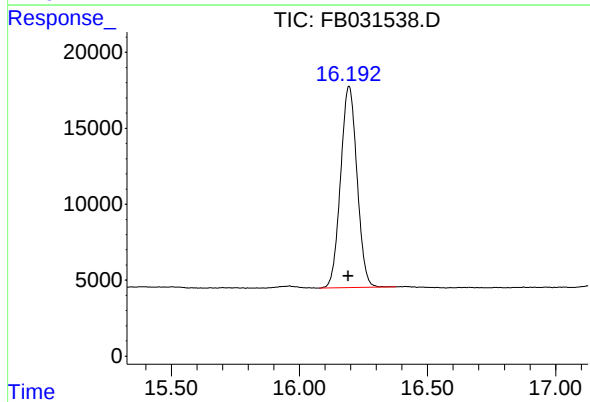

#10 1,2,4-Trimethylbenzene

R.T.: 16.194 min
Delta R.T.: 0.003 min
Response: 588806
Conc: 19.87 ng/ml