

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB030419\
 Data File : FB020035.D
 Signal(s) : FID2B.CH
 Acq On : 4 Mar 2019 14:41
 Operator : MJ/SJ
 Sample : K1668-03MS
 Misc : 5.00g/5.00ml DI WATER
 ALS Vial : 9 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Mar 05 02:15:53 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030119.M
 Quant Title :
 QLast Update : Fri Mar 01 06:28:25 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.042	218308	19.481 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.897	463346	22.270 ng/ml
2) t 2,2,4-Trimethylpentane	7.656	337620	16.770 ng/ml
3) t n-Heptane	7.998	80440	4.313 ng/ml
4) t Benzene	8.134	188790	9.006 ng/ml
6) t Toluene	10.890	501868	26.481 ng/ml
7) t Ethylbenzene	13.341	232006	10.215 ng/ml
8) t m-Xylene	13.475	342602	14.611 ng/ml
9) t O-Xylene	14.207	407492	17.501 ng/ml
10) t 1,2,4-Trimethylbenzene	16.493	287825	12.501 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB030419\
Data File : FB020035.D
Signal(s) : FID2B.CH
Acq On : 4 Mar 2019 14:41
Operator : MJ/SJ
Sample : K1668-03MS
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 9 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Mar 05 02:15:53 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030119.M
Quant Title :
QLast Update : Fri Mar 01 06:28:25 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

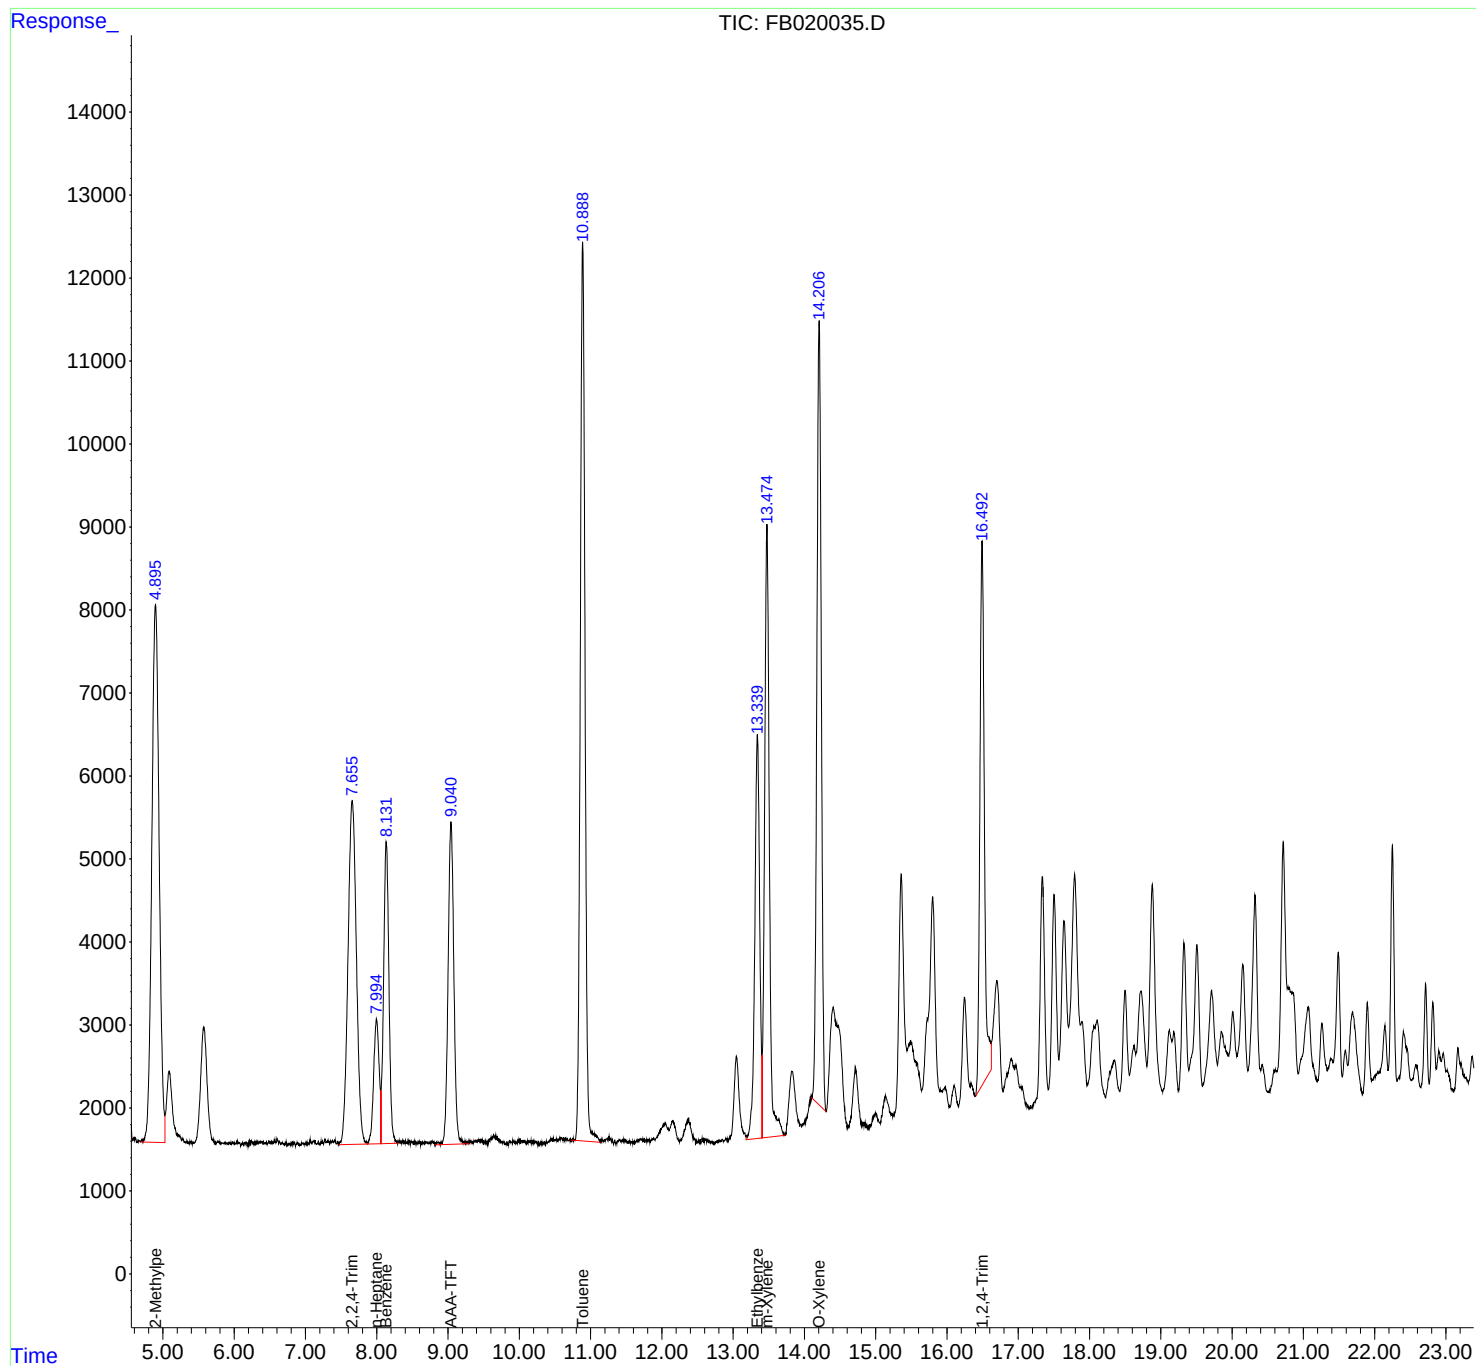

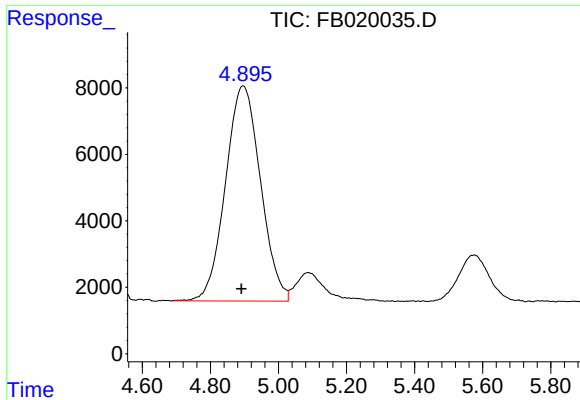


#1 2-Methylpentane

R.T.: 4.897 min
Delta R.T.: 0.006 min
Response: 463346
Conc: 22.27 ng/ml

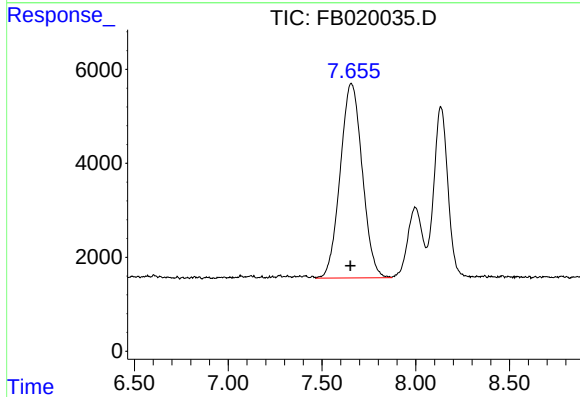


#2 2,2,4-Trimethylpentane

R.T.: 7.656 min
Delta R.T.: 0.005 min
Response: 337620
Conc: 16.77 ng/ml

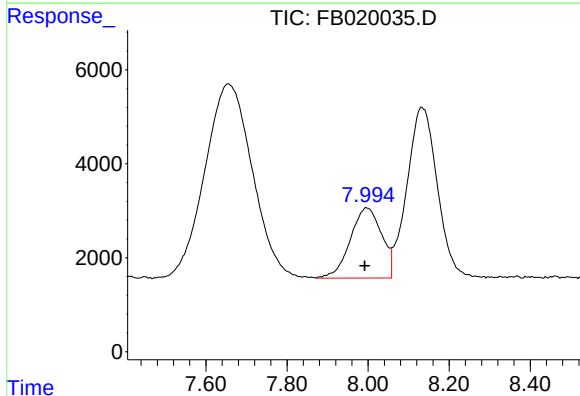


#3 n-Heptane

R.T.: 7.998 min
Delta R.T.: 0.006 min
Response: 80440
Conc: 4.31 ng/ml

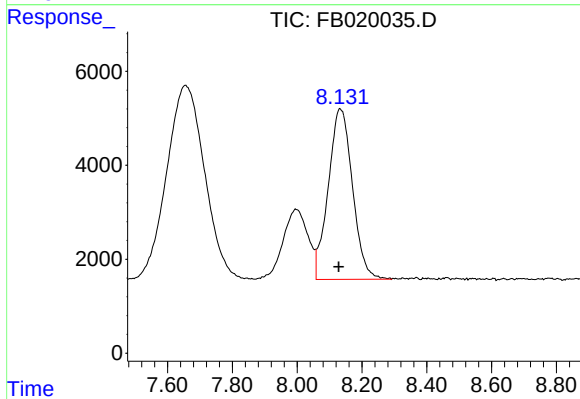


#4 Benzene

R.T.: 8.134 min
Delta R.T.: 0.005 min
Response: 188790
Conc: 9.01 ng/ml

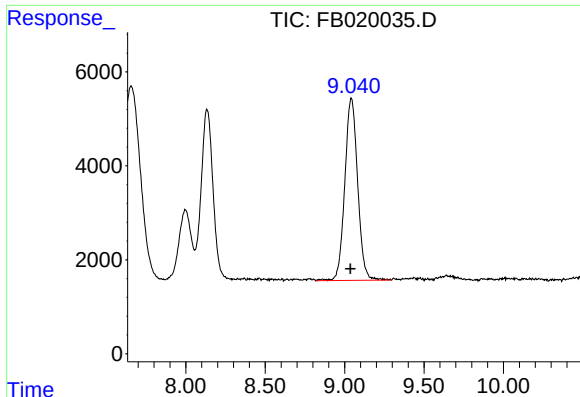


#5 AAA-TFT

R.T.: 9.042 min
Delta R.T.: 0.006 min
Response: 218308
Conc: 19.48 ng/ml

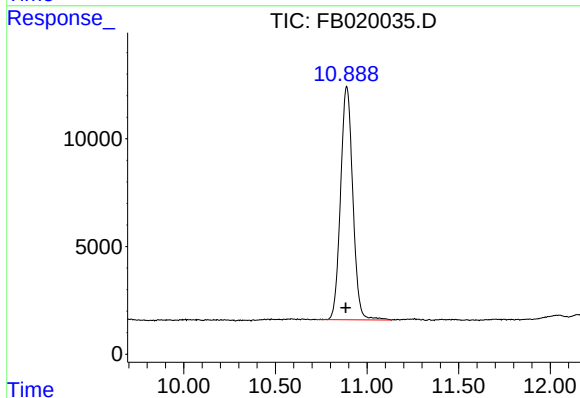


#6 Toluene

R.T.: 10.890 min
Delta R.T.: 0.006 min
Response: 501868
Conc: 26.48 ng/ml

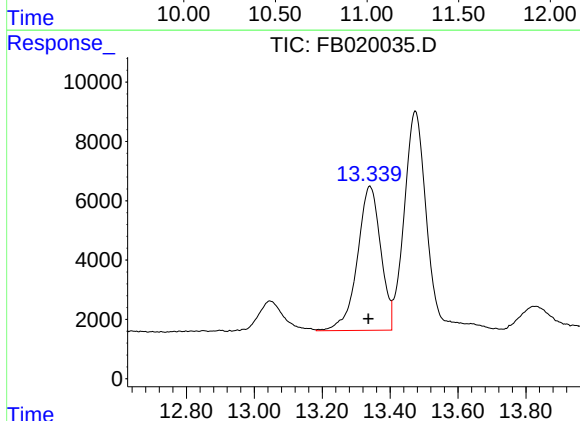


#7 Ethylbenzene

R.T.: 13.341 min
Delta R.T.: 0.005 min
Response: 232006
Conc: 10.22 ng/ml

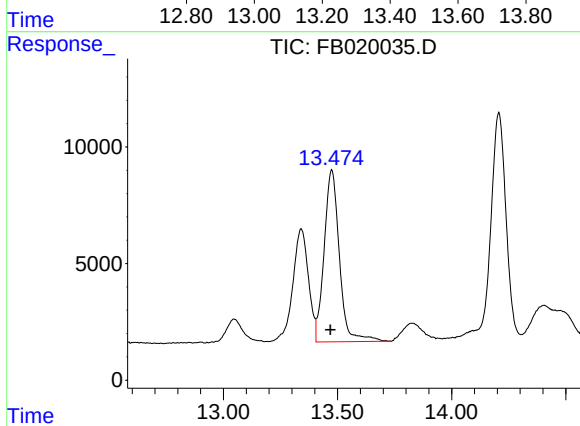


#8 m-Xylene

R.T.: 13.475 min
Delta R.T.: 0.006 min
Response: 342602
Conc: 14.61 ng/ml

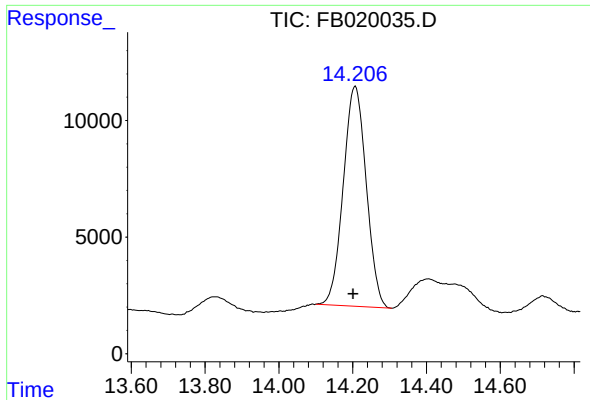

#9 O-Xylene

R.T.: 14.207 min
Delta R.T.: 0.006 min
Response: 407492
Conc: 17.50 ng/ml

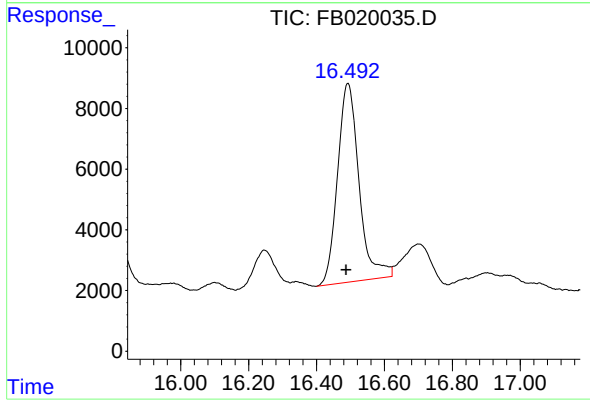

#10 1,2,4-Trimethylbenzene

R.T.: 16.493 min
Delta R.T.: 0.006 min
Response: 287825
Conc: 12.50 ng/ml