

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB030420\
 Data File : FB023781.D
 Signal(s) : FID2B.CH
 Acq On : 4 Mar 2020 9:57
 Operator : DD/AJ
 Sample : BSF0304S1
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Mar 05 00:20:32 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB020620.M
 Quant Title :
 QLast Update : Thu Feb 06 11:13:47 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.797	403462	19.817 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.688	809759	26.911 ng/ml
2) t 2,2,4-Trimethylpentane	7.415	944113	28.933 ng/ml
3) t n-Heptane	7.756	296255	9.208 ng/ml
4) t Benzene	7.890	387433	9.472 ng/ml
6) t Toluene	10.629	1133465	28.554 ng/ml
7) t Ethylbenzene	13.070	359603	9.673 ng/ml
8) t m-Xylene	13.203	694081	19.436 ng/ml
9) t O-Xylene	13.931	669040	19.398 ng/ml
10) t 1,2,4-Trimethylbenzene	16.209	563264	19.238 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB030420\
Data File : FB023781.D
Signal(s) : FID2B.CH
Acq On : 4 Mar 2020 9:57
Operator : DD/AJ
Sample : BSF0304S1
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Mar 05 00:20:32 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB020620.M
Quant Title :
QLast Update : Thu Feb 06 11:13:47 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

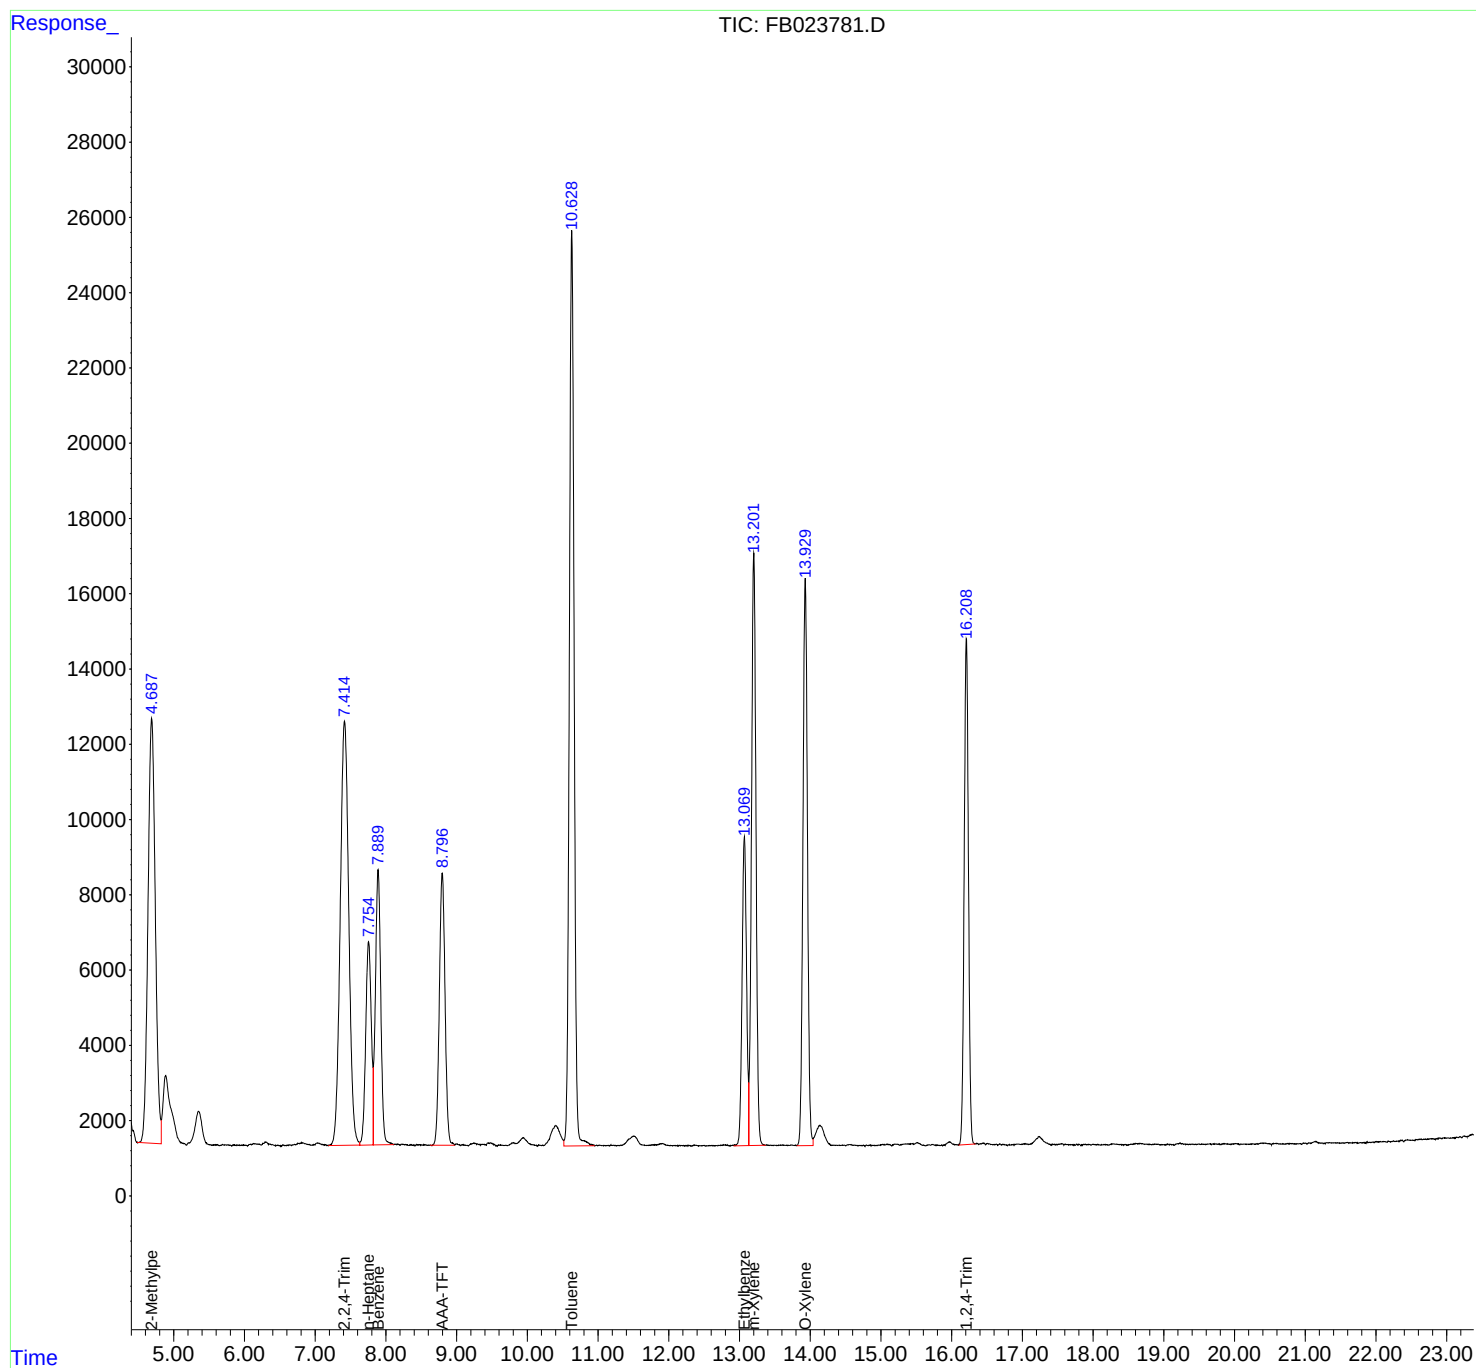

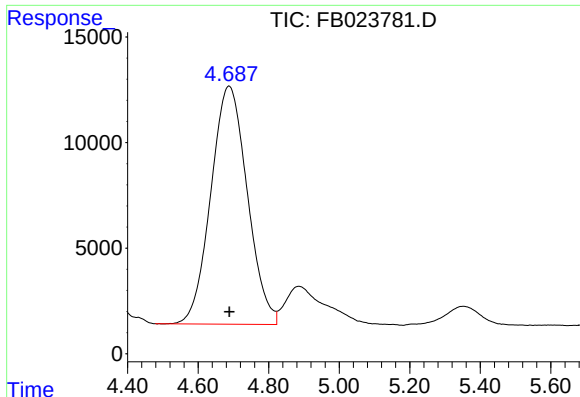


#1 2-Methylpentane

R.T.: 4.688 min
Delta R.T.: 0.000 min
Response: 809759
Conc: 26.91 ng/ml

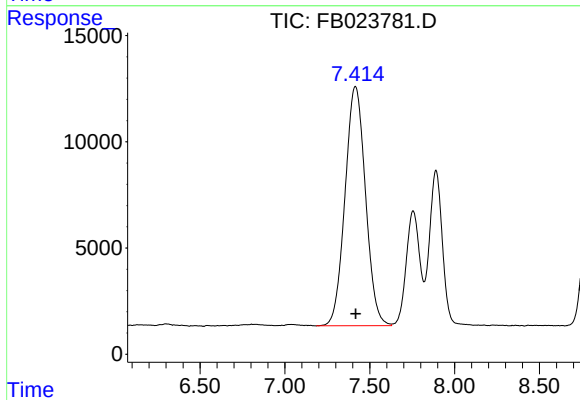


#2 2,2,4-Trimethylpentane

R.T.: 7.415 min
Delta R.T.: -0.003 min
Response: 944113
Conc: 28.93 ng/ml

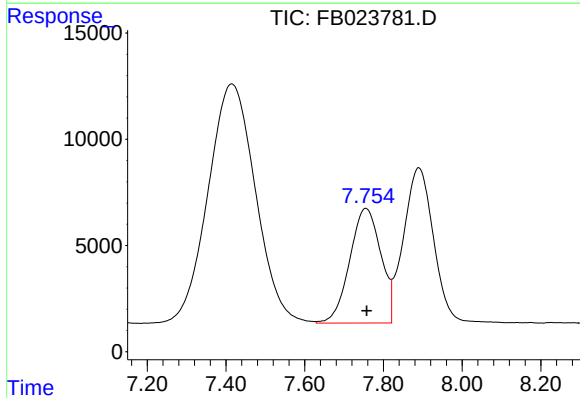


#3 n-Heptane

R.T.: 7.756 min
Delta R.T.: -0.002 min
Response: 296255
Conc: 9.21 ng/ml

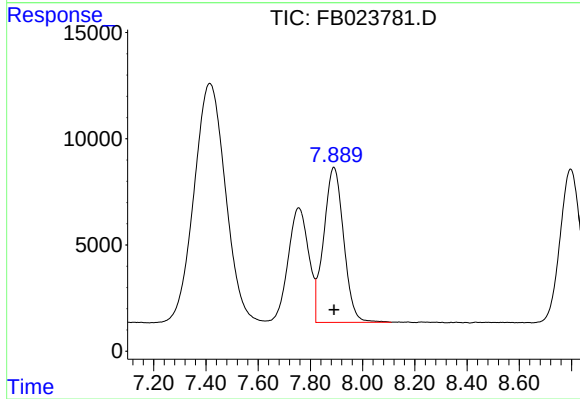


#4 Benzene

R.T.: 7.890 min
Delta R.T.: -0.001 min
Response: 387433
Conc: 9.47 ng/ml

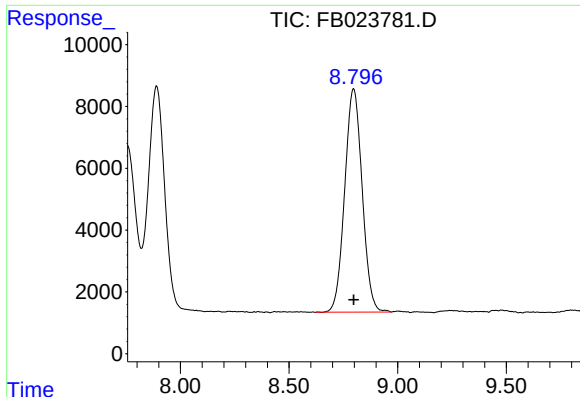


#5 AAA-TFT

R.T.: 8.797 min
Delta R.T.: -0.001 min
Response: 403462
Conc: 19.82 ng/ml

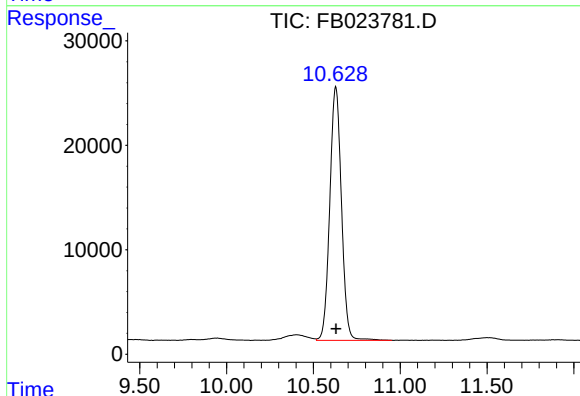


#6 Toluene

R.T.: 10.629 min
Delta R.T.: -0.001 min
Response: 1133465
Conc: 28.55 ng/ml

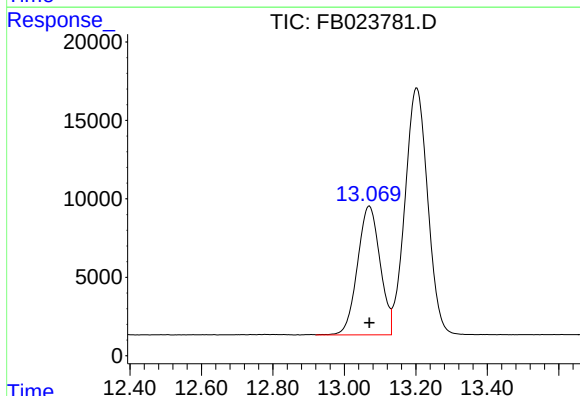


#7 Ethylbenzene

R.T.: 13.070 min
Delta R.T.: 0.000 min
Response: 359603
Conc: 9.67 ng/ml

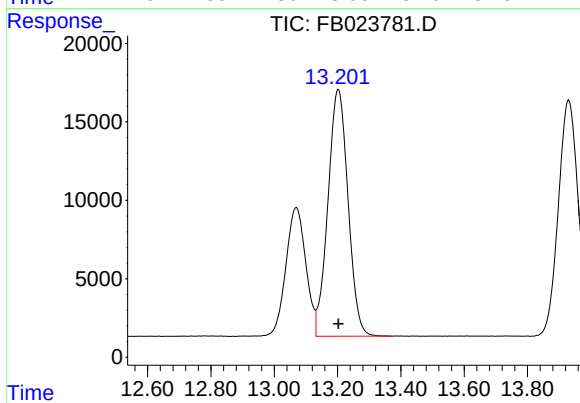


#8 m-Xylene

R.T.: 13.203 min
Delta R.T.: 0.000 min
Response: 694081
Conc: 19.44 ng/ml

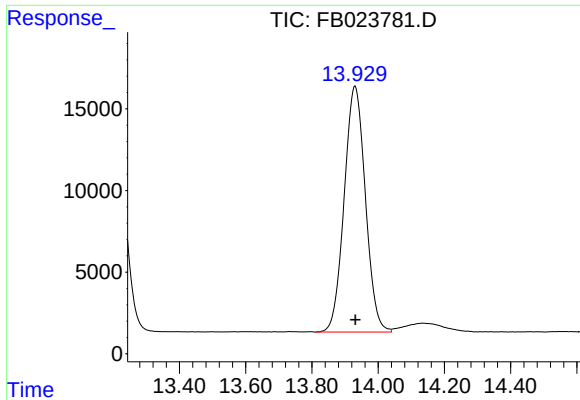

#9 O-Xylene

R.T.: 13.931 min
Delta R.T.: 0.000 min
Response: 669040
Conc: 19.40 ng/ml

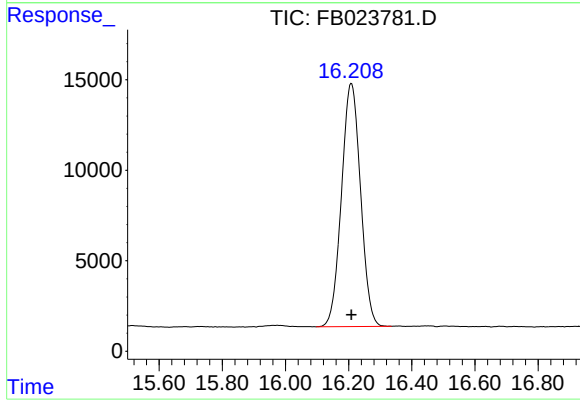

#10 1,2,4-Trimethylbenzene

R.T.: 16.209 min
Delta R.T.: 0.000 min
Response: 563264
Conc: 19.24 ng/ml