

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB030425\  
Data File : FB031541.D  
Signal(s) : FID2B.CH  
Acq On : 4 Mar 2025 11:14  
Operator : YP/AJ  
Sample : VBF0304W1  
Misc :  
ALS Vial : 2 Sample Multiplier: 1

Instrument :  
FID\_B  
ClientSampleId :

Integration File: Calibration.e  
Quant Time: Mar 05 02:06:38 2025  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB021125.M  
Quant Title :  
QLast Update : Tue Feb 11 12:33:57 2025  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 5 g/ml  
Signal Phase : RTX-502.2  
Signal Info : 60mx0.53mmx3.00um

| Compound                     | R.T.   | Response | Conc Units   |
|------------------------------|--------|----------|--------------|
| -----                        |        |          |              |
| System Monitoring Compounds  |        |          |              |
| 5) s AAA-TFT                 | 8.786  | 394351   | 16.774 ng/ml |
| Target Compounds             |        |          |              |
| 6) t Toluene                 | 10.609 | 7022     | 0.171 ng/ml  |
| 8) t m-Xylene                | 13.186 | 8045     | 0.205 ng/ml  |
| 9) t O-Xylene                | 13.918 | 10322    | 0.276 ng/ml  |
| 10) t 1,2,4-Trimethylbenzene | 16.188 | 18942    | 0.639 ng/ml  |
| -----                        |        |          |              |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB030425\  
Data File : FB031541.D  
Signal(s) : FID2B.CH  
Acq On : 4 Mar 2025 11:14  
Operator : YP/AJ  
Sample : VBF0304W1  
Misc :  
ALS Vial : 2 Sample Multiplier: 1

Instrument :  
FID\_B  
ClientSampleId :

Integration File: Calibration.e  
Quant Time: Mar 05 02:06:38 2025  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB021125.M  
Quant Title :  
QLast Update : Tue Feb 11 12:33:57 2025  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 5 g/ml  
Signal Phase : RTX-502.2  
Signal Info : 60mx0.53mmx3.00um

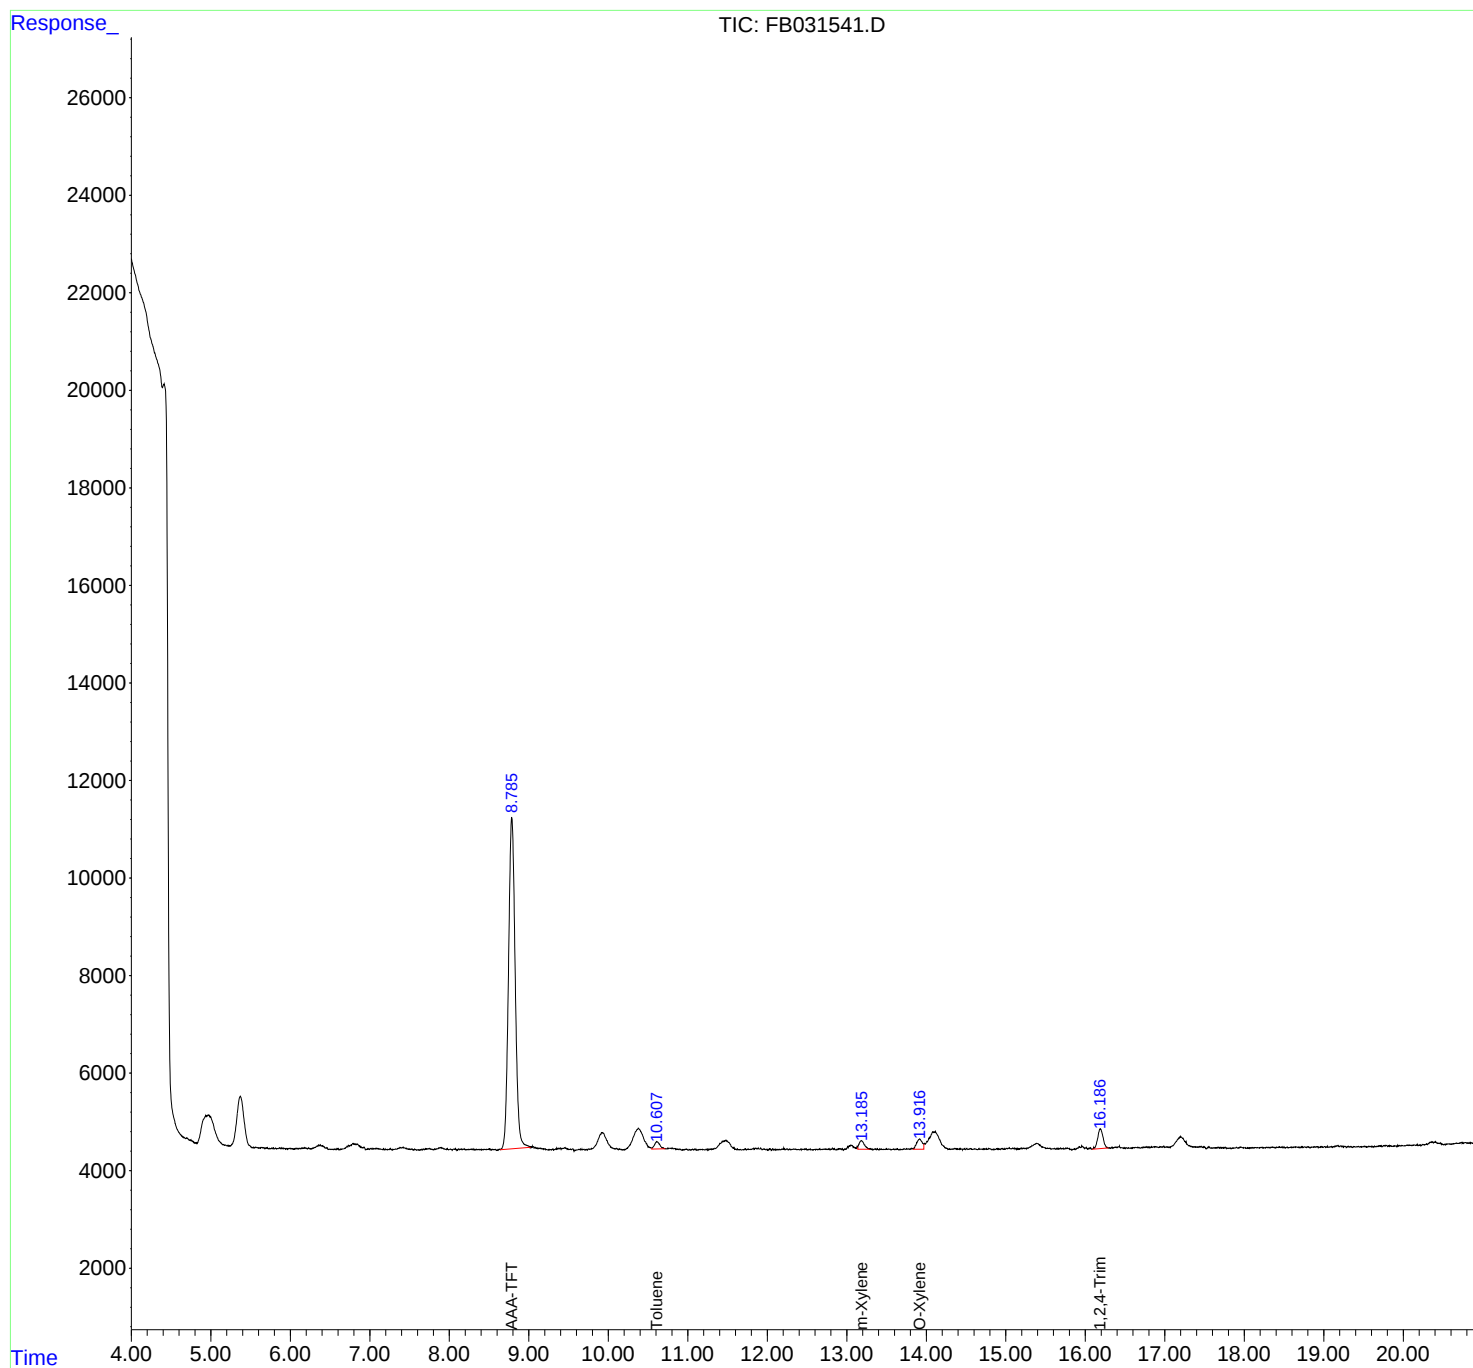


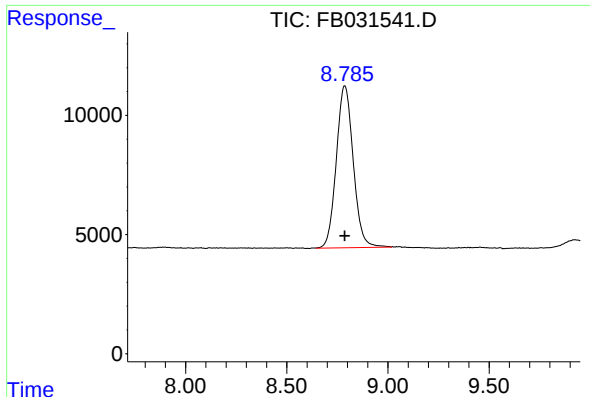

#5 AAA-TFT


R.T.: 8.786 min  
Delta R.T.: 0.000 min  
Response: 394351  
Conc: 16.77 ng/ml

Instrument :  
FID\_B  
ClientSampleId :

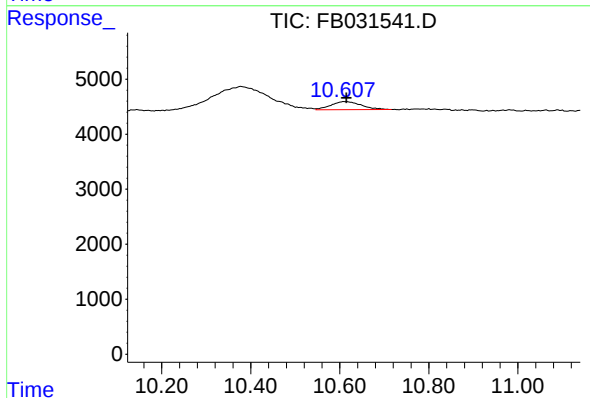


#6 Toluene

R.T.: 10.609 min  
Delta R.T.: -0.006 min  
Response: 7022  
Conc: 0.17 ng/ml

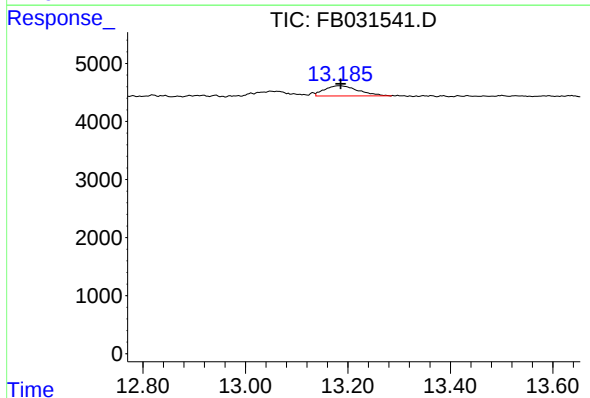


#8 m-Xylene

R.T.: 13.186 min  
Delta R.T.: 0.000 min  
Response: 8045  
Conc: 0.20 ng/ml

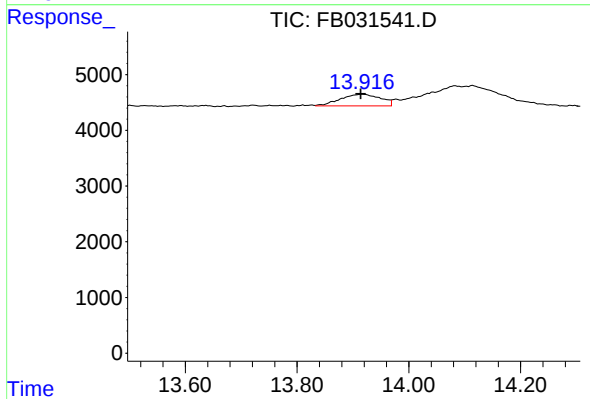

#9 O-Xylene

R.T.: 13.918 min  
Delta R.T.: 0.004 min  
Response: 10322  
Conc: 0.28 ng/ml

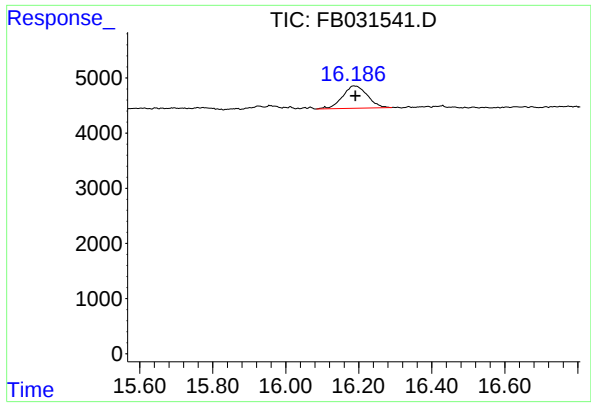

#10 1,2,4-Trimethylbenzene

R.T.: 16.188 min  
Delta R.T.: -0.003 min  
Response: 18942  
Conc: 0.64 ng/ml

Instrument :  
FID\_B  
ClientSampleId :