

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB030619\
 Data File : FB020078.D
 Signal(s) : FID2B.CH
 Acq On : 6 Mar 2019 17:49
 Operator : MJ/SJ
 Sample : K1753-02MS
 Misc : 5.03g/5.00ml DI WATER
 ALS Vial : 11 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Mar 07 08:06:24 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030119.M
 Quant Title :
 QLast Update : Fri Mar 01 06:28:25 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.040	27092	2.418 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.907	61456	2.954 ng/ml
2) t 2,2,4-Trimethylpentane	7.662	58044	2.883 ng/ml
3) t n-Heptane	7.984	9192	0.493 ng/ml
4) t Benzene	8.140	17973	0.857 ng/ml
6) t Toluene	10.893	51648	2.725 ng/ml
7) t Ethylbenzene	13.349	17040	0.750 ng/ml
8) t m-Xylene	13.475	35413	1.510 ng/ml
9) t O-Xylene	14.203	30662	1.317 ng/ml
10) t 1,2,4-Trimethylbenzene	16.491	22149	0.962 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB030619\
Data File : FB020078.D
Signal(s) : FID2B.CH
Acq On : 6 Mar 2019 17:49
Operator : MJ/SJ
Sample : K1753-02MS
Misc : 5.03g/5.00ml DI WATER
ALS Vial : 11 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Mar 07 08:06:24 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030119.M
Quant Title :
QLast Update : Fri Mar 01 06:28:25 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

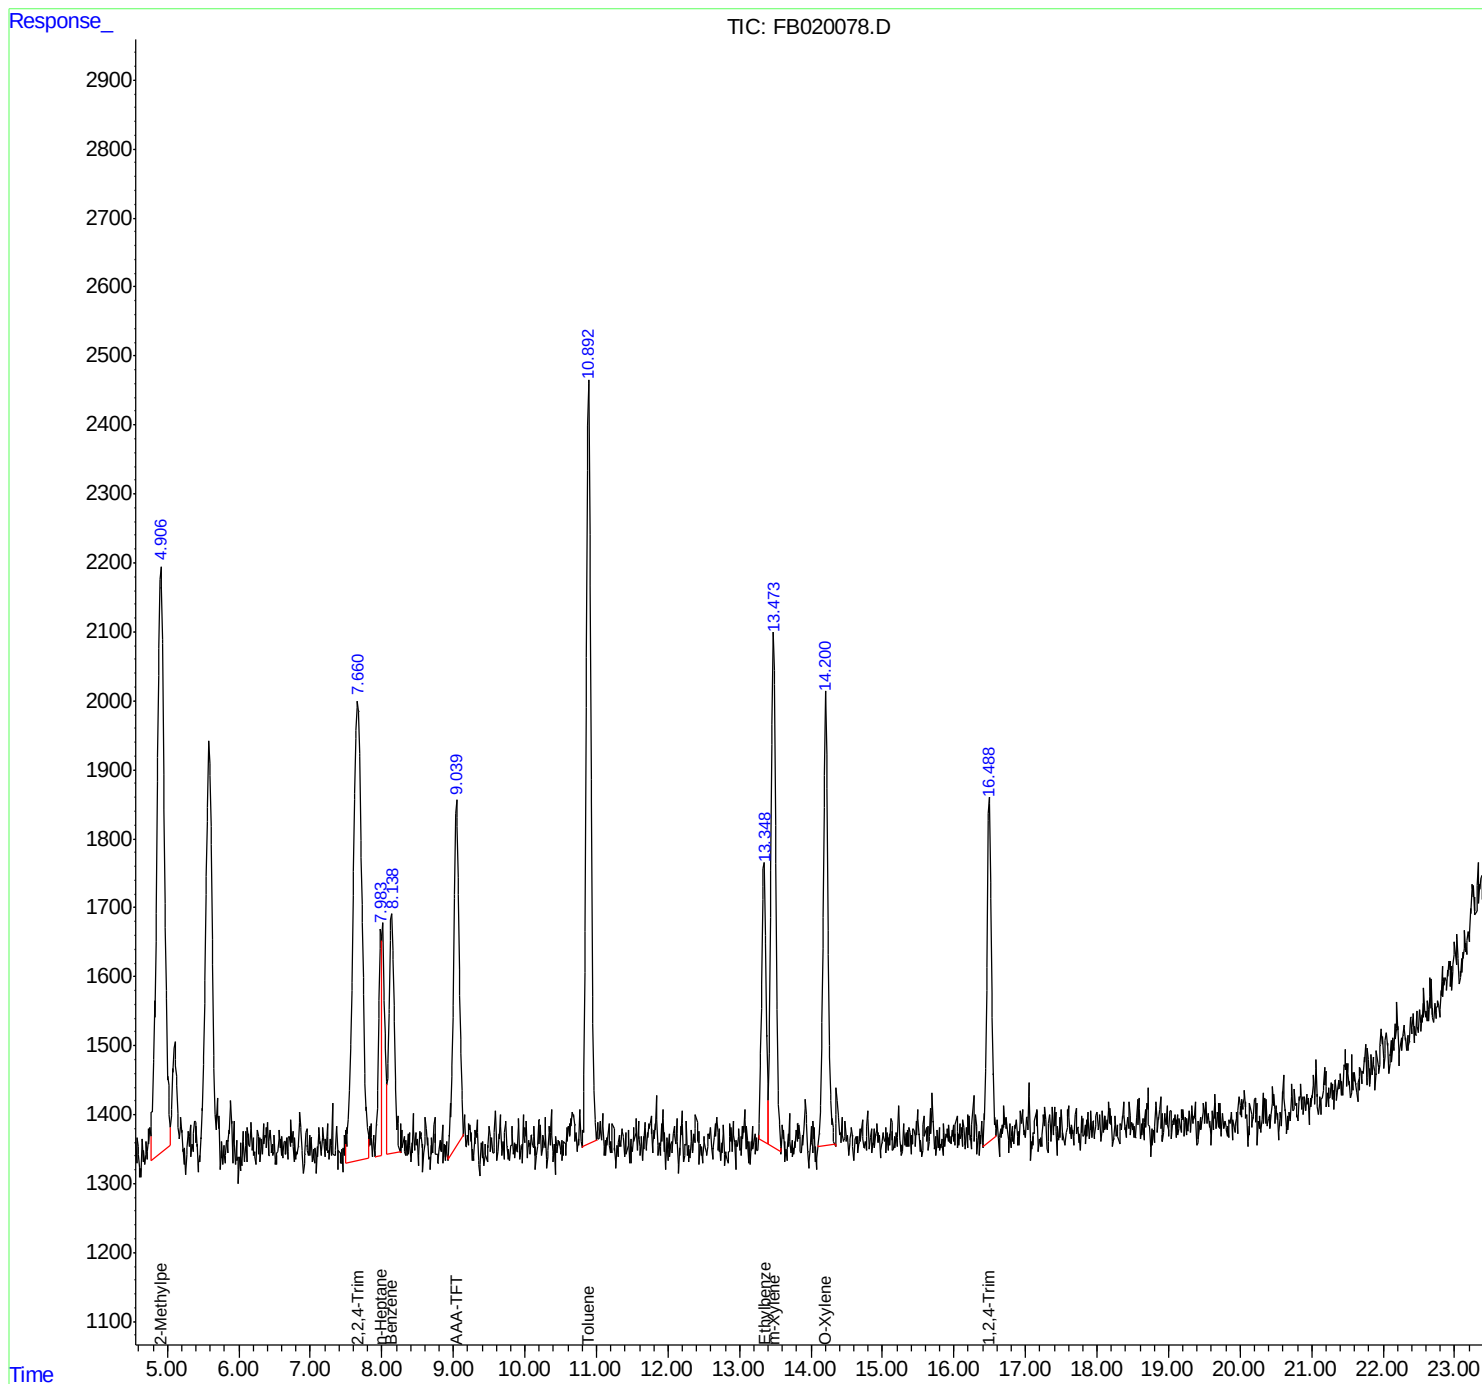

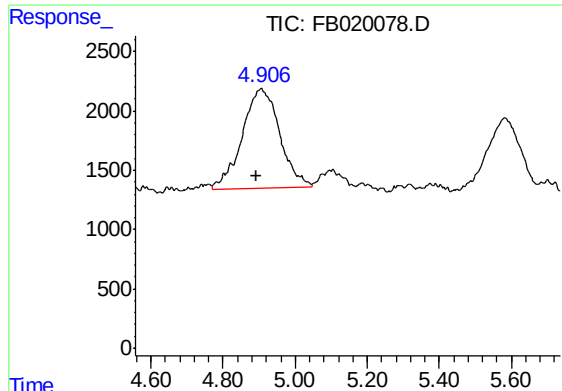


#1 2-Methylpentane

R.T.: 4.907 min
Delta R.T.: 0.016 min
Response: 61456
Conc: 2.95 ng/ml

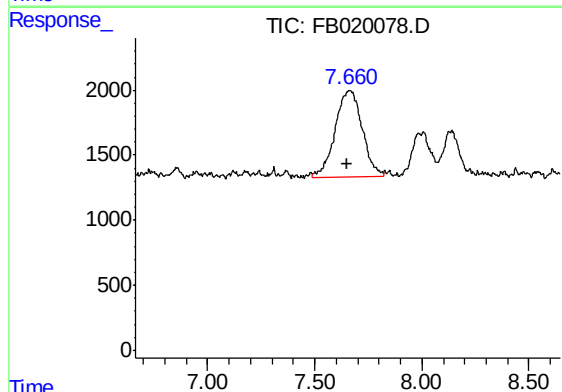


#2 2,2,4-Trimethylpentane

R.T.: 7.662 min
Delta R.T.: 0.011 min
Response: 58044
Conc: 2.88 ng/ml

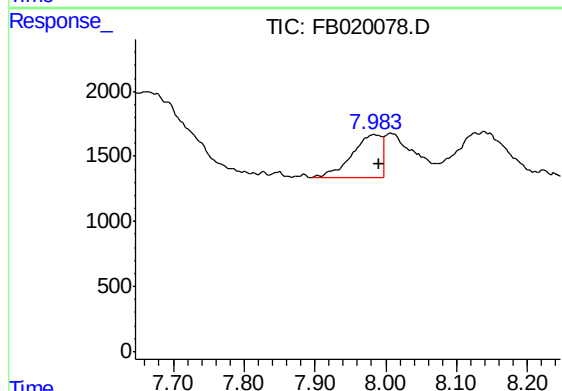


#3 n-Heptane

R.T.: 7.984 min
Delta R.T.: -0.008 min
Response: 9192
Conc: 0.49 ng/ml

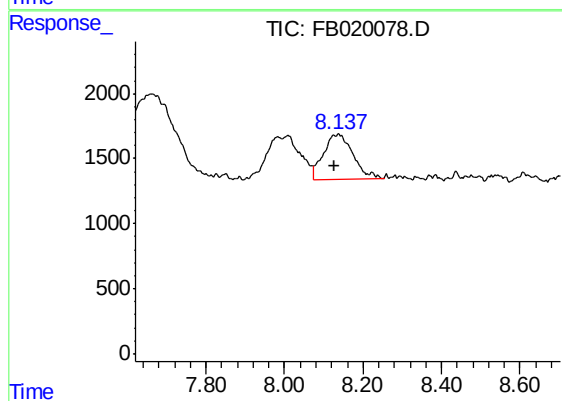


#4 Benzene

R.T.: 8.140 min
Delta R.T.: 0.011 min
Response: 17973
Conc: 0.86 ng/ml

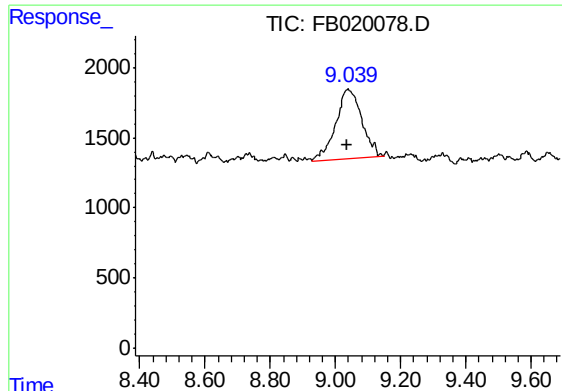


#5 AAA-TFT

R.T.: 9.040 min
Delta R.T.: 0.003 min
Response: 27092
Conc: 2.42 ng/ml

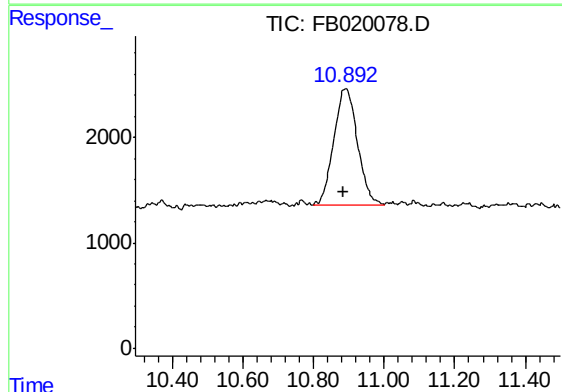


#6 Toluene

R.T.: 10.893 min
Delta R.T.: 0.009 min
Response: 51648
Conc: 2.73 ng/ml

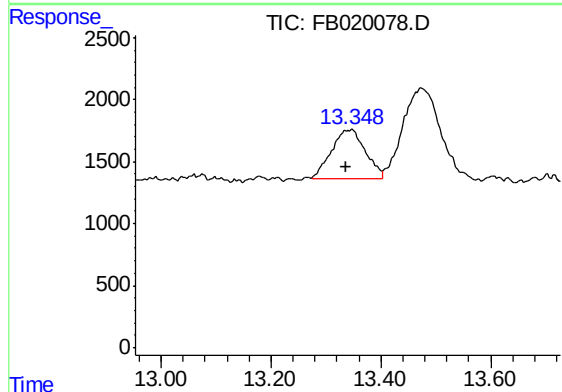


#7 Ethylbenzene

R.T.: 13.349 min
Delta R.T.: 0.013 min
Response: 17040
Conc: 0.75 ng/ml

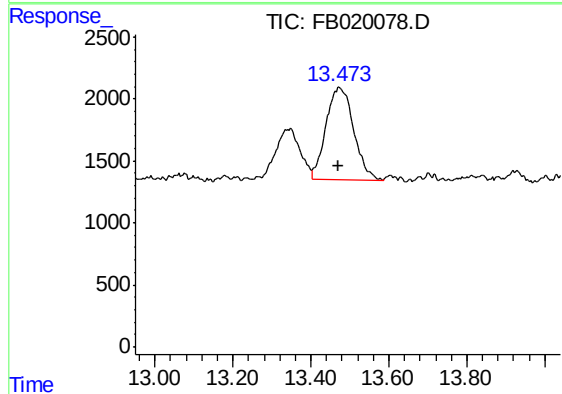


#8 m-Xylene

R.T.: 13.475 min
Delta R.T.: 0.006 min
Response: 35413
Conc: 1.51 ng/ml

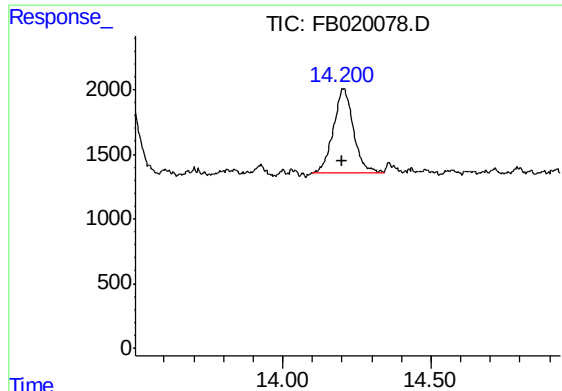

#9 O-Xylene

R.T.: 14.203 min
Delta R.T.: 0.002 min
Response: 30662
Conc: 1.32 ng/ml

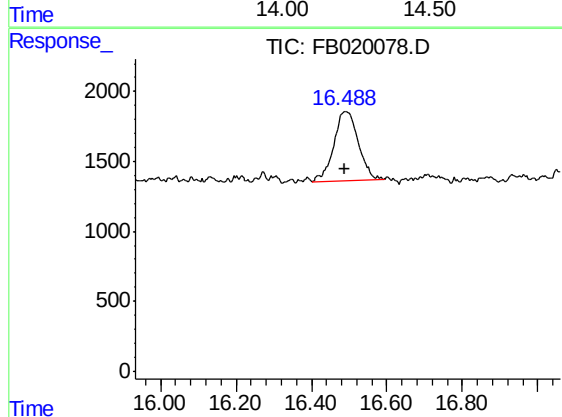

#10 1,2,4-Trimethylbenzene

R.T.: 16.491 min
Delta R.T.: 0.003 min
Response: 22149
Conc: 0.96 ng/ml